


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN101420\
Data File : BN012262.D
Acq On : 16 Oct 2020 12:08
Operator : CG/JU
Sample : PB132225BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK25

Manual Integrations
APPROVED

mohammad
10/19/2020 1:21:20 PM

Quant Time: Oct 16 13:09:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 10:51:19 2020
Response via : Initial Calibration

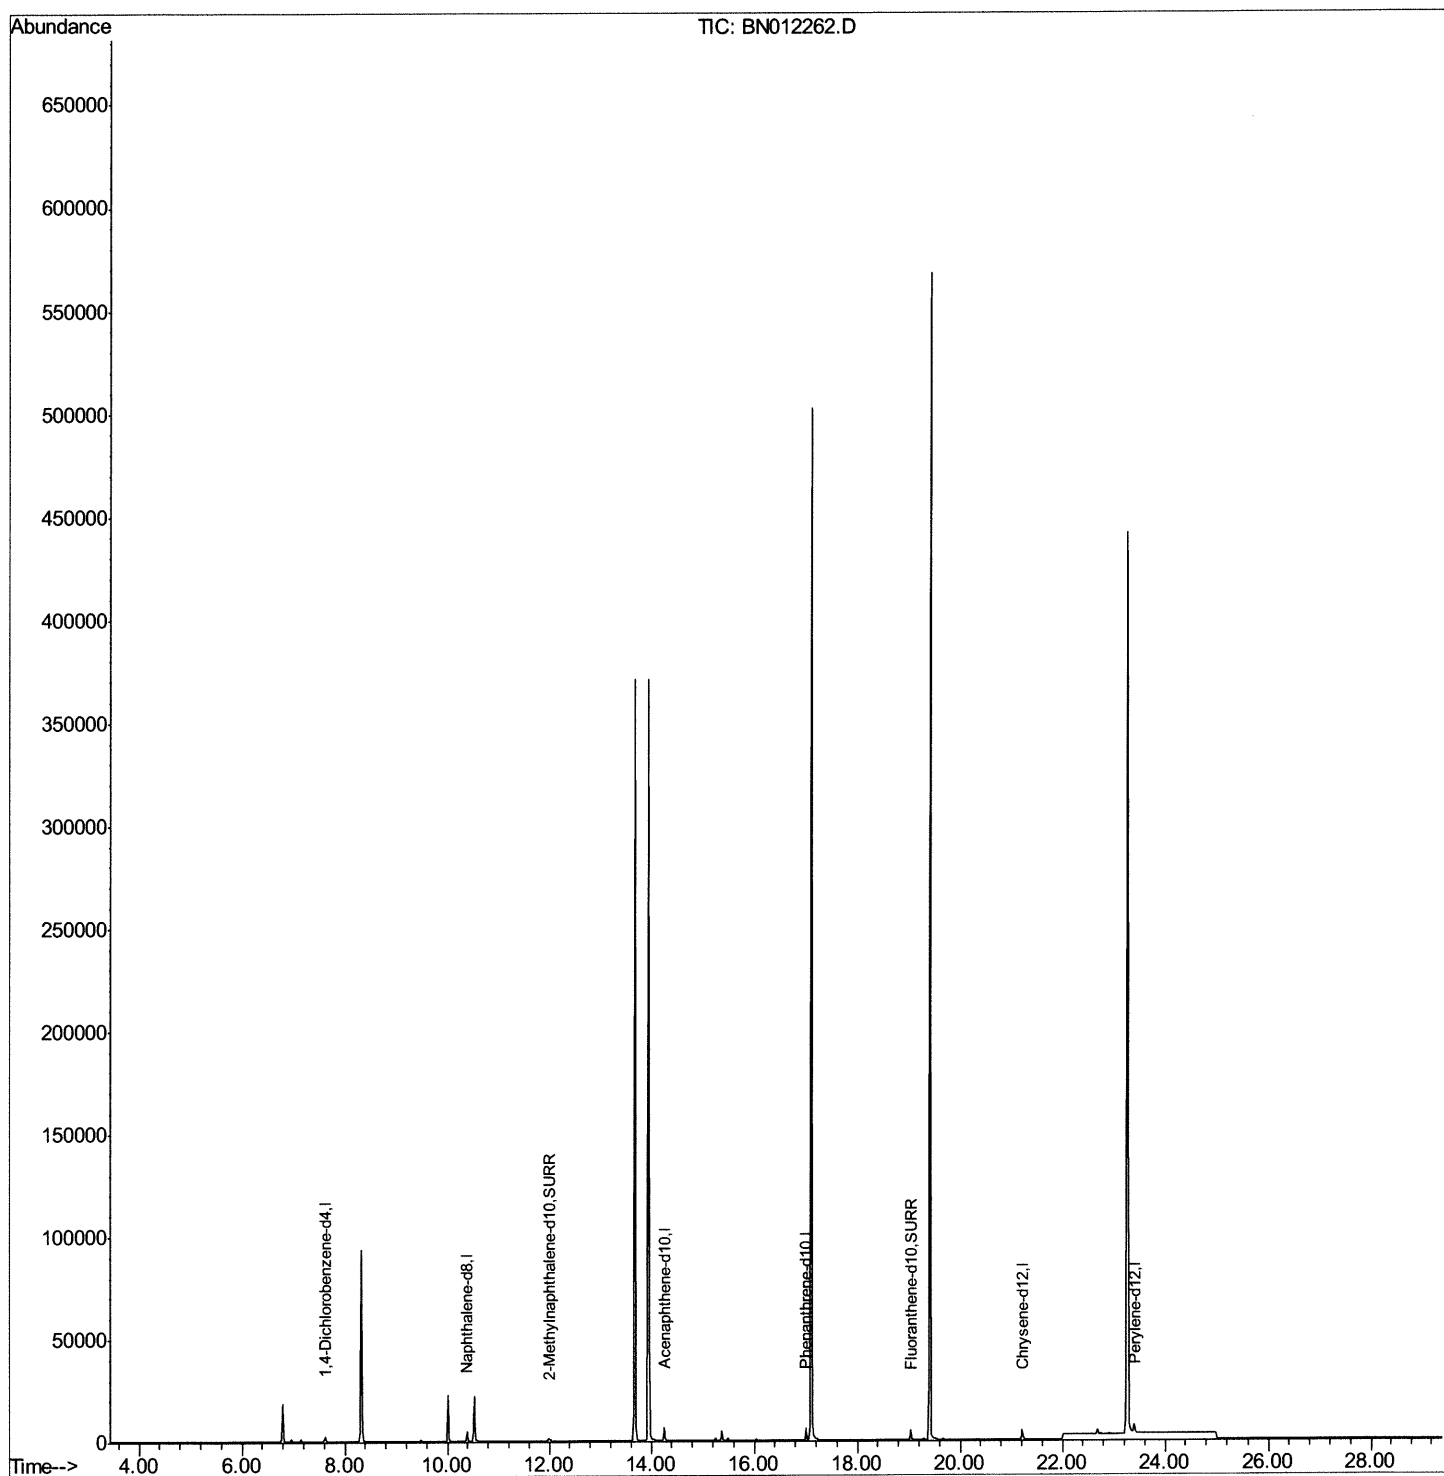

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN101420\
 Data File : BN012262.D
 Acq On : 16 Oct 2020 12:08
 Operator : CG/JU
 Sample : PB132225BL
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 SBLK25

Manual Integrations
APPROVED

mohammad
 10/19/2020 1:21:20 PM

Quant Time: Oct 16 13:05:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 16 10:51:19 2020
 Response via : Initial Calibration

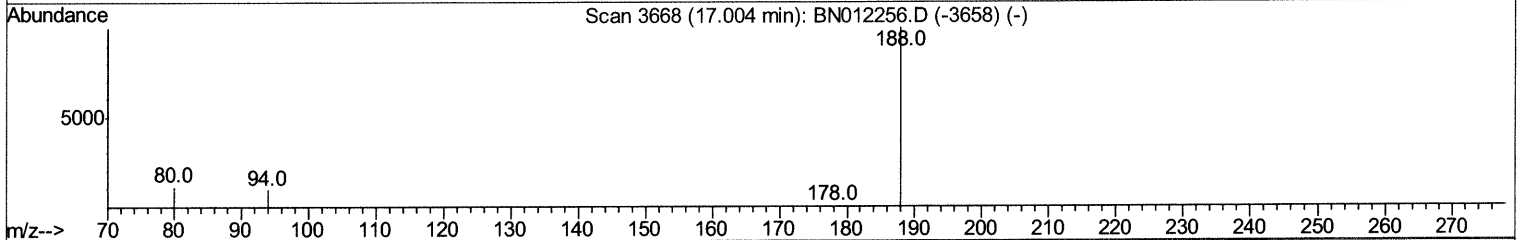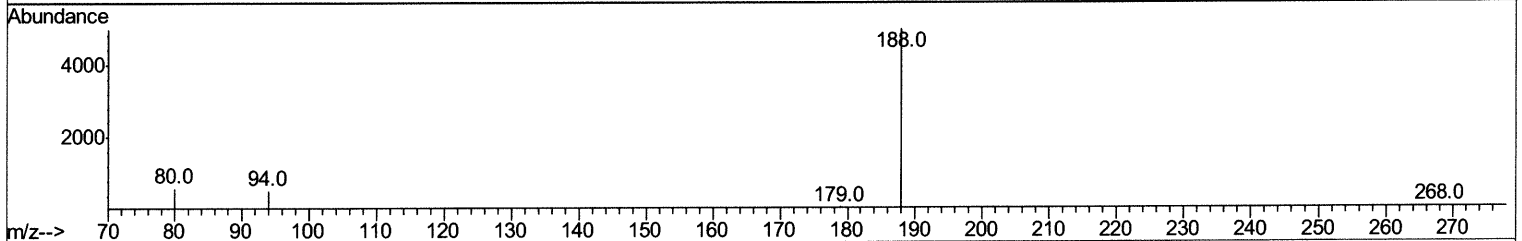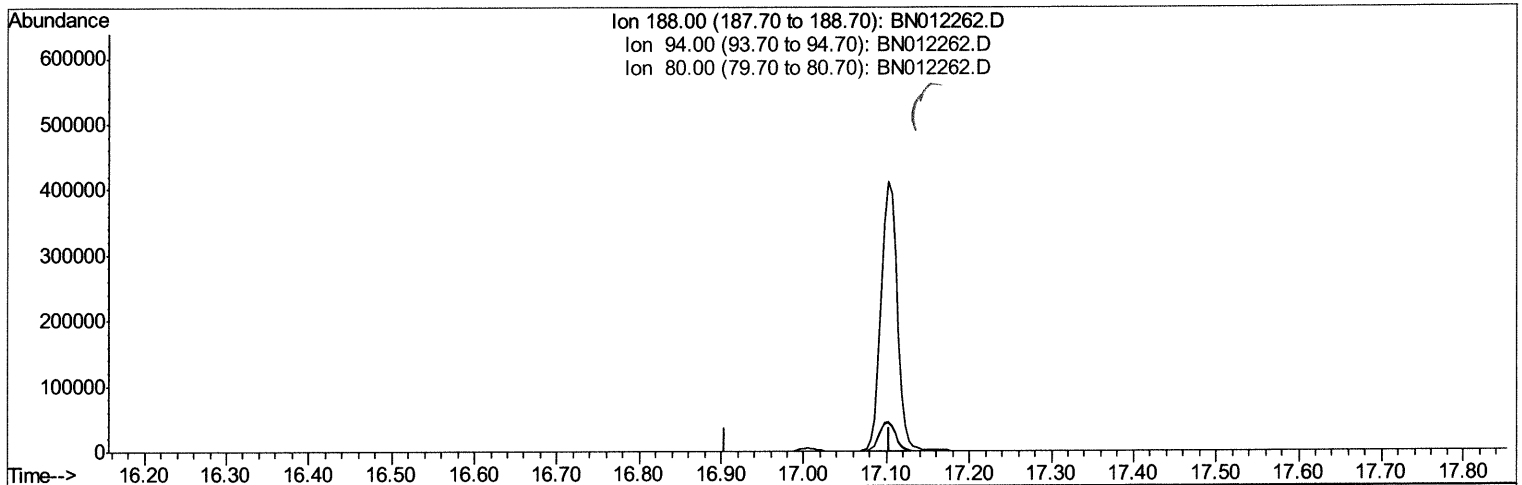

TIC: BN012262.D

(10) Phenanthrene-d10 (I)
 17.004min (-17.004) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.20	0.00#
80.00	12.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN101420\
Data File : BN012262.D
Acq On : 16 Oct 2020 12:08
Operator : CG/JU
Sample : PB132225BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK25

Manual Integrations
APPROVED

mohammad
10/19/2020 1:21:20 PM

Quant Time: Oct 16 13:05:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 10:51:19 2020
Response via : Initial Calibration

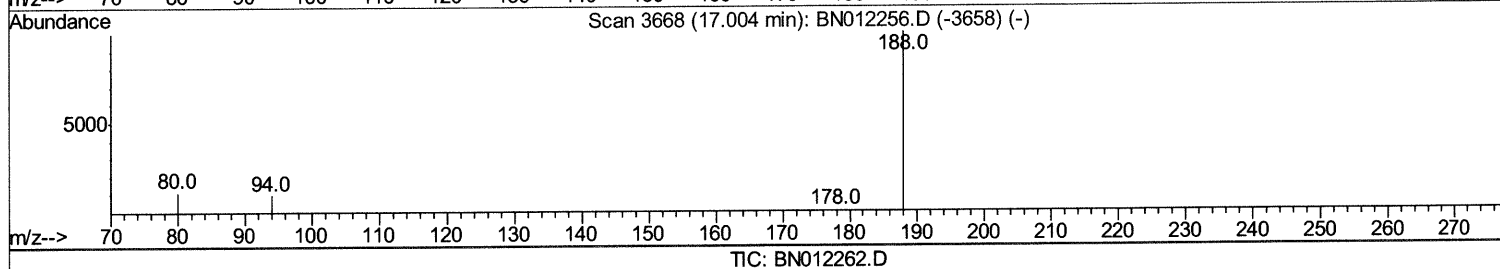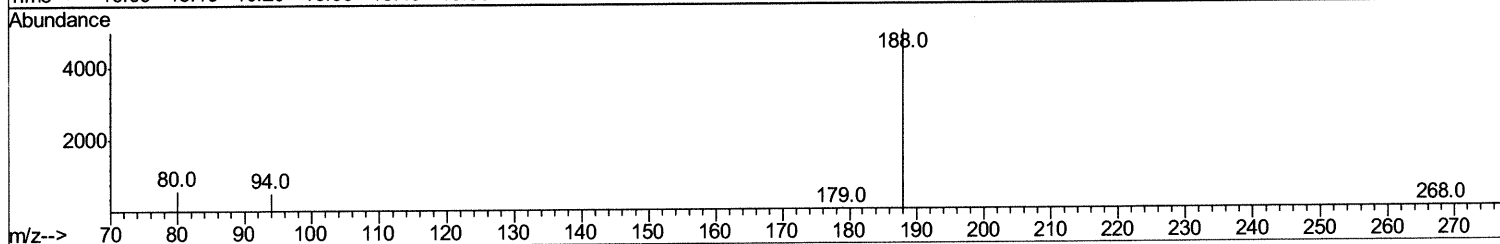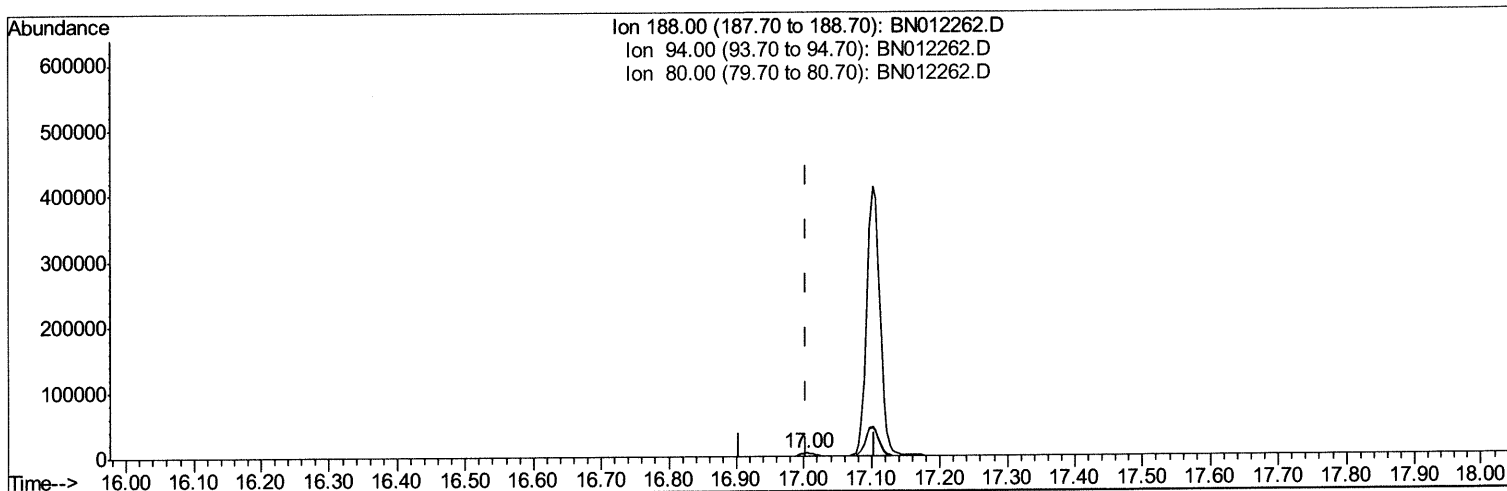

(10) Phenanthrene-d10 (I)

17.005min (+0.000) 0.40ng/ul m 10/20/20 54

response 7019

Ion	Exp%	Act%
188.00	100	100
94.00	11.20	10.77
80.00	12.20	11.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN101420\
Data File : BN012262.D
Acq On : 16 Oct 2020 12:08
Operator : CG/JU
Sample : PB132225BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK25

Manual Integrations
APPROVED

mohammad
10/19/2020 1:21:20 PM

Quant Time: Oct 16 13:09:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 10:51:19 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	1421	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136	5929	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	3455	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	7019m>	0.40	ng/ul >	0.00 10/20/20 JU
16) Chrysene-d12	21.21	240	5414	0.40	ng/ul	0.00
20) Perylene-d12	23.39	264	6128	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.99	152	2562	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.04	212	5580	0.29	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed