
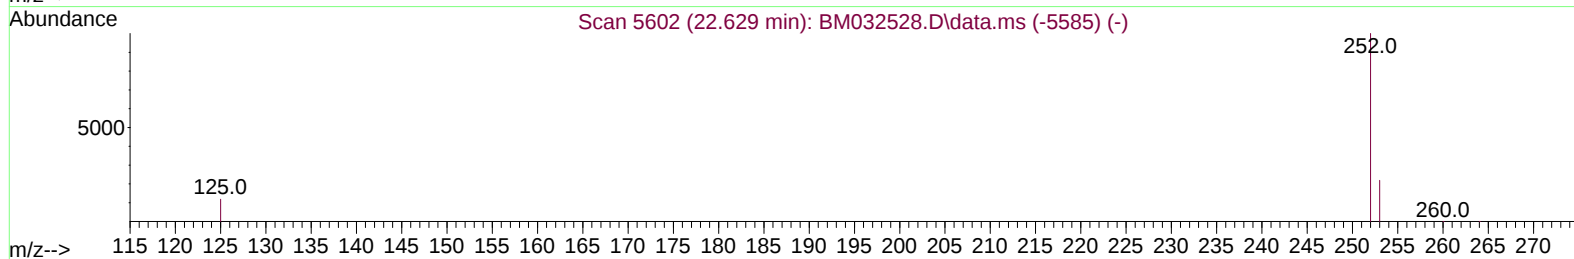
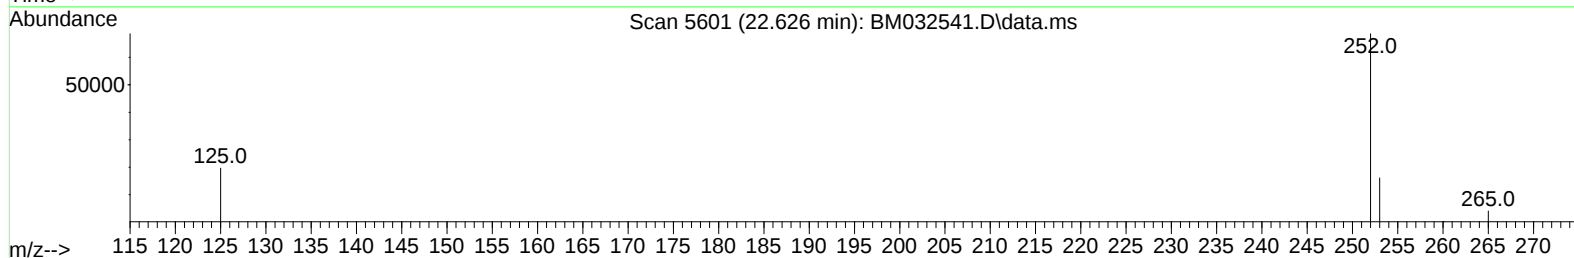


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101521\
Data File : BM032541.D
Acq On : 16 Oct 2021 00:30
Operator : CG/JU
Sample : M4029-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Oct 18 04:10:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 15 12:37:00 2021
Response via : Initial Calibration

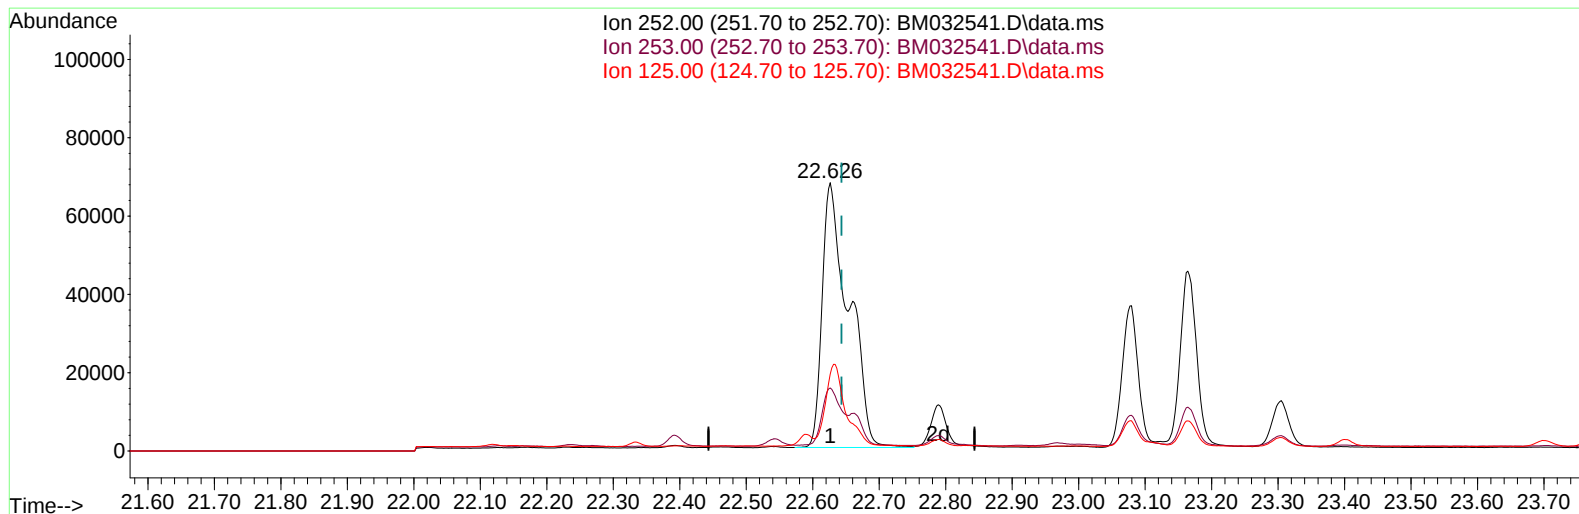

TIC: BM032541.D\data.ms

(24) Benzo(b)fluoranthene

22.626min (-0.017) 3.19 ng/u1

response 187020

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.90	23.52
125.00	17.80	28.66
0.00	0.00	0.00