

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101421\
 Data File : BN016951.D
 Acq On : 14 Oct 2021 15:09
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Oct 14 15:43:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 14 14:27:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.615	152	18227	0.40	ng	0.00
7) Naphthalene-d8	10.381	136	78673	0.40	ng	0.00
13) Acenaphthene-d10	14.243	164	42146	0.40	ng	0.00
19) Phenanthrene-d10	16.993	188	77961	0.40	ng	0.00
29) Chrysene-d12	21.196	240	80486	0.40	ng	0.00
35) Perylene-d12	23.426	264	76816	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.217	112	76611	1.85	ng	0.00
5) Phenol-d6	6.794	99	86591	1.88	ng	0.00
8) Nitrobenzene-d5	8.759	82	87429	1.75	ng	0.00
11) 2-Methylnaphthalene-d10	11.972	152	188119	1.71	ng	0.00
14) 2,4,6-Tribromophenol	15.741	330	35435	1.85	ng	0.00
15) 2-Fluorobiphenyl	12.860	172	263752	1.65	ng	0.00
27) Fluoranthene-d10	19.028	212	346163	1.77	ng	0.00
31) Terphenyl-d14	19.644	244	297173	1.68	ng	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.207	88	19245	1.58	ng	# 51
3) n-Nitrosodimethylamine	3.530	42	25549	1.83	ng	98
6) bis(2-Chloroethyl)ether	7.052	93	84077	1.70	ng	100
9) Naphthalene	10.432	128	348094	1.70	ng	100
10) Hexachlorobutadiene	10.711	225	66181	1.64	ng	# 100
12) 2-Methylnaphthalene	12.047	142	220493	1.70	ng	100
16) Acenaphthylene	13.952	152	311669	1.82	ng	100
17) Acenaphthene	14.307	154	197482	1.69	ng	99
18) Fluorene	15.296	166	242067	1.73	ng	99
20) 4,6-Dinitro-2-methylph...	15.385	198	22201	2.33	ng	# 87
21) 4-Bromophenyl-phenylether	16.190	248	81131	1.78	ng	98
22) Hexachlorobenzene	16.300	284	89309	1.69	ng	100
23) Atrazine	16.470	200	59745	2.09	ng	99
24) Pentachlorophenol	16.640	266	32758	1.83	ng	100
25) Phenanthrene	17.030	178	371997	1.68	ng	100
26) Anthracene	17.127	178	343821	1.82	ng	100
28) Fluoranthene	19.058	202	425711	1.78	ng	100
30) Pyrene	19.425	202	426743	1.67	ng	100
32) Benzo(a)anthracene	21.185	228	431933	1.78	ng	97
33) Chrysene	21.227	228	431642	1.65	ng	100
34) Bis(2-ethylhexyl)phtha...	21.132	149	212805	1.99	ng	100
36) Indeno(1,2,3-cd)pyrene	25.672	276	489372	1.68	ng	100
37) Benzo(b)fluoranthene	22.755	252	446783	1.82	ng	100
38) Benzo(k)fluoranthene	22.800	252	427900	1.75	ng	99
39) Benzo(a)pyrene	23.327	252	394832	1.76	ng	99
40) Dibenzo(a,h)anthracene	25.692	278	398343	1.69	ng	100
41) Benzo(g,h,i)perylene	26.363	276	429653	1.70	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101421\
Data File : BN016951.D
Acq On : 14 Oct 2021 15:09
Operator : CG/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Quant Time: Oct 14 15:43:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 14:27:18 2021
Response via : Initial Calibration

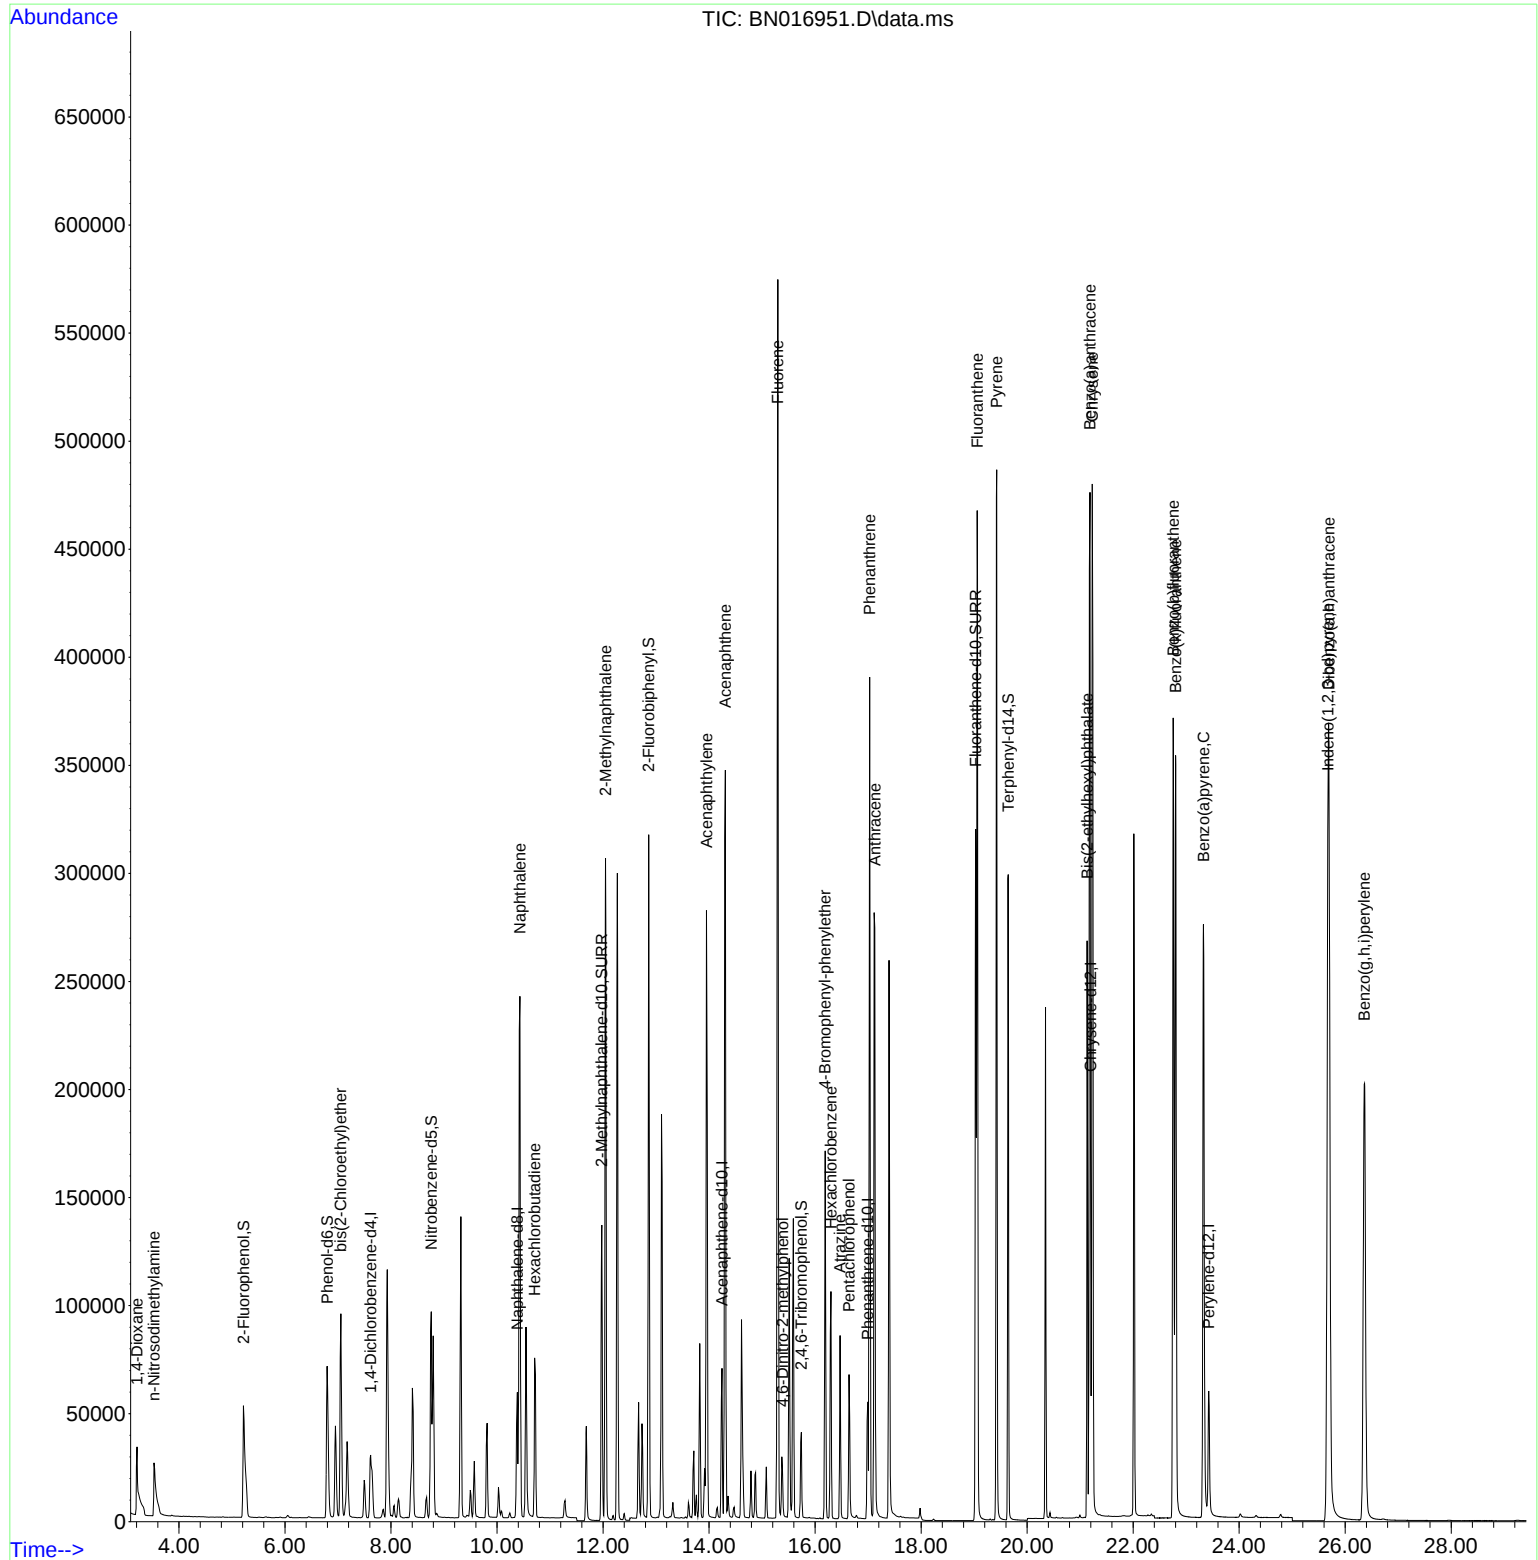







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.615 min Scan# 492
 Delta R.T. -0.000 min
 Lab File: BN016951.D
 Acq: 14 Oct 2021 15:09

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:152 Resp: 18227




Ion	Ratio	Lower	Upper
152	100		
150	154.2	122.2	183.4
115	57.9	46.1	69.1

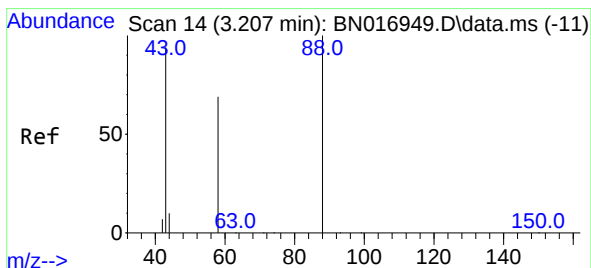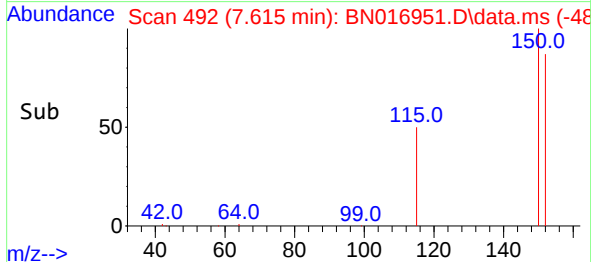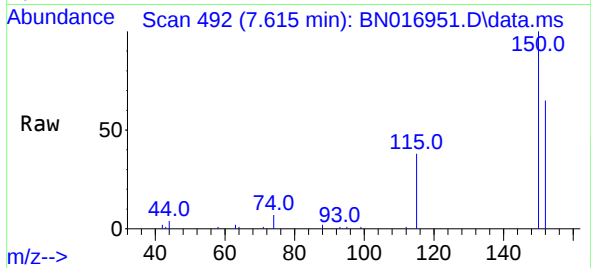


#2
 1,4-Dioxane
 Concen: 1.58 ng
 RT: 3.207 min Scan# 14
 Delta R.T. -0.000 min
 Lab File: BN016951.D
 Acq: 14 Oct 2021 15:09

Tgt Ion: 88 Resp: 19245

Ion	Ratio	Lower	Upper
88	100		
43	44.1	107.1	160.7#
58	76.0	62.4	93.6


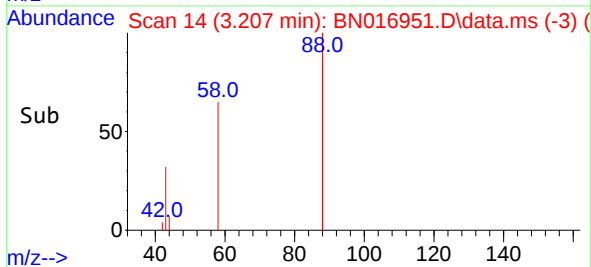

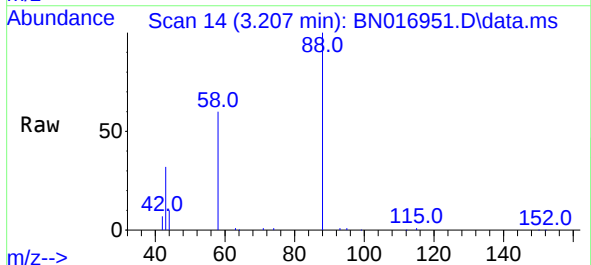




#3
n-Nitrosodimethylamine
Concen: 1.83 ng
RT: 3.530 min Scan# 49
Delta R.T. -0.009 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 25549
Ion Ratio Lower Upper
42 100
74 146.3 114.9 172.3
44 6.7 5.4 8.2



#4
2-Fluorophenol
Concen: 1.85 ng
RT: 5.217 min Scan# 232
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion: 112 Resp: 76611
Ion Ratio Lower Upper
112 100
64 56.0 44.7 67.1
63 28.1 22.6 33.8









#5
Phenol-d6
Concen: 1.88 ng
RT: 6.794 min Scan# 403
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 86591
Ion Ratio Lower Upper
99 100
42 17.7 14.2 21.4
71 30.6 24.6 36.8

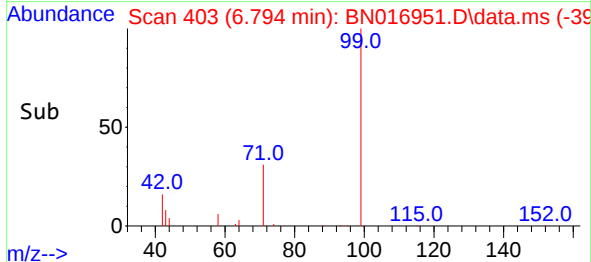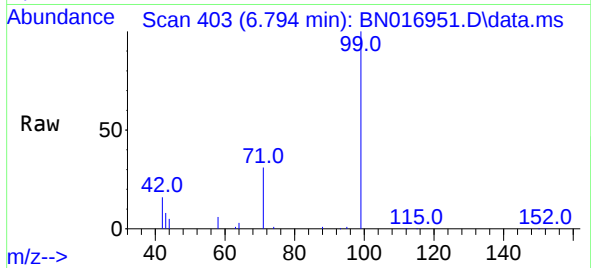

#6
bis(2-Chloroethyl)ether
Concen: 1.70 ng
RT: 7.052 min Scan# 431
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09


Tgt Ion: 93 Resp: 84077
Ion Ratio Lower Upper
93 100
63 75.4 60.0 90.0
95 32.9 26.5 39.7








#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.381 min Scan# 731
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6







Tgt Ion:	136	Resp:	78673
Ion Ratio	100	Lower	Upper
136	100		
137	11.0	8.8	13.2
54	5.5	4.3	6.5
68	4.8	3.7	5.5



#8
Nitrobenzene-d5
Concen: 1.75 ng
RT: 8.759 min Scan# 603
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:	82	Resp:	87429
Ion Ratio	100	Lower	Upper
82	100		
128	48.2	37.0	55.4
54	43.8	36.2	54.4









#9
Naphthalene
Concen: 1.70 ng
RT: 10.432 min Scan# 735
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:128 Resp: 348094




Ion	Ratio	Lower	Upper
128	100		
129	11.0	8.9	13.3
127	12.6	10.2	15.2




#10
Hexachlorobutadiene
Concen: 1.64 ng
RT: 10.711 min Scan# 757
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:225 Resp: 66181

Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.1	51.2	76.8







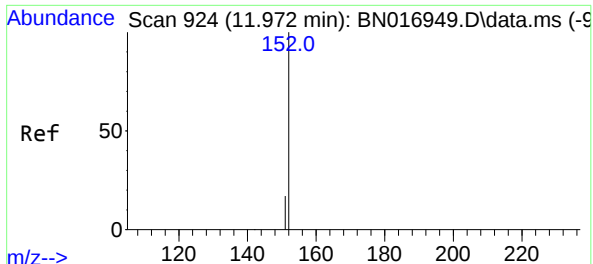

#11
2-Methylnaphthalene-d10
Concen: 1.71 ng
RT: 11.972 min Scan# 924
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 188119
Ion Ratio Lower Upper
152 100
151 20.3 16.3 24.5

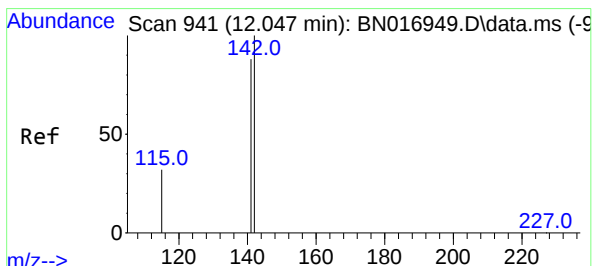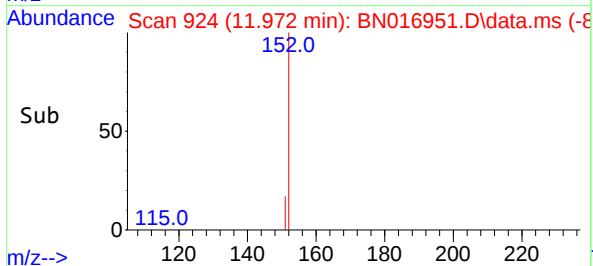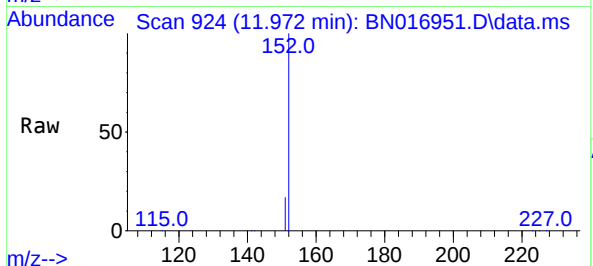

#12
2-Methylnaphthalene
Concen: 1.70 ng
RT: 12.047 min Scan# 941
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:142 Resp: 220493
Ion Ratio Lower Upper
142 100
141 87.4 70.2 105.4
115 32.6 26.1 39.1


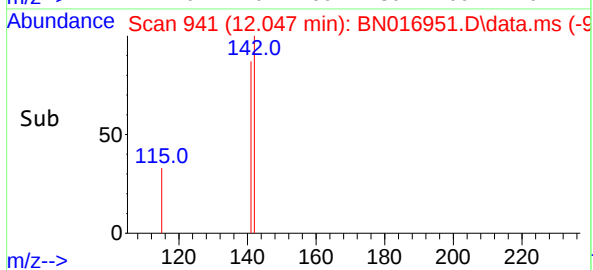

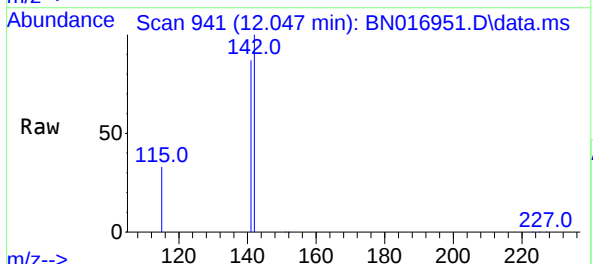




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.243 min Scan# 1181
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 42146
Ion Ratio Lower Upper
164 100
162 98.8 79.1 118.7
160 43.3 34.7 52.1

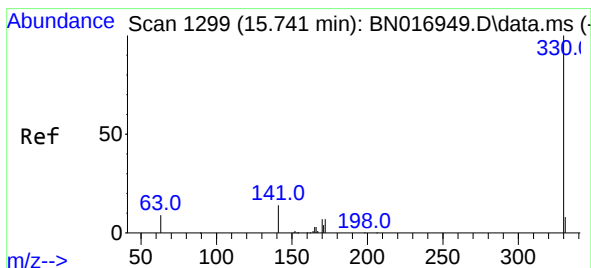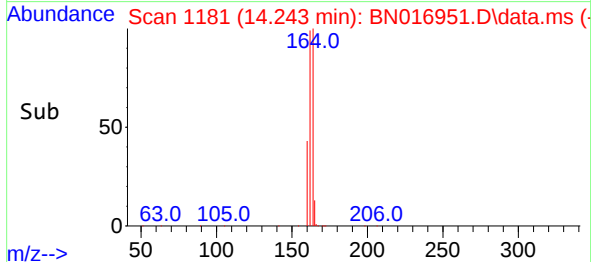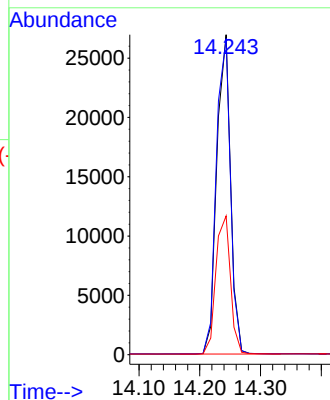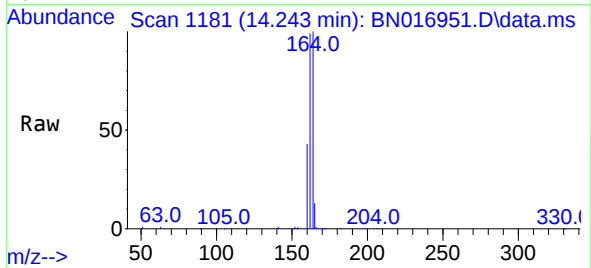

#14
2,4,6-Tribromophenol
Concen: 1.85 ng
RT: 15.741 min Scan# 1299
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:330 Resp: 35435
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.1 24.2 36.2


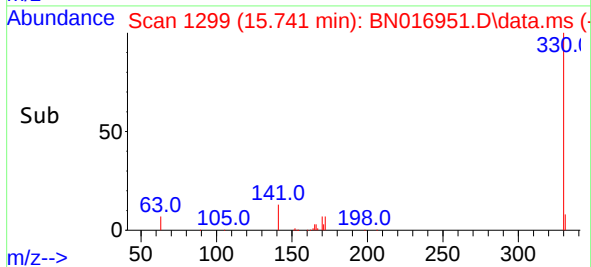
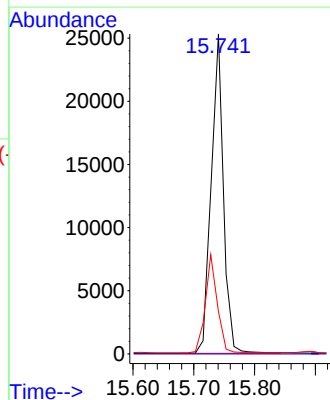
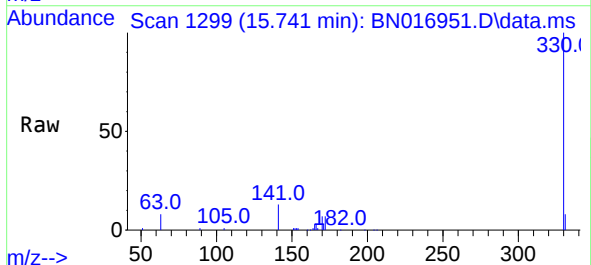


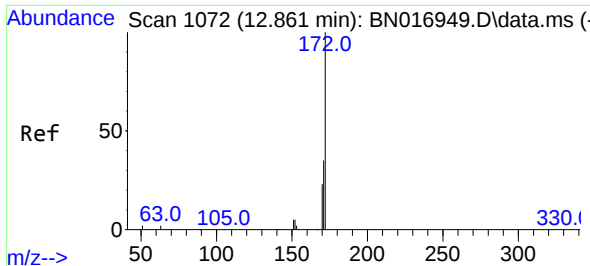

#15
2-Fluorobiphenyl
Concen: 1.65 ng
RT: 12.860 min Scan# 1072
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:172 Resp: 263752
Ion Ratio Lower Upper
172 100
171 35.2 27.9 41.9
170 23.5 18.6 27.8

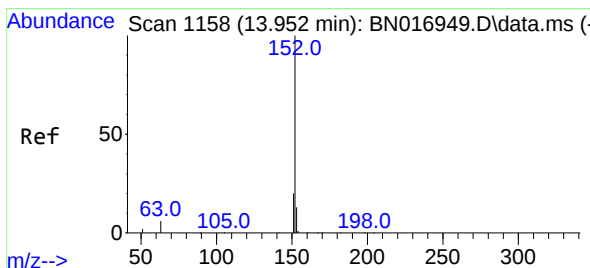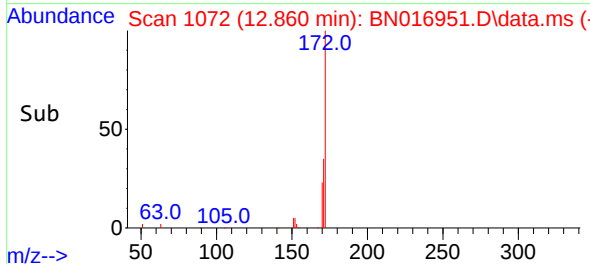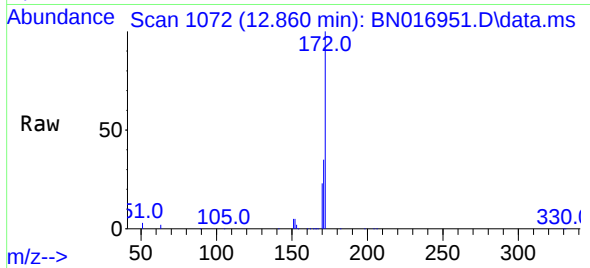

#16
Acenaphthylene
Concen: 1.82 ng
RT: 13.952 min Scan# 1158
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:152 Resp: 311669
Ion Ratio Lower Upper
152 100
151 19.4 15.4 23.2
153 13.0 10.5 15.7


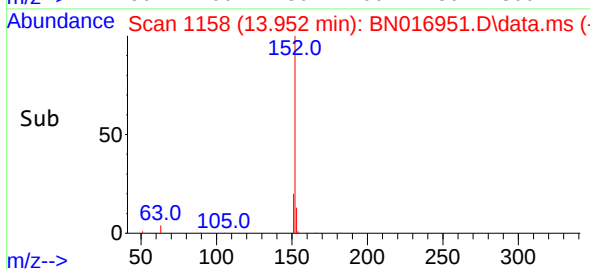

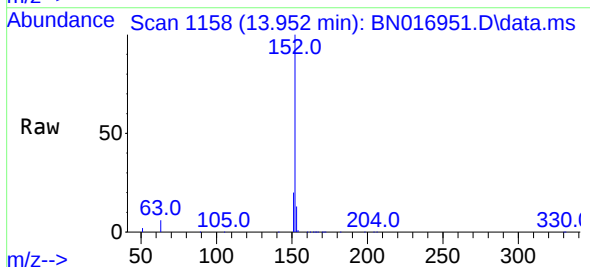


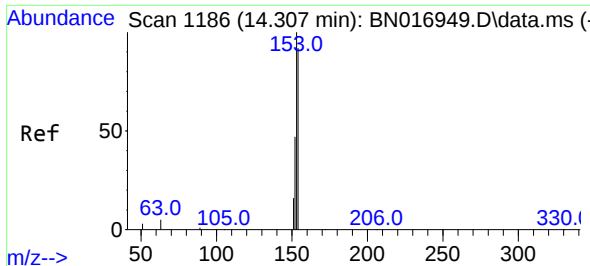

#17
Acenaphthene
Concen: 1.69 ng
RT: 14.307 min Scan# 1186
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:154 Resp: 197482
Ion Ratio Lower Upper
154 100
153 112.1 90.6 135.8
152 53.7 44.2 66.2

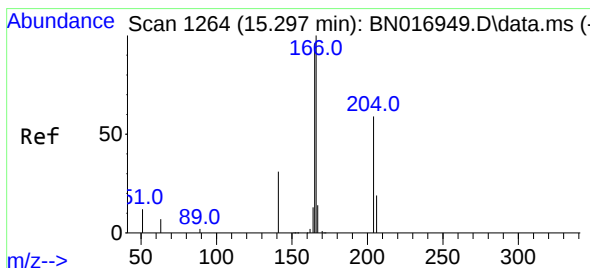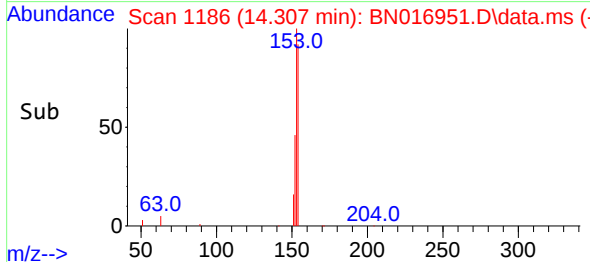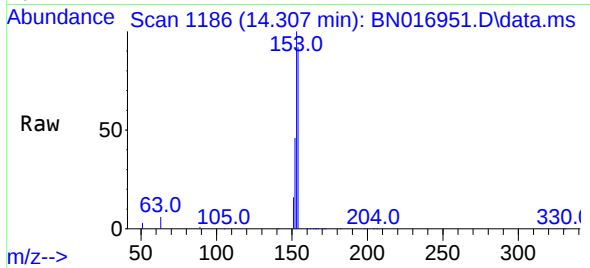

#18
Fluorene
Concen: 1.73 ng
RT: 15.296 min Scan# 1264
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:166 Resp: 242067
Ion Ratio Lower Upper
166 100
165 97.3 78.4 117.6
167 13.5 10.7 16.1


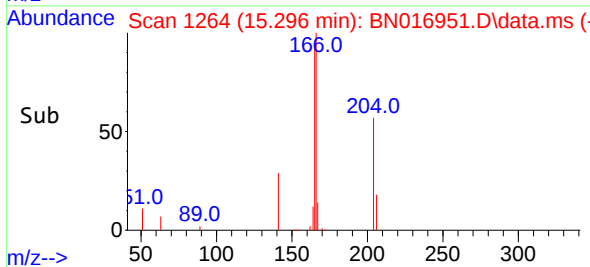

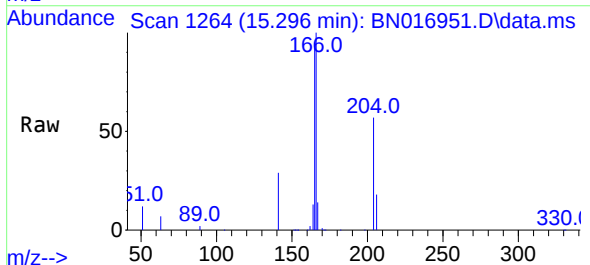


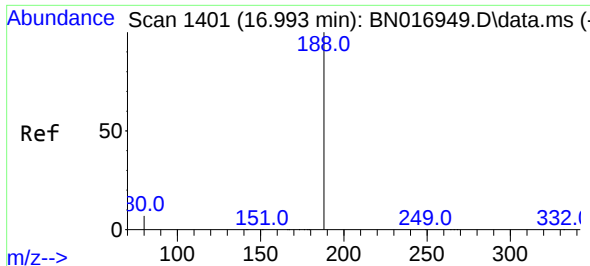

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.993 min Scan# 1401
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:188 Resp: 77961
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.9 5.6 8.4

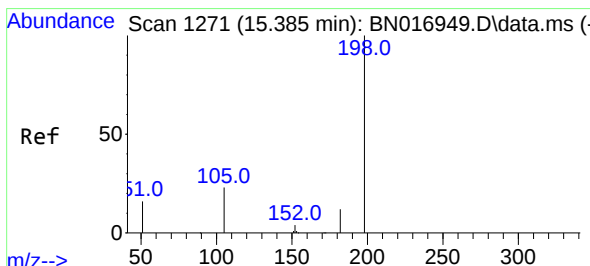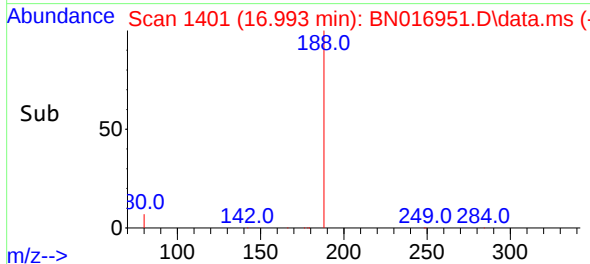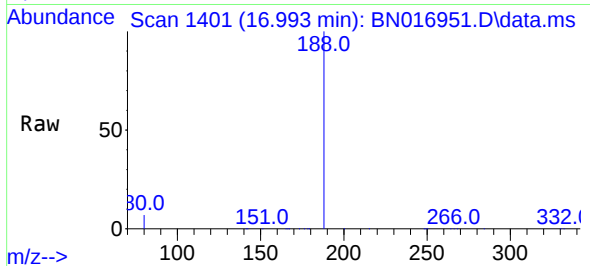

#20
4,6-Dinitro-2-methylphenol
Concen: 2.33 ng
RT: 15.385 min Scan# 1271
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:198 Resp: 22201
Ion Ratio Lower Upper
198 100
182 8.9 11.5 17.3#
77 0.0 0.0 0.0


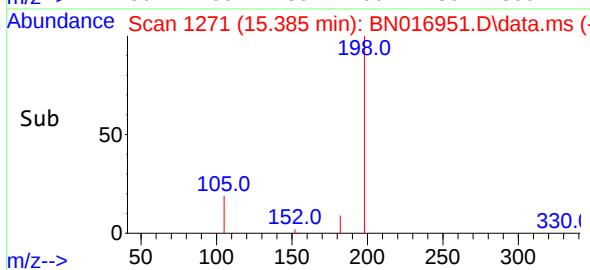

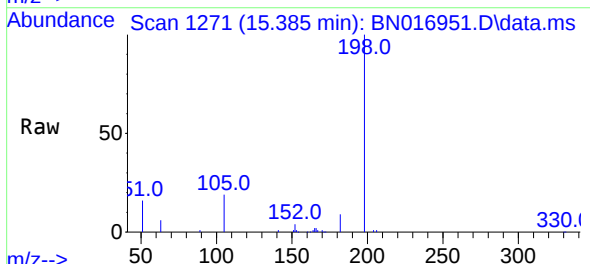




#21
4-Bromophenyl-phenylether
Concen: 1.78 ng
RT: 16.190 min Scan# 1335
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:248 Resp: 81131
Ion Ratio Lower Upper
248 100
250 95.0 76.1 114.1
141 54.8 46.6 70.0



#22
Hexachlorobenzene
Concen: 1.69 ng
RT: 16.300 min Scan# 1344
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:284 Resp: 89309
Ion Ratio Lower Upper
284 100
142 32.1 25.9 38.9
249 29.2 23.3 34.9









#23
Atrazine
Concen: 2.09 ng
RT: 16.470 min Scan# 1358
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:200 Resp: 59745
Ion Ratio Lower Upper
200 100
173 27.4 21.7 32.5
215 47.5 38.6 57.8



#24
Pentachlorophenol
Concen: 1.83 ng
RT: 16.640 min Scan# 1372
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:266 Resp: 32758
Ion Ratio Lower Upper
266 100
264 62.9 50.3 75.5
268 64.1 51.1 76.7







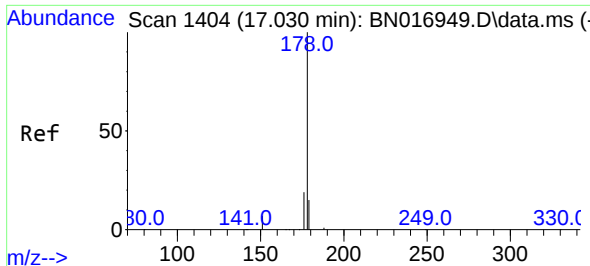

#25
Phenanthrene
Concen: 1.68 ng
RT: 17.030 min Scan# 1404
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:178 Resp: 371997
Ion Ratio Lower Upper
178 100
176 18.9 15.0 22.4
179 15.4 12.2 18.4

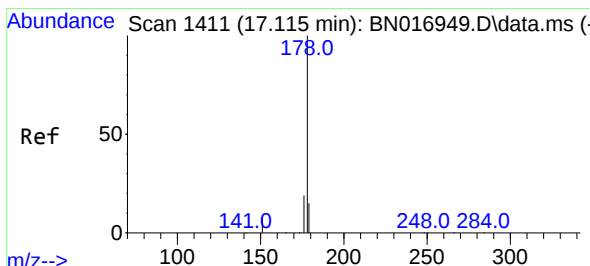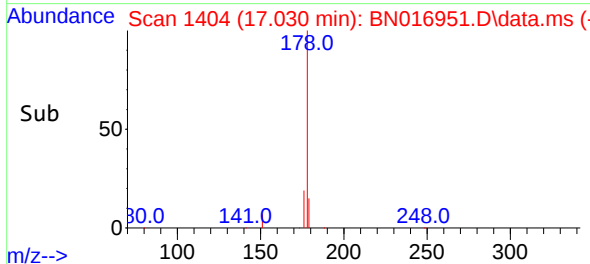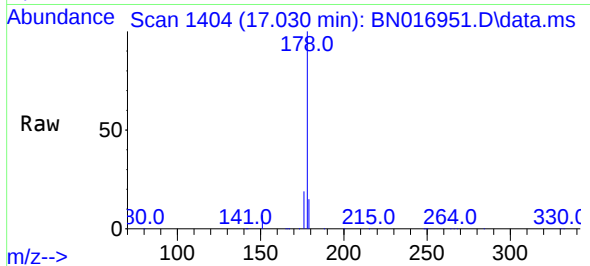

#26
Anthracene
Concen: 1.82 ng
RT: 17.127 min Scan# 1412
Delta R.T. 0.012 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:178 Resp: 343821
Ion Ratio Lower Upper
178 100
176 18.2 14.6 21.8
179 15.3 12.3 18.5


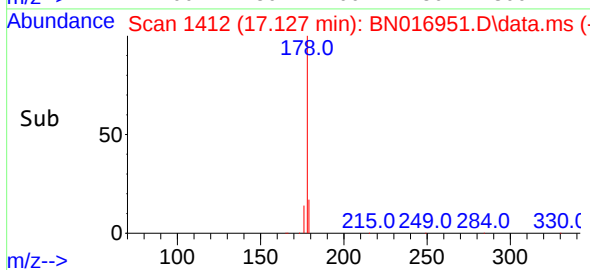

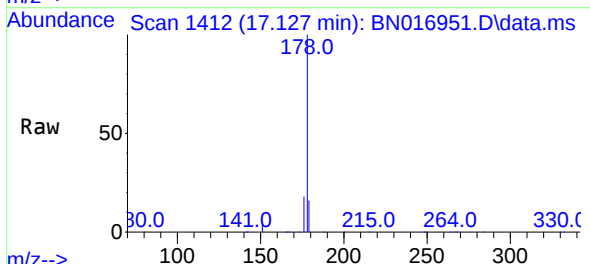




#27
Fluoranthene-d10
Concen: 1.77 ng
RT: 19.028 min Scan# 1689
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:212 Resp: 346163
Ion Ratio Lower Upper
212 100
106 13.7 10.9 16.3
104 7.5 6.0 9.0

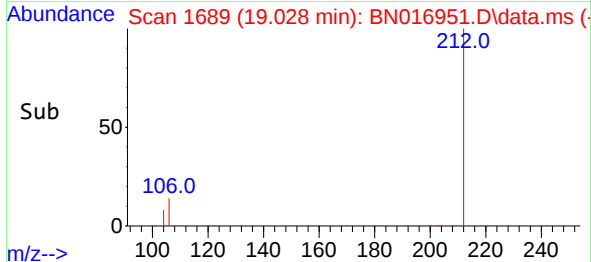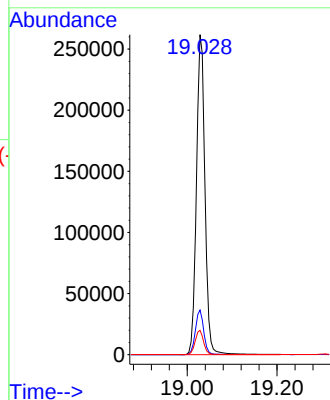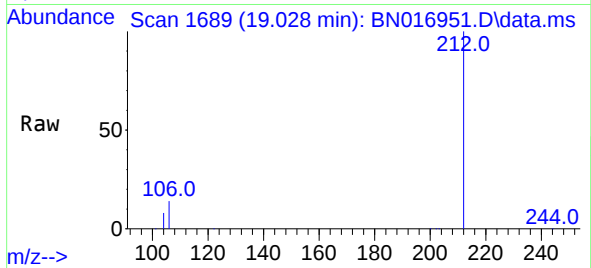

#28
Fluoranthene
Concen: 1.78 ng
RT: 19.058 min Scan# 1695
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:202 Resp: 425711
Ion Ratio Lower Upper
202 100
101 11.5 9.1 13.7
203 17.4 13.8 20.8


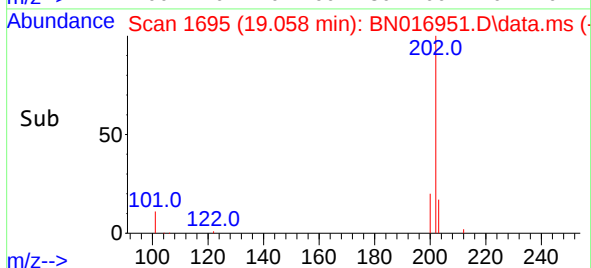
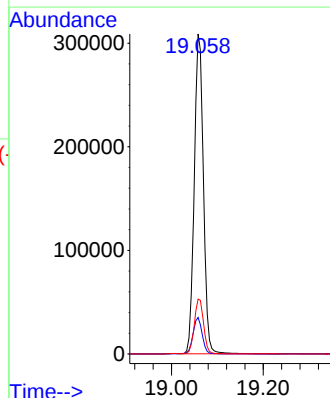





#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.196 min Scan# 1998
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:240 Resp: 80486
Ion Ratio Lower Upper
240 100
120 9.1 6.5 9.7
236 26.0 20.8 31.2

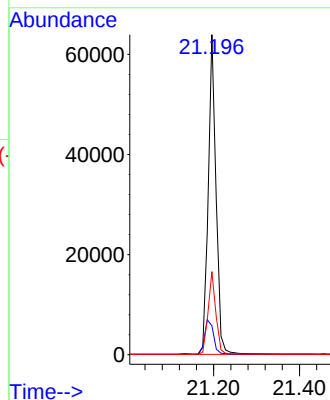

#30
Pyrene
Concen: 1.67 ng
RT: 19.425 min Scan# 1769
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:202 Resp: 426743
Ion Ratio Lower Upper
202 100
200 20.6 16.4 24.6
203 17.4 14.0 21.0



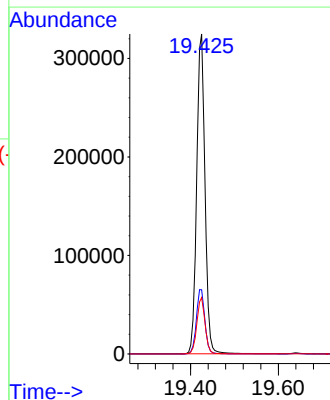





#31
Terphenyl-d14
Concen: 1.68 ng
RT: 19.644 min Scan# 1813
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:244 Resp: 297173
Ion Ratio Lower Upper
244 100
212 6.9 5.6 8.4
122 10.9 9.2 13.8



#32
Benzo(a)anthracene
Concen: 1.78 ng
RT: 21.185 min Scan# 1997
Delta R.T. 0.011 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:228 Resp: 431933
Ion Ratio Lower Upper
228 100
226 25.3 21.9 32.9
229 20.2 15.3 22.9







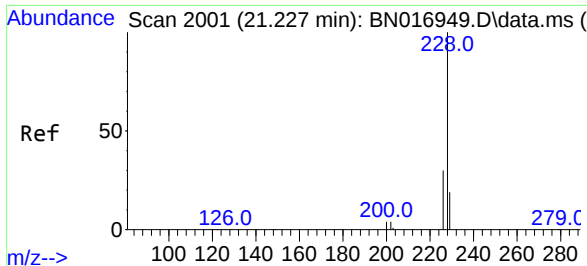

#33
Chrysene
Concen: 1.65 ng
RT: 21.227 min Scan# 2001
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:228 Resp: 431642
Ion Ratio Lower Upper
228 100
226 30.4 24.2 36.4
229 19.3 15.3 22.9

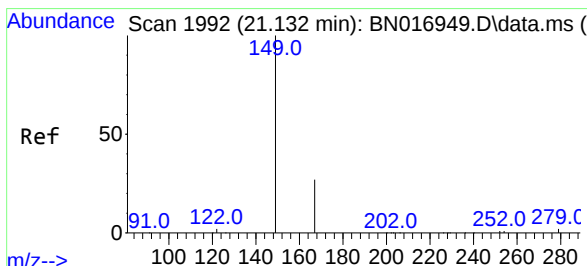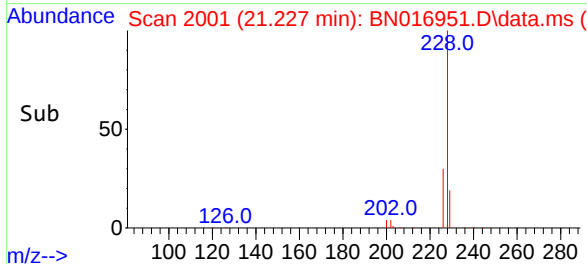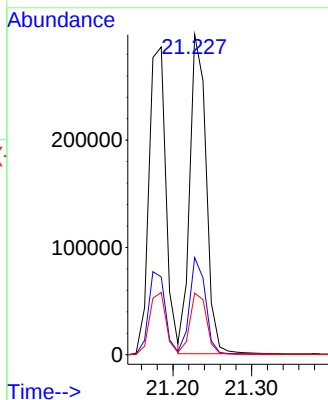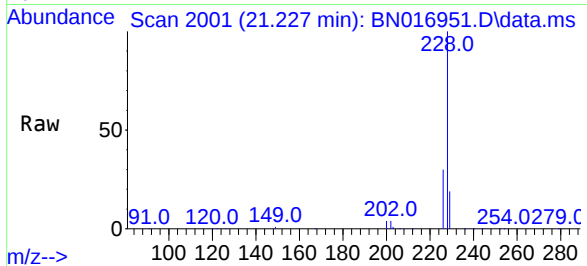

#34
Bis(2-ethylhexyl)phthalate
Concen: 1.99 ng
RT: 21.132 min Scan# 1992
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09


Tgt Ion:149 Resp: 212805
Ion Ratio Lower Upper
149 100
167 27.8 22.0 33.0
279 4.3 3.4 5.2

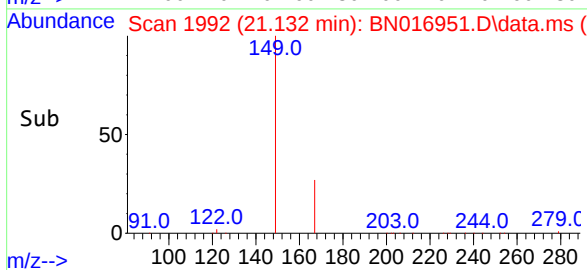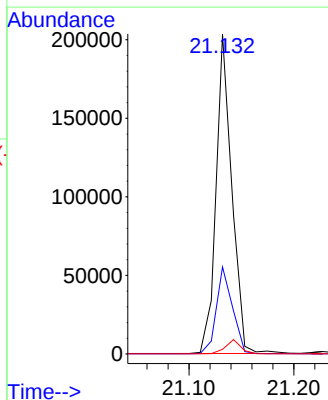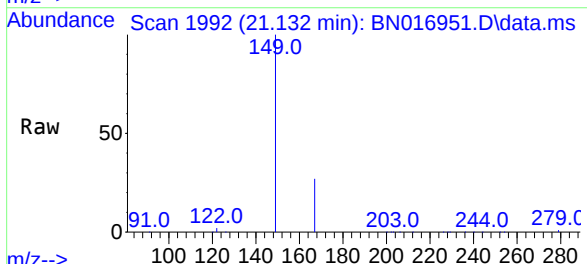






#35
Perylene-d12
Concen: 0.40 ng
RT: 23.426 min Scan# 2410
Delta R.T. 0.003 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6



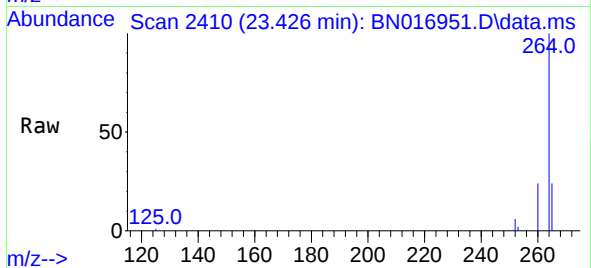



Tgt Ion:264 Resp: 76816
Ion Ratio Lower Upper
264 100
260 24.4 19.6 29.4
265 23.7 18.8 28.2



#36
Indeno(1,2,3-cd)pyrene
Concen: 1.68 ng
RT: 25.672 min Scan# 3066
Delta R.T. -0.003 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:276 Resp: 489372
Ion Ratio Lower Upper
276 100
138 24.3 19.4 29.2
277 25.1 20.1 30.1









#37
Benzo(b)fluoranthene
Concen: 1.82 ng
RT: 22.755 min Scan# 2214
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 446783
Ion Ratio Lower Upper
252 100
253 21.9 17.7 26.5
125 9.9 7.9 11.9



#38
Benzo(k)fluoranthene
Concen: 1.75 ng
RT: 22.800 min Scan# 2227
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09


Tgt Ion:252 Resp: 427900
Ion Ratio Lower Upper
252 100
253 21.7 17.9 26.9
125 10.0 8.4 12.6








#39
Benzo(a)pyrene
Concen: 1.76 ng
RT: 23.327 min Scan# 2381
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6



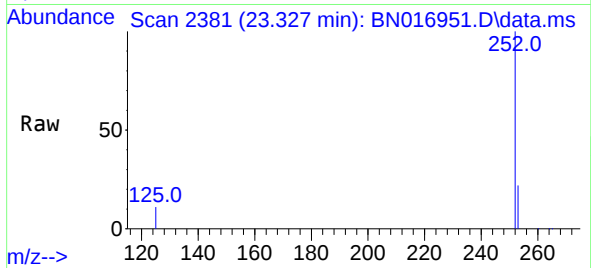



Tgt Ion:252 Resp: 394832
Ion Ratio Lower Upper
252 100
253 22.0 17.8 26.8
125 10.8 9.0 13.6

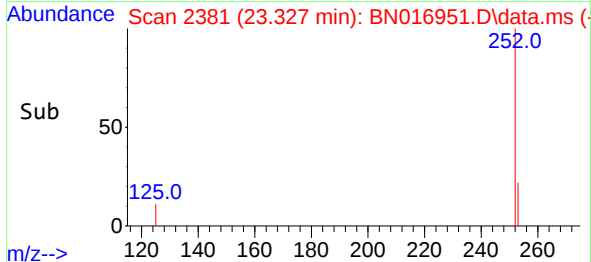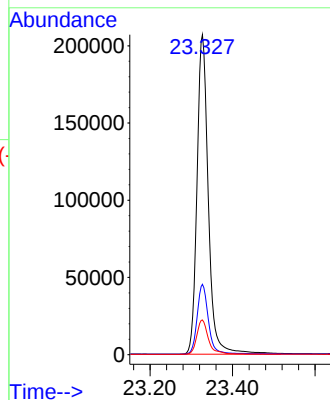

#40
Dibenzo(a,h)anthracene
Concen: 1.69 ng
RT: 25.692 min Scan# 3072
Delta R.T. -0.000 min
Lab File: BN016951.D
Acq: 14 Oct 2021 15:09

Tgt Ion:278 Resp: 398343
Ion Ratio Lower Upper
278 100
139 16.2 13.0 19.6
279 23.7 19.1 28.7

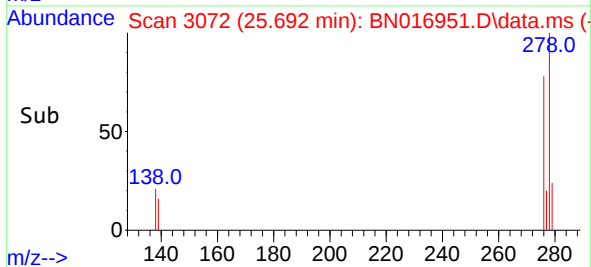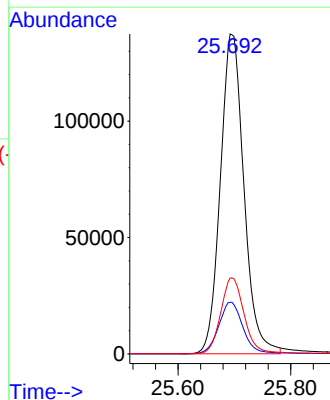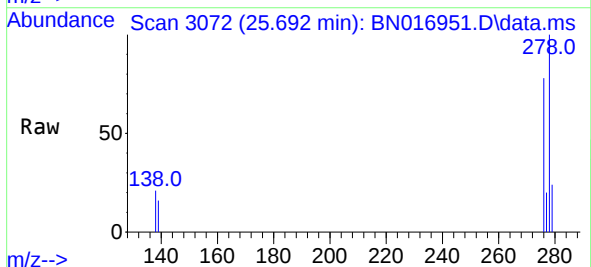

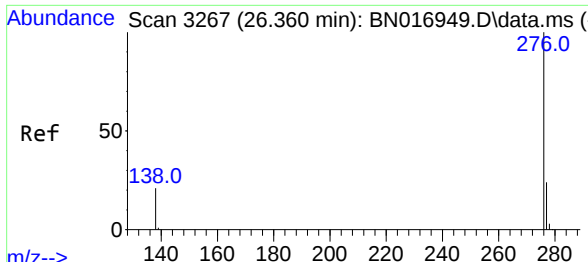

#41
 Benzo(g,h,i)perylene
 Concen: 1.70 ng
 RT: 26.363 min Scan# 3268
 Delta R.T. 0.003 min
 Lab File: BN016951.D
 Acq: 14 Oct 2021 15:09

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:	276	Resp:	429653
Ion	Ratio	Lower	Upper
276	100		
277	23.7	19.1	28.7
138	21.0	16.8	25.2

