

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101421\
 Data File : BN016965.D
 Acq On : 15 Oct 2021 00:55
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Oct 15 01:49:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 14 17:01:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.614	152	20709	0.40	ng	0.00
7) Naphthalene-d8	10.381	136	90594	0.40	ng	0.00
13) Acenaphthene-d10	14.243	164	46932	0.40	ng	0.00
19) Phenanthrene-d10	16.993	188	86646	0.40	ng	0.00
29) Chrysene-d12	21.195	240	87095	0.40	ng	# 0.00
35) Perylene-d12	23.419	264	90559	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.217	112	18583	0.36	ng	0.00
5) Phenol-d6	6.794	99	20537	0.36	ng	0.00
8) Nitrobenzene-d5	8.759	82	20009	0.35	ng	0.00
11) 2-Methylnaphthalene-d10	11.971	152	49320	0.38	ng	0.00
14) 2,4,6-Tribromophenol	15.740	330	7068	0.33	ng	0.00
15) 2-Fluorobiphenyl	12.860	172	71002	0.40	ng	0.00
27) Fluoranthene-d10	19.028	212	84184	0.38	ng	0.00
31) Terphenyl-d14	19.638	244	76157	0.39	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.207	88	4926	0.37	ng	# 46
3) n-Nitrosodimethylamine	3.539	42	6266	0.37	ng	100
6) bis(2-Chloroethyl)ether	7.052	93	22571	0.39	ng	99
9) Naphthalene	10.432	128	94553	0.37	ng	100
10) Hexachlorobutadiene	10.710	225	18082	0.39	ng	# 100
12) 2-Methylnaphthalene	12.047	142	60230	0.40	ng	99
16) Acenaphthylene	13.951	152	71945	0.37	ng	100
17) Acenaphthene	14.306	154	51174	0.39	ng	100
18) Fluorene	15.296	166	62057	0.40	ng	100
20) 4,6-Dinitro-2-methylph...	15.385	198	2885	0.40	ng	99
21) 4-Bromophenyl-phenylether	16.190	248	20061	0.39	ng	98
22) Hexachlorobenzene	16.299	284	23882	0.40	ng	99
23) Atrazine	16.470	200	12175	0.34	ng	99
24) Pentachlorophenol	16.640	266	6069	0.41	ng	100
25) Phenanthrene	17.029	178	100055	0.40	ng	100
26) Anthracene	17.115	178	81565	0.38	ng	100
28) Fluoranthene	19.058	202	110613	0.41	ng	100
30) Pyrene	19.420	202	110613	0.40	ng	100
32) Benzo(a)anthracene	21.174	228	103604	0.39	ng	99
33) Chrysene	21.227	228	115241	0.41	ng	98
34) Bis(2-ethylhexyl)phtha...	21.131	149	35859	0.38	ng	100
36) Indeno(1,2,3-cd)pyrene	25.664	276	135638	0.41	ng	99
37) Benzo(b)fluoranthene	22.748	252	113545	0.38	ng	100
38) Benzo(k)fluoranthene	22.793	252	119891	0.40	ng	98
39) Benzo(a)pyrene	23.320	252	101682	0.38	ng	99
40) Dibenzo(a,h)anthracene	25.688	278	110142	0.41	ng	99
41) Benzo(g,h,i)perylene	26.352	276	117158	0.40	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101421\
Data File : BN016965.D
Acq On : 15 Oct 2021 00:55
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Oct 15 01:49:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 17:01:23 2021
Response via : Initial Calibration









#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.614 min Scan# 492
Delta R.T. -0.001 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 20709
Ion Ratio Lower Upper
152 100
150 153.4 122.2 183.4
115 58.2 46.1 69.1



#2
1,4-Dioxane
Concen: 0.37 ng
RT: 3.207 min Scan# 14
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion: 88 Resp: 4926
Ion Ratio Lower Upper
88 100
43 32.5 107.1 160.7#
58 77.0 62.4 93.6









#3
n-Nitrosodimethylamine
Concen: 0.37 ng
RT: 3.539 min Scan# 50
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 42 Resp: 6266




Ion	Ratio	Lower	Upper
42	100		
74	144.0	114.9	172.3
44	7.3	5.4	8.2




#4
2-Fluorophenol
Concen: 0.36 ng
RT: 5.217 min Scan# 232
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion: 112 Resp: 18583

Ion	Ratio	Lower	Upper
112	100		
64	56.3	44.7	67.1
63	28.0	22.6	33.8









#5
Phenol-d6
Concen: 0.36 ng
RT: 6.794 min Scan# 403
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	99	Resp:	20537
Ion	Ratio	Lower	Upper
99	100		
42	17.9	14.2	21.4
71	30.8	24.6	36.8



#6
bis(2-Chloroethyl)ether
Concen: 0.39 ng
RT: 7.052 min Scan# 431
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55


Tgt Ion:	93	Resp:	22571
Ion	Ratio	Lower	Upper
93	100		
63	75.6	60.0	90.0
95	33.1	26.5	39.7








#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.381 min Scan# 731
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:	136	Resp:	90594
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.8	13.2
54	5.2	4.3	6.5
68	4.7	3.7	5.5



#8
Nitrobenzene-d5
Concen: 0.35 ng
RT: 8.759 min Scan# 603
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:	82	Resp:	20009
Ion	Ratio	Lower	Upper
82	100		
128	46.1	37.0	55.4
54	45.0	36.2	54.4









#9
Naphthalene
Concen: 0.37 ng
RT: 10.432 min Scan# 735
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	128	Resp:	94553
Ion	Ratio	Lower	Upper
128	100		
129	11.0	8.9	13.3
127	12.6	10.2	15.2



#10
Hexachlorobutadiene
Concen: 0.39 ng
RT: 10.710 min Scan# 757
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:	225	Resp:	18082
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.2	51.2	76.8







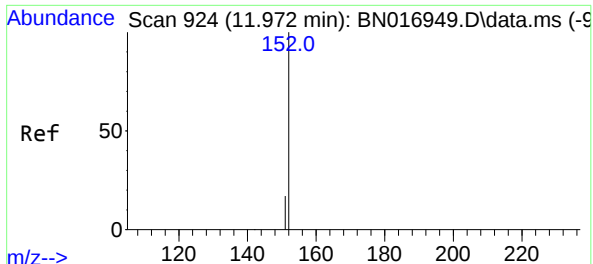

#11
2-Methylnaphthalene-d10
Concen: 0.38 ng
RT: 11.971 min Scan# 924
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 49320
Ion Ratio Lower Upper
152 100
151 20.5 16.3 24.5

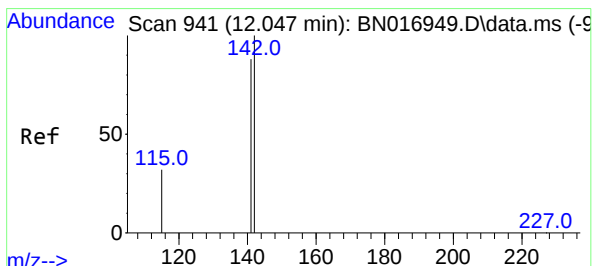

#12
2-Methylnaphthalene
Concen: 0.40 ng
RT: 12.047 min Scan# 941
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:142 Resp: 60230
Ion Ratio Lower Upper
142 100
141 88.4 70.2 105.4
115 32.9 26.1 39.1









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.243 min Scan# 1181
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 46932
Ion Ratio Lower Upper
164 100
162 98.8 79.1 118.7
160 43.2 34.7 52.1



#14
2,4,6-Tribromophenol
Concen: 0.33 ng
RT: 15.740 min Scan# 1299
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:330 Resp: 7068
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.2 24.2 36.2







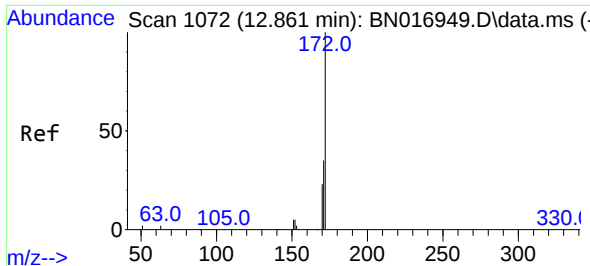

#15
2-Fluorobiphenyl
Concen: 0.40 ng
RT: 12.860 min Scan# 1072
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:172 Resp: 71002
Ion Ratio Lower Upper
172 100
171 35.0 27.9 41.9
170 23.3 18.6 27.8



#16
Acenaphthylene
Concen: 0.37 ng
RT: 13.951 min Scan# 1158
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:152 Resp: 71945
Ion Ratio Lower Upper
152 100
151 19.6 15.4 23.2
153 13.0 10.5 15.7









#17
Acenaphthene
Concen: 0.39 ng
RT: 14.306 min Scan# 1186
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 51174
Ion Ratio Lower Upper
154 100
153 113.7 90.6 135.8
152 55.3 44.2 66.2



#18
Fluorene
Concen: 0.40 ng
RT: 15.296 min Scan# 1264
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:166 Resp: 62057
Ion Ratio Lower Upper
166 100
165 98.2 78.4 117.6
167 13.5 10.7 16.1







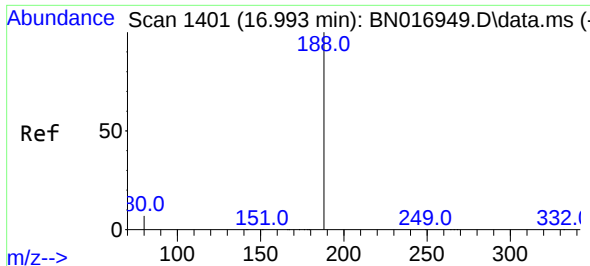

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.993 min Scan# 1401
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 86646
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.6 5.6 8.4



#20
4,6-Dinitro-2-methylphenol
Concen: 0.40 ng
RT: 15.385 min Scan# 1271
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:198 Resp: 2885
Ion Ratio Lower Upper
198 100
182 14.0 11.5 17.3
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.39 ng
RT: 16.190 min Scan# 1335
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	248	Resp:	20061
Ion	Ratio	Lower	Upper
248	100		
250	96.2	76.1	114.1
141	55.3	46.6	70.0



#22
Hexachlorobenzene
Concen: 0.40 ng
RT: 16.299 min Scan# 1344
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:	284	Resp:	23882
Ion	Ratio	Lower	Upper
284	100		
142	31.9	25.9	38.9
249	29.5	23.3	34.9









#23
Atrazine
Concen: 0.34 ng
RT: 16.470 min Scan# 1358
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:200 Resp: 12175
Ion Ratio Lower Upper
200 100
173 25.9 21.7 32.5
215 48.7 38.6 57.8



#24
Pentachlorophenol
Concen: 0.41 ng
RT: 16.640 min Scan# 1372
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:266 Resp: 6069
Ion Ratio Lower Upper
266 100
264 62.9 50.3 75.5
268 64.6 51.1 76.7







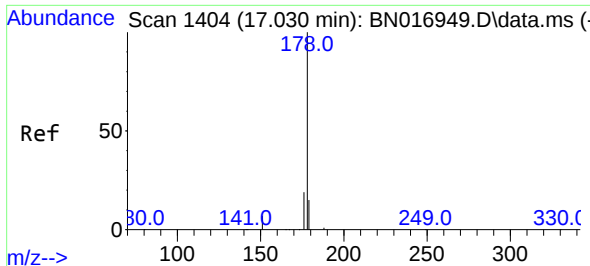

#25
Phenanthrene
Concen: 0.40 ng
RT: 17.029 min Scan# 1404
Delta R.T. -0.001 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 100055
Ion Ratio Lower Upper
178 100
176 18.8 15.0 22.4
179 15.4 12.2 18.4

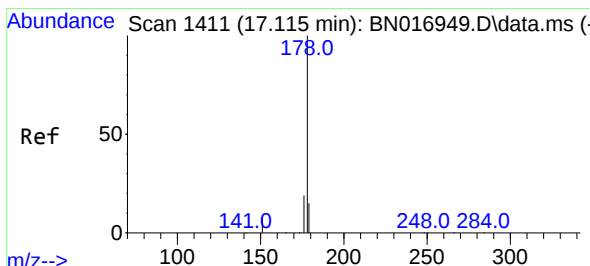

#26
Anthracene
Concen: 0.38 ng
RT: 17.115 min Scan# 1411
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:178 Resp: 81565
Ion Ratio Lower Upper
178 100
176 18.2 14.6 21.8
179 15.4 12.3 18.5









#27
Fluoranthene-d10
Concen: 0.38 ng
RT: 19.028 min Scan# 1689
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 84184
Ion Ratio Lower Upper
212 100
106 13.5 10.9 16.3
104 7.4 6.0 9.0



#28
Fluoranthene
Concen: 0.41 ng
RT: 19.058 min Scan# 1695
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:202 Resp: 110613
Ion Ratio Lower Upper
202 100
101 11.5 9.1 13.7
203 17.3 13.8 20.8









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.195 min Scan# 1998
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 87095
Ion Ratio Lower Upper
240 100
120 5.9 6.5 9.7#
236 25.2 20.8 31.2



#30
Pyrene
Concen: 0.40 ng
RT: 19.420 min Scan# 1768
Delta R.T. -0.005 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:202 Resp: 110613
Ion Ratio Lower Upper
202 100
200 20.6 16.4 24.6
203 17.4 14.0 21.0









#31
Terphenyl-d14
Concen: 0.39 ng
RT: 19.638 min Scan# 1812
Delta R.T. -0.005 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:244 Resp: 76157
Ion Ratio Lower Upper
244 100
212 7.3 5.6 8.4
122 12.6 9.2 13.8



#32
Benzo(a)anthracene
Concen: 0.39 ng
RT: 21.174 min Scan# 1996
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:228 Resp: 103604
Ion Ratio Lower Upper
228 100
226 27.1 21.9 32.9
229 19.5 15.3 22.9









#33
Chrysene
Concen: 0.41 ng
RT: 21.227 min Scan# 2001
Delta R.T. -0.000 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:228 Resp: 115241




Ion	Ratio	Lower	Upper
228	100		
226	29.0	24.2	36.4
229	19.5	15.3	22.9




#34
Bis(2-ethylhexyl)phthalate
Concen: 0.38 ng
RT: 21.131 min Scan# 1992
Delta R.T. -0.001 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:149 Resp: 35859


Ion	Ratio	Lower	Upper
149	100		
167	27.3	22.0	33.0
279	4.2	3.4	5.2








#35
Perylene-d12
Concen: 0.40 ng
RT: 23.419 min Scan# 2408
Delta R.T. -0.004 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:264 Resp: 90559
Ion Ratio Lower Upper
264 100
260 24.4 19.6 29.4
265 22.8 18.8 28.2



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.41 ng
RT: 25.664 min Scan# 3064
Delta R.T. -0.011 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55


Tgt Ion:276 Resp: 135638
Ion Ratio Lower Upper
276 100
138 25.2 19.4 29.2
277 25.3 20.1 30.1








#37
Benzo(b)fluoranthene
Concen: 0.38 ng
RT: 22.748 min Scan# 2212
Delta R.T. -0.007 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:252 Resp: 113545
Ion Ratio Lower Upper
252 100
253 22.3 17.7 26.5
125 10.0 7.9 11.9



#38
Benzo(k)fluoranthene
Concen: 0.40 ng
RT: 22.793 min Scan# 2225
Delta R.T. -0.007 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55


Tgt Ion:252 Resp: 119891
Ion Ratio Lower Upper
252 100
253 22.5 17.9 26.9
125 12.4 8.4 12.6








#39
Benzo(a)pyrene
Concen: 0.38 ng
RT: 23.320 min Scan# 2379
Delta R.T. -0.007 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:252 Resp: 101682
Ion Ratio Lower Upper
252 100
253 22.1 17.8 26.8
125 11.0 9.0 13.6



#40
Dibenzo(a,h)anthracene
Concen: 0.41 ng
RT: 25.688 min Scan# 3071
Delta R.T. -0.004 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Tgt Ion:278 Resp: 110142
Ion Ratio Lower Upper
278 100
139 17.0 13.0 19.6
279 23.9 19.1 28.7



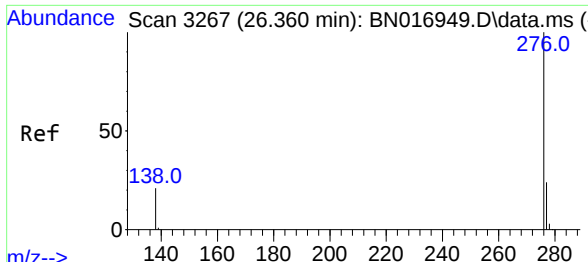

#41
Benzo(g,h,i)perylene
Concen: 0.40 ng
RT: 26.352 min Scan# 3265
Delta R.T. -0.007 min
Lab File: BN016965.D
Acq: 15 Oct 2021 00:55

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:276 Resp: 117158
Ion Ratio Lower Upper
276 100
277 23.8 19.1 28.7
138 21.2 16.8 25.2

