

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101421\
 Data File : BN016971.D
 Acq On : 15 Oct 2021 04:32
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Manual Integrations
 APPROVED

mohammad
 10/18/2021 8:47:27 AM

Quant Time: Oct 15 05:48:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 14 17:01:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.606	152	22266	0.40	ng	0.00
7) Naphthalene-d8	10.381	136	99207	0.40	ng	0.00
13) Acenaphthene-d10	14.231	164	52813	0.40	ng	-0.01
19) Phenanthrene-d10	16.981	188	97728	0.40	ng	#-0.01
29) Chrysene-d12	21.196	240	101435	0.40	ng	# 0.00
35) Perylene-d12	23.420	264	105887	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.218	112	21292	0.38	ng	0.00
5) Phenol-d6	6.794	99	23803	0.39	ng	0.00
8) Nitrobenzene-d5	8.747	82	25445	0.40	ng	-0.01
11) 2-Methylnaphthalene-d10	11.972	152	54985	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.741	330	9229	0.39	ng	0.00
15) 2-Fluorobiphenyl	12.861	172	78138	0.39	ng	0.00
27) Fluoranthene-d10	19.028	212	100880	0.41	ng	0.00
31) Terphenyl-d14	19.639	244	87908	0.39	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.207	88	5483m	0.38	ng	
3) n-Nitrosodimethylamine	3.530	42	7158	0.39	ng	97
6) bis(2-Chloroethyl)ether	7.052	93	24644	0.40	ng	99
9) Naphthalene	10.419	128	102639	0.37	ng	99
10) Hexachlorobutadiene	10.711	225	20070	0.40	ng	# 100
12) 2-Methylnaphthalene	12.047	142	66419	0.40	ng	100
16) Acenaphthylene	13.952	152	86001	0.39	ng	100
17) Acenaphthene	14.294	154	56875	0.39	ng	99
18) Fluorene	15.297	166	69538	0.39	ng	100
20) 4,6-Dinitro-2-methylph...	15.385	198	4061	0.43	ng	98
21) 4-Bromophenyl-phenylether	16.190	248	22930	0.39	ng	93
22) Hexachlorobenzene	16.300	284	26190	0.39	ng	99
23) Atrazine	16.470	200	16346	0.40	ng	98
24) Pentachlorophenol	16.640	266	8279	0.45	ng	100
25) Phenanthrene	17.030	178	110141	0.39	ng	100
26) Anthracene	17.115	178	97205	0.41	ng	100
28) Fluoranthene	19.058	202	127575	0.42	ng	100
30) Pyrene	19.420	202	129596	0.40	ng	100
32) Benzo(a)anthracene	21.174	228	130536	0.42	ng	99
33) Chrysene	21.228	228	132227	0.40	ng	99
34) Bis(2-ethylhexyl)phtha...	21.132	149	78338	0.55	ng	99
36) Indeno(1,2,3-cd)pyrene	25.672	276	158001	0.40	ng	99
37) Benzo(b)fluoranthene	22.752	252	136967	0.39	ng	100
38) Benzo(k)fluoranthene	22.797	252	139573	0.40	ng	98
39) Benzo(a)pyrene	23.324	252	127843	0.41	ng	100
40) Dibenzo(a,h)anthracene	25.692	278	128217	0.40	ng	99
41) Benzo(g,h,i)perylene	26.356	276	135987	0.39	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101421\
Data File : BN016971.D
Acq On : 15 Oct 2021 04:32
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED


mohammad
10/18/2021 8:47:27 AM

Quant Time: Oct 15 05:48:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 17:01:23 2021
Response via : Initial Calibration









#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.606 min Scan# 491
Delta R.T. -0.009 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32





Tgt Ion: 152 Resp: 22266
Ion Ratio Lower Upper
152 100
150 157.9 122.2 183.4
115 60.9 46.1 69.1



#2
1,4-Dioxane
Concen: 0.38 ng m
RT: 3.207 min Scan# 14
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Tgt Ion: 88 Resp: 5483
Ion Ratio Lower Upper
88 100
43 26.1 107.1 160.7#
58 65.9 62.4 93.6



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
10/18/2021 8:47:27 AM



#3
n-Nitrosodimethylamine
Concen: 0.39 ng
RT: 3.530 min Scan# 49
Delta R.T. -0.009 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32





Tgt Ion: 42 Resp: 7158

Ion	Ratio	Lower	Upper
42	100		
74	147.9	114.9	172.3
44	6.8	5.4	8.2

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED




mohammad
10/18/2021 8:47:27 AM




#4
2-Fluorophenol
Concen: 0.38 ng
RT: 5.218 min Scan# 232
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32

Tgt Ion: 112 Resp: 21292

Ion	Ratio	Lower	Upper
112	100		
64	56.5	44.7	67.1
63	28.2	22.6	33.8









#5
Phenol-d6
Concen: 0.39 ng
RT: 6.794 min Scan# 403
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32

Tgt Ion:	99	Resp:	23803
Ion	Ratio	Lower	Upper
99	100		
42	17.9	14.2	21.4
71	31.0	24.6	36.8

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
10/18/2021 8:47:27 AM



#6
bis(2-Chloroethyl)ether
Concen: 0.40 ng
RT: 7.052 min Scan# 431
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32


Tgt Ion:	93	Resp:	24644
Ion	Ratio	Lower	Upper
93	100		
63	75.6	60.0	90.0
95	33.2	26.5	39.7





#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.381 min Scan# 731
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Tgt Ion:	136	Resp:	99207
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.8	13.2
54	4.7	4.3	6.5
68	4.2	3.7	5.5

Manual Integrations
APPROVED



mohammad
10/18/2021 8:47:27 AM




#8
Nitrobenzene-d5
Concen: 0.40 ng
RT: 8.747 min Scan# 602
Delta R.T. -0.013 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32



Tgt Ion:	82	Resp:	25445
Ion	Ratio	Lower	Upper
82	100		
128	35.7	37.0	55.4#
54	53.4	36.2	54.4









#9
Naphthalene
Concen: 0.37 ng
RT: 10.419 min Scan# 734
Delta R.T. -0.013 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32

Tgt Ion:	128	Resp:	102639
Ion	Ratio	Lower	Upper
128	100		
129	11.0	8.9	13.3
127	13.3	10.2	15.2

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
10/18/2021 8:47:27 AM



#10
Hexachlorobutadiene
Concen: 0.40 ng
RT: 10.711 min Scan# 757
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32

Tgt Ion:	225	Resp:	20070
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.7	51.2	76.8



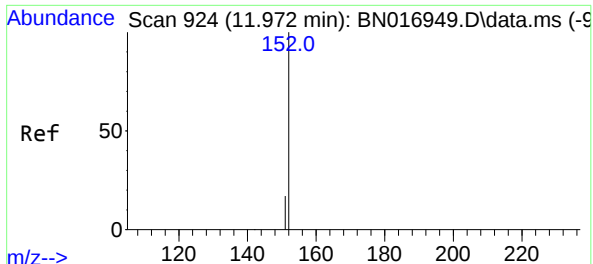





#11
2-Methylnaphthalene-d10
Concen: 0.39 ng
RT: 11.972 min Scan# 924
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32

Tgt Ion:152 Resp: 54985
Ion Ratio Lower Upper
152 100
151 20.3 16.3 24.5

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
10/18/2021 8:47:27 AM




#12
2-Methylnaphthalene
Concen: 0.40 ng
RT: 12.047 min Scan# 941
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32

Tgt Ion:142 Resp: 66419
Ion Ratio Lower Upper
142 100
141 87.5 70.2 105.4
115 32.3 26.1 39.1









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.231 min Scan# 1180
Delta R.T. -0.013 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32





Tgt Ion:164 Resp: 52813
Ion Ratio Lower Upper
164 100
162 104.6 79.1 118.7
160 48.6 34.7 52.1



#14
2,4,6-Tribromophenol
Concen: 0.39 ng
RT: 15.741 min Scan# 1299
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Tgt Ion:330 Resp: 9229
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 29.8 24.2 36.2




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED




mohammad
10/18/2021 8:47:27 AM

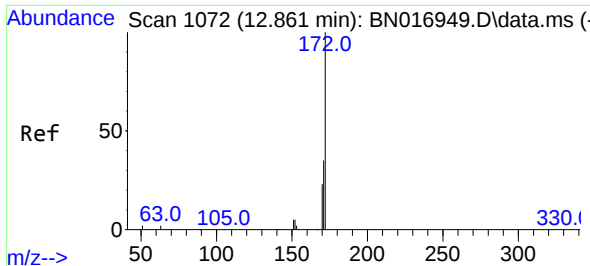


#15
2-Fluorobiphenyl
Concen: 0.39 ng
RT: 12.861 min Scan# 1072
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32





Tgt Ion:172 Resp: 78138
Ion Ratio Lower Upper
172 100
171 34.6 27.9 41.9
170 22.8 18.6 27.8



#16
Acenaphthylene
Concen: 0.39 ng
RT: 13.952 min Scan# 1158
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Tgt Ion:152 Resp: 86001
Ion Ratio Lower Upper
152 100
151 19.5 15.4 23.2
153 13.0 10.5 15.7



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Manual Integrations
APPROVED

mohammad
10/18/2021 8:47:27 AM

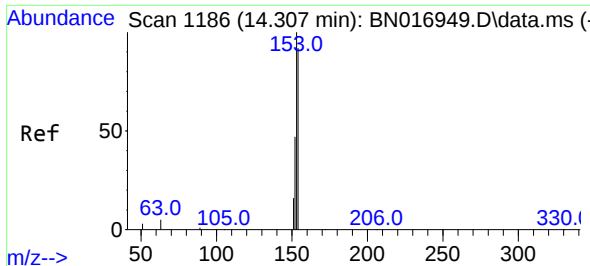

#17
Acenaphthene
Concen: 0.39 ng
RT: 14.294 min Scan# 1185
Delta R.T. -0.013 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



Tgt Ion:154 Resp: 56875
Ion Ratio Lower Upper
154 100
153 113.0 90.6 135.8
152 54.2 44.2 66.2




Manual Integrations
APPROVED


mohammad
10/18/2021 8:47:27 AM



#18
Fluorene
Concen: 0.39 ng
RT: 15.297 min Scan# 1264
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32


Tgt Ion:166 Resp: 69538
Ion Ratio Lower Upper
166 100
165 97.9 78.4 117.6
167 13.4 10.7 16.1



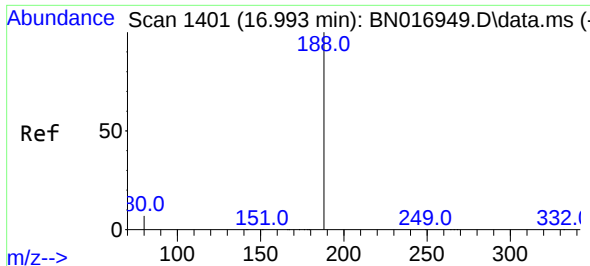

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.981 min Scan# 1400
Delta R.T. -0.012 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Tgt Ion:188 Resp: 97728
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.0 5.6 8.4#

Manual Integrations
APPROVED



mohammad
10/18/2021 8:47:27 AM




#20
4,6-Dinitro-2-methylphenol
Concen: 0.43 ng
RT: 15.385 min Scan# 1271
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Tgt Ion:198 Resp: 4061
Ion Ratio Lower Upper
198 100
182 13.7 11.5 17.3
77 0.0 0.0 0.0





#21
4-Bromophenyl-phenylether
Concen: 0.39 ng
RT: 16.190 min Scan# 1335
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Tgt Ion:248 Resp: 22930
Ion Ratio Lower Upper
248 100
250 97.9 76.1 114.1
141 48.3 46.6 70.0

Manual Integrations
APPROVED



mohammad
10/18/2021 8:47:27 AM




#22
Hexachlorobenzene
Concen: 0.39 ng
RT: 16.300 min Scan# 1344
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Tgt Ion:284 Resp: 26190
Ion Ratio Lower Upper
284 100
142 32.0 25.9 38.9
249 29.6 23.3 34.9









#23
Atrazine
Concen: 0.40 ng
RT: 16.470 min Scan# 1358
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32





Tgt Ion:200 Resp: 16346
Ion Ratio Lower Upper
200 100
173 24.9 21.7 32.5
215 48.9 38.6 57.8



#24
Pentachlorophenol
Concen: 0.45 ng
RT: 16.640 min Scan# 1372
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Tgt Ion:266 Resp: 8279
Ion Ratio Lower Upper
266 100
264 62.9 50.3 75.5
268 64.4 51.1 76.7



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Manual Integrations
APPROVED

mohammad
10/18/2021 8:47:27 AM

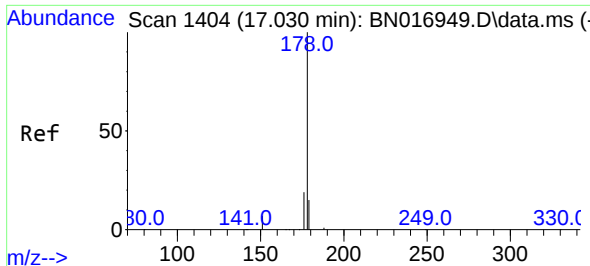

#25
Phenanthrene
Concen: 0.39 ng
RT: 17.030 min Scan# 1404
Delta R.T. -0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Tgt Ion:178 Resp: 110141
Ion Ratio Lower Upper
178 100
176 18.9 15.0 22.4
179 15.6 12.2 18.4

Manual Integrations
APPROVED



mohammad
10/18/2021 8:47:27 AM




#26
Anthracene
Concen: 0.41 ng
RT: 17.115 min Scan# 1411
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32



Tgt Ion:178 Resp: 97205
Ion Ratio Lower Upper
178 100
176 18.2 14.6 21.8
179 15.2 12.3 18.5









#27
Fluoranthene-d10
Concen: 0.41 ng
RT: 19.028 min Scan# 1689
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32

Tgt Ion:212 Resp: 100880
Ion Ratio Lower Upper
212 100
106 13.6 10.9 16.3
104 7.4 6.0 9.0

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
10/18/2021 8:47:27 AM



#28
Fluoranthene
Concen: 0.42 ng
RT: 19.058 min Scan# 1695
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32

Tgt Ion:202 Resp: 127575
Ion Ratio Lower Upper
202 100
101 11.5 9.1 13.7
203 17.3 13.8 20.8









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.196 min Scan# 1998
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32

Tgt Ion:240 Resp: 101435
Ion Ratio Lower Upper
240 100
120 6.3 6.5 9.7#
236 25.1 20.8 31.2

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
10/18/2021 8:47:27 AM




#30
Pyrene
Concen: 0.40 ng
RT: 19.420 min Scan# 1768
Delta R.T. -0.005 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32

Tgt Ion:202 Resp: 129596
Ion Ratio Lower Upper
202 100
200 20.5 16.4 24.6
203 17.5 14.0 21.0









#31
Terphenyl-d14
Concen: 0.39 ng
RT: 19.639 min Scan# 1812
Delta R.T. -0.005 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32





Tgt Ion:244 Resp: 87908
Ion Ratio Lower Upper
244 100
212 7.1 5.6 8.4
122 12.9 9.2 13.8



#32
Benzo(a)anthracene
Concen: 0.42 ng
RT: 21.174 min Scan# 1996
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Tgt Ion:228 Resp: 130536
Ion Ratio Lower Upper
228 100
226 26.9 21.9 32.9
229 19.3 15.3 22.9



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Manual Integrations
APPROVED

mohammad
10/18/2021 8:47:27 AM



#33
Chrysene
Concen: 0.40 ng
RT: 21.228 min Scan# 2001
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Tgt Ion:228 Resp: 132227
Ion Ratio Lower Upper
228 100
226 29.7 24.2 36.4
229 19.3 15.3 22.9

Manual Integrations
APPROVED



mohammad
10/18/2021 8:47:27 AM




#34
Bis(2-ethylhexyl)phthalate
Concen: 0.55 ng
RT: 21.132 min Scan# 1992
Delta R.T. -0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Tgt Ion:149 Resp: 78338
Ion Ratio Lower Upper
149 100
167 27.8 22.0 33.0
279 4.4 3.4 5.2





#35
Perylene-d12
Concen: 0.40 ng
RT: 23.420 min Scan# 2408
Delta R.T. -0.003 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



Tgt Ion:264 Resp: 105887
Ion Ratio Lower Upper
264 100
260 24.7 19.6 29.4
265 23.0 18.8 28.2




Manual Integrations
APPROVED


mohammad
10/18/2021 8:47:27 AM




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.40 ng
RT: 25.672 min Scan# 3066
Delta R.T. -0.003 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32

Tgt Ion:276 Resp: 158001
Ion Ratio Lower Upper
276 100
138 25.3 19.4 29.2
277 25.2 20.1 30.1









#37
Benzo(b)fluoranthene
Concen: 0.39 ng
RT: 22.752 min Scan# 2213
Delta R.T. -0.003 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32





Tgt Ion:252 Resp: 136967
Ion Ratio Lower Upper
252 100
253 22.0 17.7 26.5
125 10.2 7.9 11.9



#38
Benzo(k)fluoranthene
Concen: 0.40 ng
RT: 22.797 min Scan# 2226
Delta R.T. -0.003 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32




Tgt Ion:252 Resp: 139573
Ion Ratio Lower Upper
252 100
253 22.6 17.9 26.9
125 12.4 8.4 12.6



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC





Manual Integrations
APPROVED

mohammad
10/18/2021 8:47:27 AM






#39
Benzo(a)pyrene
Concen: 0.41 ng
RT: 23.324 min Scan# 2380
Delta R.T. -0.003 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32

Tgt Ion:252 Resp: 127843
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.8
125 11.4 9.0 13.6



#40
Dibenzo(a,h)anthracene
Concen: 0.40 ng
RT: 25.692 min Scan# 3072
Delta R.T. 0.000 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32


Tgt Ion:278 Resp: 128217
Ion Ratio Lower Upper
278 100
139 17.0 13.0 19.6
279 23.8 19.1 28.7




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED



mohammad
10/18/2021 8:47:27 AM

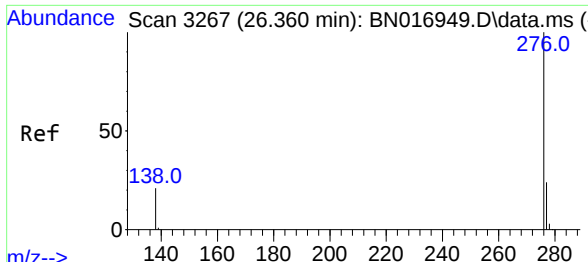

#41
Benzo(g,h,i)perylene
Concen: 0.39 ng
RT: 26.356 min Scan# 3266
Delta R.T. -0.003 min
Lab File: BN016971.D
Acq: 15 Oct 2021 04:32



Tgt Ion: 276 Resp: 135987
Ion Ratio Lower Upper
276 100
277 23.6 19.1 28.7
138 21.1 16.8 25.2



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
10/18/2021 8:47:27 AM