
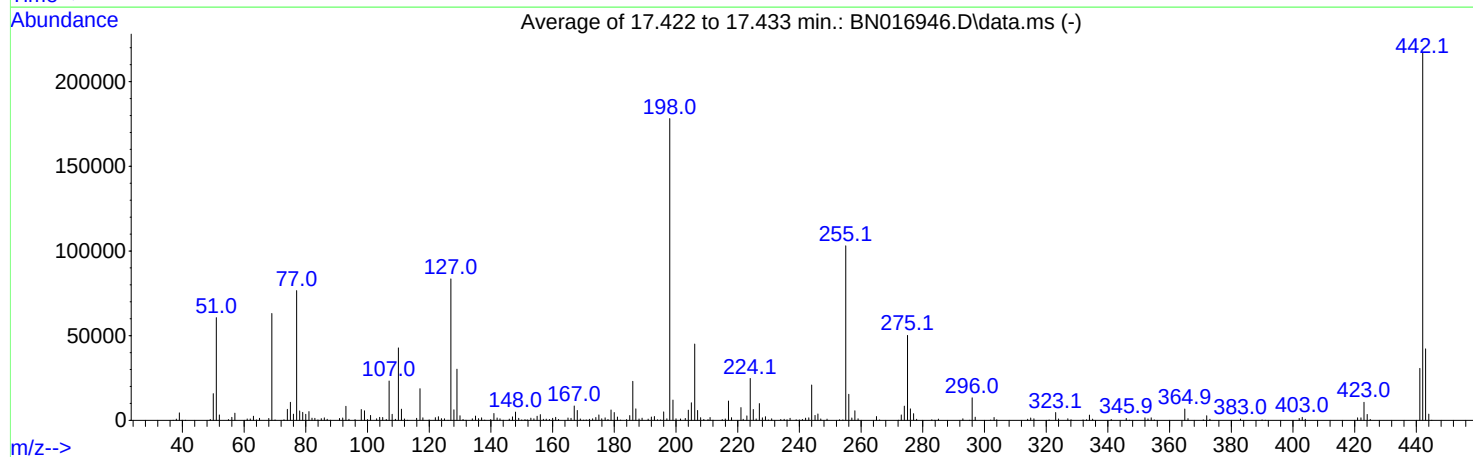


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101421\
 Data File : BN016946.D
 Acq On : 14 Oct 2021 12:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 14 17:01:23 2021

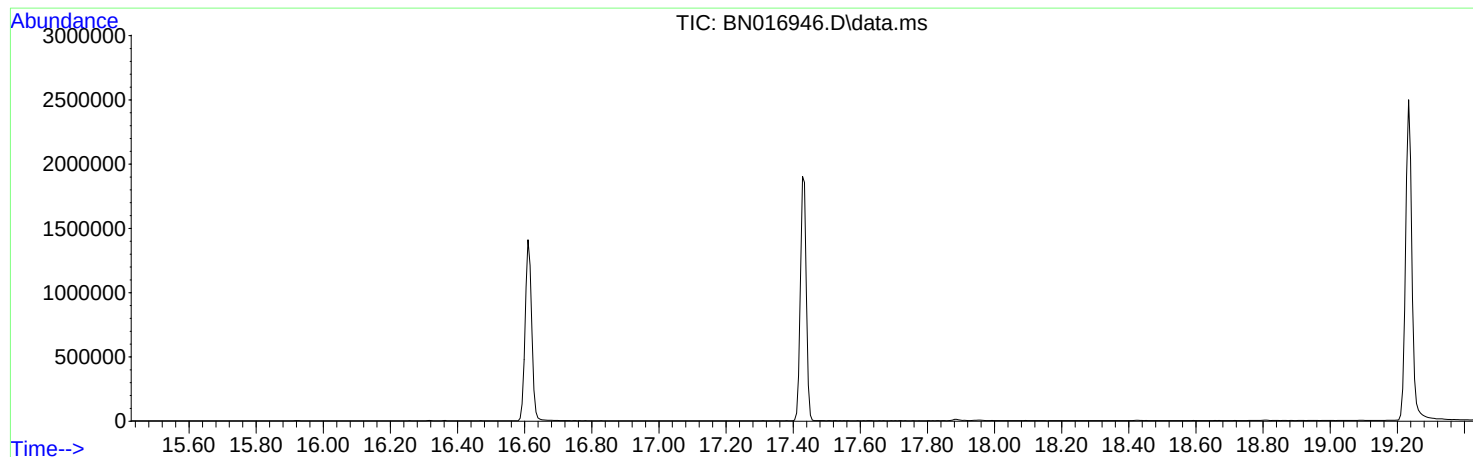




AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	60683	PASS
68	69	0.00	2	1.8	1126	PASS
69	198	0.00	100	35.4	63093	PASS
70	69	0.00	2	0.5	313	PASS
127	198	10	80	46.9	83477	PASS
197	198	0.00	2	0.6	985	PASS
198	198	100	100	100.0	178168	PASS
199	198	5	9	6.8	12042	PASS
275	198	10	60	28.2	50181	PASS
365	198	1	100	3.8	6751	PASS
441	198	0.01	100	17.2	30729	PASS
442	442	50	100	100.0	217200	PASS
443	442	15	24	19.5	42251	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101421\
Data File : BN016946.D
Acq On : 14 Oct 2021 12:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 15 04:51:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 17:23:48 2021
Response via : Initial Calibration

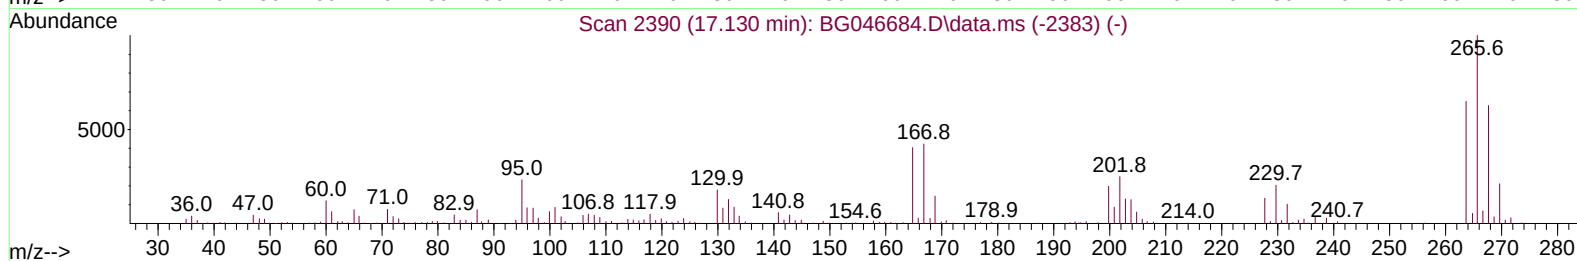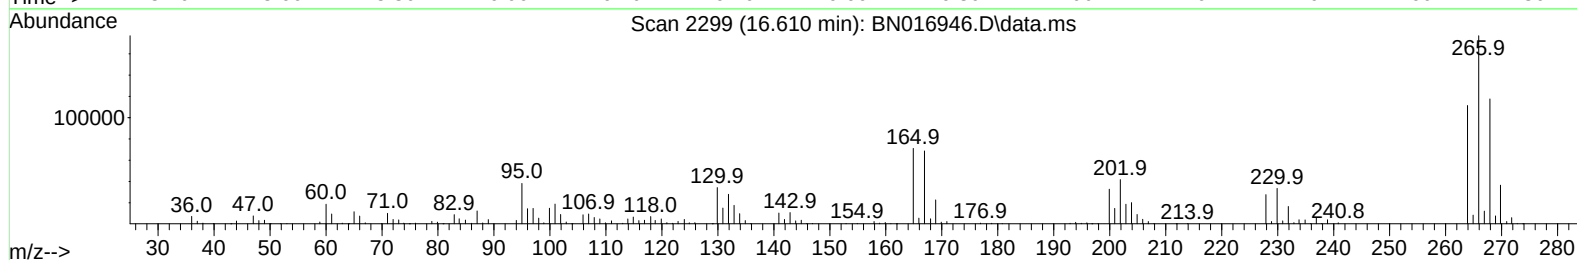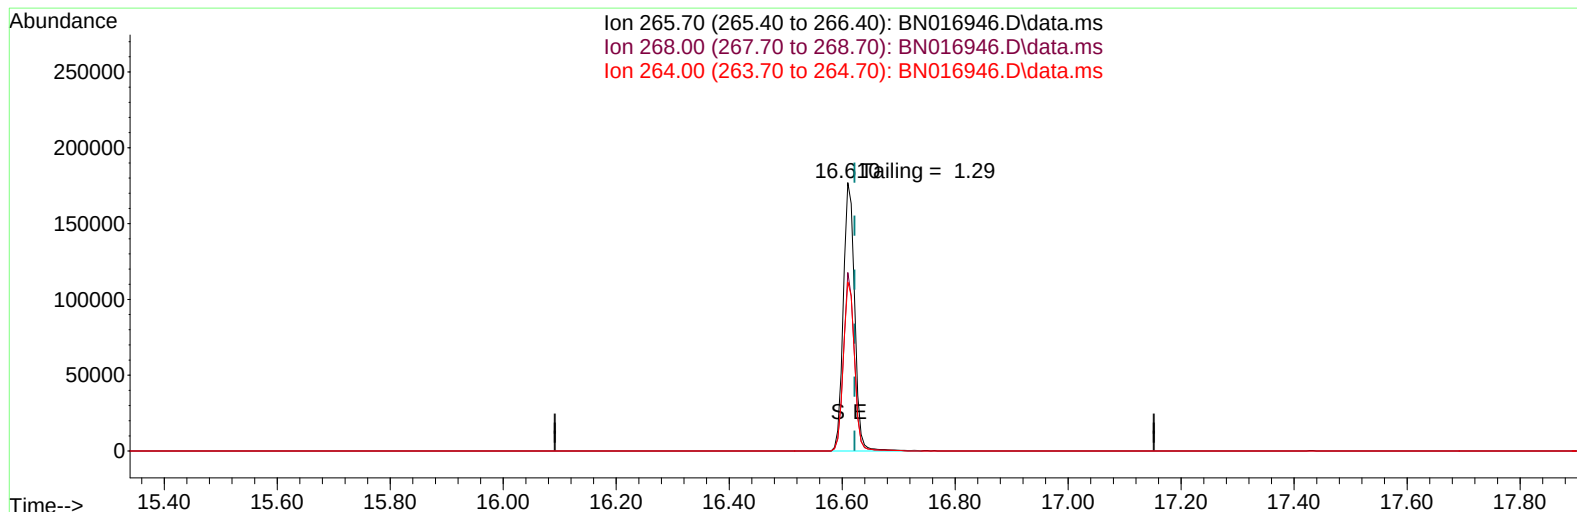

TIC: BN016946.D\data.ms

(70) Pentachlorophenol (C)

16.610min (-0.012) 29948.30 ng




response 246073

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.47
264.00	61.60	62.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101421\
Data File : BN016946.D
Acq On : 14 Oct 2021 12:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 15 04:51:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 17:23:48 2021
Response via : Initial Calibration

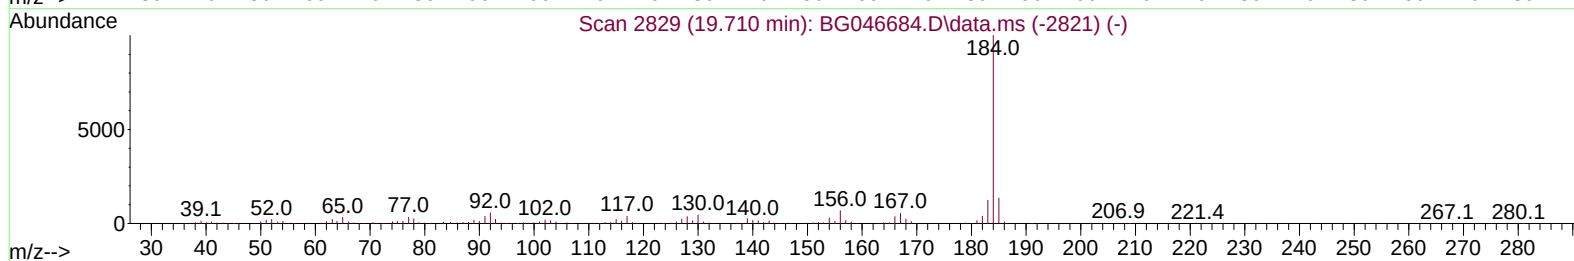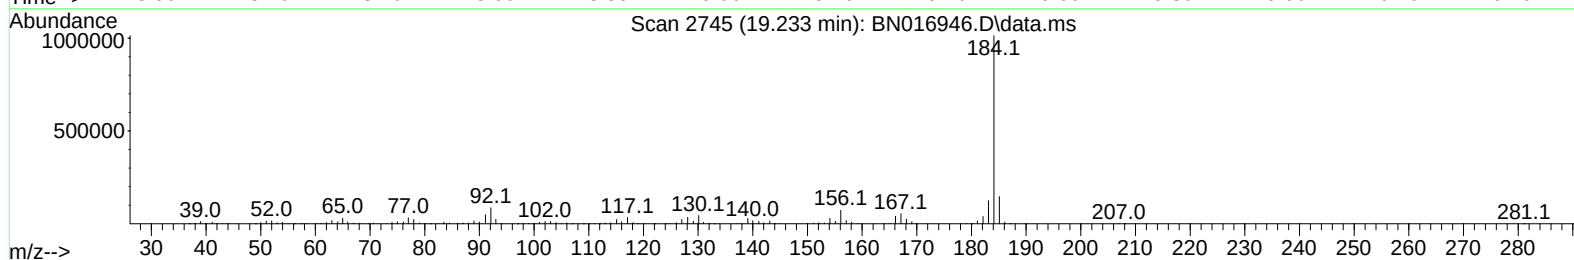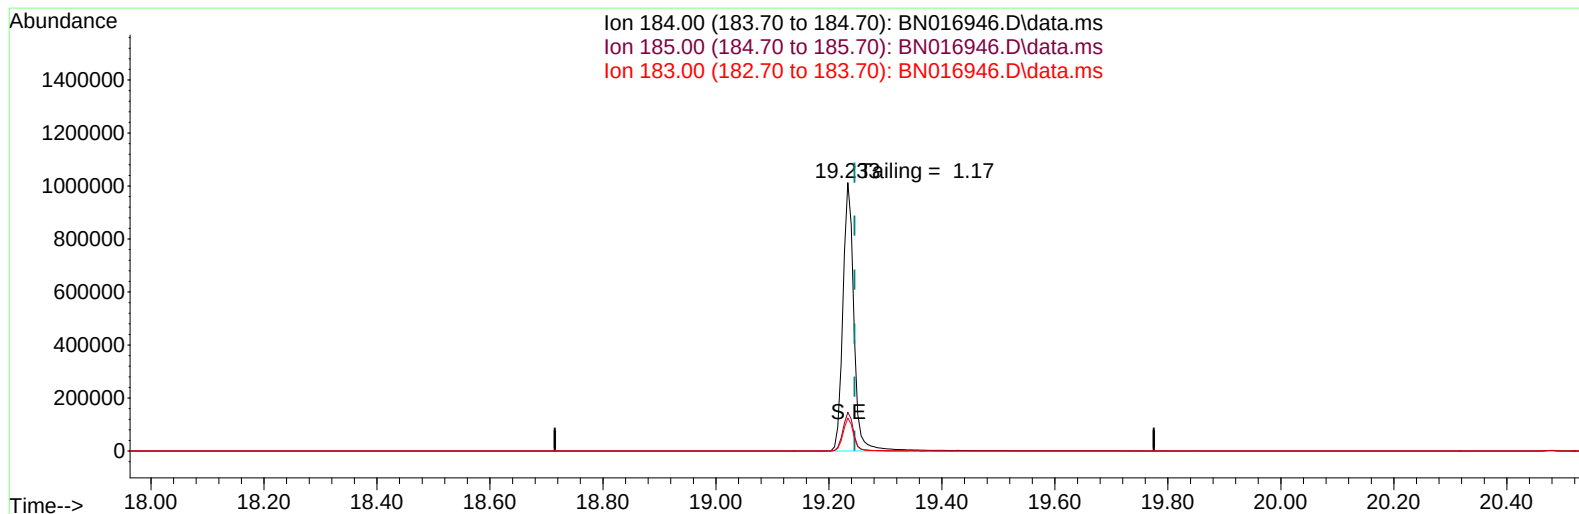

TIC: BN016946.D\data.ms

(77) Benzidine

19.233min (-0.012) 0.00 ng

response 1372636

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.46
183.00	13.20	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/14/2021	BNA_N	<u>BN016946.D</u>
Compound Name	Response	Retention Time
DDT	689823	20.48
DDD	2822	20.086
DDE	0	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2822	692645	0.41

Instrument :
BNA_N
ClientSampleId :
DFTPP