

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
 Data File : BN022089.D
 Acq On : 13 Oct 2022 15:37
 Operator : CG/JU
 Sample : N4984-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGNJ1

Quant Time: Oct 13 22:40:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 13 03:08:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	130109	20.000	ng/ul	0.00
20) Naphthalene-d8	10.786	136	634082	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.633	164	443219	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	934401	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	881972	20.000	ng/ul	0.00
88) Perylene-d12	24.056	264	903211	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	16694	4.863	ng/uL	0.00
4) Pyridine-d5	3.710	84	37480	3.510	ng/ul	0.02
7) Phenol-d5	7.110	99	94491	7.429	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	296920	37.253	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	262725	29.790	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	181263	17.934	ng/ul	0.00
21) Nitrobenzene-d5	9.139	128	179302	38.564	ng/ul	0.00
24) 2-Nitrophenol-d4	9.869	143	180246	37.823	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.404	165	301289	33.681	ng/ul	0.00
31) 4-Chloroaniline-d4	10.933	131	324515	22.189	ng/ul	0.00
46) Dimethylphthalate-d6	14.045	166	1159800	37.539	ng/ul	0.00
49) Acenaphthylene-d8	14.327	160	1264596	36.653	ng/ul	0.00
54) 4-Nitrophenol-d4	14.827	143	32646	4.950	ng/ul	0.00
60) Fluorene-d10	15.621	176	1009808	38.750	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	151886	28.493	ng/ul	0.00
73) Anthracene-d10	17.486	188	1654120	40.736	ng/ul	0.00
81) Pyrene-d10	19.786	212	1746928	39.783	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.892	264	1791938	40.455	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.798	105	16318	1.011	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022089.D
Acq On : 13 Oct 2022 15:37
Operator : CG/JU
Sample : N4984-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGNJ1

Quant Time: Oct 13 22:40:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 13 03:08:08 2022
Response via : Initial Calibration

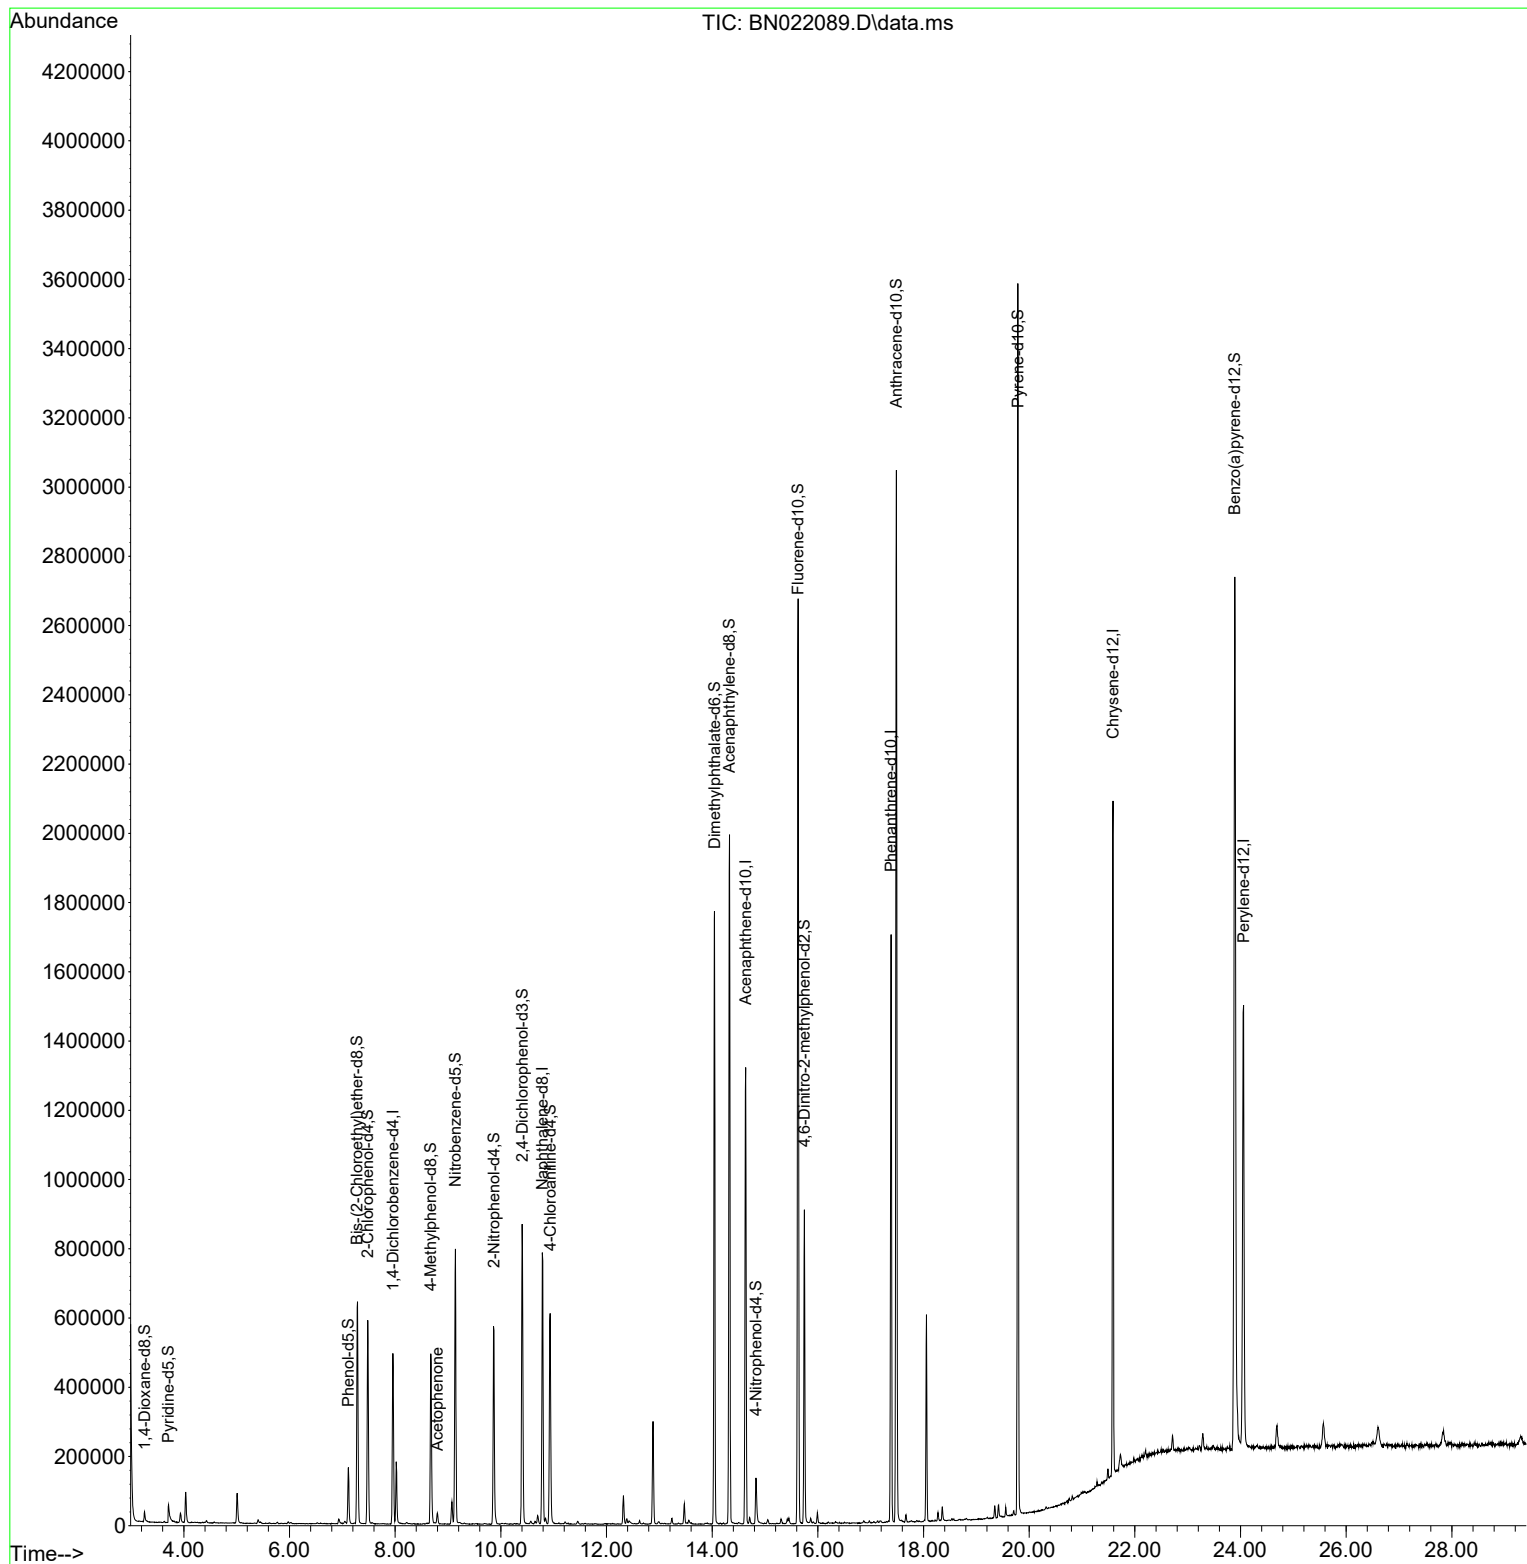

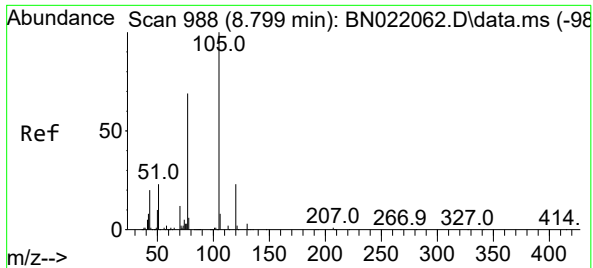

#16
 Acetophenone
 Concen: 1.011 ng/ul
 RT: 8.798 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BN022089.D
 Acq: 13 Oct 2022 15:37

Instrument :
 BNA_N
 ClientSampleId :
 BGNJ1

Tgt Ion:	105	Resp:	16318
Ion	Ratio	Lower	Upper
105	100		
77	87.3	64.9	97.3
51	30.6	21.8	32.6

