

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
 Data File : BN022090.D
 Acq On : 13 Oct 2022 16:15
 Operator : CG/JU
 Sample : N4984-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGNM3

Quant Time: Oct 13 22:40:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 13 03:08:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	99442	20.000	ng/ul	0.00
20) Naphthalene-d8	10.787	136	468991	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.633	164	318530	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	712240	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	739679	20.000	ng/ul	-0.01
88) Perylene-d12	24.051	264	865843	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	14212	5.417	ng/uL	0.00
4) Pyridine-d5	3.705	84	78589	9.629	ng/ul	0.01
7) Phenol-d5	7.116	99	62856	6.466	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	176098	28.907	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	154831	22.970	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	107260	13.885	ng/ul	0.00
21) Nitrobenzene-d5	9.140	128	100273	29.158	ng/ul	0.00
24) 2-Nitrophenol-d4	9.863	143	98227	27.868	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.404	165	163294	24.681	ng/ul	0.00
31) 4-Chloroaniline-d4	10.934	131	458340	42.372	ng/ul	0.00
46) Dimethylphthalate-d6	14.039	166	666077	29.998	ng/ul	0.00
49) Acenaphthylene-d8	14.328	160	710942	28.672	ng/ul	0.00
54) 4-Nitrophenol-d4	14.833	143	22195	4.683	ng/ul	0.00
60) Fluorene-d10	15.622	176	586543	31.319	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	82296	20.254	ng/ul	0.00
73) Anthracene-d10	17.486	188	980017	31.663	ng/ul	0.00
81) Pyrene-d10	19.786	212	1112857	30.219	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.892	264	1318375	31.048	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.093	77	10424	2.171	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022090.D
Acq On : 13 Oct 2022 16:15
Operator : CG/JU
Sample : N4984-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGNM3


Quant Time: Oct 13 22:40:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 13 03:08:08 2022
Response via : Initial Calibration

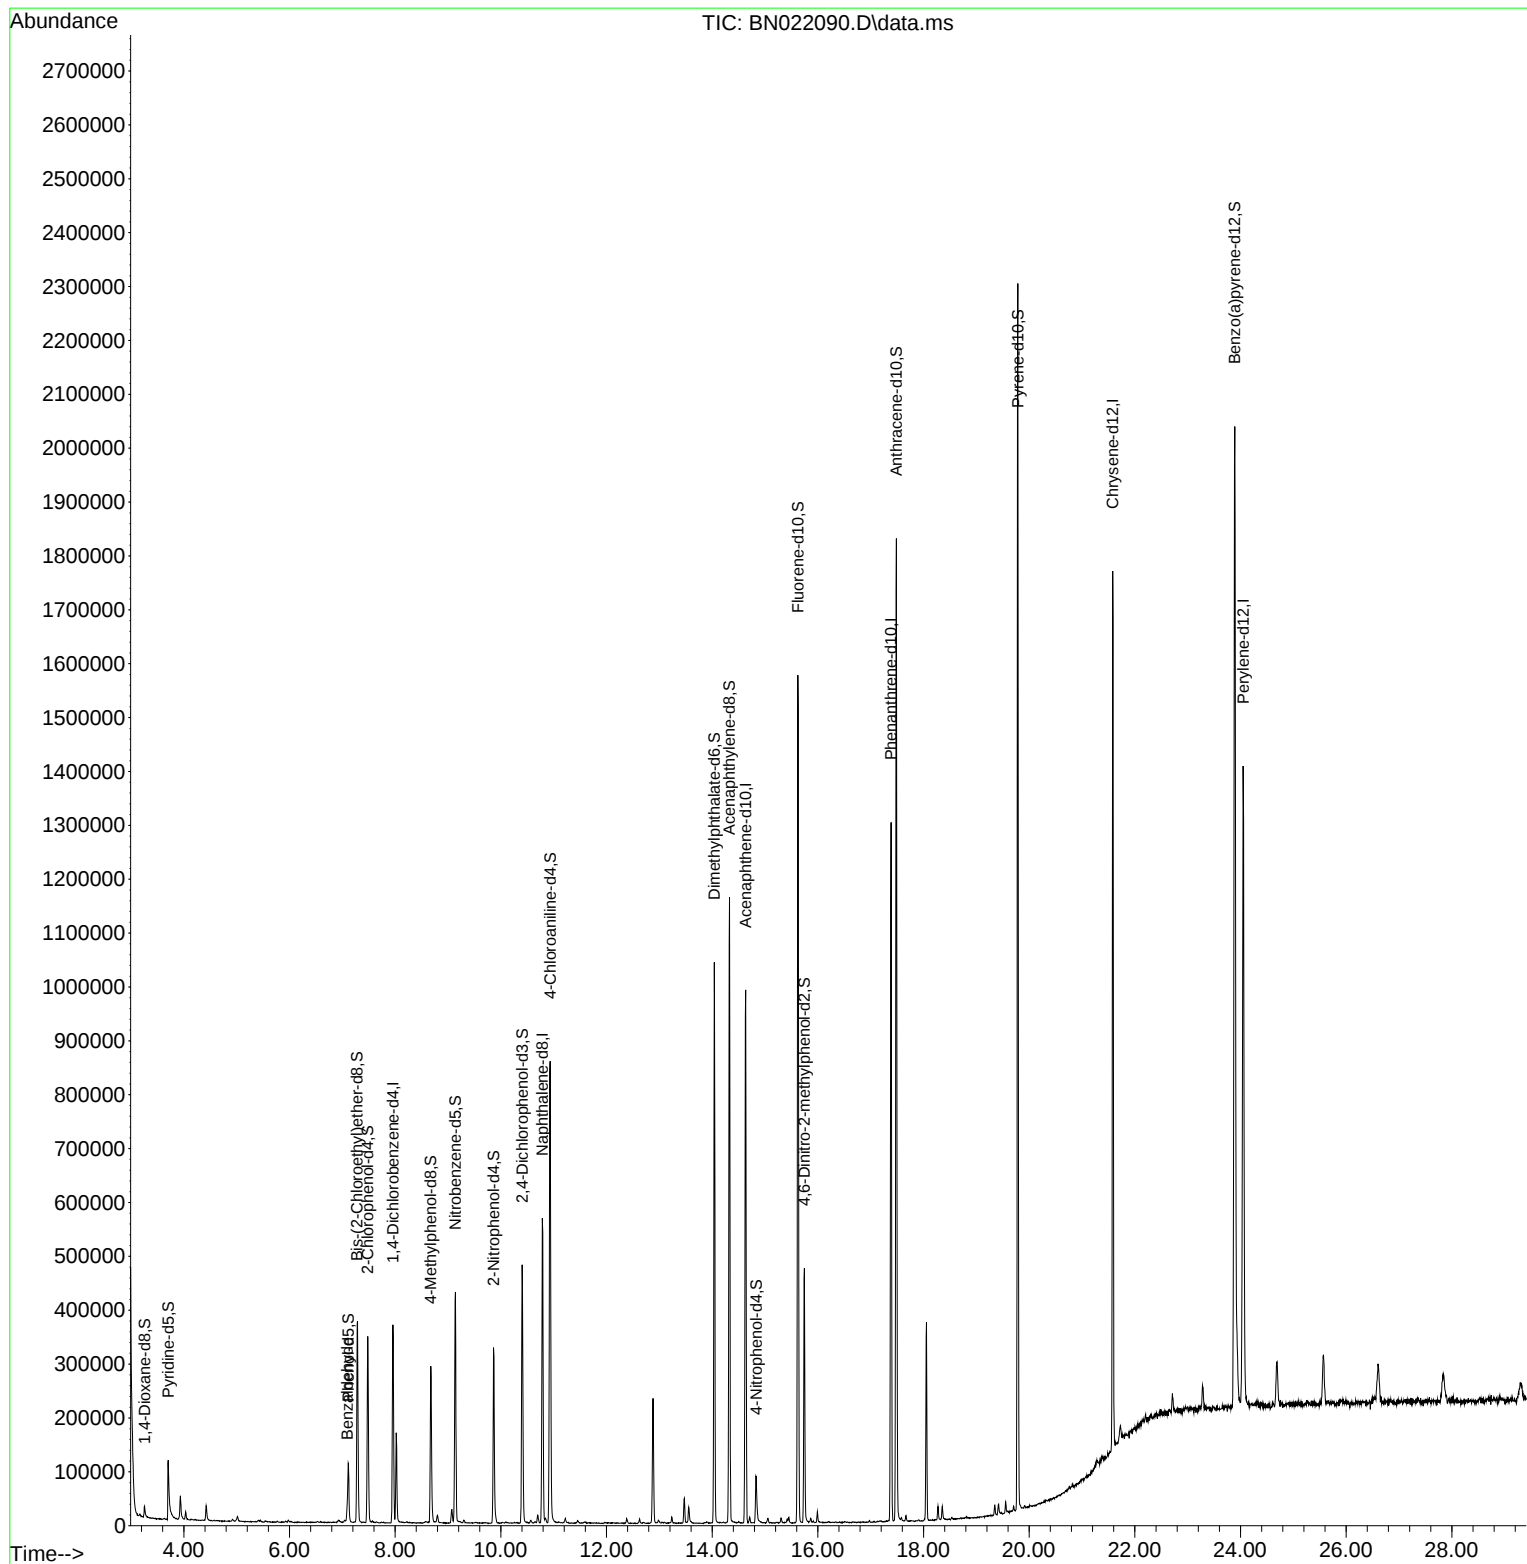

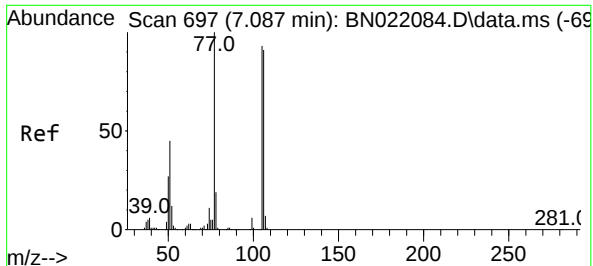

#6
Benzaldehyde
Concen: 2.171 ng/ul
RT: 7.093 min Scan# 698
Delta R.T. -0.000 min
Lab File: BN022090.D
Acq: 13 Oct 2022 16:15

Instrument :
BNA_N
ClientSampleId :
BGNM3

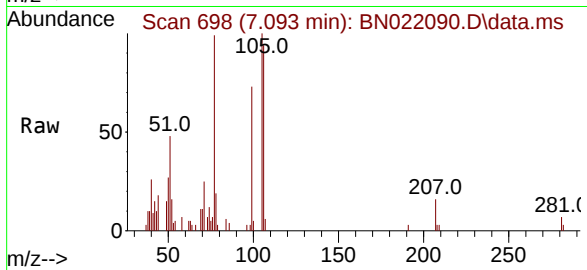

Tgt Ion:	77	Resp:	10424
Ion	Ratio	Lower	Upper
77	100		
105	101.0	78.6	118.0
106	95.3	75.4	113.2

