

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
 Data File : BN022091.D
 Acq On : 13 Oct 2022 16:54
 Operator : CG/JU
 Sample : N4984-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGNM1

Quant Time: Oct 13 22:40:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 13 03:08:08 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	120351	20.000	ng/u1	0.00
20) Naphthalene-d8	10.787	136	580281	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.634	164	393027	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.386	188	805463	20.000	ng/u1	0.00
79) Chrysene-d12	21.580	240	774495	20.000	ng/u1	-0.01
88) Perylene-d12	24.051	264	833439	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	16970	5.344	ng/uL	0.00
4) Pyridine-d5	3.699	84	102188	10.346	ng/u1	0.00
7) Phenol-d5	7.116	99	102833	8.740	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	308451	41.837	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	274400	33.637	ng/u1	0.00
15) 4-Methylphenol-d8	8.675	113	192147	20.553	ng/u1	0.00
21) Nitrobenzene-d5	9.140	128	181225	42.591	ng/u1	0.00
24) 2-Nitrophenol-d4	9.869	143	178697	40.975	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.404	165	306518	37.443	ng/u1	0.00
31) 4-Chloroaniline-d4	10.934	131	433444	32.385	ng/u1	0.00
46) Dimethylphthalate-d6	14.045	166	1205304	43.994	ng/u1	0.00
49) Acenaphthylene-d8	14.328	160	1300837	42.519	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	37042	6.334	ng/u1	0.00
60) Fluorene-d10	15.628	176	1002233	43.371	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	140743	30.629	ng/u1	0.00
73) Anthracene-d10	17.486	188	1601340	45.749	ng/u1	0.00
81) Pyrene-d10	19.786	212	1781497	46.200	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.892	264	1869626	45.742	ng/u1	0.00
Target Compounds						
16) Acetophenone	8.799	105	17151	1.148	ng/u1	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022091.D
Acq On : 13 Oct 2022 16:54
Operator : CG/JU
Sample : N4984-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGNM1

Quant Time: Oct 13 22:40:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 13 03:08:08 2022
Response via : Initial Calibration

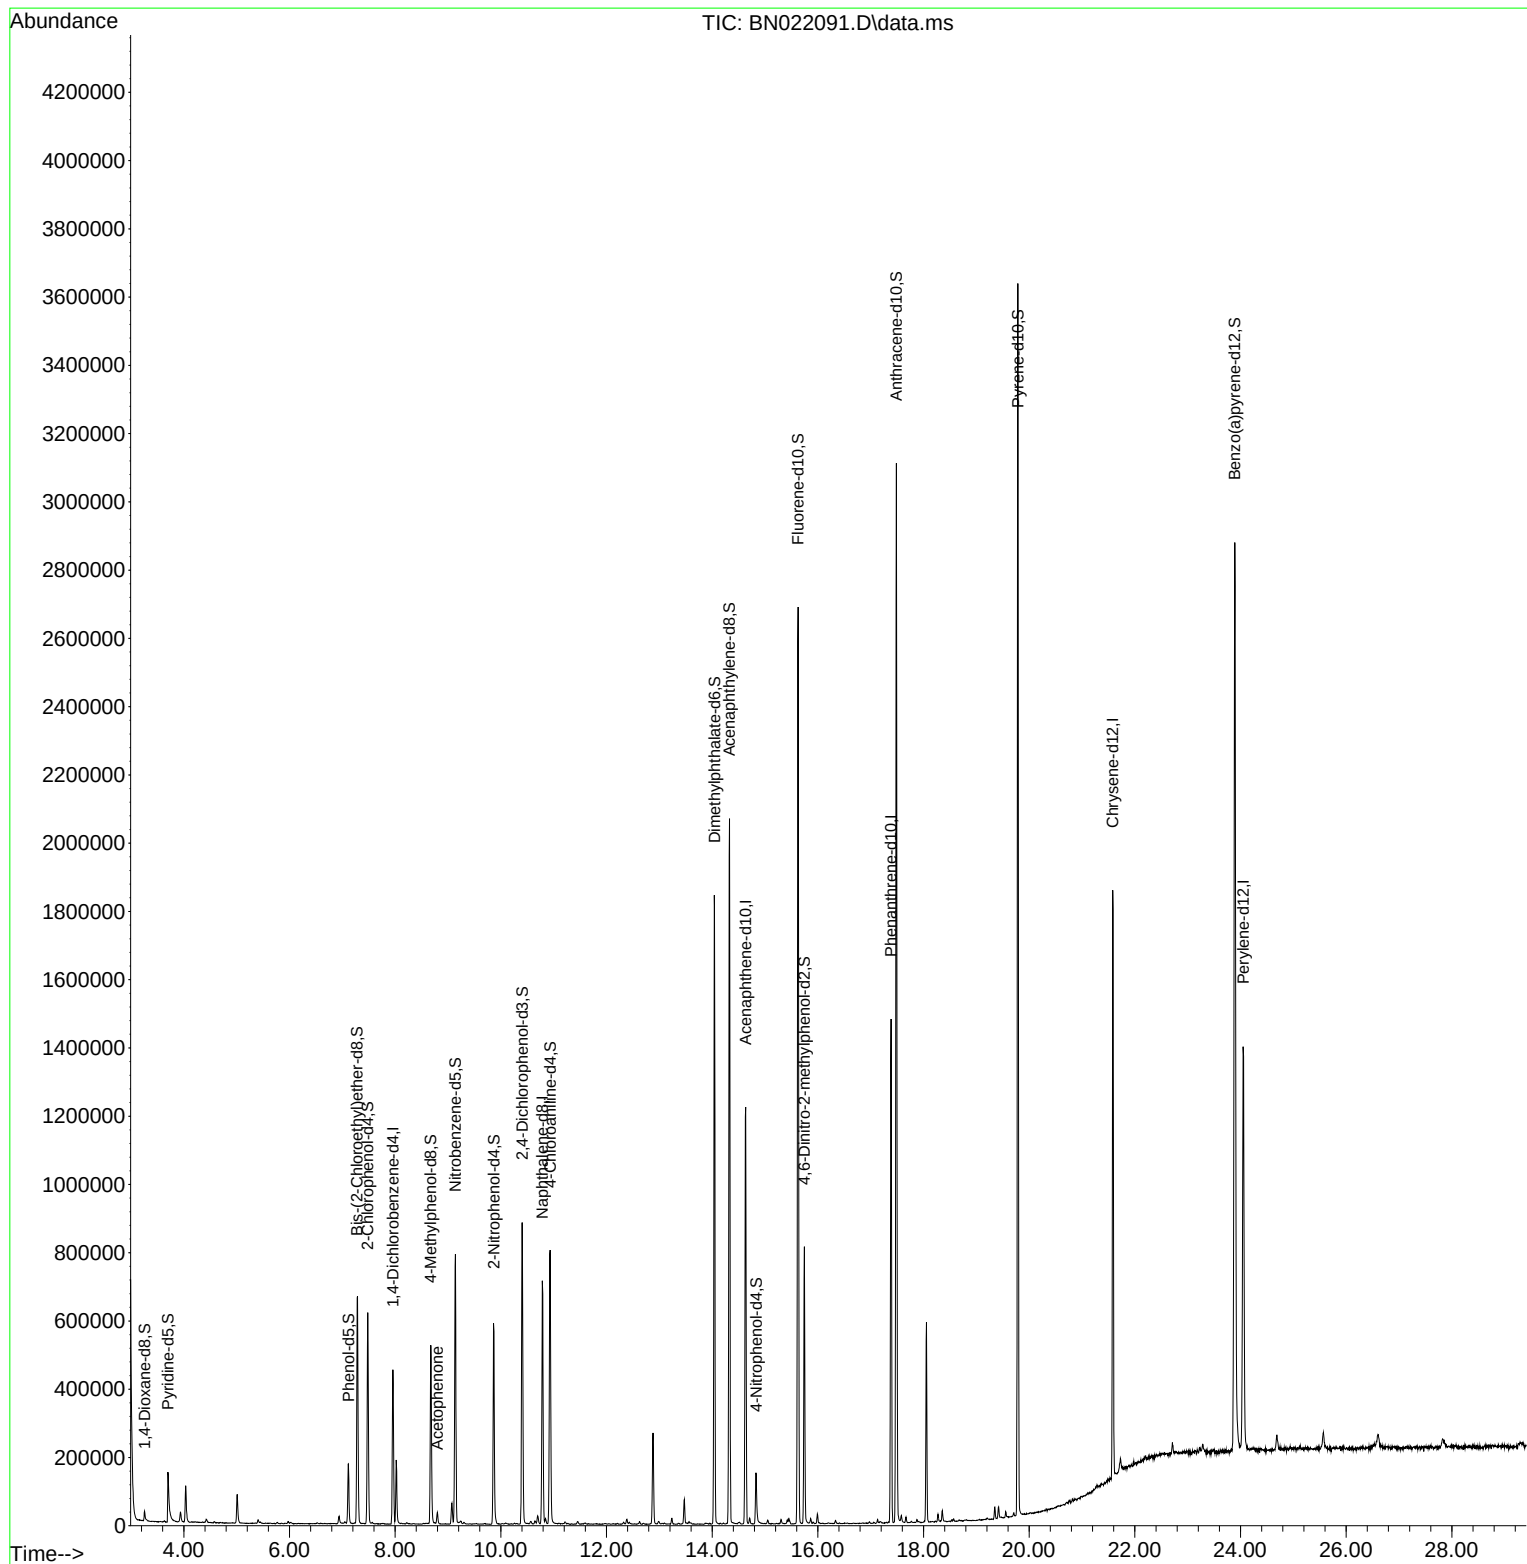

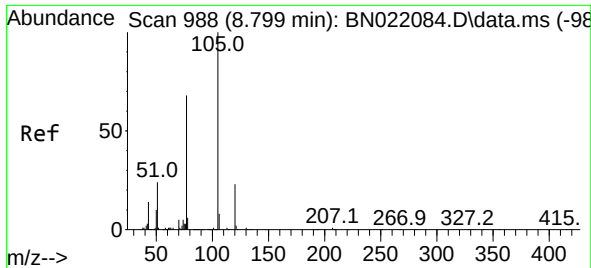

#16
 Acetophenone
 Concen: 1.148 ng/ul
 RT: 8.799 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BN022091.D
 Acq: 13 Oct 2022 16:54

Instrument :
 BNA_N
 ClientSampleId :
 BGNM1

Tgt Ion:	105	Resp:	17151
Ion	Ratio	Lower	Upper
105	100		
77	85.1	64.9	97.3
51	28.1	21.8	32.6

