

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
 Data File : BN022130.D
 Acq On : 14 Oct 2022 19:24
 Operator : CG/JU
 Sample : N5023-09
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC2

Quant Time: Oct 15 00:28:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 13 03:08:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	150658	20.000	ng/ul	0.00
20) Naphthalene-d8	10.787	136	702113	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.627	164	456332	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	938295	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	822113	20.000	ng/ul	0.00
88) Perylene-d12	24.051	264	705717	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	19392	4.878	ng/uL	0.00
4) Pyridine-d5	3.699	84	109056	8.820	ng/ul	0.00
7) Phenol-d5	7.110	99	382983	26.003	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	236020	25.573	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	284708	27.880	ng/ul	0.00
15) 4-Methylphenol-d8	8.675	113	294977	25.205	ng/ul	0.00
21) Nitrobenzene-d5	9.134	128	151150	29.359	ng/ul	0.00
24) 2-Nitrophenol-d4	9.863	143	169103	32.046	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.404	165	277999	28.066	ng/ul	0.00
31) 4-Chloroaniline-d4	10.928	131	412730	25.487	ng/ul	0.00
46) Dimethylphthalate-d6	14.039	166	908697	28.566	ng/ul	0.00
49) Acenaphthylene-d8	14.322	160	1005868	28.317	ng/ul	0.00
54) 4-Nitrophenol-d4	14.827	143	166178	24.475	ng/ul	0.00
60) Fluorene-d10	15.622	176	778025	28.998	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	106407	19.878	ng/ul	0.00
73) Anthracene-d10	17.486	188	1206970	29.601	ng/ul	0.00
81) Pyrene-d10	19.780	212	1353311	33.063	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.892	264	1081845	31.258	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.140	94	18348	1.174	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022130.D
Acq On : 14 Oct 2022 19:24
Operator : CG/JU
Sample : N5023-09
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC2

Quant Time: Oct 15 00:28:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 13 03:08:08 2022
Response via : Initial Calibration

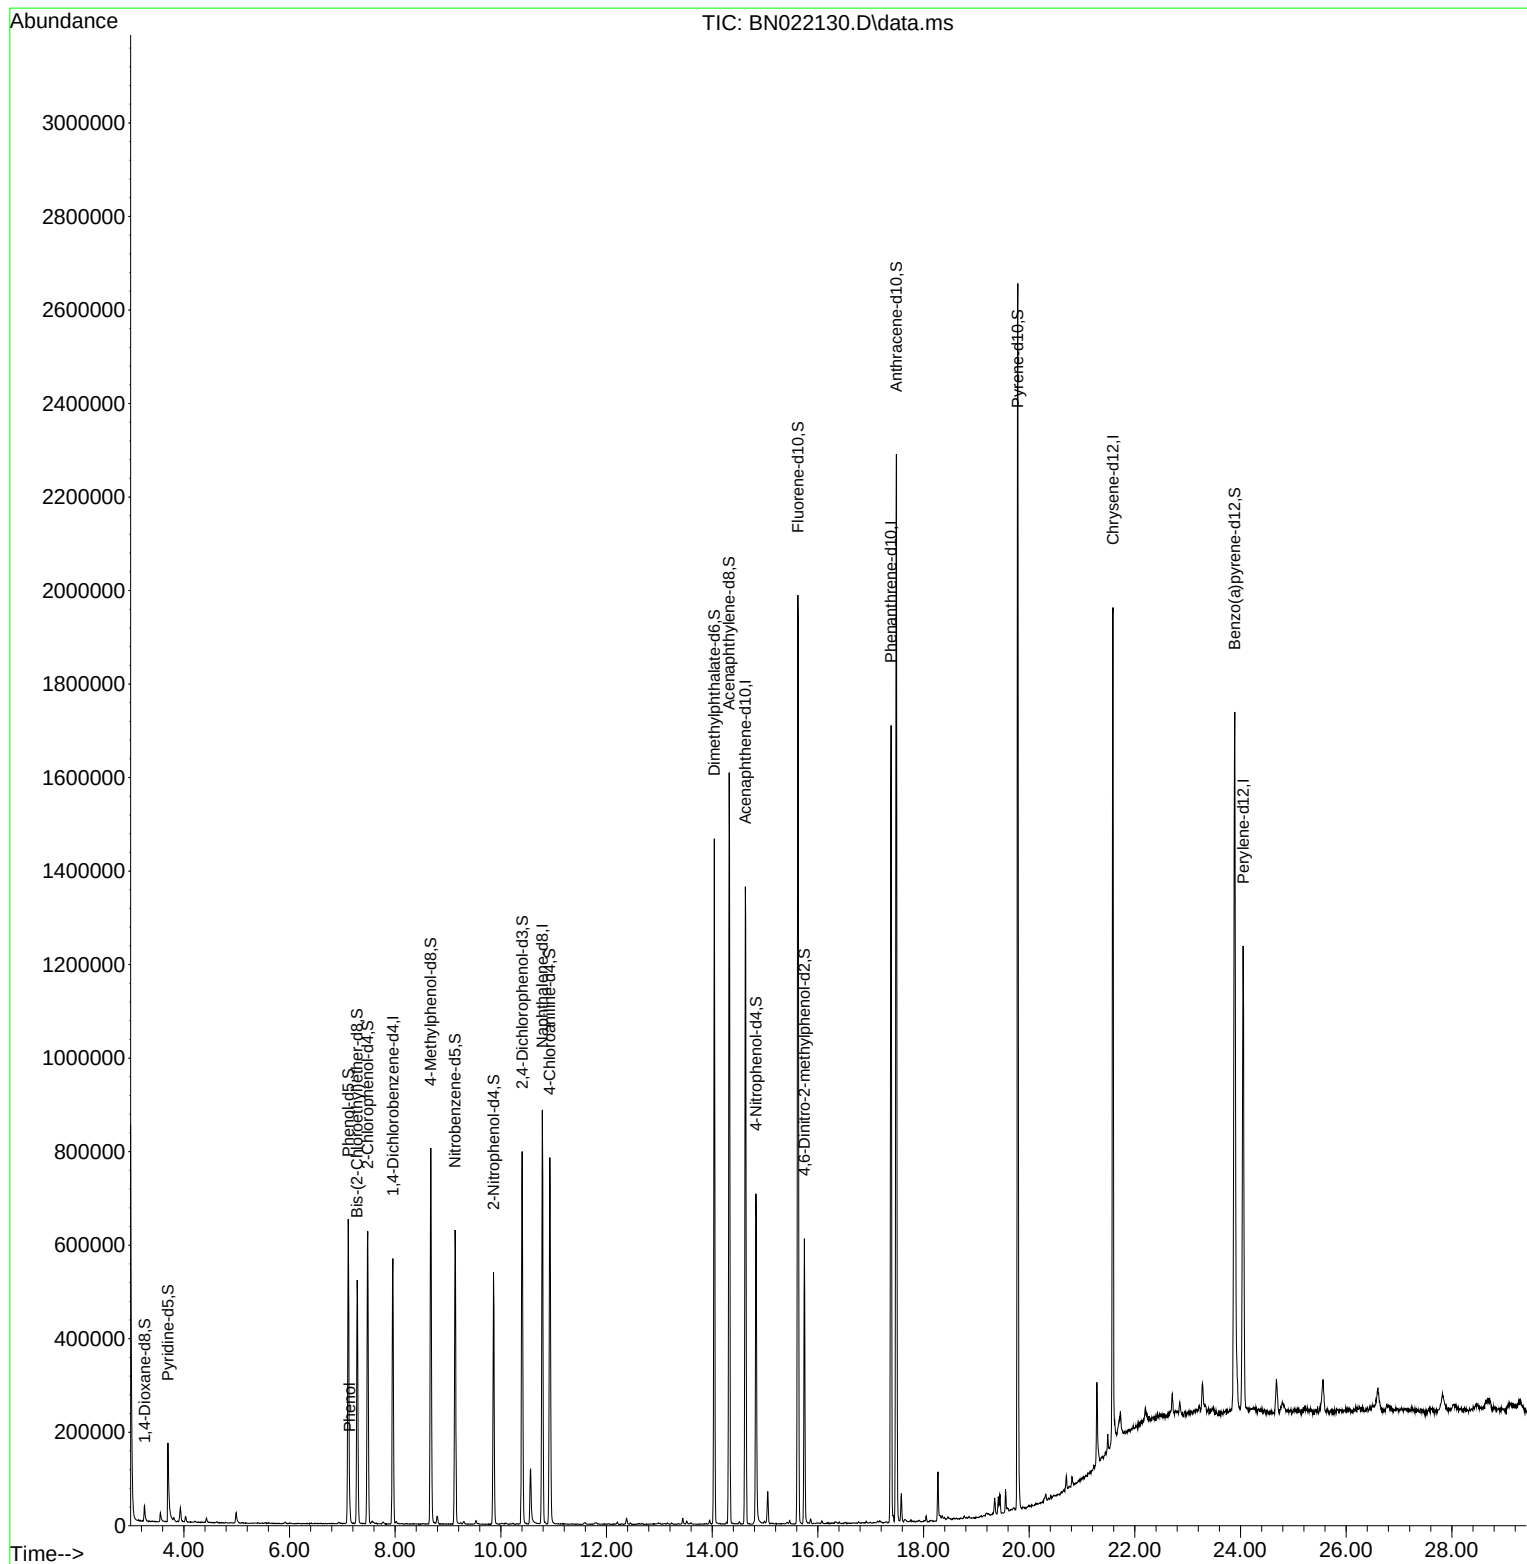

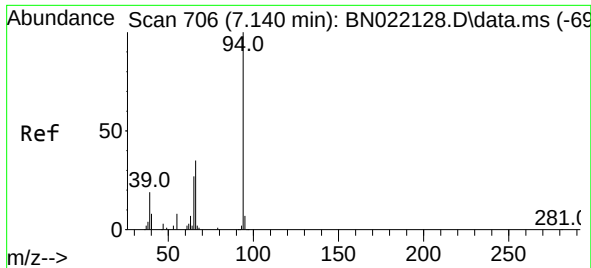

#8
Phenol
Concen: 1.174 ng/ul
RT: 7.140 min Scan# 706
Delta R.T. -0.000 min
Lab File: BN022130.D
Acq: 14 Oct 2022 19:24

Instrument :
BNA_N
ClientSampleId :
C0BC2

Tgt Ion: 94 Resp: 18348
Ion Ratio Lower Upper
94 100
65 24.9 22.1 33.1
66 38.8 29.0 43.6

