

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
 Data File : BN022086.D
 Acq On : 13 Oct 2022 13:43
 Operator : CG/JU
 Sample : PB148241BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	58	rVB	39856	62574	1.41%	0.143%
2	3.693	117	120	144	rBV	456687	811543	18.26%	1.851%
3	4.034	174	178	183	rBV	9050	11779	0.27%	0.027%
4	7.110	695	701	716	rBV	652788	1048624	23.59%	2.392%
5	7.287	723	731	744	rBV	543574	890483	20.04%	2.031%
6	7.481	756	764	779	rBV	658951	1036079	23.31%	2.363%
7	7.957	838	845	857	rBV	574134	924734	20.81%	2.109%
8	8.675	961	967	982	rBV	803310	1281639	28.84%	2.923%
9	9.140	1035	1046	1060	rBV	611550	1028407	23.14%	2.346%
10	9.863	1162	1169	1181	rBV	498212	812024	18.27%	1.852%
11	10.404	1254	1261	1276	rBV	747307	1255818	28.26%	2.864%
12	10.787	1318	1326	1335	rBV	864374	1462969	32.92%	3.337%
13	10.934	1343	1351	1367	rBV	750317	1340233	30.15%	3.057%
14	12.387	1593	1598	1603	rBV	10097	17142	0.39%	0.039%
15	14.039	1873	1879	1890	rBV	1478751	2039538	45.89%	4.652%
16	14.328	1921	1928	1936	rBV	1609186	2340123	52.65%	5.337%
17	14.634	1973	1980	1990	rBV	1439422	2069221	46.56%	4.719%
18	14.828	2006	2013	2037	rBV	783876	1133151	25.50%	2.584%
19	15.628	2142	2149	2160	rVB	1999091	3008304	67.69%	6.861%
20	15.745	2163	2169	2186	rBV	769548	1009472	22.71%	2.302%
21	15.869	2186	2190	2198	rVB3	7848	11473	0.26%	0.026%
22	17.386	2441	2448	2457	rVV	1732576	2498095	56.21%	5.697%
23	17.486	2458	2465	2483	rBV	2505278	3451437	77.66%	7.872%
24	17.763	2510	2512	2519	rVB6	2287	4932	0.11%	0.011%
25	18.363	2609	2614	2617	rBV4	3418	6250	0.14%	0.014%
26	19.351	2777	2782	2786	rBV2	24631	33547	0.75%	0.077%
27	19.421	2789	2794	2799	rBV2	25731	34963	0.79%	0.080%
28	19.710	2840	2843	2847	rVB5	7796	8402	0.19%	0.019%
29	19.786	2850	2856	2869	rVV	2869618	3911597	88.01%	8.921%
30	21.586	3156	3162	3170	rBV2	2078104	2864869	64.46%	6.534%
31	23.892	3546	3554	3569	rBV2	2139484	4444520	100.00%	10.137%
32	24.051	3574	3581	3591	rVB2	1456935	2991863	67.32%	6.824%




Sum of corrected areas: 43845805

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022086.D
Acq On : 13 Oct 2022 13:43
Operator : CG/JU
Sample : PB148241BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK241

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

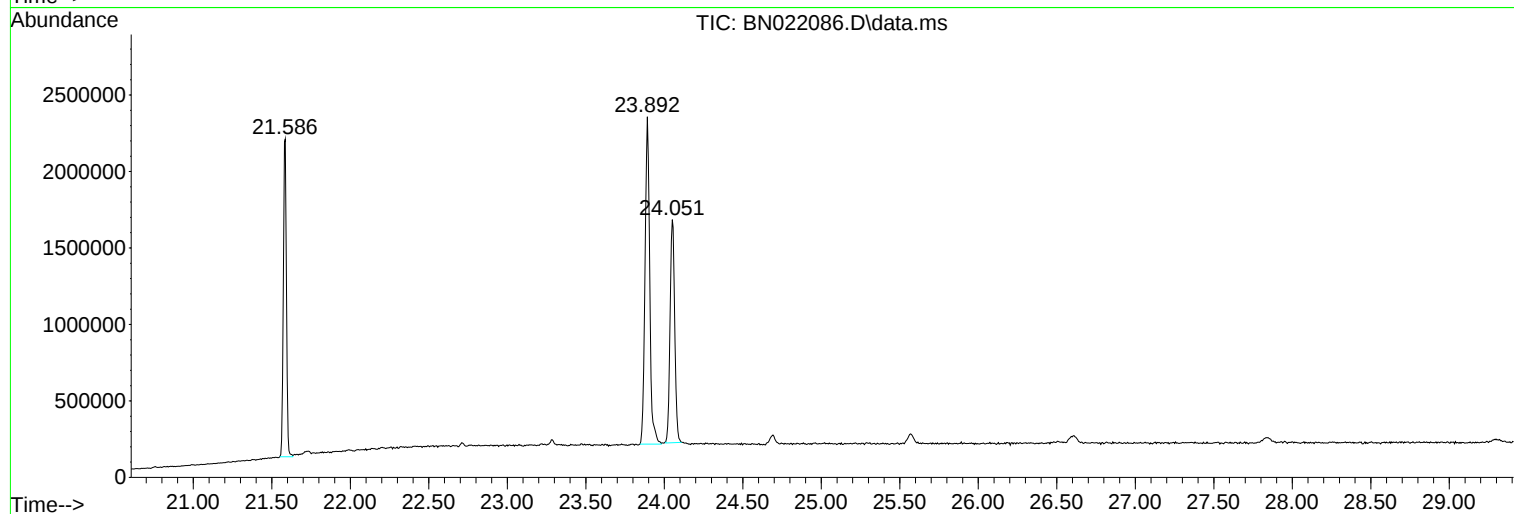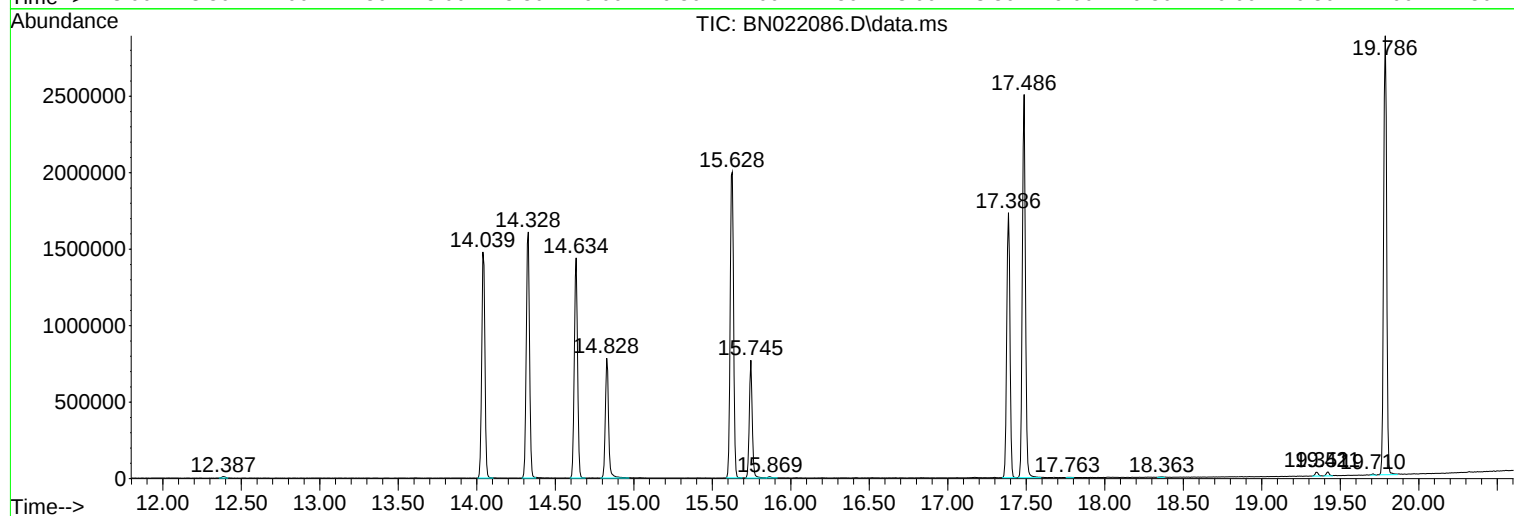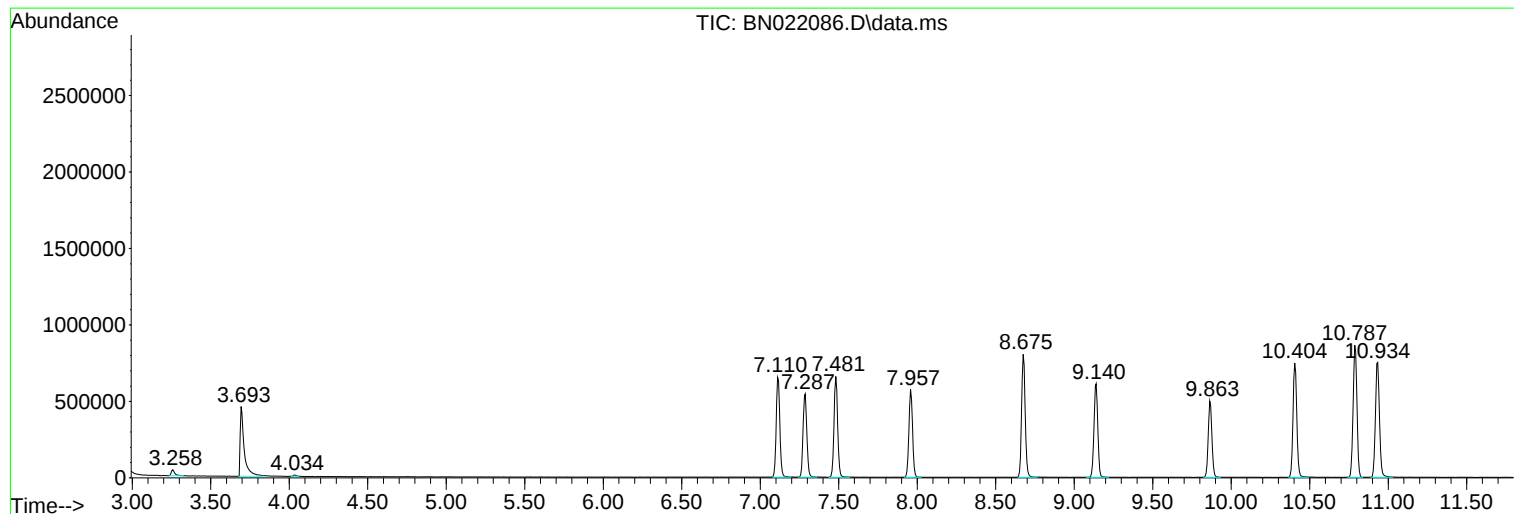

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022086.D
Acq On : 13 Oct 2022 13:43
Operator : CG/JU
Sample : PB148241BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK241

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022086.D
Acq On : 13 Oct 2022 13:43
Operator : CG/JU
Sample : PB148241BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK241

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc