

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
 Data File : BN022102.D
 Acq On : 14 Oct 2022 00:33
 Operator : CG/JU
 Sample : PB148290BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK290

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	42	46	55	rBV	37783	55637	1.17%	0.121%
2	3.693	117	120	144	rBV	483923	823905	17.35%	1.793%
3	4.034	174	178	182	rBV	10010	14235	0.30%	0.031%
4	7.110	694	701	711	rBV	677544	1056798	22.25%	2.300%
5	7.281	724	730	739	rBV	553924	882261	18.58%	1.920%
6	7.481	756	764	778	rVB	632526	1026207	21.61%	2.233%
7	7.957	836	845	857	rBV	631224	1031199	21.71%	2.244%
8	8.675	960	967	975	rBV	822936	1301568	27.41%	2.832%
9	9.134	1038	1045	1060	rBV	636491	1038531	21.87%	2.260%
10	9.863	1162	1169	1184	rBV	515002	826530	17.40%	1.799%
11	10.404	1253	1261	1273	rBV	758010	1284674	27.05%	2.796%
12	10.787	1318	1326	1334	rVB	1007420	1655032	34.85%	3.602%
13	10.928	1343	1350	1370	rBV	808759	1367354	28.79%	2.976%
14	12.381	1592	1597	1604	rBV	11150	19837	0.42%	0.043%
15	13.522	1784	1791	1794	rBV5	3677	5974	0.13%	0.013%
16	14.039	1872	1879	1892	rBV	1496456	2025275	42.64%	4.407%
17	14.322	1920	1927	1944	rBV	1676059	2399112	50.52%	5.221%
18	14.628	1973	1979	1989	rVB	1586365	2318508	48.82%	5.046%
19	14.827	2006	2013	2025	rBV	800520	1130428	23.80%	2.460%
20	15.622	2140	2148	2162	rVB	2146236	3045068	64.12%	6.627%
21	15.745	2162	2169	2184	rVV	729855	1000923	21.08%	2.178%
22	15.863	2184	2189	2195	rVB2	9405	15035	0.32%	0.033%
23	16.410	2277	2282	2289	rBV6	2538	4942	0.10%	0.011%
24	17.169	2407	2411	2415	rBV3	3402	4761	0.10%	0.010%
25	17.380	2441	2447	2458	rBV	1909061	2777705	58.49%	6.045%
26	17.486	2458	2465	2478	rBV	2301729	3430486	72.23%	7.465%
27	19.345	2777	2781	2787	rBV	25467	35110	0.74%	0.076%
28	19.415	2789	2793	2797	rBV	25203	33541	0.71%	0.073%
29	19.704	2839	2842	2845	rBV4	7095	8551	0.18%	0.019%
30	19.780	2849	2855	2868	rBV	2843107	3972239	83.64%	8.644%
31	21.580	3155	3161	3169	rBV	2474729	3208793	67.56%	6.983%
32	23.886	3545	3553	3570	rBV2	2195397	4749255	100.00%	10.335%
33	24.051	3573	3581	3589	rVV	1653247	3402503	71.64%	7.404%




Sum of corrected areas: 45951977

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022102.D
Acq On : 14 Oct 2022 00:33
Operator : CG/JU
Sample : PB148290BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK290

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

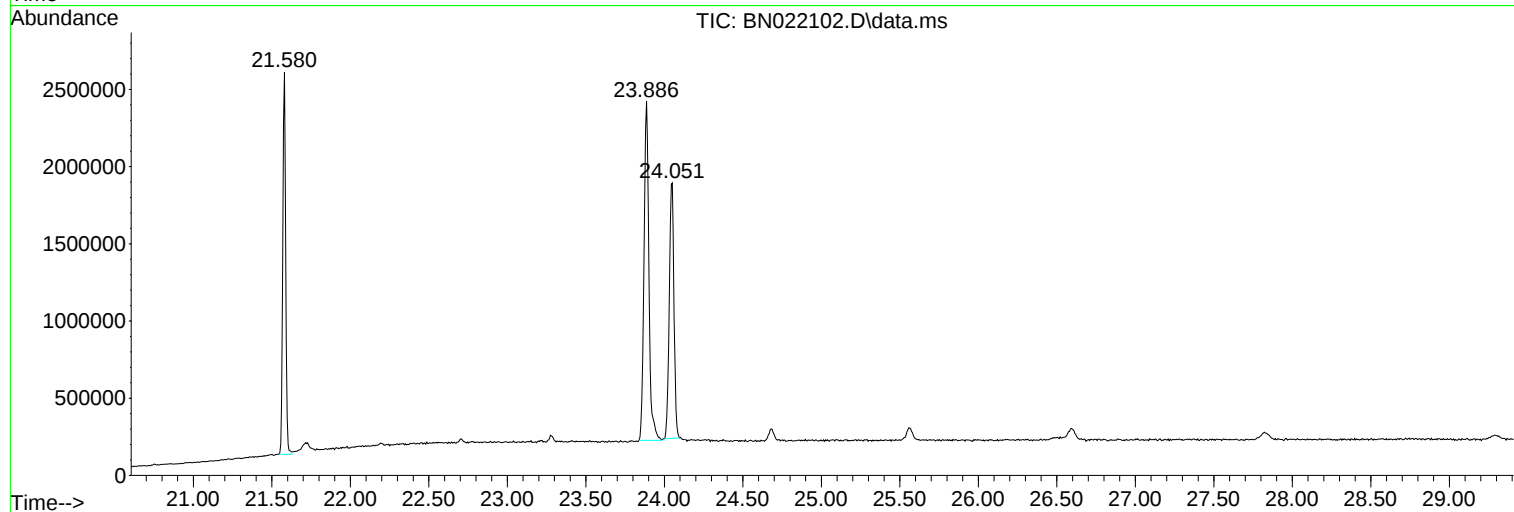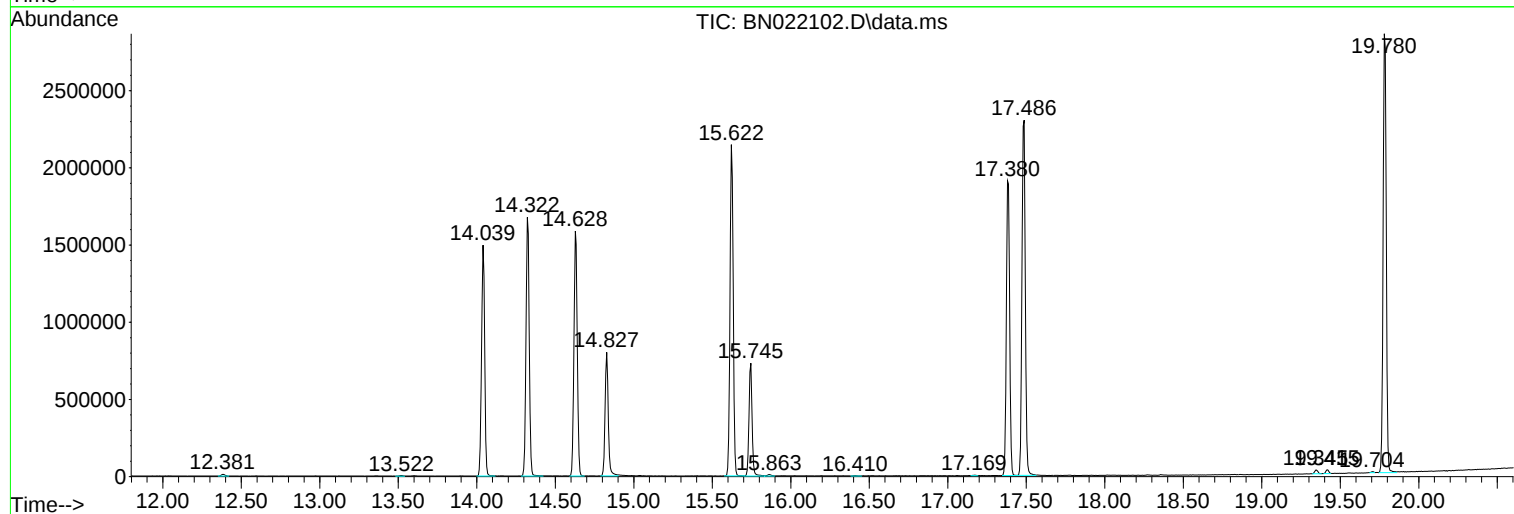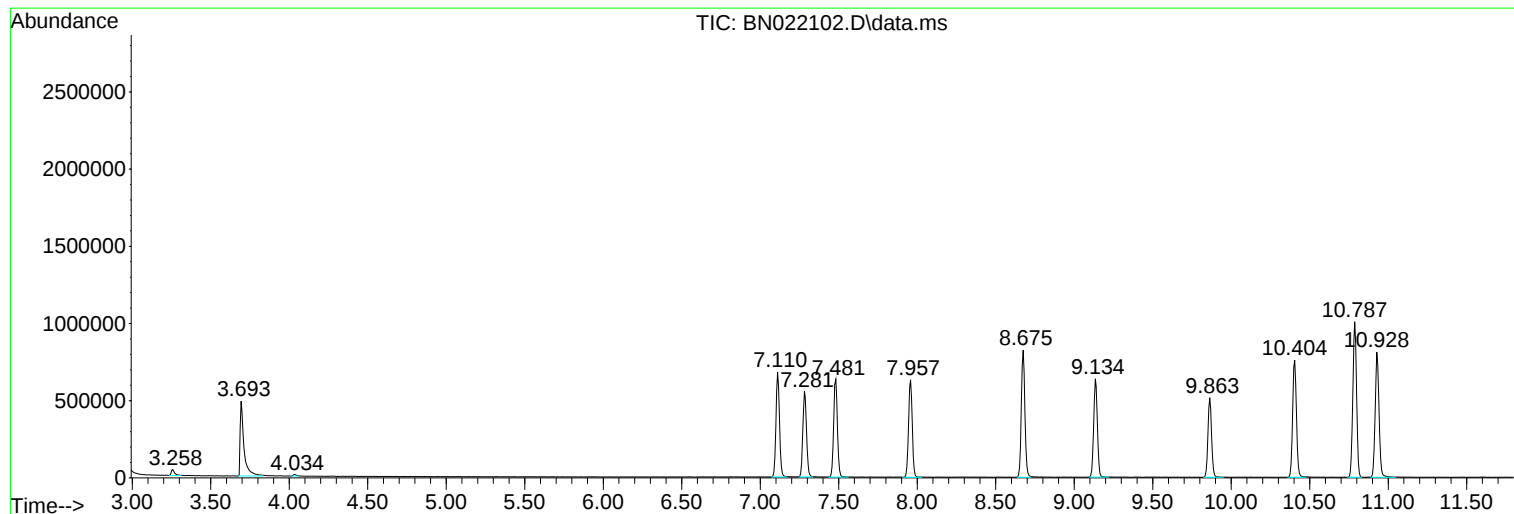

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022102.D
Acq On : 14 Oct 2022 00:33
Operator : CG/JU
Sample : PB148290BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK290

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022102.D
Acq On : 14 Oct 2022 00:33
Operator : CG/JU
Sample : PB148290BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK290

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc