

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
 Data File : BN022119.D
 Acq On : 14 Oct 2022 11:49
 Operator : CG/JU
 Sample : PB148256BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK256

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	57	rVB	51941	75336	1.42%	0.131%
2	3.687	116	119	143	rBV	687130	1127922	21.31%	1.957%
3	4.034	174	178	182	rVB	10437	13842	0.26%	0.024%
4	7.110	694	701	711	rBV	929289	1464200	27.66%	2.541%
5	7.281	723	730	743	rVB	781259	1212474	22.91%	2.104%
6	7.475	756	763	775	rBV	904934	1433967	27.09%	2.488%
7	7.951	837	844	854	rBV	650542	1033950	19.53%	1.794%
8	8.675	959	967	977	rBV	1128356	1859789	35.13%	3.227%
9	9.134	1037	1045	1059	rBV	918925	1498211	28.30%	2.600%
10	9.863	1161	1169	1179	rBV	762350	1265038	23.90%	2.195%
11	10.398	1253	1260	1276	rBV	1114584	1878029	35.48%	3.259%
12	10.786	1318	1326	1335	rVB	1005023	1740586	32.88%	3.020%
13	10.928	1341	1350	1368	rBV	1216800	2058483	38.89%	3.572%
14	12.380	1592	1597	1604	rVB2	20133	32577	0.62%	0.057%
15	14.039	1872	1879	1890	rBV	2092252	2871518	54.25%	4.983%
16	14.322	1920	1927	1936	rBV2	2398469	3513803	66.38%	6.097%
17	14.627	1972	1979	1989	rBV	1668781	2459967	46.47%	4.269%
18	14.827	2006	2013	2032	rBV	1141534	1658692	31.34%	2.878%
19	15.039	2044	2049	2055	rVB6	4810	8094	0.15%	0.014%
20	15.621	2141	2148	2159	rBV	2993748	4272843	80.72%	7.415%
21	15.745	2163	2169	2183	rBV	1067077	1473511	27.84%	2.557%
22	15.863	2183	2189	2196	rVB2	13449	19720	0.37%	0.034%
23	17.386	2441	2448	2457	rBV	2036059	2947300	55.68%	5.114%
24	17.486	2457	2465	2478	rBV	3114462	4632362	87.51%	8.038%
25	17.768	2510	2513	2520	rVB6	3778	6648	0.13%	0.012%
26	19.345	2777	2781	2788	rBV3	40104	50820	0.96%	0.088%
27	19.415	2788	2793	2799	rBV	44834	61089	1.15%	0.106%
28	19.704	2839	2842	2845	rBV	11839	12827	0.24%	0.022%
29	19.786	2849	2856	2867	rBV	3620068	5255495	99.29%	9.120%
30	21.580	3156	3161	3167	rBV2	2547609	3233340	61.08%	5.611%
31	23.886	3545	3553	3567	rVB2	2421310	5293312	100.00%	9.185%
32	24.045	3573	3580	3589	rVB2	1457982	2989014	56.47%	5.187%
33	24.680	3685	3688	3698	rVB	92294	172620	3.26%	0.300%




Sum of corrected areas: 57627379

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022119.D
Acq On : 14 Oct 2022 11:49
Operator : CG/JU
Sample : PB148256BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK256

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

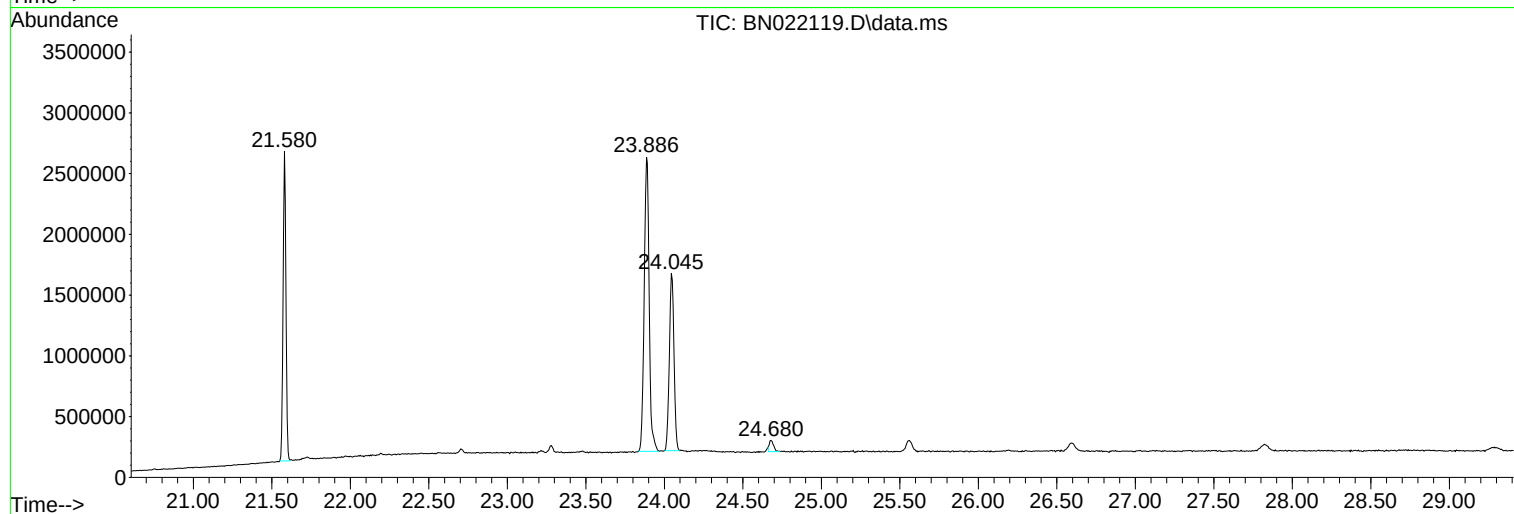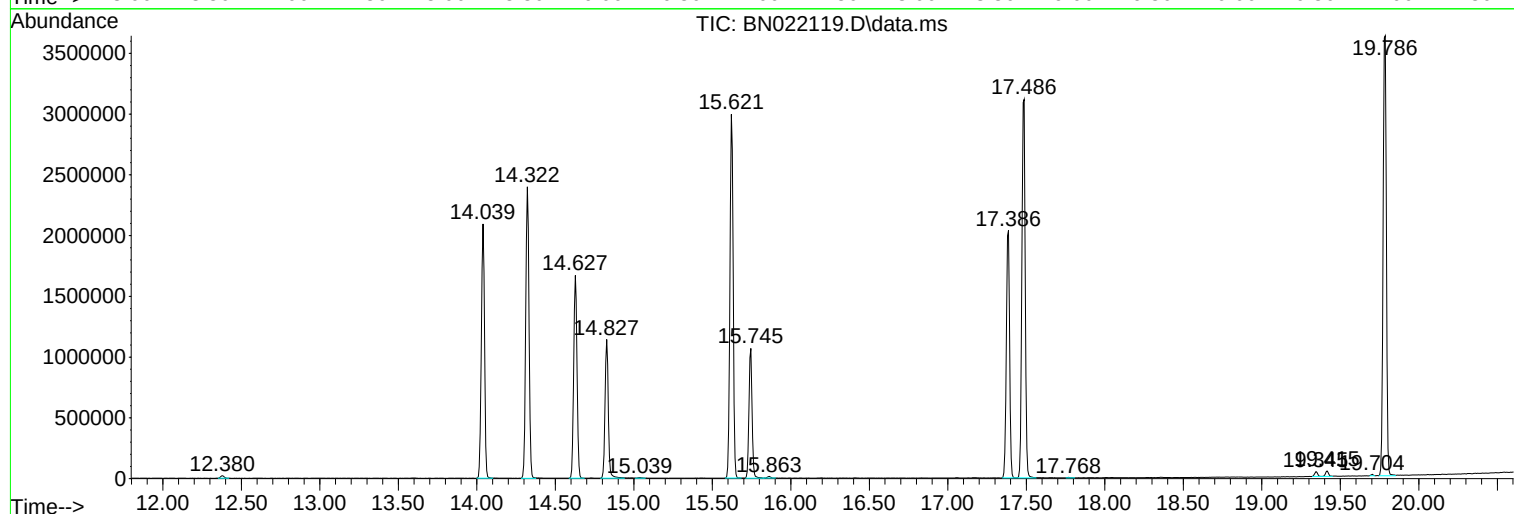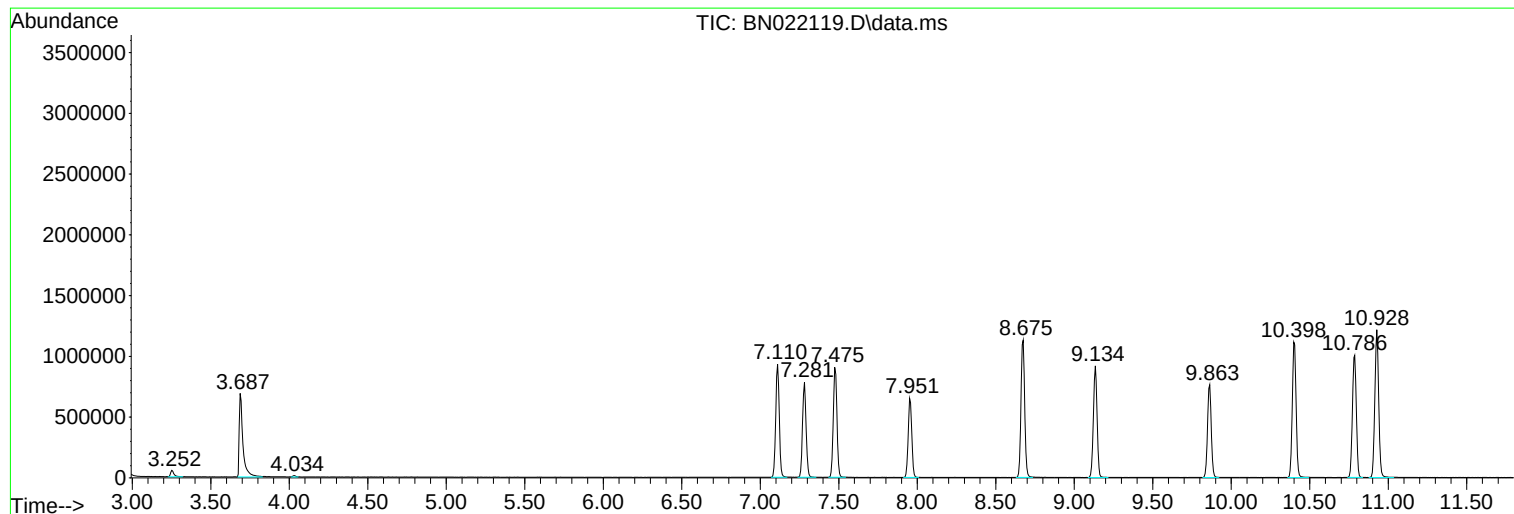

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022119.D
Acq On : 14 Oct 2022 11:49
Operator : CG/JU
Sample : PB148256BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK256

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022119.D
Acq On : 14 Oct 2022 11:49
Operator : CG/JU
Sample : PB148256BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK256

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------