

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
 Data File : BN022129.D
 Acq On : 14 Oct 2022 18:46
 Operator : CG/JU
 Sample : PB148269BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022129.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	42	45	57	rVB	37516	57661	1.52%	0.129%
2	3.693	116	120	147	rBV	534634	884578	23.32%	1.976%
3	4.034	174	178	184	rVB2	9675	14753	0.39%	0.033%
4	7.110	694	701	715	rBV	724019	1176347	31.02%	2.628%
5	7.281	723	730	742	rVB	605172	942616	24.85%	2.106%
6	7.481	756	764	775	rBV	718611	1152340	30.38%	2.574%
7	7.957	838	845	856	rBV	662910	1042850	27.50%	2.330%
8	8.675	960	967	980	rBV	922790	1500803	39.57%	3.353%
9	9.134	1036	1045	1053	rBV	720202	1186667	31.29%	2.651%
10	9.863	1162	1169	1181	rBV	612062	1008666	26.59%	2.253%
11	10.404	1254	1261	1272	rBV	921223	1528965	40.31%	3.416%
12	10.787	1318	1326	1334	rBV	999427	1671648	44.08%	3.734%
13	10.928	1342	1350	1364	rBV	939794	1626542	42.89%	3.634%
14	12.381	1592	1597	1604	rVB2	16765	27156	0.72%	0.061%
15	13.604	1798	1805	1808	rBV3	2746	4815	0.13%	0.011%
16	14.039	1872	1879	1892	rBV	1623149	2172622	57.28%	4.854%
17	14.322	1920	1927	1939	rBV	1819873	2730156	71.98%	6.099%
18	14.633	1972	1980	1989	rBV	1495117	2278721	60.08%	5.091%
19	14.833	2007	2014	2038	rBV	821053	1245031	32.83%	2.781%
20	15.039	2046	2049	2056	rVB5	3434	6052	0.16%	0.014%
21	15.622	2142	2148	2160	rVB	2241675	3295993	86.90%	7.363%
22	15.745	2163	2169	2183	rBV	693379	931811	24.57%	2.082%
23	15.863	2186	2189	2198	rVB	10317	14536	0.38%	0.032%
24	17.174	2406	2412	2414	rVV2	3653	5229	0.14%	0.012%
25	17.386	2441	2448	2455	rBV	1857145	2645301	69.75%	5.910%
26	17.486	2458	2465	2478	rVV2	2471467	3559434	93.85%	7.952%
27	17.645	2487	2492	2503	rVB8	7709	17380	0.46%	0.039%
28	17.769	2509	2513	2517	rBV3	3113	4970	0.13%	0.011%
29	18.351	2610	2612	2620	rVB4	4513	7329	0.19%	0.016%
30	19.345	2777	2781	2786	rBV	29325	39735	1.05%	0.089%
31	19.416	2788	2793	2798	rBV	34595	46954	1.24%	0.105%
32	19.704	2839	2842	2845	rBV5	5709	7168	0.19%	0.016%
33	19.786	2849	2856	2866	rVV	2770324	3792704	100.00%	8.473%
34	21.486	3142	3145	3149	rBV	92047	97644	2.57%	0.218%
35	21.580	3156	3161	3168	rBV	1995321	2570122	67.76%	5.742%
36	23.892	3546	3554	3572	rVV2	1514969	3323447	87.63%	7.425%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022129.D
Acq On : 14 Oct 2022 18:46
Operator : CG/JU
Sample : PB148269BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK269

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Title : SVOA CALIBRATION

37	24.051	3574	3581	3593	rVB	1063865	2144349	56.54%	4.790%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 44763095

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022129.D
Acq On : 14 Oct 2022 18:46
Operator : CG/JU
Sample : PB148269BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK269

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

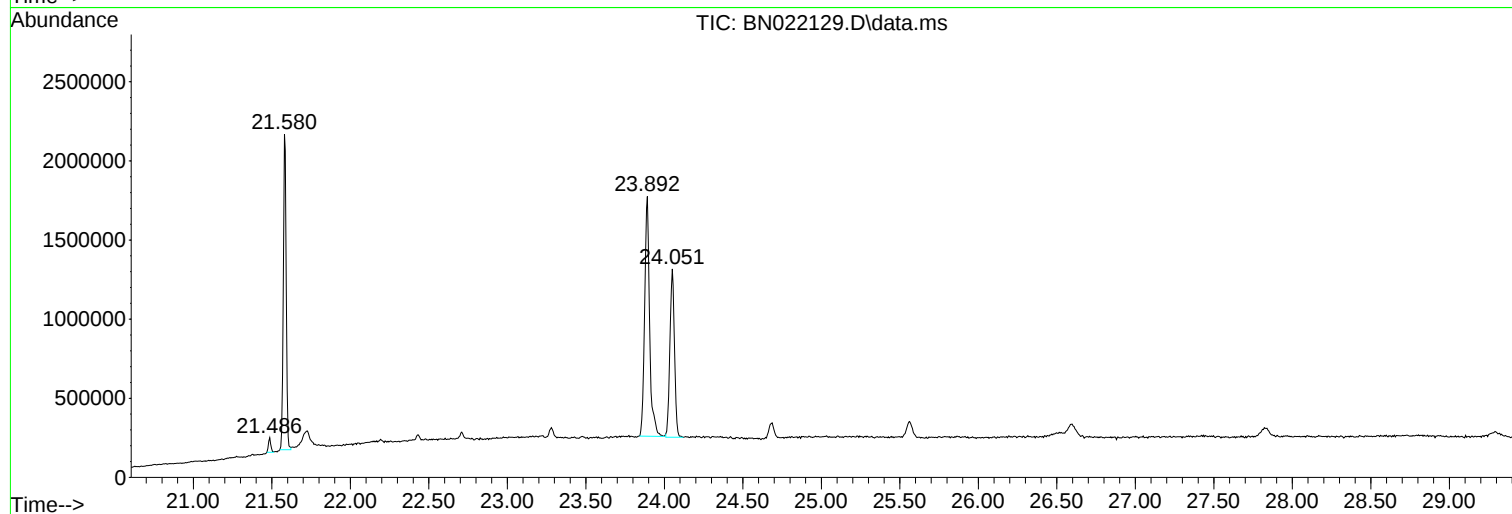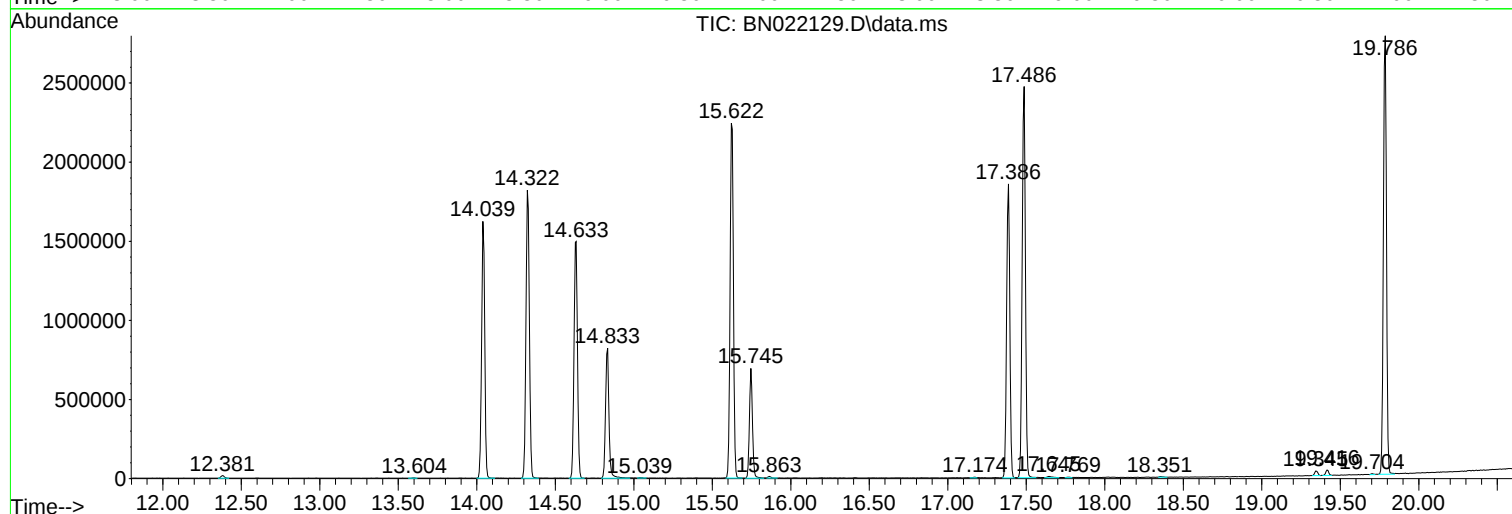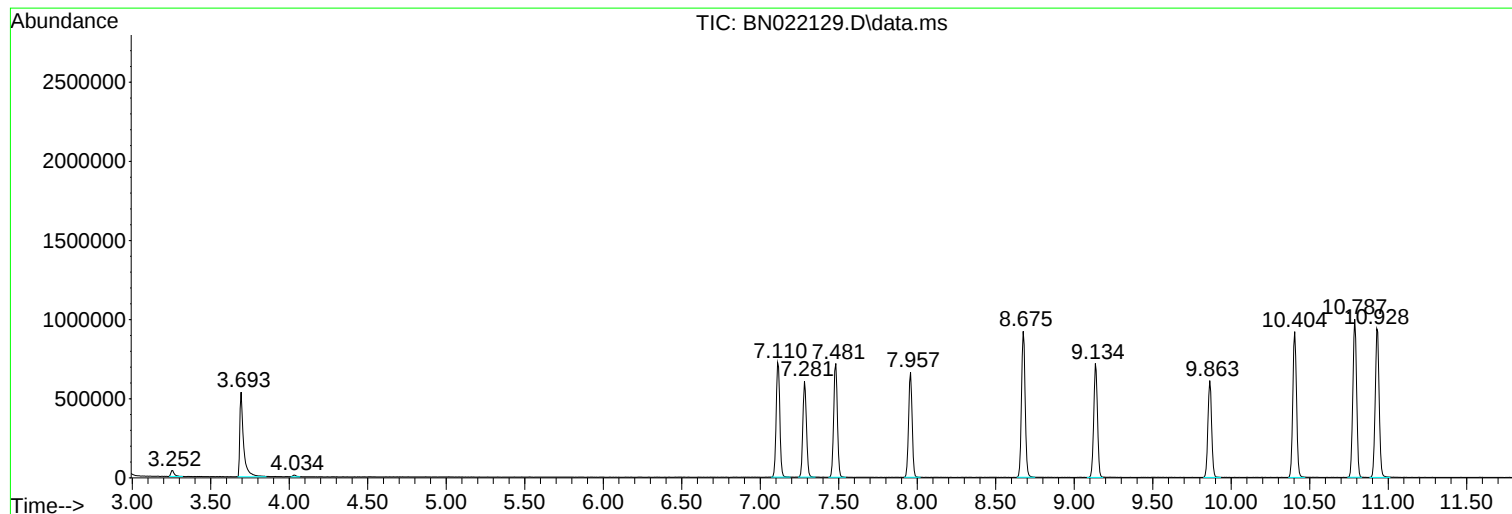

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022129.D
Acq On : 14 Oct 2022 18:46
Operator : CG/JU
Sample : PB148269BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK269

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101422\
Data File : BN022129.D
Acq On : 14 Oct 2022 18:46
Operator : CG/JU
Sample : PB148269BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK269

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------