

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
 Data File : BN034573.D
 Acq On : 14 Oct 2024 16:13
 Operator : RC/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Oct 14 17:39:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 16:58:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.358	152	5343	0.400	ng	0.00
7) Naphthalene-d8	10.116	136	15688	0.400	ng	# 0.00
13) Acenaphthene-d10	14.008	164	9488	0.400	ng	-0.01
19) Phenanthrene-d10	16.771	188	20373	0.400	ng	-0.01
29) Chrysene-d12	21.008	240	3865	0.400	ng	# 0.00
35) Perylene-d12	23.104	264	12249	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.004	112	69455	4.795	ng	0.00
5) Phenol-d6	6.564	99	87872	5.853	ng	0.00
8) Nitrobenzene-d5	8.493	82	57986	5.668	ng	-0.02
11) 2-Methylnaphthalene-d10	11.712	152	122004	5.189	ng	-0.01
14) 2,4,6-Tribromophenol	15.517	330	29679	7.058	ng	-0.01
15) 2-Fluorobiphenyl	12.618	172	157382	4.810	ng	-0.02
27) Fluoranthene-d10	18.820	212	256499	5.178	ng	0.00
31) Terphenyl-d14	19.442	244	173803	6.270	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.018	88	26990	4.188	ng	98
3) n-Nitrosodimethylamine	3.314	42	28302	4.822	ng	# 97
6) bis(2-Chloroethyl)ether	6.809	93	66318	5.401	ng	95
9) Naphthalene	10.159	128	200654	4.889	ng	99
10) Hexachlorobutadiene	10.458	225	41506	4.637	ng	# 100
12) 2-Methylnaphthalene	11.787	142	137789	5.210	ng	99
16) Acenaphthylene	13.720	152	213808	5.543	ng	100
17) Acenaphthene	14.072	154	138183	5.059	ng	99
18) Fluorene	15.077	166	181240	5.193	ng	99
20) 4,6-Dinitro-2-methylph...	16.262	198	1440	5.145	ng	# 14
21) 4-Bromophenyl-phenylether	15.977	248	57947	5.240	ng	99
22) Hexachlorobenzene	16.076	284	71798	4.810	ng	97
23) Atrazine	16.262	200	48966	5.560	ng	93
24) Pentachlorophenol	16.436	266	32007	7.495	ng	96
25) Phenanthrene	16.808	178	275276	5.121	ng	100
26) Anthracene	16.908	178	259020	5.553	ng	99
28) Fluoranthene	18.848	202	315099	5.147	ng	99
30) Pyrene	19.215	202	320399	8.448	ng	100
33) Chrysene	21.035	228	254990	7.363	ng	98
36) Indeno(1,2,3-cd)pyrene	25.151	276	238548	5.014	ng	99
37) Benzo(b)fluoranthene	22.481	252	231677	5.658	ng	# 90
38) Benzo(k)fluoranthene	22.522	252	239725	5.139	ng	# 90
39) Benzo(a)pyrene	23.010	252	189742	5.338	ng	# 84
40) Dibenzo(a,h)anthracene	25.168	278	188016	5.164	ng	93
41) Benzo(g,h,i)perylene	25.773	276	207886	4.776	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
Data File : BN034573.D
Acq On : 14 Oct 2024 16:13
Operator : RC/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Oct 14 17:39:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 16:58:38 2024
Response via : Initial Calibration









#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.358 min Scan# 61
Delta R.T. -0.007 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 5343
Ion Ratio Lower Upper
152 100
150 158.8 122.0 183.0
115 63.0 48.3 72.5



#2
1,4-Dioxane
Concen: 4.188 ng
RT: 3.018 min Scan# 19
Delta R.T. -0.007 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion: 88 Resp: 26990
Ion Ratio Lower Upper
88 100
43 28.2 22.8 34.2
58 73.0 56.4 84.6







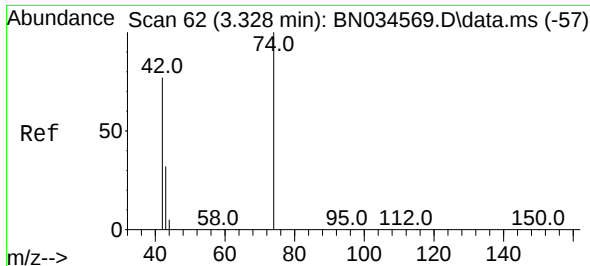

#3
 n-Nitrosodimethylamine
 Concen: 4.822 ng
 RT: 3.314 min Scan# 60
 Delta R.T. -0.015 min
 Lab File: BN034573.D
 Acq: 14 Oct 2024 16:13




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion: 42 Resp: 28302
 Ion Ratio Lower Upper
 42 100
 74 127.4 99.0 148.6
 44 6.1 6.6 9.8#

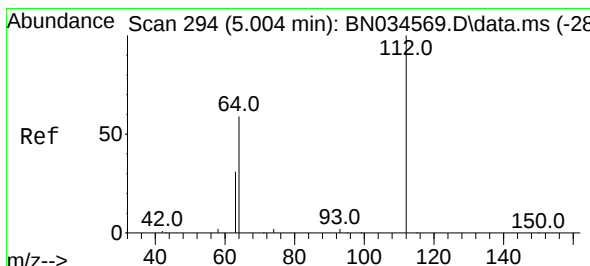

#4
 2-Fluorophenol
 Concen: 4.795 ng
 RT: 5.004 min Scan# 294
 Delta R.T. -0.000 min
 Lab File: BN034573.D
 Acq: 14 Oct 2024 16:13

Tgt Ion: 112 Resp: 69455
 Ion Ratio Lower Upper
 112 100
 64 55.3 44.6 66.8
 63 29.0 23.8 35.6









#5
Phenol-d6
Concen: 5.853 ng
RT: 6.564 min Scan# 510
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 87872
Ion Ratio Lower Upper
99 100
42 18.6 15.0 22.6
71 33.9 28.0 42.0



#6
bis(2-Chloroethyl)ether
Concen: 5.401 ng
RT: 6.809 min Scan# 544
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion: 93 Resp: 66318
Ion Ratio Lower Upper
93 100
63 75.3 64.6 96.8
95 33.2 27.9 41.9









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.116 min Scan# 921
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	15688
Ion Ratio	Lower	Upper	
136	100		
137	11.3	9.4	14.0
54	6.0	6.2	9.4#
68	4.6	4.6	6.8



#8
Nitrobenzene-d5
Concen: 5.668 ng
RT: 8.493 min Scan# 769
Delta R.T. -0.021 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:	82	Resp:	57986
Ion Ratio	Lower	Upper	
82	100		
128	37.3	38.0	57.0#
54	55.6	40.6	60.8









#9
Naphthalene
Concen: 4.889 ng
RT: 10.159 min Scan# 911
Delta R.T. -0.011 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 200654
Ion Ratio Lower Upper
128 100
129 10.9 9.3 13.9
127 13.1 10.8 16.2



#10
Hexachlorobutadiene
Concen: 4.637 ng
RT: 10.458 min Scan# 953
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:225 Resp: 41506
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.0 51.4 77.0





#11

2-Methylnaphthalene-d10

Concen: 5.189 ng

RT: 11.712 min Scan# 1106

Delta R.T. -0.011 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13

Instrument :

BNA_N

ClientSampleId :





SSTDICC5.0

Tgt Ion:152 Resp: 122004

Ion Ratio Lower Upper

152 100

151 20.6 16.7 25.1



#12

2-Methylnaphthalene

Concen: 5.210 ng

RT: 11.787 min Scan# 1126

Delta R.T. -0.011 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13




Tgt Ion:142 Resp: 137789


Ion Ratio Lower Upper

142 100

141 89.2 70.6 105.8

115 35.1 29.2 43.8





#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.008 min Scan# 14

Delta R.T. -0.011 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:164 Resp: 9488

Ion Ratio Lower Upper

164 100

162 103.8 79.7 119.5

160 48.7 37.9 56.9



#14

2,4,6-Tribromophenol

Concen: 7.058 ng

RT: 15.517 min Scan# 1615

Delta R.T. -0.012 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13




Tgt Ion:330 Resp: 29679


Ion Ratio Lower Upper

330 100

332 98.5 104.3 156.5#

141 34.0 29.4 44.0



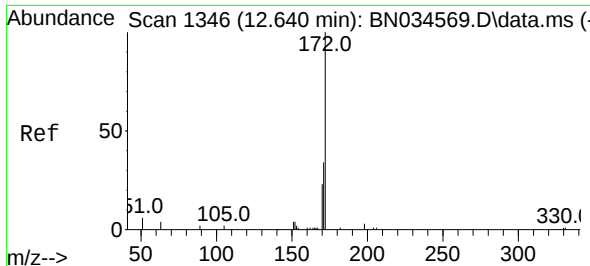

#15

2-Fluorobiphenyl

Concen: 4.810 ng

RT: 12.618 min Scan# 1444

Delta R.T. -0.021 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:172 Resp: 157382

Ion Ratio Lower Upper

172 100

171 35.6 27.1 40.7

170 23.6 18.5 27.7

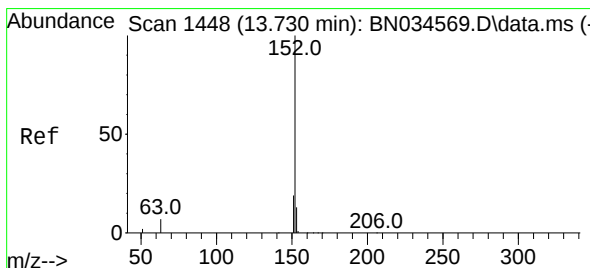

#16

Acenaphthylene

Concen: 5.543 ng

RT: 13.720 min Scan# 1447

Delta R.T. -0.011 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13




Tgt Ion:152 Resp: 213808


Ion Ratio Lower Upper

152 100

151 19.5 15.5 23.3

153 13.0 10.4 15.6









#17
Acenaphthene
Concen: 5.059 ng
RT: 14.072 min Scan# 1480
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 138183
Ion Ratio Lower Upper
154 100
153 113.8 91.5 137.3
152 55.1 45.8 68.8



#18
Fluorene
Concen: 5.193 ng
RT: 15.077 min Scan# 1574
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:166 Resp: 181240
Ion Ratio Lower Upper
166 100
165 97.4 78.6 118.0
167 13.4 10.8 16.2





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.771 min Scan# 1

Delta R.T. -0.012 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:188 Resp: 20373

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.4 6.3 9.5



#20

4,6-Dinitro-2-methylphenol

Concen: 5.145 ng

RT: 16.262 min Scan# 1675

Delta R.T. -0.013 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13




Tgt Ion:198 Resp: 1440


Ion Ratio Lower Upper

198 100

51 26.0 174.8 262.2#

105 287.5 167.9 251.9#







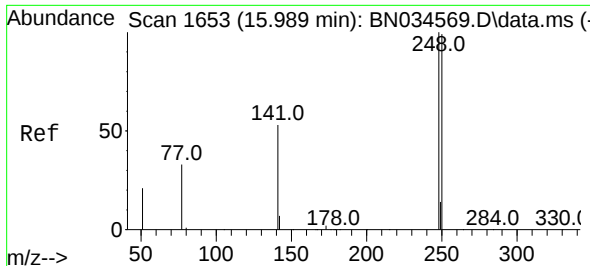

#21
4-Bromophenyl-phenylether
Concen: 5.240 ng
RT: 15.977 min Scan# 1652
Delta R.T. -0.012 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 57947
Ion Ratio Lower Upper
248 100
250 98.3 79.8 119.6
141 56.3 44.3 66.5

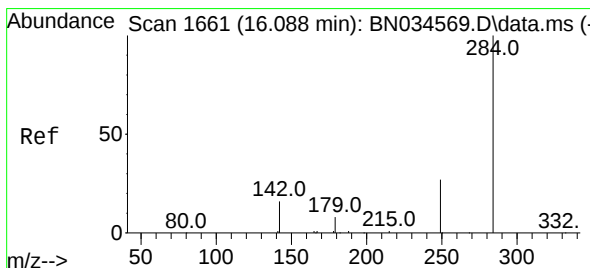

#22
Hexachlorobenzene
Concen: 4.810 ng
RT: 16.076 min Scan# 1660
Delta R.T. -0.012 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:284 Resp: 71798
Ion Ratio Lower Upper
284 100
142 33.2 28.4 42.6
249 30.4 25.0 37.4









#23
 Atrazine
 Concen: 5.560 ng
 RT: 16.262 min Scan# 1675
 Delta R.T. -0.025 min
 Lab File: BN034573.D
 Acq: 14 Oct 2024 16:13




Instrument : BNA_N
 ClientSampleId : SSTDICC5.0


Tgt Ion:	200	Resp:	48966
Ion Ratio	Lower	Upper	
200	100		
173	33.4	22.9	34.3
215	44.8	38.8	58.2



#24
 Pentachlorophenol
 Concen: 7.495 ng
 RT: 16.436 min Scan# 1689
 Delta R.T. -0.025 min
 Lab File: BN034573.D
 Acq: 14 Oct 2024 16:13

Tgt Ion:	266	Resp:	32007
Ion Ratio	Lower	Upper	
266	100		
264	62.7	46.6	69.8
268	63.6	52.0	78.0









#25
Phenanthrene
Concen: 5.121 ng
RT: 16.808 min Scan# 1719
Delta R.T. -0.012 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 275276
Ion Ratio Lower Upper
178 100
176 19.0 15.3 22.9
179 15.2 12.2 18.4



#26
Anthracene
Concen: 5.553 ng
RT: 16.908 min Scan# 1727
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:178 Resp: 259020
Ion Ratio Lower Upper
178 100
176 18.2 14.3 21.5
179 15.2 12.0 18.0





#27

Fluoranthene-d10

Concen: 5.178 ng

RT: 18.820 min Scan# 1923

Delta R.T. -0.005 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:212 Resp: 256499

Ion Ratio Lower Upper

212 100

106 14.2 11.1 16.7

104 8.0 6.5 9.7



#28

Fluoranthene

Concen: 5.147 ng

RT: 18.848 min Scan# 1929

Delta R.T. -0.005 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13




Tgt Ion:202 Resp: 315099


Ion Ratio Lower Upper

202 100

101 11.2 8.8 13.2

203 17.3 13.4 20.0









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.008 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 3865
Ion Ratio Lower Upper
240 100
120 9.8 10.1 15.1#
236 27.8 22.6 34.0



#30
Pyrene
Concen: 8.448 ng
RT: 19.215 min Scan# 2008
Delta R.T. -0.005 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:202 Resp: 320399
Ion Ratio Lower Upper
202 100
200 20.7 16.6 24.8
203 17.9 14.3 21.5





#31

Terphenyl-d14

Concen: 6.270 ng

RT: 19.442 min Scan# 2057

Delta R.T. -0.010 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:244 Resp: 173803

Ion Ratio Lower Upper

244 100

212 8.4 7.7 11.5

122 14.1 12.6 19.0



#33

Chrysene

Concen: 7.363 ng

RT: 21.035 min Scan# 2397

Delta R.T. -0.000 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13




Tgt Ion:228 Resp: 254990


Ion Ratio Lower Upper

228 100

226 29.1 24.4 36.6

229 19.8 15.8 23.6









#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.104 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BN034573.D
 Acq: 14 Oct 2024 16:13




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:264 Resp: 12249
 Ion Ratio Lower Upper
 264 100
 260 25.8 20.9 31.3
 265 68.3 61.6 92.4



#36
 Indeno(1,2,3-cd)pyrene
 Concen: 5.014 ng
 RT: 25.151 min Scan# 3489
 Delta R.T. -0.015 min
 Lab File: BN034573.D
 Acq: 14 Oct 2024 16:13


Tgt Ion:276 Resp: 238548
 Ion Ratio Lower Upper
 276 100
 138 28.0 22.0 33.0
 277 25.0 20.1 30.1








#37
Benzo(b)fluoranthene
Concen: 5.658 ng
RT: 22.481 min Scan# 2579
Delta R.T. -0.009 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0







Tgt Ion:252 Resp: 231677
Ion Ratio Lower Upper
252 100
253 22.0 21.3 31.9
125 11.3 12.7 19.1#



#38
Benzo(k)fluoranthene
Concen: 5.139 ng
RT: 22.522 min Scan# 2590
Delta R.T. -0.009 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:252 Resp: 239725
Ion Ratio Lower Upper
252 100
253 21.7 21.0 31.6
125 11.2 13.3 19.9#





#39

Benzo(a)pyrene

Concen: 5.338 ng

RT: 23.010 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN034573.D


Acq: 14 Oct 2024 16:13

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0






Tgt Ion:252 Resp: 189742

Ion Ratio Lower Upper

252 100

253 22.1 23.8 35.8#

125 12.6 17.2 25.8#



#40

Dibenzo(a,h)anthracene

Concen: 5.164 ng

RT: 25.168 min Scan# 3495

Delta R.T. -0.012 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13




Tgt Ion:278 Resp: 188016


Ion Ratio Lower Upper

278 100

139 18.6 16.0 24.0


279 23.7 23.4 35.0





#41
Benzo(g,h,i)perylene
Concen: 4.776 ng
RT: 25.773 min Scan# 31
Delta R.T. -0.015 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Tgt Ion:276 Resp: 207886
Ion Ratio Lower Upper
276 100
277 23.7 19.8 29.8
138 24.1 19.2 28.8

