

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
 Data File : BN034574.D
 Acq On : 14 Oct 2024 16:49
 Operator : RC/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN101424

Quant Time: Oct 14 17:54:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 17:52:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.365	152	4606	0.400	ng	0.00
7) Naphthalene-d8	10.116	136	14096	0.400	ng	0.00
13) Acenaphthene-d10	14.015	164	8828	0.400	ng	0.00
19) Phenanthrene-d10	16.778	188	18205	0.400	ng	# 0.00
29) Chrysene-d12	21.006	240	7980	0.400	ng	0.00
35) Perylene-d12	23.110	264	10560	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.011	112	4730	0.379	ng	0.00
5) Phenol-d6	6.571	99	4725	0.365	ng	0.00
8) Nitrobenzene-d5	8.514	82	3272	0.356	ng	0.00
11) 2-Methylnaphthalene-d10	11.727	152	8412	0.398	ng	0.00
14) 2,4,6-Tribromophenol	15.537	330	1324	0.338	ng	0.00
15) 2-Fluorobiphenyl	12.636	172	11468	0.377	ng	0.00
27) Fluoranthene-d10	18.827	212	17598	0.398	ng	0.00
31) Terphenyl-d14	19.454	244	11229	0.391	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.018	88	2275	0.410	ng	97
3) n-Nitrosodimethylamine	3.328	42	1907	0.377	ng	# 93
6) bis(2-Chloroethyl)ether	6.817	93	3440	0.325	ng	95
9) Naphthalene	10.169	128	14448	0.392	ng	100
10) Hexachlorobutadiene	10.458	225	3184	0.396	ng	# 100
12) 2-Methylnaphthalene	11.803	142	9414	0.396	ng	99
16) Acenaphthylene	13.727	152	13201	0.368	ng	100
17) Acenaphthene	14.079	154	9850	0.388	ng	100
18) Fluorene	15.074	166	12916	0.398	ng	99
20) 4,6-Dinitro-2-methylph...	16.282	198	104	0.416	ng	81
21) 4-Bromophenyl-phenylether	15.984	248	3808	0.385	ng	# 91
22) Hexachlorobenzene	16.083	284	5495	0.412	ng	98
23) Atrazine	16.282	200	3012	0.383	ng	99
24) Pentachlorophenol	16.455	266	1055	0.276	ng	96
25) Phenanthrene	16.815	178	19243	0.401	ng	100
26) Anthracene	16.915	178	16076	0.386	ng	99
28) Fluoranthene	18.855	202	21727	0.397	ng	99
30) Pyrene	19.222	202	21695	0.277	ng	100
33) Chrysene	21.042	228	20933	0.293	ng	99
36) Indeno(1,2,3-cd)pyrene	25.166	276	15385	0.375	ng	99
37) Benzo(b)fluoranthene	22.488	252	13430	0.380	ng	99
38) Benzo(k)fluoranthene	22.532	252	17060	0.424	ng	98
39) Benzo(a)pyrene	23.017	252	11938	0.390	ng	99
40) Dibenzo(a,h)anthracene	25.183	278	11570	0.369	ng	98
41) Benzo(g,h,i)perylene	25.783	276	14245	0.380	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
Data File : BN034574.D
Acq On : 14 Oct 2024 16:49
Operator : RC/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ICVBN101424


Quant Time: Oct 14 17:54:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:52:02 2024
Response via : Initial Calibration

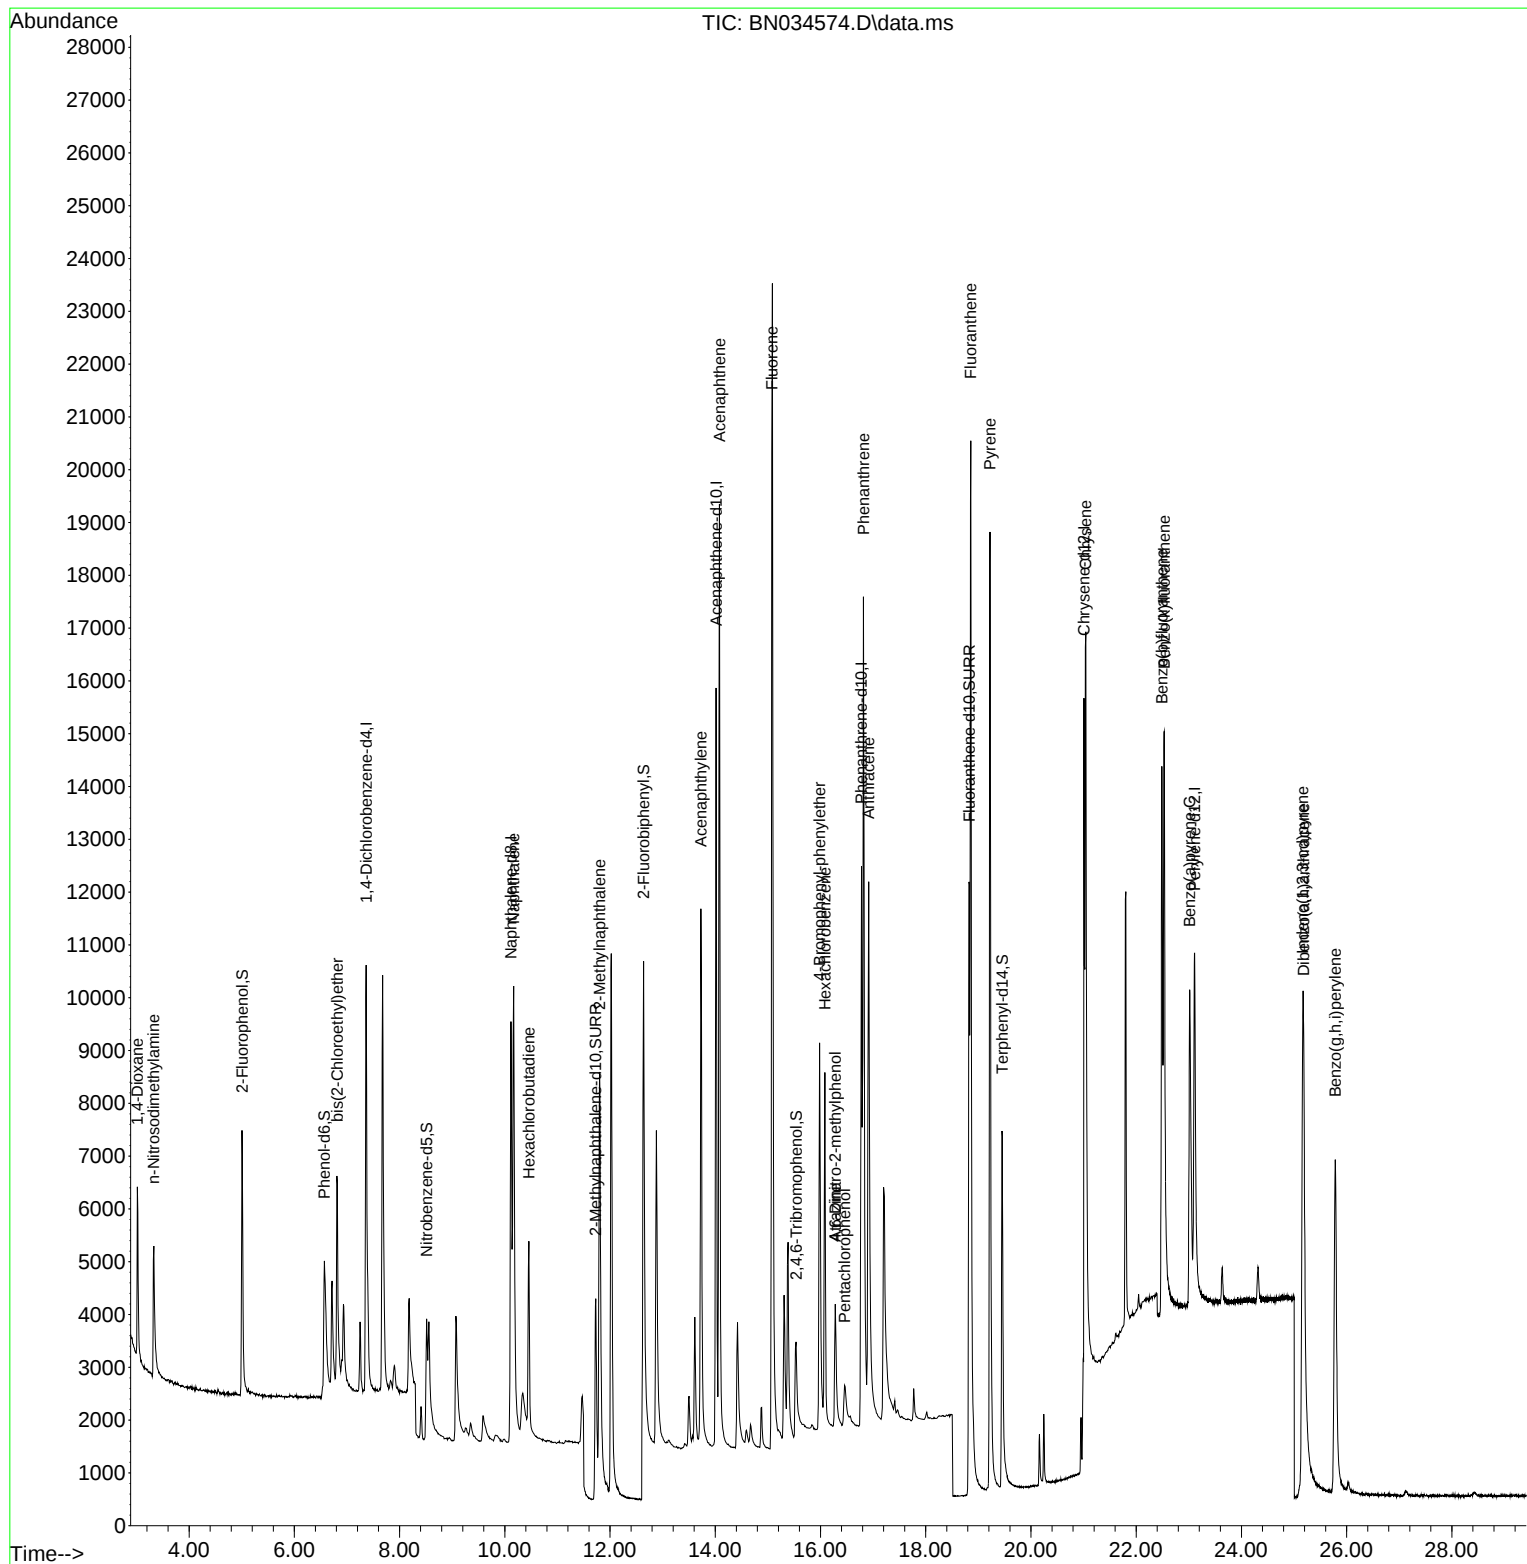






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.365 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN034574.D
 Acq: 14 Oct 2024 16:49

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN101424



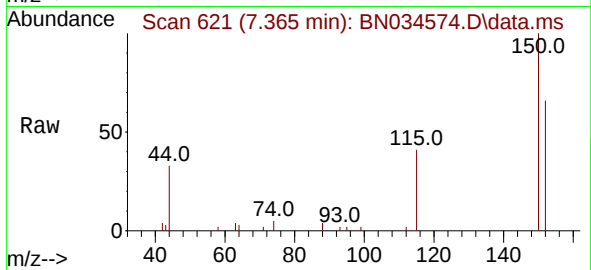



Tgt Ion:152 Resp: 4606
 Ion Ratio Lower Upper
 152 100
 150 152.3 122.0 183.0
 115 62.1 48.3 72.5

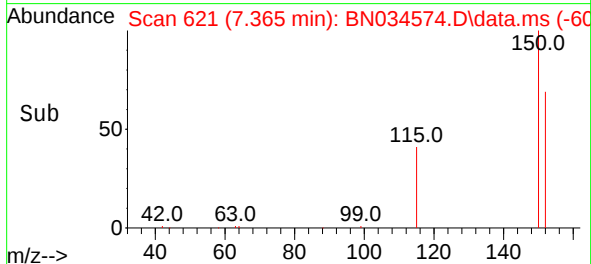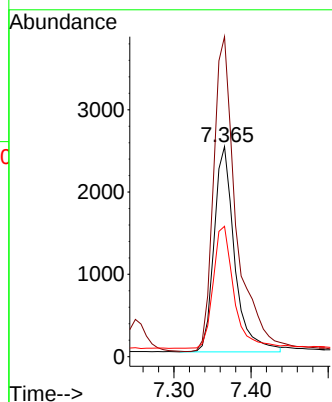

#2
 1,4-Dioxane
 Concen: 0.410 ng
 RT: 3.018 min Scan# 19
 Delta R.T. -0.007 min
 Lab File: BN034574.D
 Acq: 14 Oct 2024 16:49

Tgt Ion: 88 Resp: 2275
 Ion Ratio Lower Upper
 88 100
 43 31.0 22.8 34.2
 58 72.3 56.4 84.6


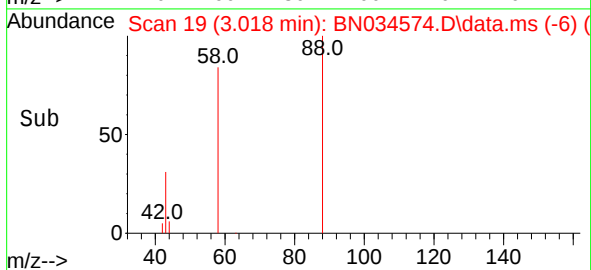

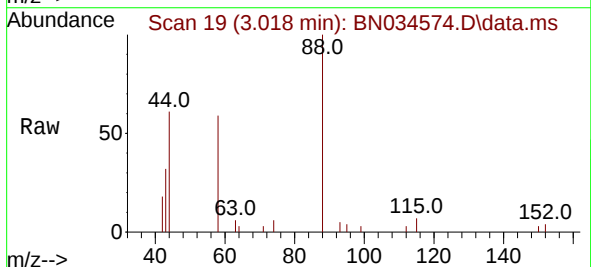


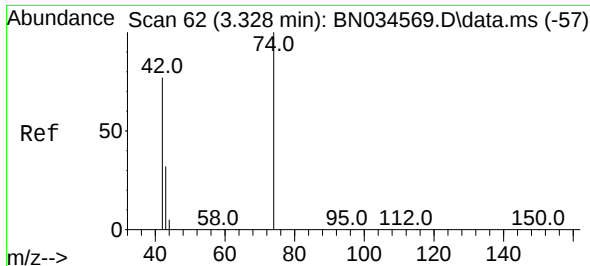

#3
n-Nitrosodimethylamine
Concen: 0.377 ng
RT: 3.328 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49




Instrument :
BNA_N
ClientSampleId :
ICVBN101424


Tgt Ion: 42 Resp: 1907
Ion Ratio Lower Upper
42 100
74 131.2 99.0 148.6
44 13.9 6.6 9.8#

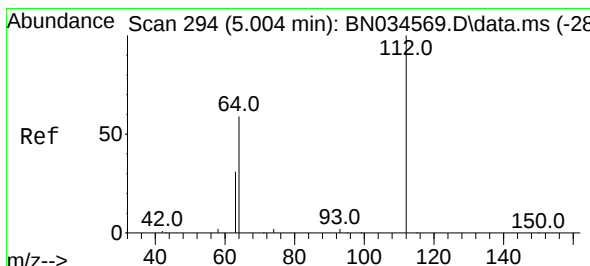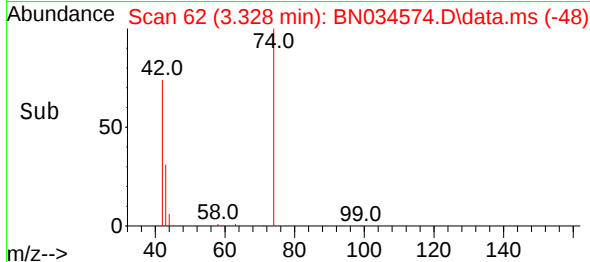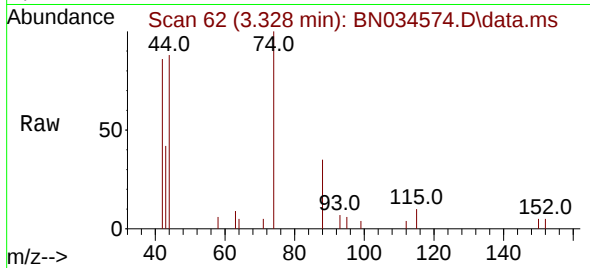

#4
2-Fluorophenol
Concen: 0.379 ng
RT: 5.011 min Scan# 295
Delta R.T. 0.007 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49

Tgt Ion: 112 Resp: 4730
Ion Ratio Lower Upper
112 100
64 56.1 44.6 66.8
63 29.2 23.8 35.6

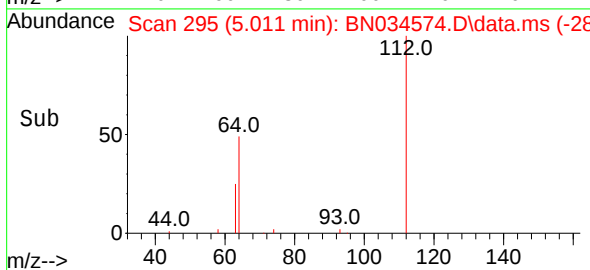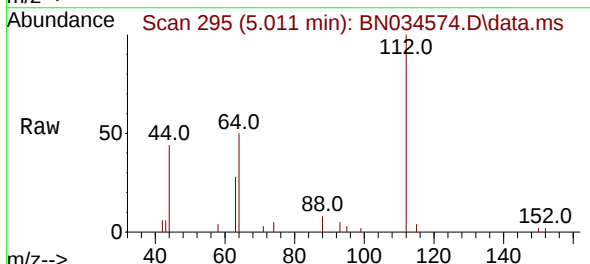



#5

Phenol-d6

Concen: 0.365 ng

RT: 6.571 min Scan# 511

Delta R.T. 0.007 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49

Instrument :

BNA_N

ClientSampleId :

ICVBN101424





Tgt Ion: 99 Resp: 4725

Ion Ratio Lower Upper

99 100

42 20.1 15.0 22.6

71 34.1 28.0 42.0

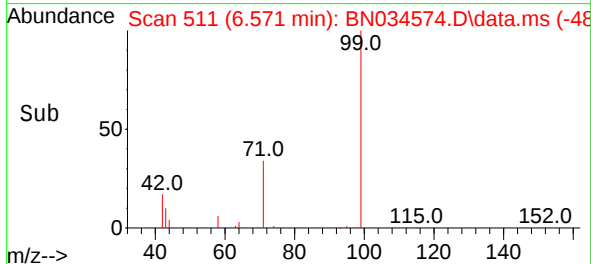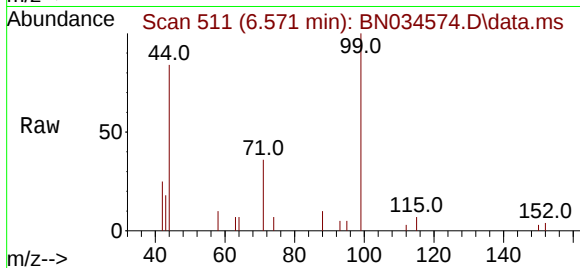

#6

bis(2-Chloroethyl)ether

Concen: 0.325 ng

RT: 6.817 min Scan# 545

Delta R.T. 0.007 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49




Tgt Ion: 93 Resp: 3440


Ion Ratio Lower Upper

93 100

63 85.1 64.6 96.8

95 38.2 27.9 41.9


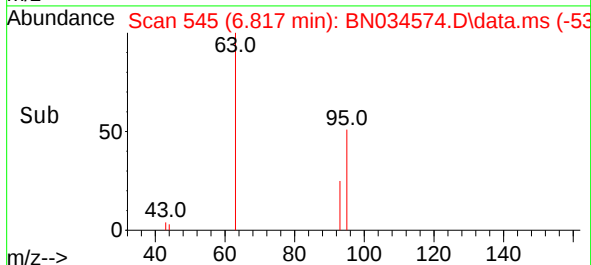
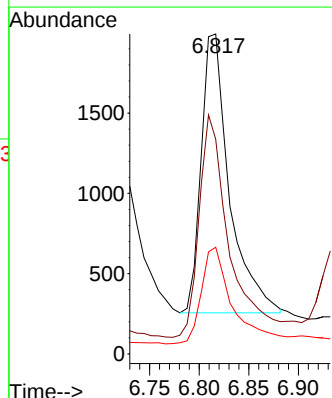
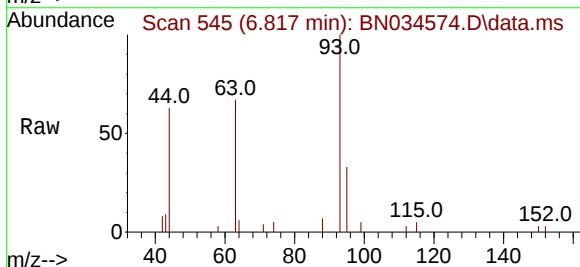




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.116 min Scan# 921
Delta R.T. 0.000 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49




Instrument :
BNA_N
ClientSampleId :
ICVBN101424


Tgt Ion:	136	Resp:	14096
Ion Ratio	Lower	Upper	
136	100		
137	11.7	9.4	14.0
54	8.2	6.2	9.4
68	6.3	4.6	6.8

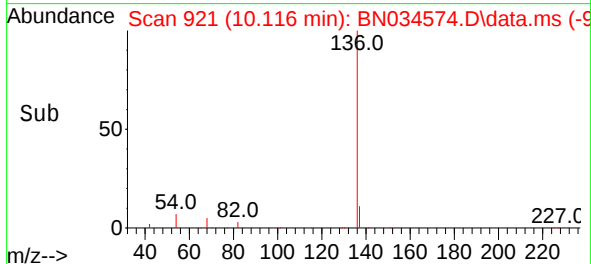

#8
Nitrobenzene-d5
Concen: 0.356 ng
RT: 8.514 min Scan# 771
Delta R.T. 0.000 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49

Tgt Ion:	82	Resp:	3272
Ion Ratio	Lower	Upper	
82	100		
128	46.0	38.0	57.0
54	53.2	40.6	60.8

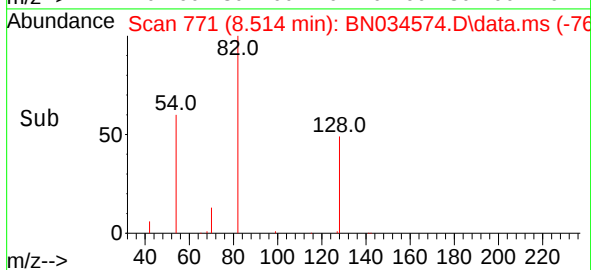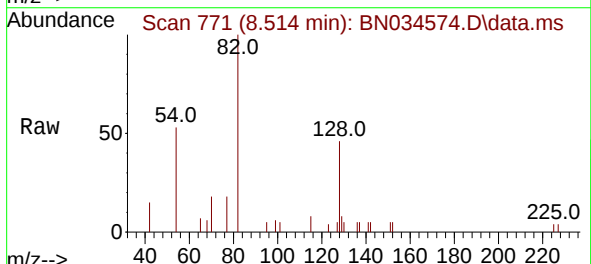



#9

Naphthalene

Concen: 0.392 ng

RT: 10.169 min Scan# 91

Delta R.T. 0.000 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49

Instrument :

BNA_N

ClientSampleId :

ICVBN101424





Tgt Ion:128 Resp: 14448

Ion Ratio Lower Upper

128 100

129 11.7 9.3 13.9

127 13.5 10.8 16.2

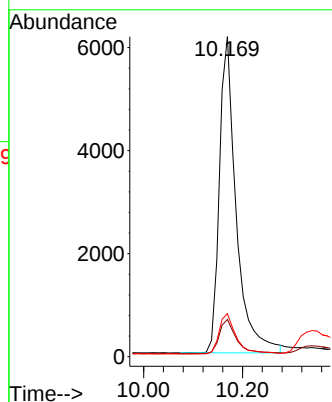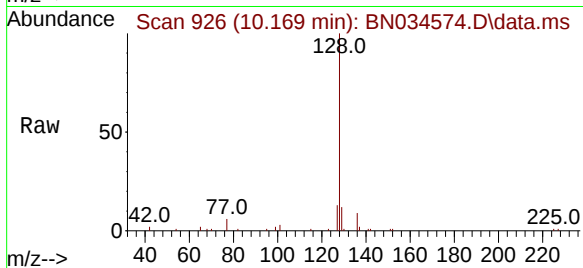

#10

Hexachlorobutadiene

Concen: 0.396 ng

RT: 10.458 min Scan# 953

Delta R.T. 0.000 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49




Tgt Ion:225 Resp: 3184


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 64.3 51.4 77.0


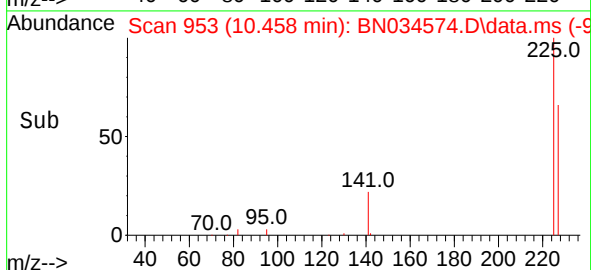

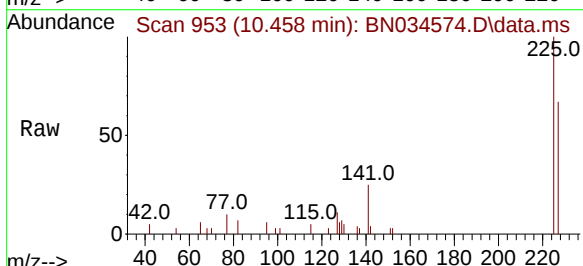


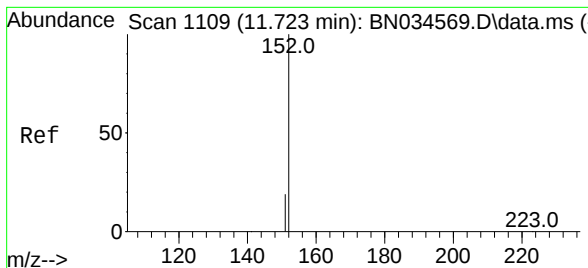

#11
2-Methylnaphthalene-d10
Concen: 0.398 ng
RT: 11.727 min Scan# 1110
Delta R.T. 0.004 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49




Instrument :
BNA_N
ClientSampleId :
ICVBN101424


Tgt Ion:152 Resp: 8412
Ion Ratio Lower Upper
152 100
151 20.7 16.7 25.1

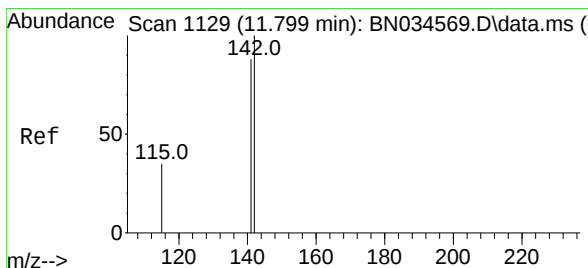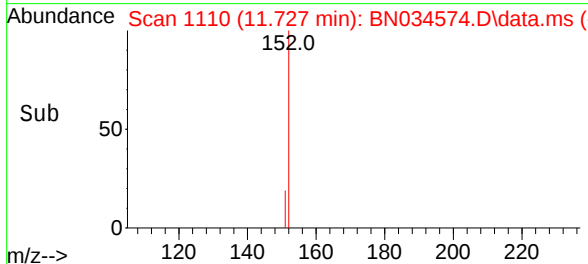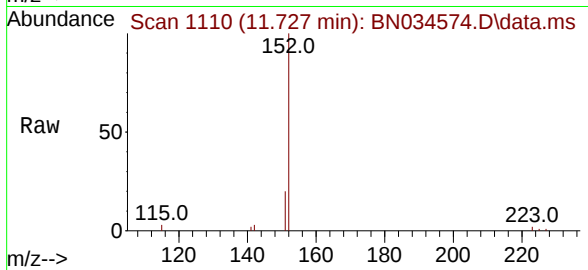

#12
2-Methylnaphthalene
Concen: 0.396 ng
RT: 11.803 min Scan# 1130
Delta R.T. 0.004 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49

Tgt Ion:142 Resp: 9414
Ion Ratio Lower Upper
142 100
141 89.0 70.6 105.8
115 35.7 29.2 43.8

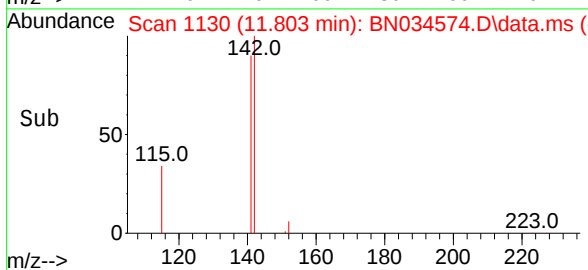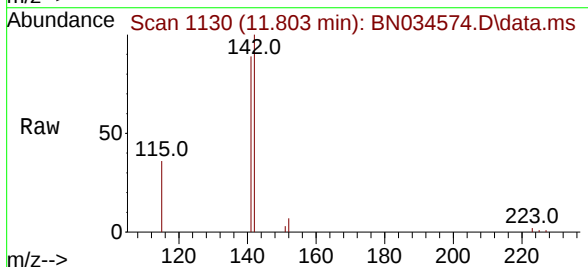



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.015 min Scan# 1475

Delta R.T. -0.004 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49

Instrument :

BNA_N

ClientSampleId :

ICVBN101424





Tgt Ion:164 Resp: 8828

Ion Ratio Lower Upper

164 100

162 100.9 79.7 119.5

160 48.5 37.9 56.9

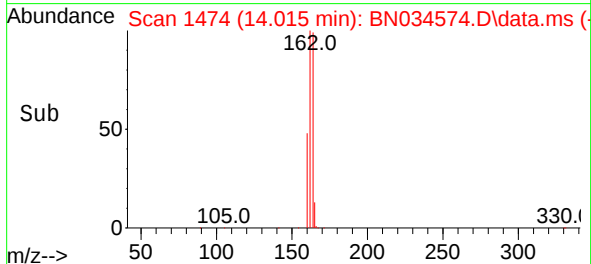

#14

2,4,6-Tribromophenol

Concen: 0.338 ng

RT: 15.537 min Scan# 1616

Delta R.T. 0.007 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49




Tgt Ion:330 Resp: 1324


Ion Ratio Lower Upper

330 100

332 122.0 104.3 156.5

141 32.3 29.4 44.0

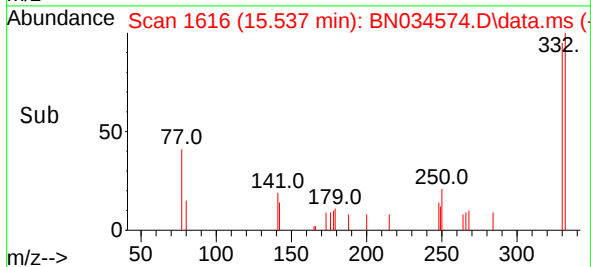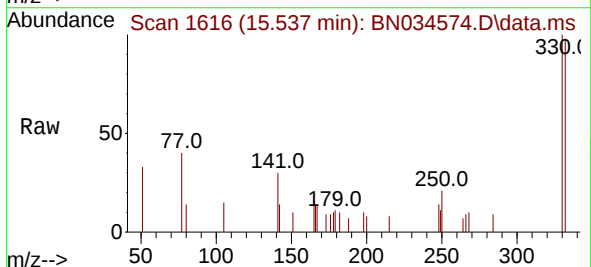

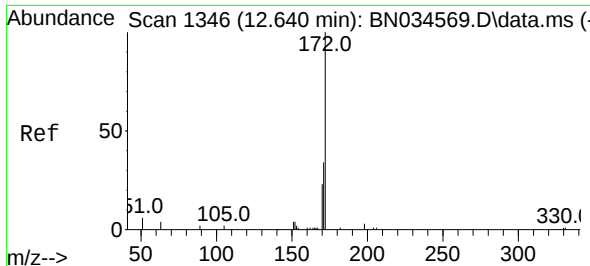

#15

2-Fluorobiphenyl

Concen: 0.377 ng

RT: 12.636 min Scan# 1446

Delta R.T. -0.004 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49

Instrument :

BNA_N

ClientSampleId :

ICVBN101424





Tgt Ion:172 Resp: 11468

Ion Ratio Lower Upper

172 100

171 35.0 27.1 40.7

170 23.5 18.5 27.7

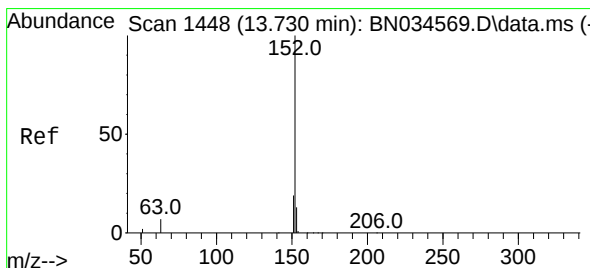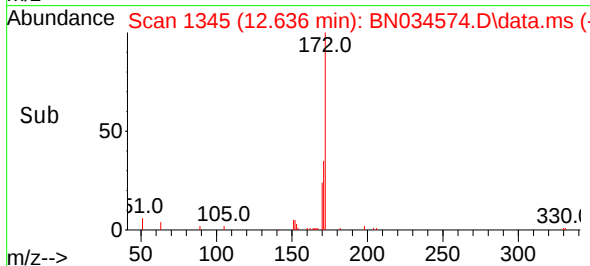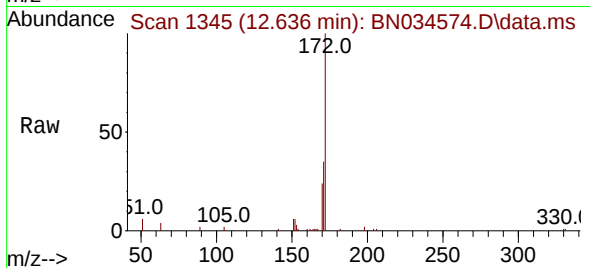

#16

Acenaphthylene

Concen: 0.368 ng

RT: 13.727 min Scan# 1447

Delta R.T. -0.004 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49




Tgt Ion:152 Resp: 13201


Ion Ratio Lower Upper

152 100

151 19.4 15.5 23.3

153 12.9 10.4 15.6


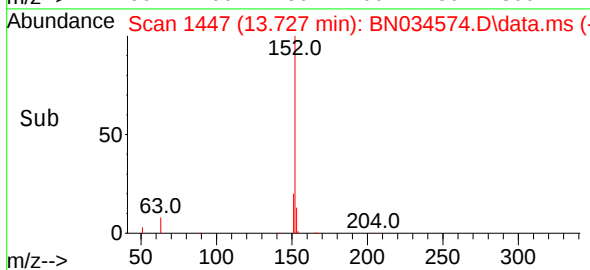

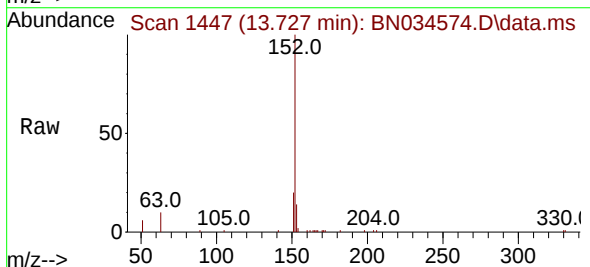




#17
Acenaphthene
Concen: 0.388 ng
RT: 14.079 min Scan# 1480
Delta R.T. 0.007 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49




Instrument :
BNA_N
ClientSampleId :
ICVBN101424


Tgt Ion:154 Resp: 9850
Ion Ratio Lower Upper
154 100
153 114.7 91.5 137.3
152 57.5 45.8 68.8

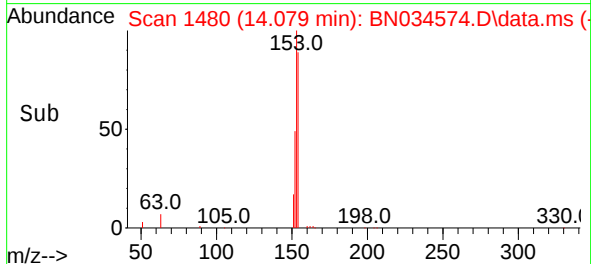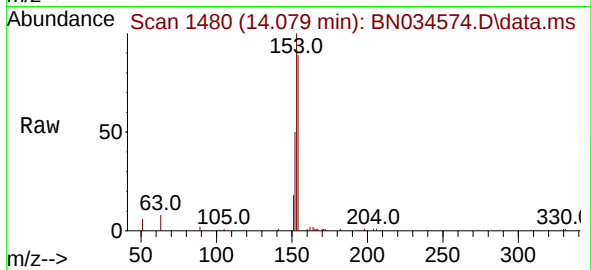

#18
Fluorene
Concen: 0.398 ng
RT: 15.074 min Scan# 1573
Delta R.T. -0.004 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49

Tgt Ion:166 Resp: 12916
Ion Ratio Lower Upper
166 100
165 99.1 78.6 118.0
167 13.4 10.8 16.2

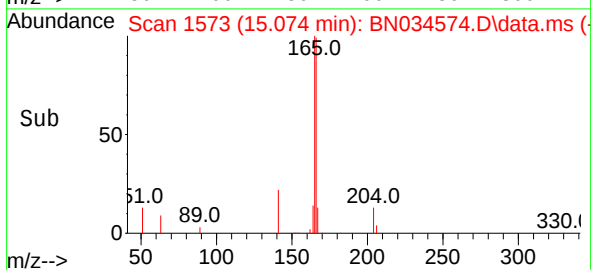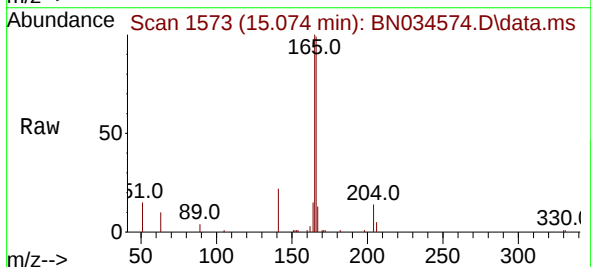

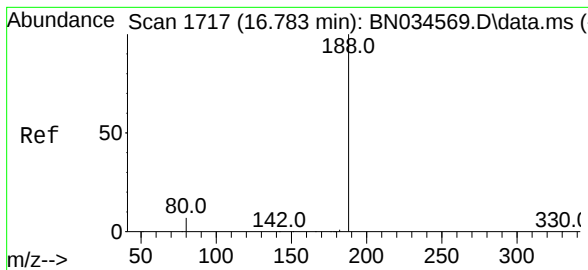

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.778 min Scan# 1717

Delta R.T. -0.005 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49

Instrument :

BNA_N

ClientSampleId :

ICVBN101424





Tgt Ion:188 Resp: 18205

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.7 6.3 9.5#

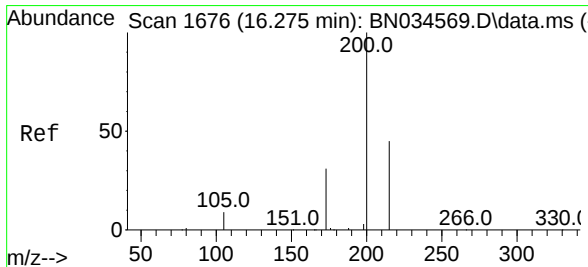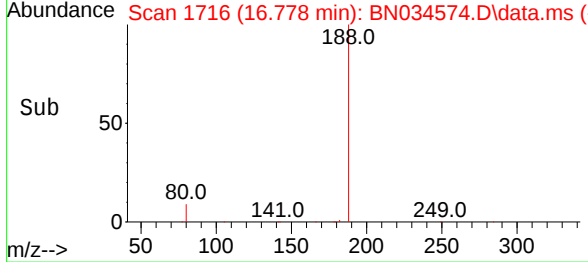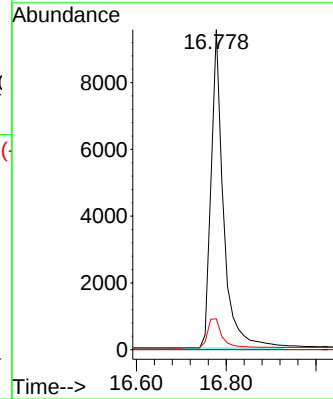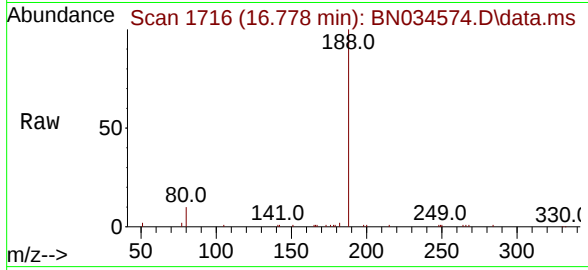

#20

4,6-Dinitro-2-methylphenol

Concen: 0.416 ng

RT: 16.282 min Scan# 1676

Delta R.T. 0.007 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49




Tgt Ion:198 Resp: 104


Ion Ratio Lower Upper

198 100

51 182.4 174.8 262.2

105 186.8 167.9 251.9


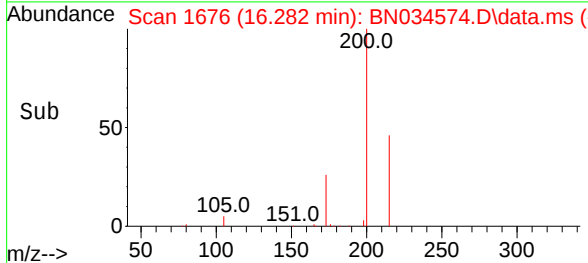
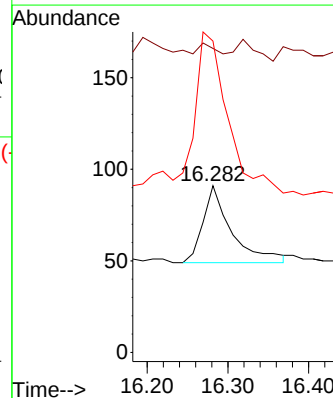
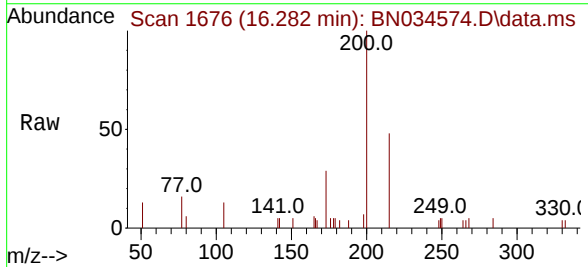


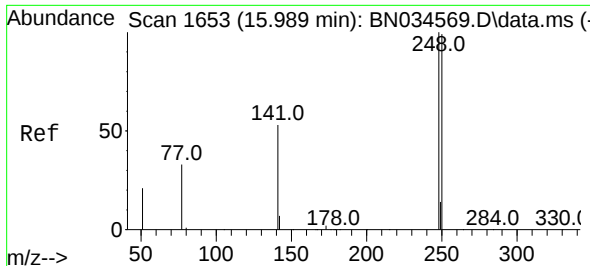

#21
4-Bromophenyl-phenylether
Concen: 0.385 ng
RT: 15.984 min Scan# 1652
Delta R.T. -0.005 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49




Instrument :
BNA_N
ClientSampleId :
ICVBN101424


Tgt Ion:248 Resp: 3808
Ion Ratio Lower Upper
248 100
250 96.9 79.8 119.6
141 70.7 44.3 66.5#

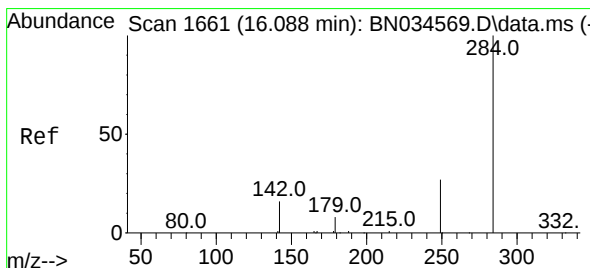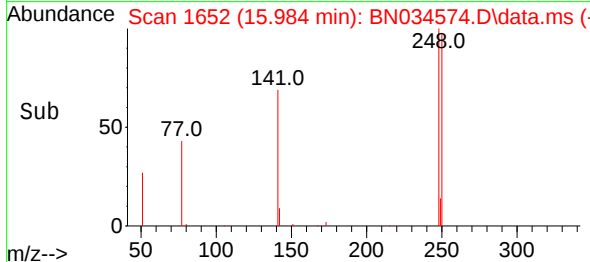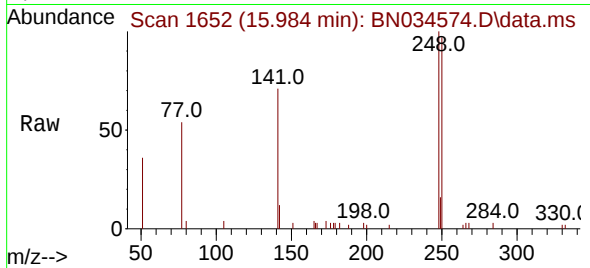

#22
Hexachlorobenzene
Concen: 0.412 ng
RT: 16.083 min Scan# 1660
Delta R.T. -0.005 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49

Tgt Ion:284 Resp: 5495
Ion Ratio Lower Upper
284 100
142 33.3 28.4 42.6
249 30.6 25.0 37.4


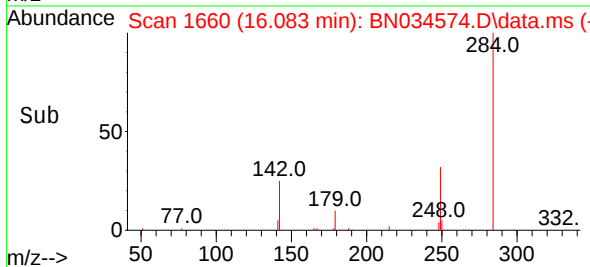

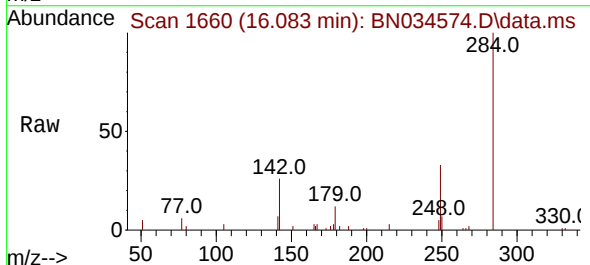


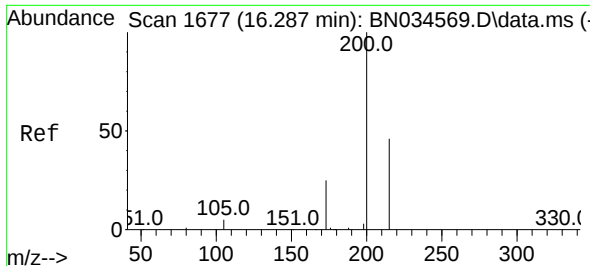

#23
Atrazine
Concen: 0.383 ng
RT: 16.282 min Scan# 1677
Delta R.T. -0.005 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49




Instrument :
BNA_N
ClientSampleId :
ICVBN101424


Tgt Ion:200 Resp: 3012
Ion Ratio Lower Upper
200 100
173 28.9 22.9 34.3
215 47.8 38.8 58.2

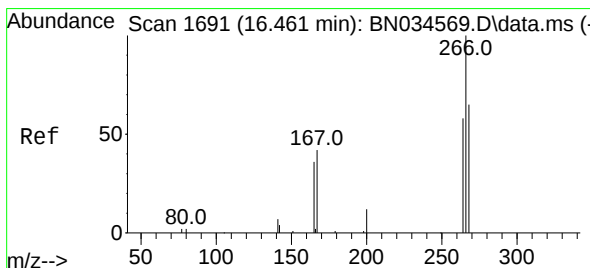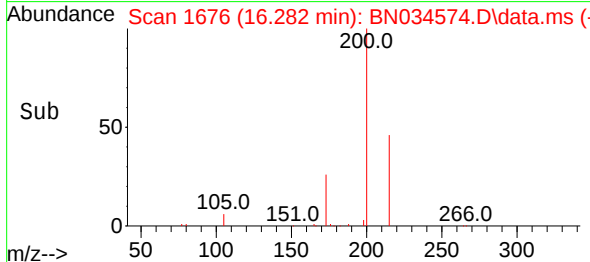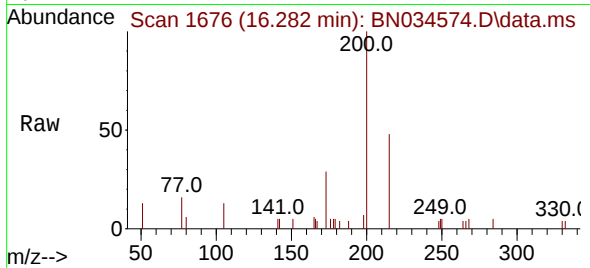

#24
Pentachlorophenol
Concen: 0.276 ng
RT: 16.455 min Scan# 1690
Delta R.T. -0.006 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49

Tgt Ion:266 Resp: 1055
Ion Ratio Lower Upper
266 100
264 63.3 46.6 69.8
268 65.8 52.0 78.0

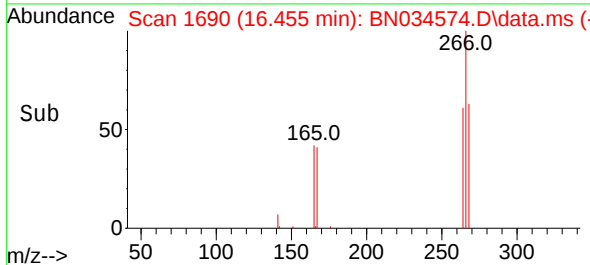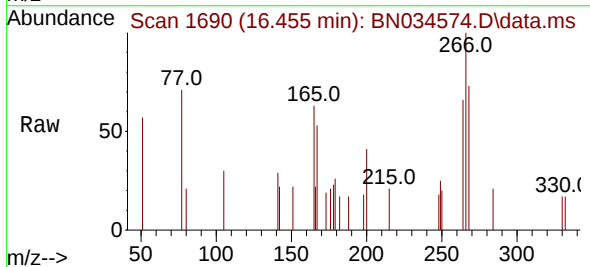

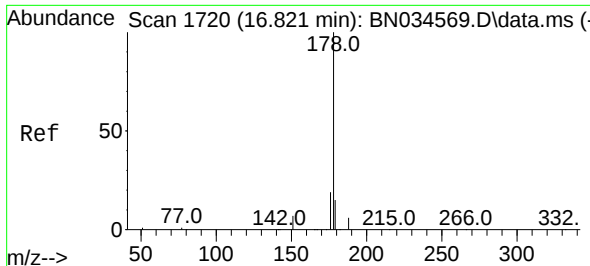

#25

Phenanthrene

Concen: 0.401 ng

RT: 16.815 min Scan# 1719

Delta R.T. -0.005 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49

Instrument :

BNA_N

ClientSampleId :

ICVBN101424





Tgt Ion:178 Resp: 19243

Ion Ratio Lower Upper

178 100

176 19.0 15.3 22.9

179 15.4 12.2 18.4

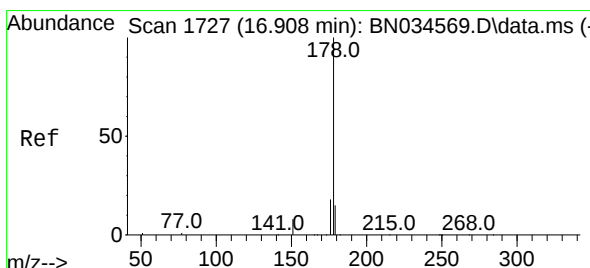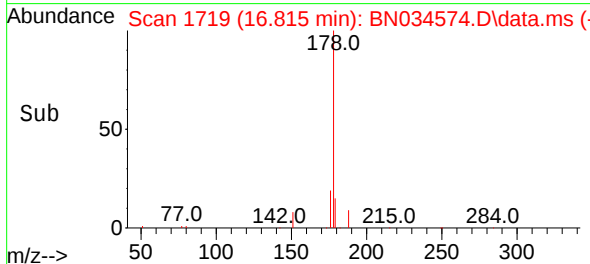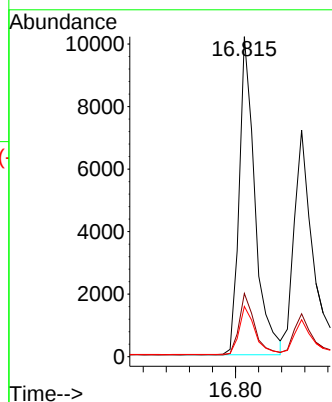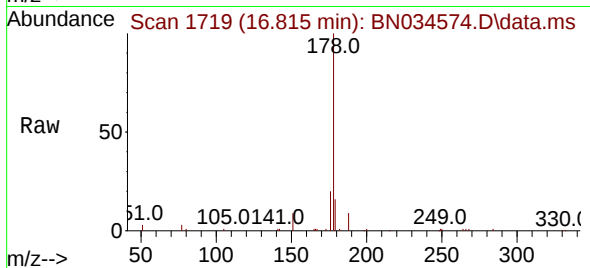

#26

Anthracene

Concen: 0.386 ng

RT: 16.915 min Scan# 1727

Delta R.T. 0.007 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49




Tgt Ion:178 Resp: 16076


Ion Ratio Lower Upper

178 100

176 18.4 14.3 21.5

179 15.1 12.0 18.0


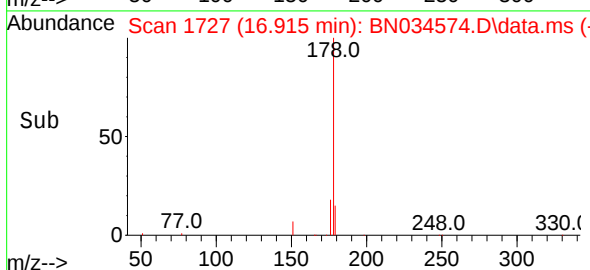
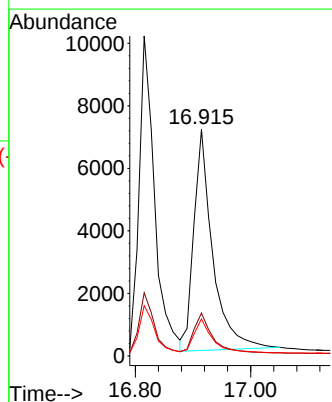
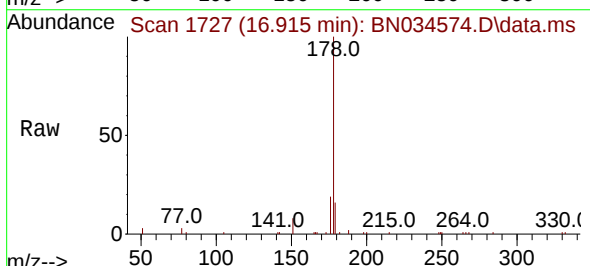


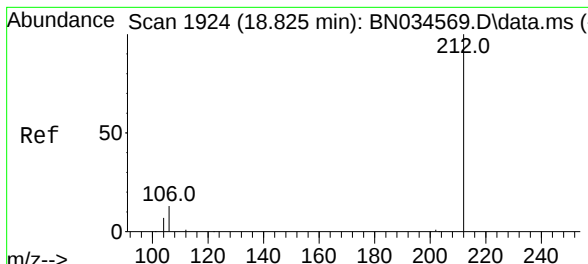

#27
Fluoranthene-d10
Concen: 0.398 ng
RT: 18.827 min Scan# 1924
Delta R.T. 0.002 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49




Instrument :
BNA_N
ClientSampleId :
ICVBN101424


Tgt Ion:212 Resp: 17598
Ion Ratio Lower Upper
212 100
106 14.2 11.1 16.7
104 8.0 6.5 9.7

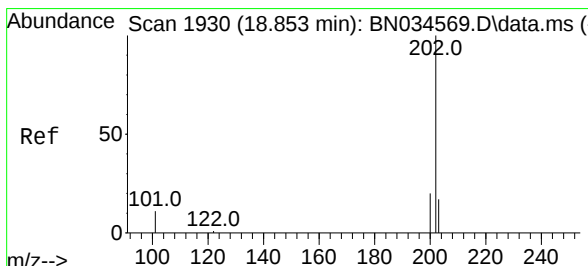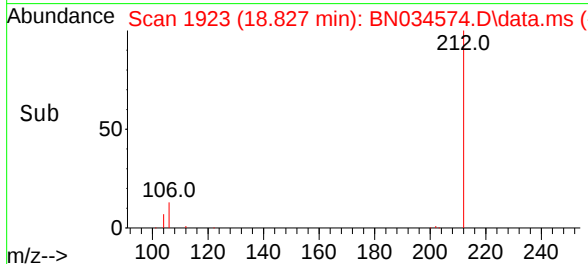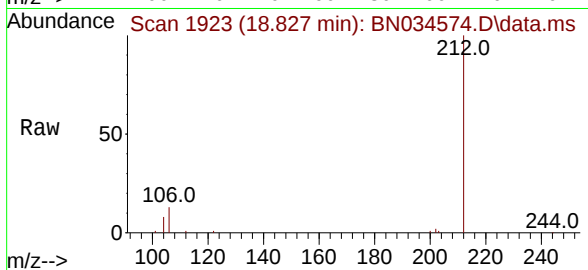

#28
Fluoranthene
Concen: 0.397 ng
RT: 18.855 min Scan# 1929
Delta R.T. 0.002 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49

Tgt Ion:202 Resp: 21727
Ion Ratio Lower Upper
202 100
101 10.9 8.8 13.2
203 17.1 13.4 20.0

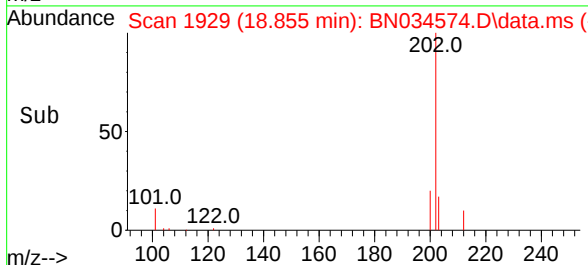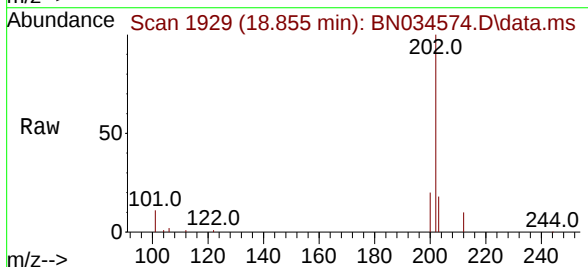

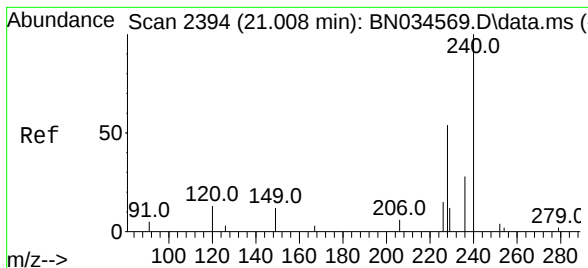

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.006 min Scan# 24

Delta R.T. -0.002 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49

Instrument :

BNA_N

ClientSampleId :

ICVBN101424





Tgt Ion:240 Resp: 7980

Ion Ratio Lower Upper

240 100

120 12.6 10.1 15.1

236 27.9 22.6 34.0

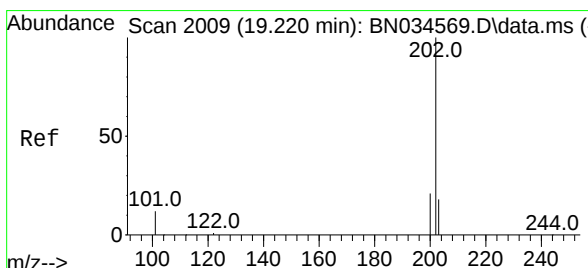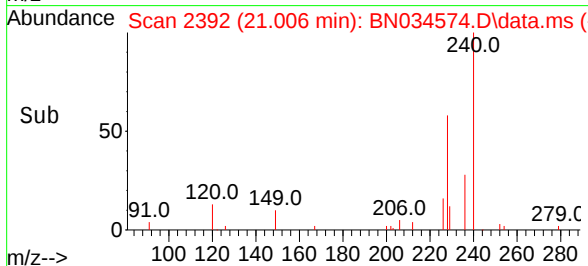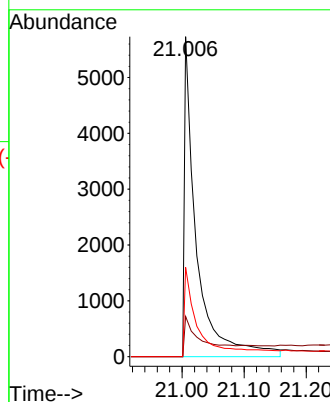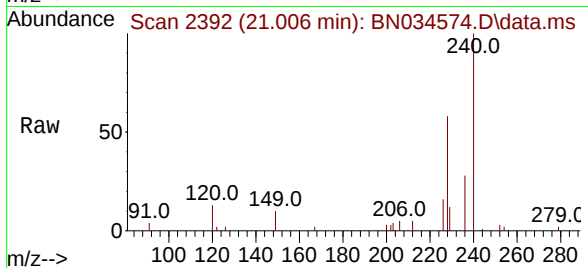

#30

Pyrene

Concen: 0.277 ng

RT: 19.222 min Scan# 2008

Delta R.T. 0.002 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49




Tgt Ion:202 Resp: 21695


Ion Ratio Lower Upper

202 100

200 20.9 16.6 24.8

203 17.9 14.3 21.5


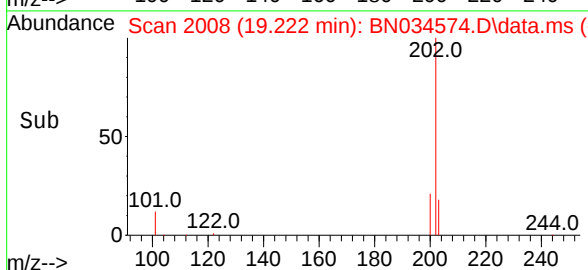

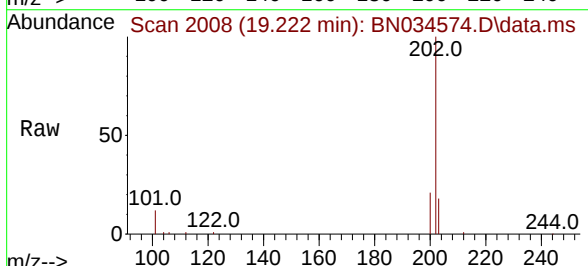




#31
 Terphenyl-d14
 Concen: 0.391 ng
 RT: 19.454 min Scan# 2059
 Delta R.T. 0.002 min
 Lab File: BN034574.D
 Acq: 14 Oct 2024 16:49




Instrument :
 BNA_N
 ClientSampleId :
 ICVBN101424


Tgt Ion:244 Resp: 11229
 Ion Ratio Lower Upper
 244 100
 212 9.0 7.7 11.5
 122 15.2 12.6 19.0

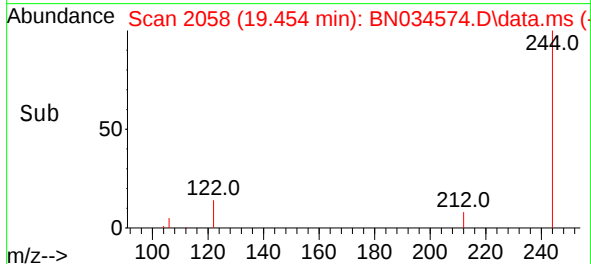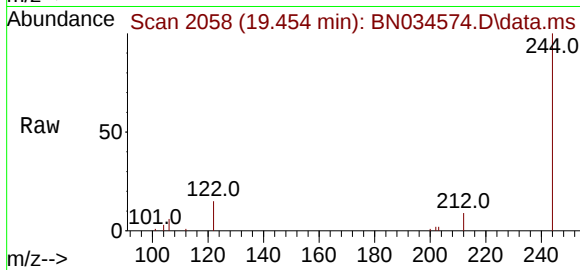

#33
 Chrysene
 Concen: 0.293 ng
 RT: 21.042 min Scan# 2396
 Delta R.T. 0.007 min
 Lab File: BN034574.D
 Acq: 14 Oct 2024 16:49


Tgt Ion:228 Resp: 20933
 Ion Ratio Lower Upper
 228 100
 226 29.5 24.4 36.6
 229 20.0 15.8 23.6

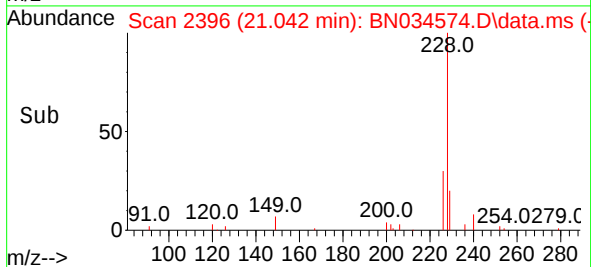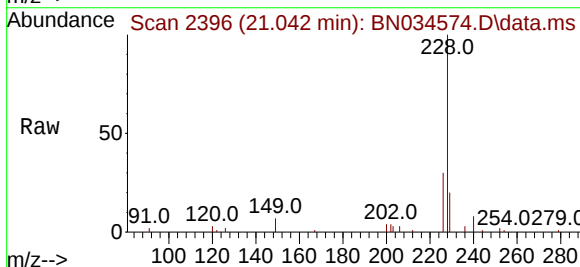






#35
Perylene-d12
Concen: 0.400 ng
RT: 23.110 min Scan# 21
Delta R.T. 0.001 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49

Instrument :
BNA_N
ClientSampleId :
ICVBN101424







Tgt Ion:264 Resp: 10560
Ion Ratio Lower Upper
264 100
260 25.7 20.9 31.3
265 79.8 61.6 92.4

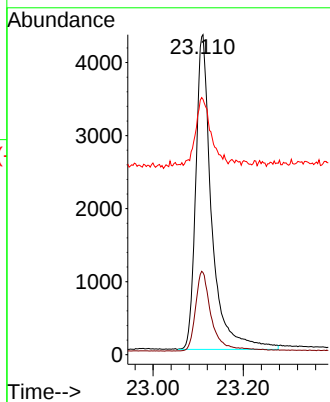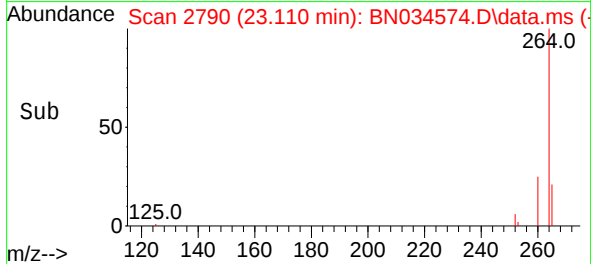

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.375 ng
RT: 25.166 min Scan# 3493
Delta R.T. 0.001 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49

Tgt Ion:276 Resp: 15385
Ion Ratio Lower Upper
276 100
138 27.9 22.0 33.0
277 25.3 20.1 30.1

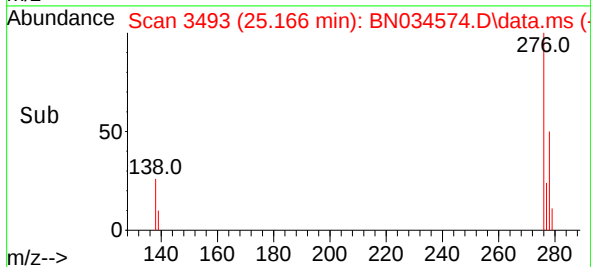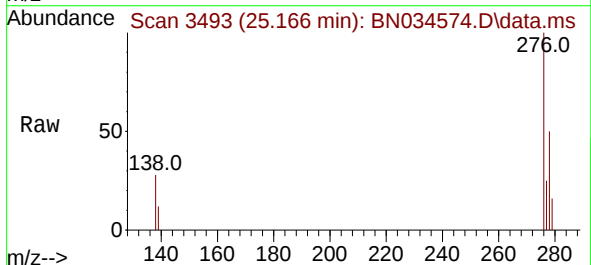



#37

Benzo(b)fluoranthene

Concen: 0.380 ng

RT: 22.488 min Scan# 2577

Delta R.T. -0.002 min

Lab File: BN034574.D


Acq: 14 Oct 2024 16:49

Instrument :

BN034574.D

ClientSampleId :

ICVBN101424

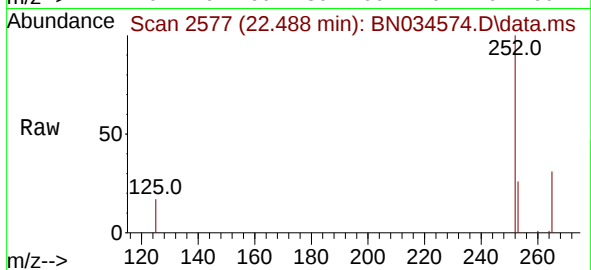




Tgt Ion:252 Resp: 13430

Ion Ratio Lower Upper

252 100

253 26.2 21.3 31.9

125 16.7 12.7 19.1

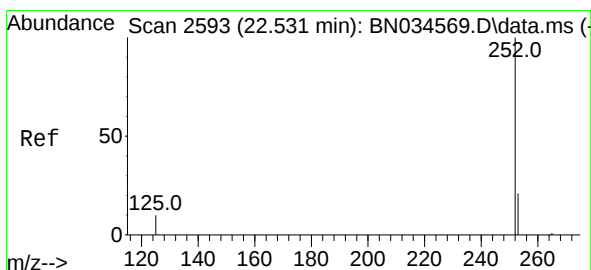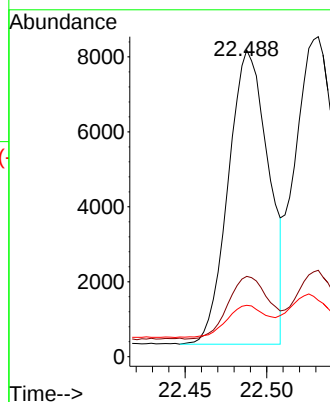

#38

Benzo(k)fluoranthene

Concen: 0.424 ng

RT: 22.532 min Scan# 2592

Delta R.T. 0.001 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49




Tgt Ion:252 Resp: 17060


Ion Ratio Lower Upper

252 100

253 27.0 21.0 31.6

125 17.6 13.3 19.9

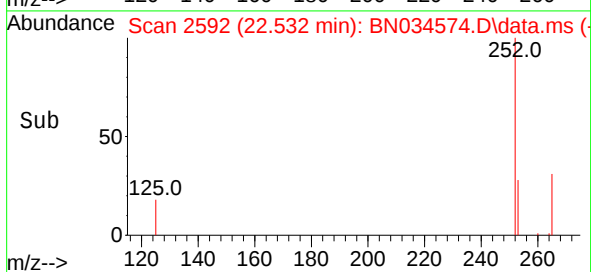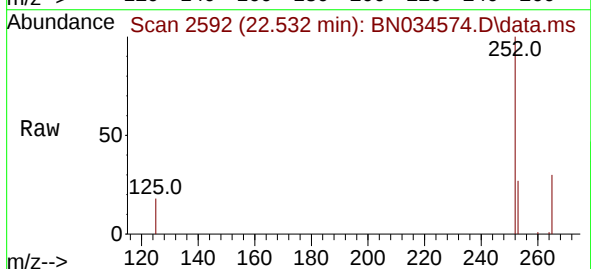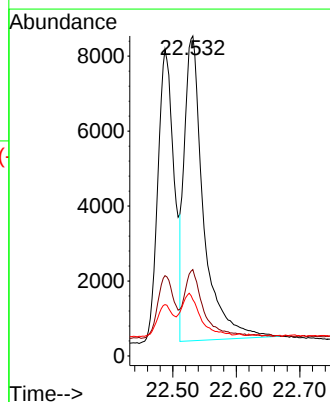



#39

Benzo(a)pyrene

Concen: 0.390 ng

RT: 23.017 min Scan# 21

Delta R.T. -0.002 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49

Instrument :

BNA_N

ClientSampleId :

ICVBN101424





Tgt Ion:252 Resp: 11938

Ion Ratio Lower Upper

252 100

253 30.2 23.8 35.8

125 22.5 17.2 25.8



#40

Dibenzo(a,h)anthracene

Concen: 0.369 ng

RT: 25.183 min Scan# 3499

Delta R.T. 0.004 min

Lab File: BN034574.D

Acq: 14 Oct 2024 16:49




Tgt Ion:278 Resp: 11570


Ion Ratio Lower Upper

278 100

139 20.9 16.0 24.0


279 30.0 23.4 35.0

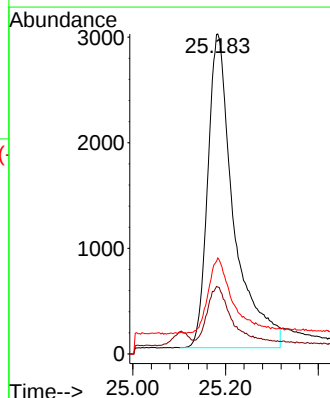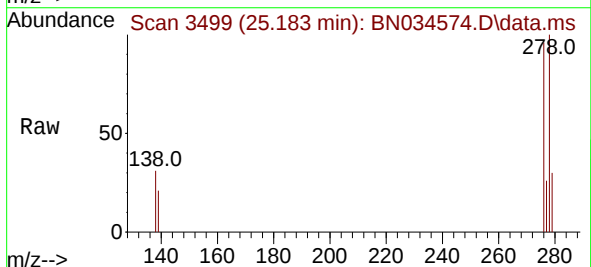

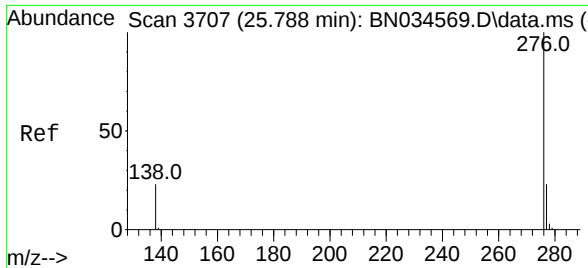

#41
Benzo(g,h,i)perylene
Concen: 0.380 ng
RT: 25.783 min Scan# 31
Delta R.T. -0.005 min
Lab File: BN034574.D
Acq: 14 Oct 2024 16:49

Instrument :
BNA_N
ClientSampleId :
ICVBN101424

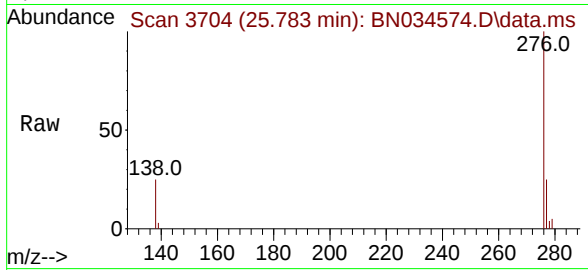

Tgt Ion:	276	Resp:	14245
Ion	Ratio	Lower	Upper
276	100		
277	24.8	19.8	29.8
138	25.0	19.2	28.8

