

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
 Data File : BN034586.D
 Acq On : 15 Oct 2024 00:07
 Operator : RC/JU
 Sample : P4282-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RW7-SP302-20241002

Quant Time: Oct 15 00:34:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 17:52:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.365	152	3755	0.400	ng	0.00
7) Naphthalene-d8	10.137	136	10712	0.400	ng	0.02
13) Acenaphthene-d10	14.019	164	6300	0.400	ng	0.00
19) Phenanthrene-d10	16.783	188	10749	0.400	ng	# 0.00
29) Chrysene-d12	21.008	240	5448	0.400	ng	0.00
35) Perylene-d12	23.104	264	8672	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.011	112	1082	0.106	ng	0.00
5) Phenol-d6	6.636	99	364	0.035	ng	0.07
8) Nitrobenzene-d5	8.536	82	2096	0.300	ng	0.02
11) 2-Methylnaphthalene-d10	11.742	152	5871	0.366	ng	0.02
14) 2,4,6-Tribromophenol	15.555	330	166	0.059	ng	0.02
15) 2-Fluorobiphenyl	12.640	172	7935	0.365	ng	0.00
27) Fluoranthene-d10	18.825	212	11949	0.457	ng	0.00
31) Terphenyl-d14	19.443	244	9330	0.432	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.018	88	477	0.105	ng	# 59
20) 4,6-Dinitro-2-methylph...	16.250	198	4	0.027	ng	# 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
Data File : BN034586.D
Acq On : 15 Oct 2024 00:07
Operator : RC/JU
Sample : P4282-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RW7-SP302-20241002


Quant Time: Oct 15 00:34:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:52:02 2024
Response via : Initial Calibration

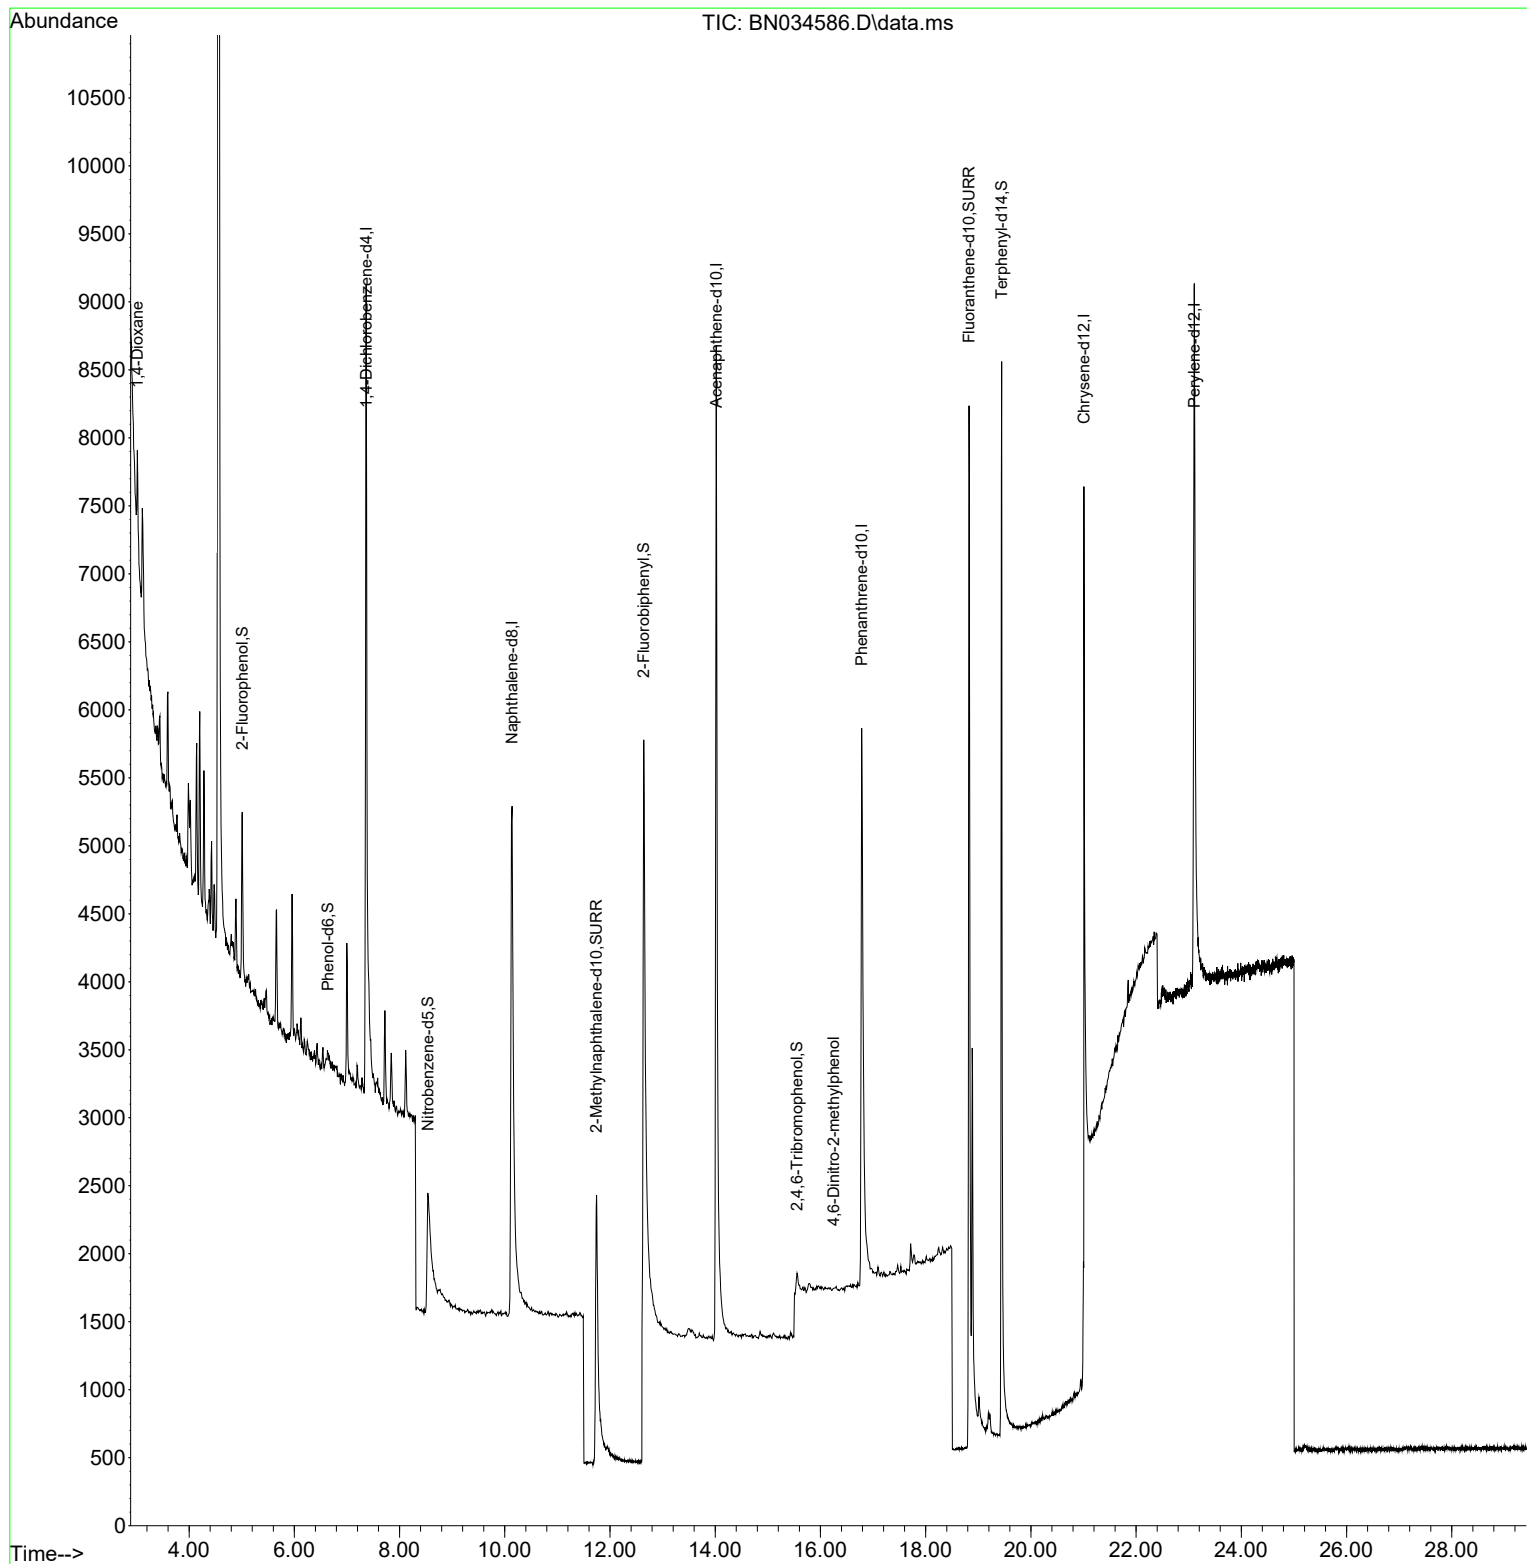



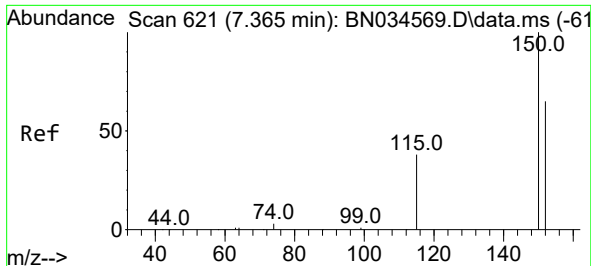


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.365 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN034586.D
 Acq: 15 Oct 2024 00:07

Instrument :
 BNA_N
 ClientSampleId :
 RW7-SP302-20241002



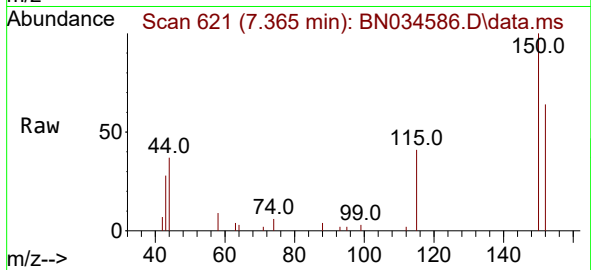



Tgt Ion:152 Resp: 3755
 Ion Ratio Lower Upper
 152 100
 150 155.3 122.0 183.0
 115 63.3 48.3 72.5

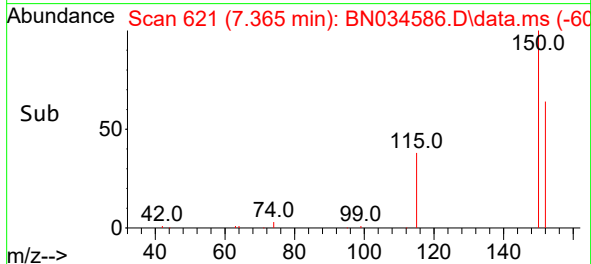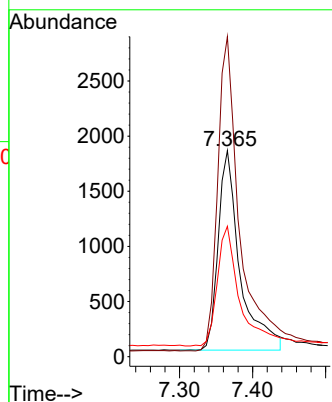

#2
 1,4-Dioxane
 Concen: 0.105 ng
 RT: 3.018 min Scan# 19
 Delta R.T. -0.007 min
 Lab File: BN034586.D
 Acq: 15 Oct 2024 00:07

Tgt Ion: 88 Resp: 477
 Ion Ratio Lower Upper
 88 100
 43 0.0 22.8 34.2#
 58 100.2 56.4 84.6#


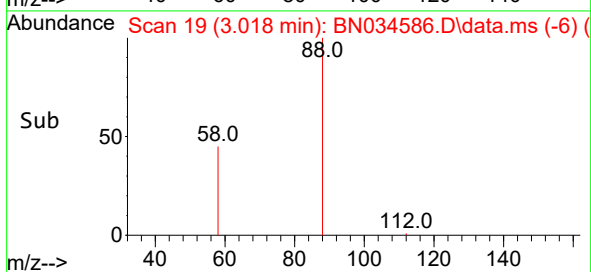
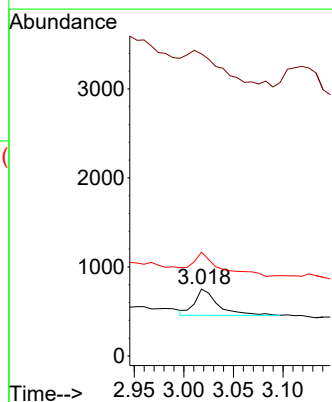
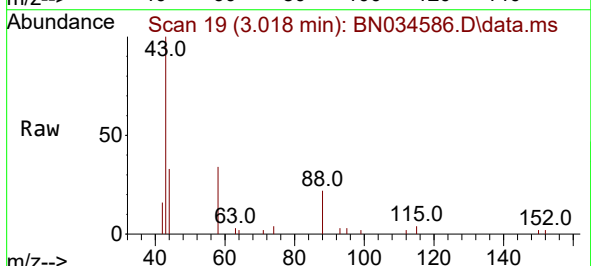


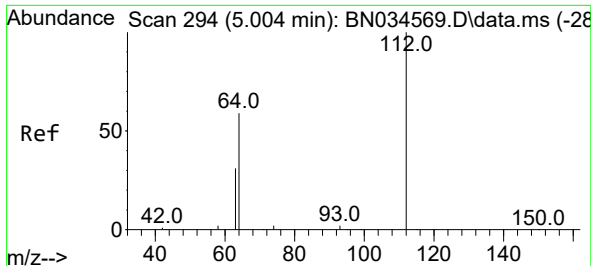

#4
2-Fluorophenol
Concen: 0.106 ng
RT: 5.011 min Scan# 294
Delta R.T. 0.007 min
Lab File: BN034586.D
Acq: 15 Oct 2024 00:07




Instrument :
BNA_N
ClientSampleId :
RW7-SP302-20241002


Tgt Ion:112 Resp: 1082
Ion Ratio Lower Upper
112 100
64 55.5 44.6 66.8
63 30.0 23.8 35.6

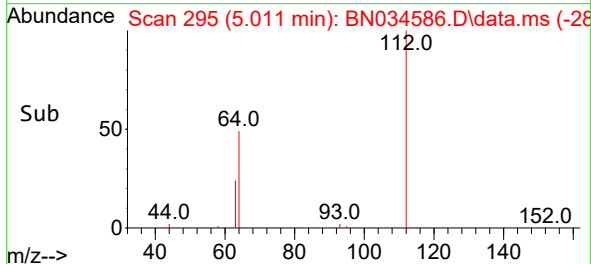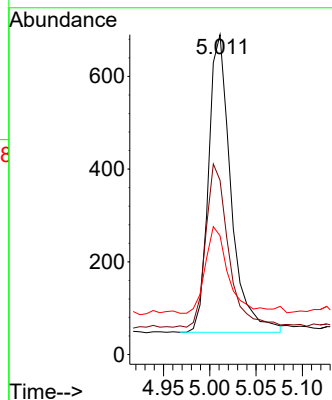

#5
Phenol-d6
Concen: 0.035 ng
RT: 6.636 min Scan# 520
Delta R.T. 0.072 min
Lab File: BN034586.D
Acq: 15 Oct 2024 00:07

Tgt Ion: 99 Resp: 364
Ion Ratio Lower Upper
99 100
42 10.7 15.0 22.6#
71 20.6 28.0 42.0#



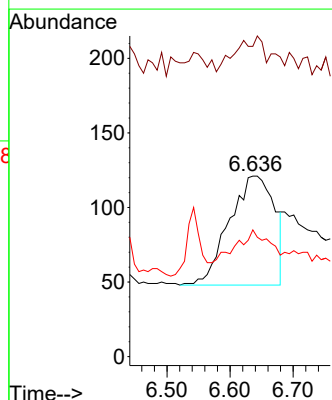
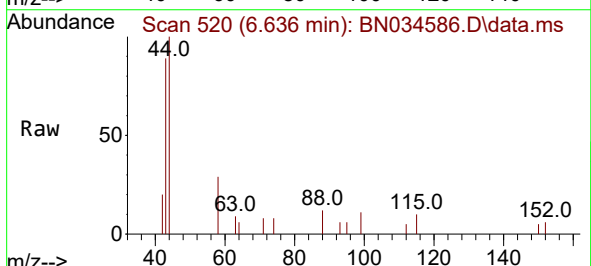


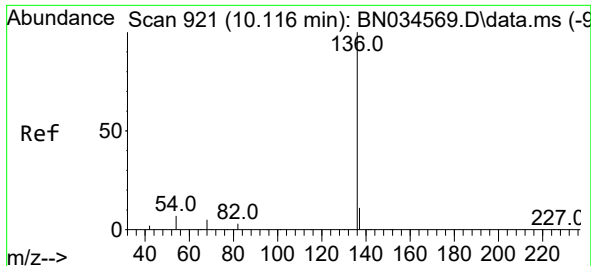

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.137 min Scan# 91
Delta R.T. 0.021 min
Lab File: BN034586.D
Acq: 15 Oct 2024 00:07




Instrument :
BNA_N
ClientSampleId :
RW7-SP302-20241002


Tgt Ion:	136	Resp:	10712
Ion Ratio	Lower	Upper	
136	100		
137	12.8	9.4	14.0
54	8.9	6.2	9.4
68	6.4	4.6	6.8

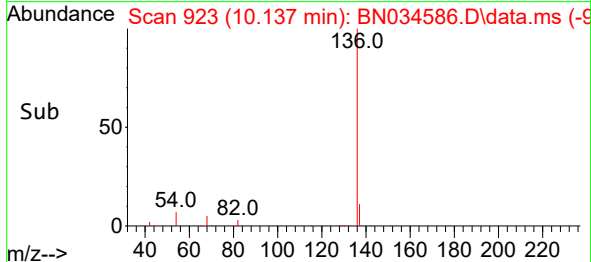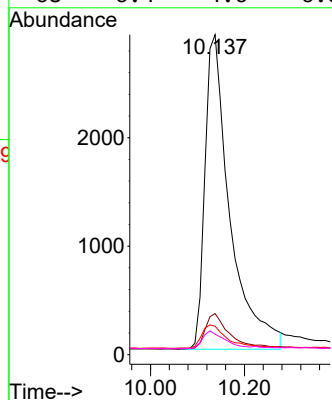

#8
Nitrobenzene-d5
Concen: 0.300 ng
RT: 8.536 min Scan# 773
Delta R.T. 0.021 min
Lab File: BN034586.D
Acq: 15 Oct 2024 00:07

Tgt Ion:	82	Resp:	2096
Ion Ratio	Lower	Upper	
82	100		
128	51.8	38.0	57.0
54	60.0	40.6	60.8

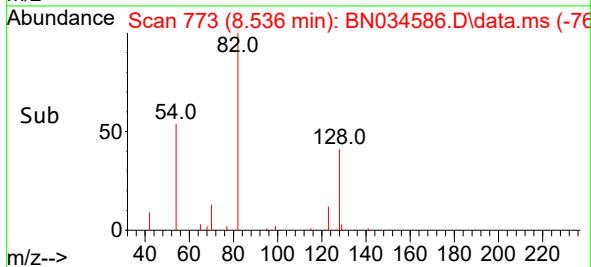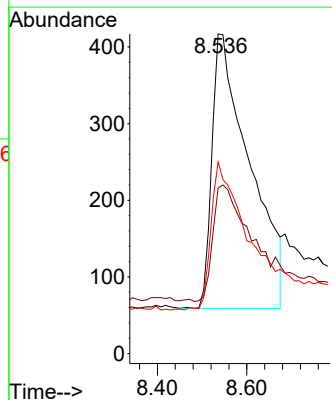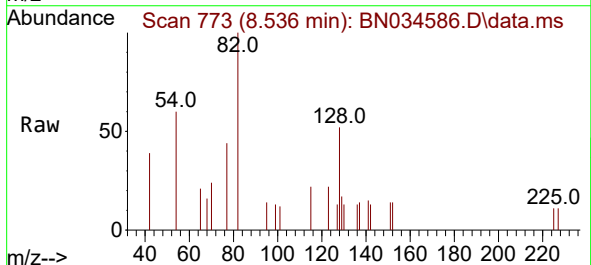

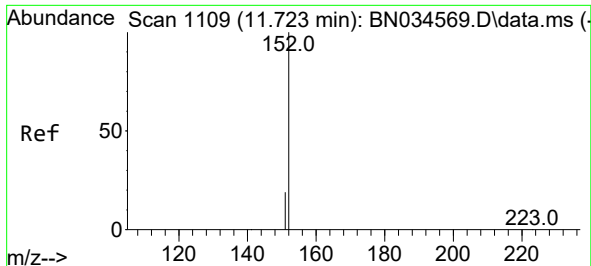

#11

2-Methylnaphthalene-d10

Concen: 0.366 ng

RT: 11.742 min Scan# 1114

Delta R.T. 0.019 min

Lab File: BN034586.D

Acq: 15 Oct 2024 00:07

Instrument :

BNA_N

ClientSampleId :





RW7-SP302-20241002

Tgt Ion:152 Resp: 5871

Ion Ratio Lower Upper

152 100

151 20.3 16.7 25.1

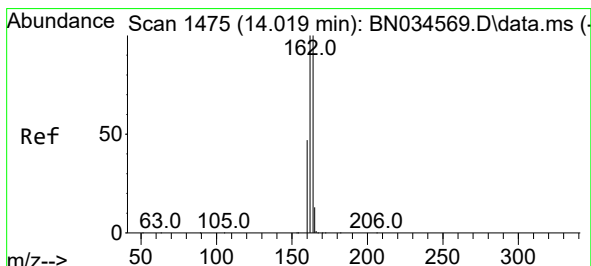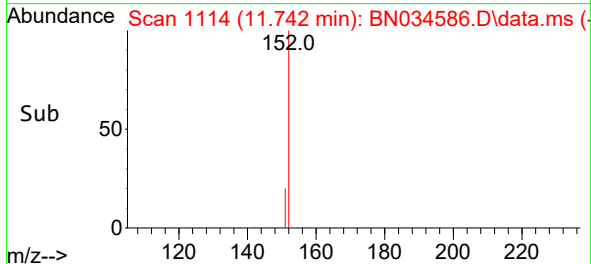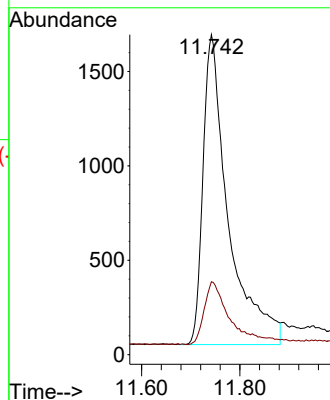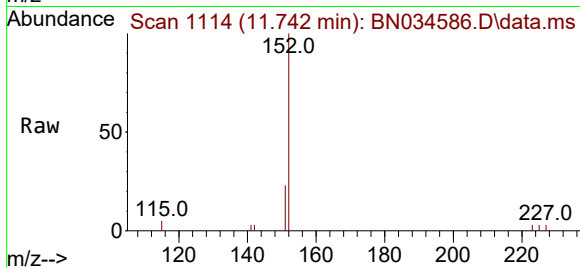

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.019 min Scan# 1475

Delta R.T. 0.000 min

Lab File: BN034586.D

Acq: 15 Oct 2024 00:07




Tgt Ion:164 Resp: 6300


Ion Ratio Lower Upper

164 100

162 104.6 79.7 119.5

160 49.5 37.9 56.9



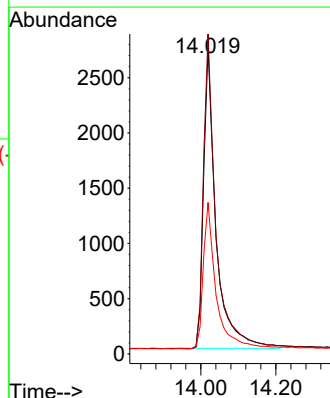
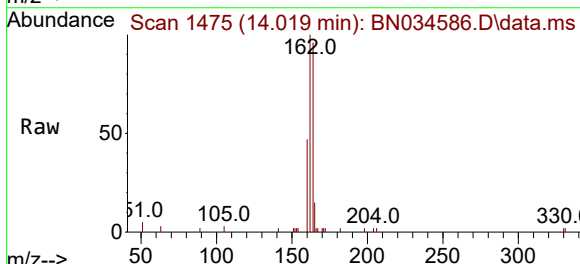


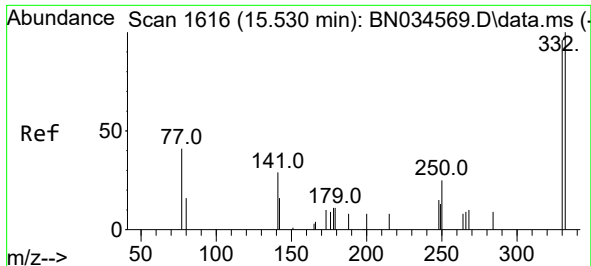

#14
2,4,6-Tribromophenol
Concen: 0.059 ng
RT: 15.555 min Scan# 1618
Delta R.T. 0.025 min
Lab File: BN034586.D
Acq: 15 Oct 2024 00:07




Instrument :
BNA_N
ClientSampleId :
RW7-SP302-20241002


Tgt Ion:330 Resp: 166
Ion Ratio Lower Upper
330 100
332 313.9 104.3 156.5#
141 41.6 29.4 44.0

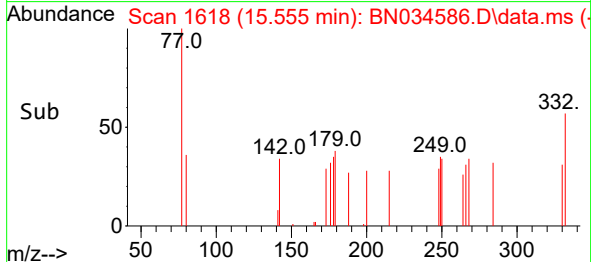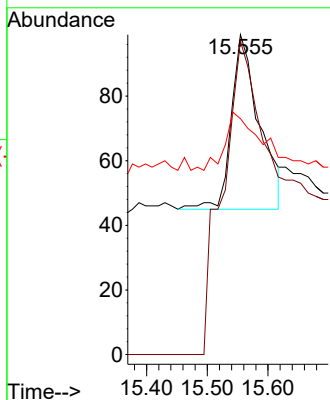

#15
2-Fluorobiphenyl
Concen: 0.365 ng
RT: 12.640 min Scan# 1346
Delta R.T. 0.000 min
Lab File: BN034586.D
Acq: 15 Oct 2024 00:07

Tgt Ion:172 Resp: 7935
Ion Ratio Lower Upper
172 100
171 36.6 27.1 40.7
170 25.0 18.5 27.7

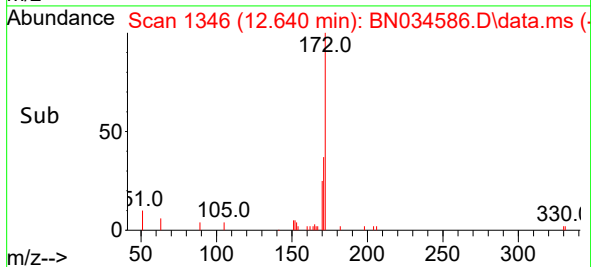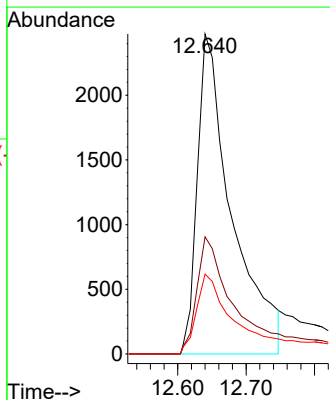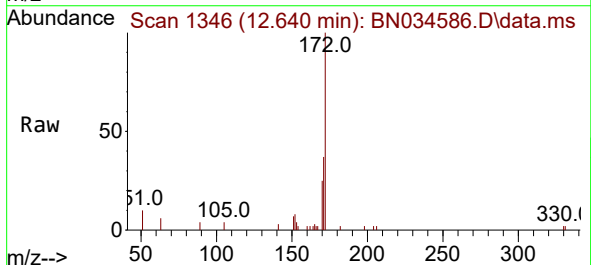

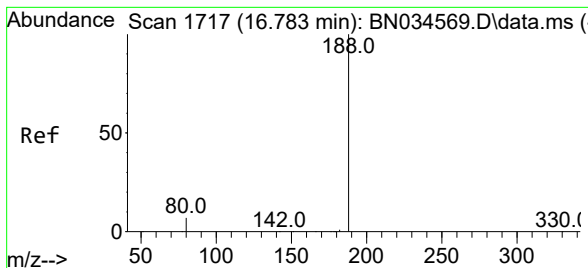

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.783 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN034586.D

Acq: 15 Oct 2024 00:07

Instrument :

BNA_N

ClientSampleId :

RW7-SP302-20241002





Tgt Ion:188 Resp: 10749

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 12.1 6.3 9.5#

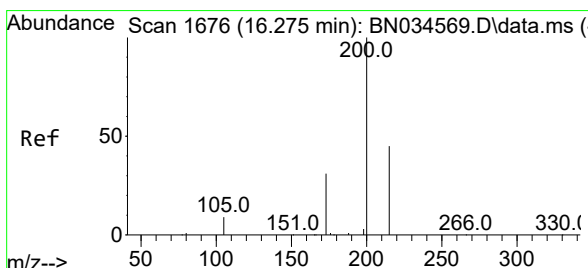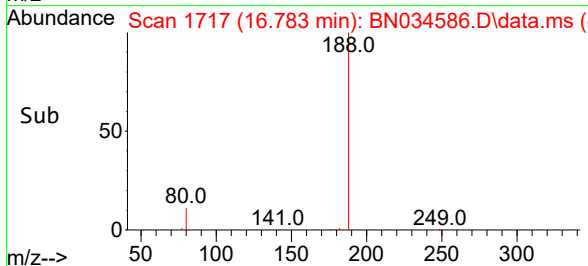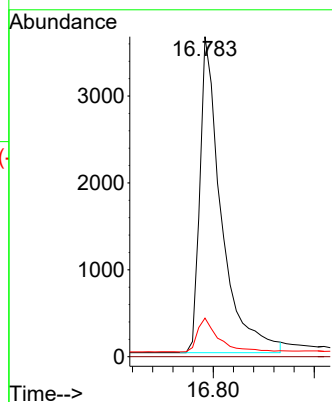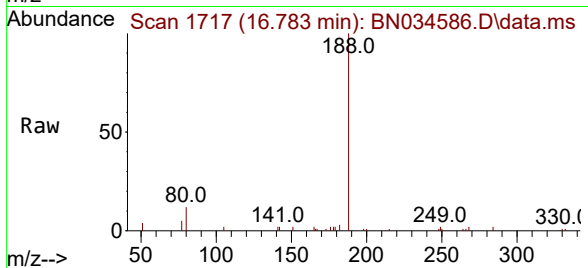

#20

4,6-Dinitro-2-methylphenol

Concen: 0.027 ng

RT: 16.250 min Scan# 1674

Delta R.T. -0.025 min

Lab File: BN034586.D

Acq: 15 Oct 2024 00:07




Tgt Ion:198 Resp: 4


Ion Ratio Lower Upper

198 100

51 297.9 174.8 262.2#

105 164.6 167.9 251.9#


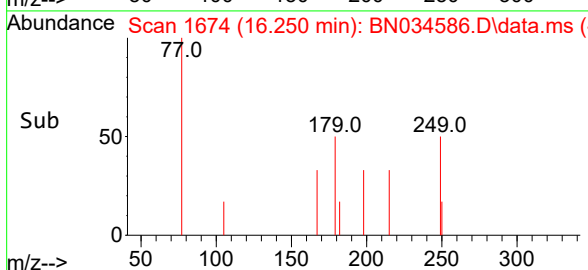
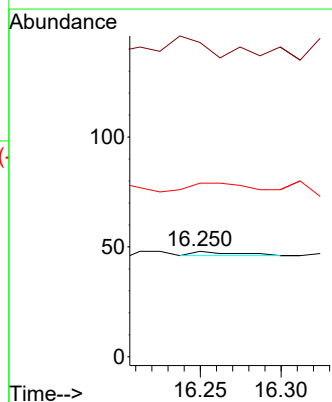
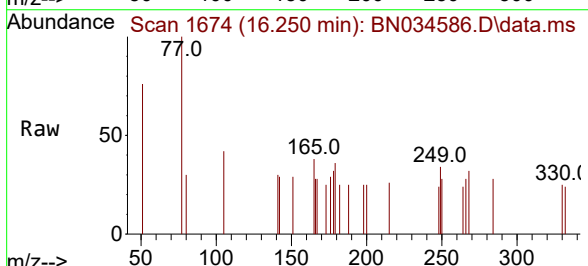


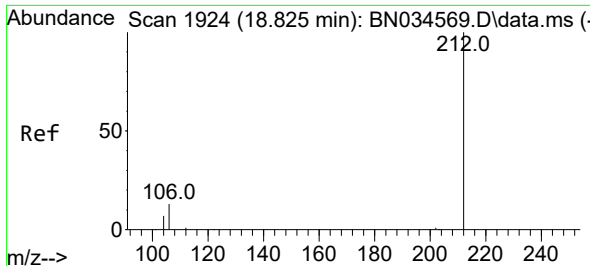

#27
Fluoranthene-d10
Concen: 0.457 ng
RT: 18.825 min Scan# 1924
Delta R.T. 0.000 min
Lab File: BN034586.D
Acq: 15 Oct 2024 00:07




Instrument :
BNA_N
ClientSampleId :
RW7-SP302-20241002


Tgt Ion:212 Resp: 11949
Ion Ratio Lower Upper
212 100
106 13.0 11.1 16.7
104 7.4 6.5 9.7

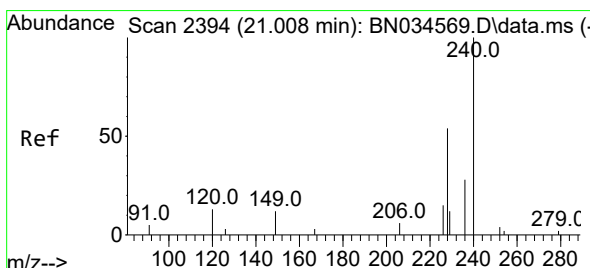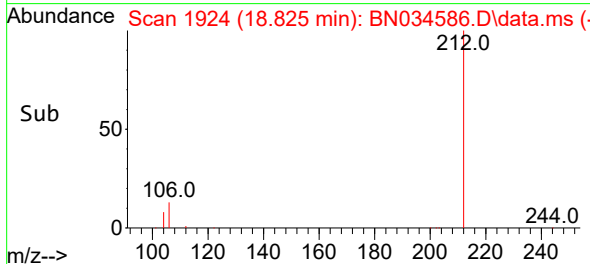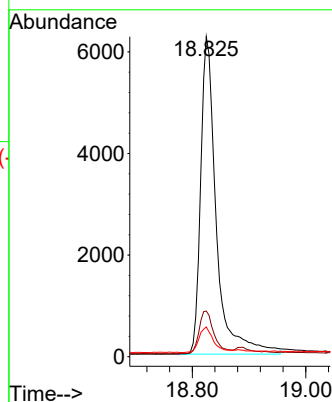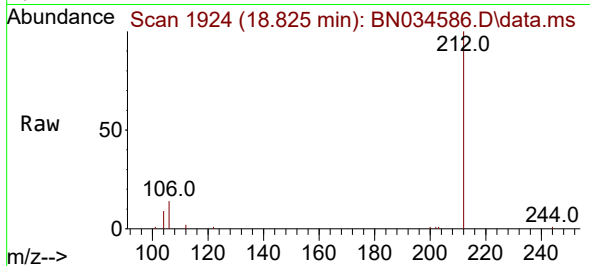

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.008 min Scan# 2394
Delta R.T. 0.000 min
Lab File: BN034586.D
Acq: 15 Oct 2024 00:07

Tgt Ion:240 Resp: 5448
Ion Ratio Lower Upper
240 100
120 13.5 10.1 15.1
236 29.0 22.6 34.0


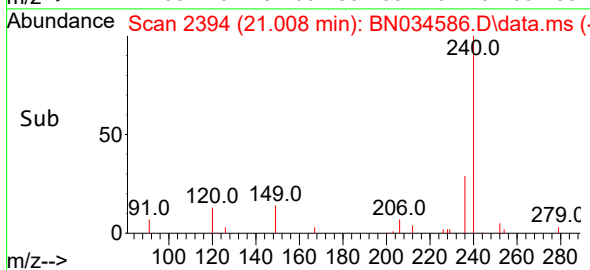
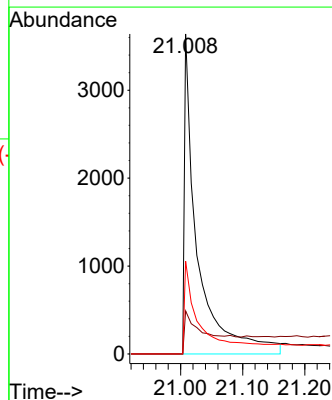
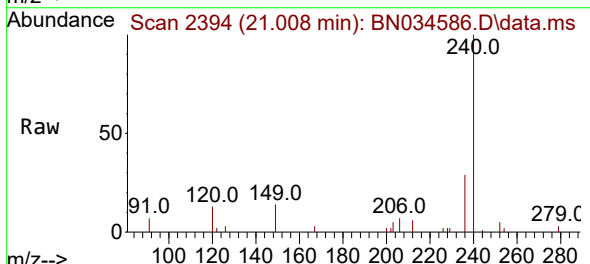


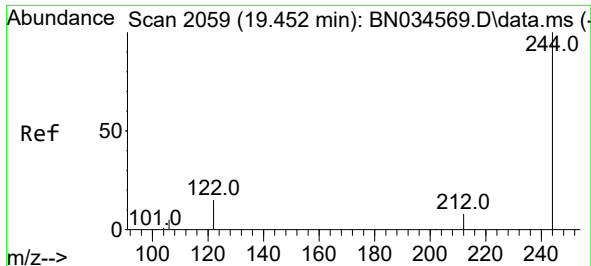

#31
Terphenyl-d14
Concen: 0.432 ng
RT: 19.443 min Scan# 2057
Delta R.T. -0.009 min
Lab File: BN034586.D
Acq: 15 Oct 2024 00:07

Instrument :
BNA_N
ClientSampleId :
RW7-SP302-20241002

Tgt Ion:244 Resp: 9330
Ion Ratio Lower Upper
244 100
212 9.4 7.7 11.5
122 15.1 12.6 19.0

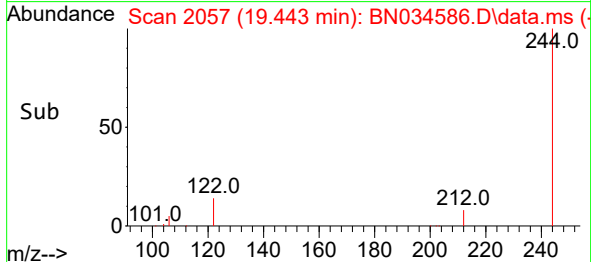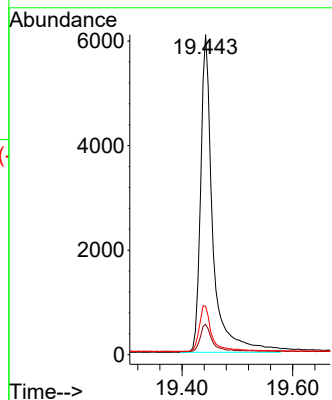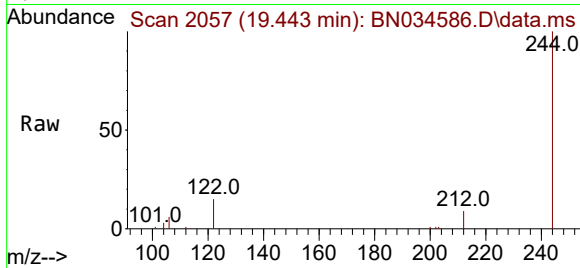

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.104 min Scan# 2789
Delta R.T. -0.006 min
Lab File: BN034586.D
Acq: 15 Oct 2024 00:07

Tgt Ion:264 Resp: 8672
Ion Ratio Lower Upper
264 100
260 26.0 20.9 31.3
265 90.1 61.6 92.4

