

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
 Data File : BN034587.D
 Acq On : 15 Oct 2024 00:44
 Operator : RC/JU
 Sample : P4241-02DL 2X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-TT189D2-GW-20240926DL

Quant Time: Oct 15 01:17:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 17:52:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.365	152	5957	0.400	ng	0.00
7) Naphthalene-d8	10.127	136	17679	0.400	ng	0.01
13) Acenaphthene-d10	14.019	164	11244	0.400	ng	0.00
19) Phenanthrene-d10	16.783	188	21118	0.400	ng	0.00
29) Chrysene-d12	21.008	240	7258	0.400	ng	0.00
35) Perylene-d12	23.101	264	15100	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.011	112	683	0.042	ng	0.00
5) Phenol-d6	6.621	99	291	0.017	ng	0.06
8) Nitrobenzene-d5	8.536	82	1413	0.123	ng	0.02
11) 2-Methylnaphthalene-d10	11.734	152	3790	0.143	ng	0.01
14) 2,4,6-Tribromophenol	15.530	330	532	0.107	ng	0.00
15) 2-Fluorobiphenyl	12.640	172	5902	0.152	ng	0.00
27) Fluoranthene-d10	18.825	212	9123	0.178	ng	0.00
31) Terphenyl-d14	19.442	244	6896	0.329	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.018	88	17829	2.481	ng	Qvalue 95
20) 4,6-Dinitro-2-methylph...	16.237	198	16	0.055	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
Data File : BN034587.D
Acq On : 15 Oct 2024 00:44
Operator : RC/JU
Sample : P4241-02DL 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BP-TT189D2-GW-20240926DL


Quant Time: Oct 15 01:17:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 17:52:02 2024
Response via : Initial Calibration

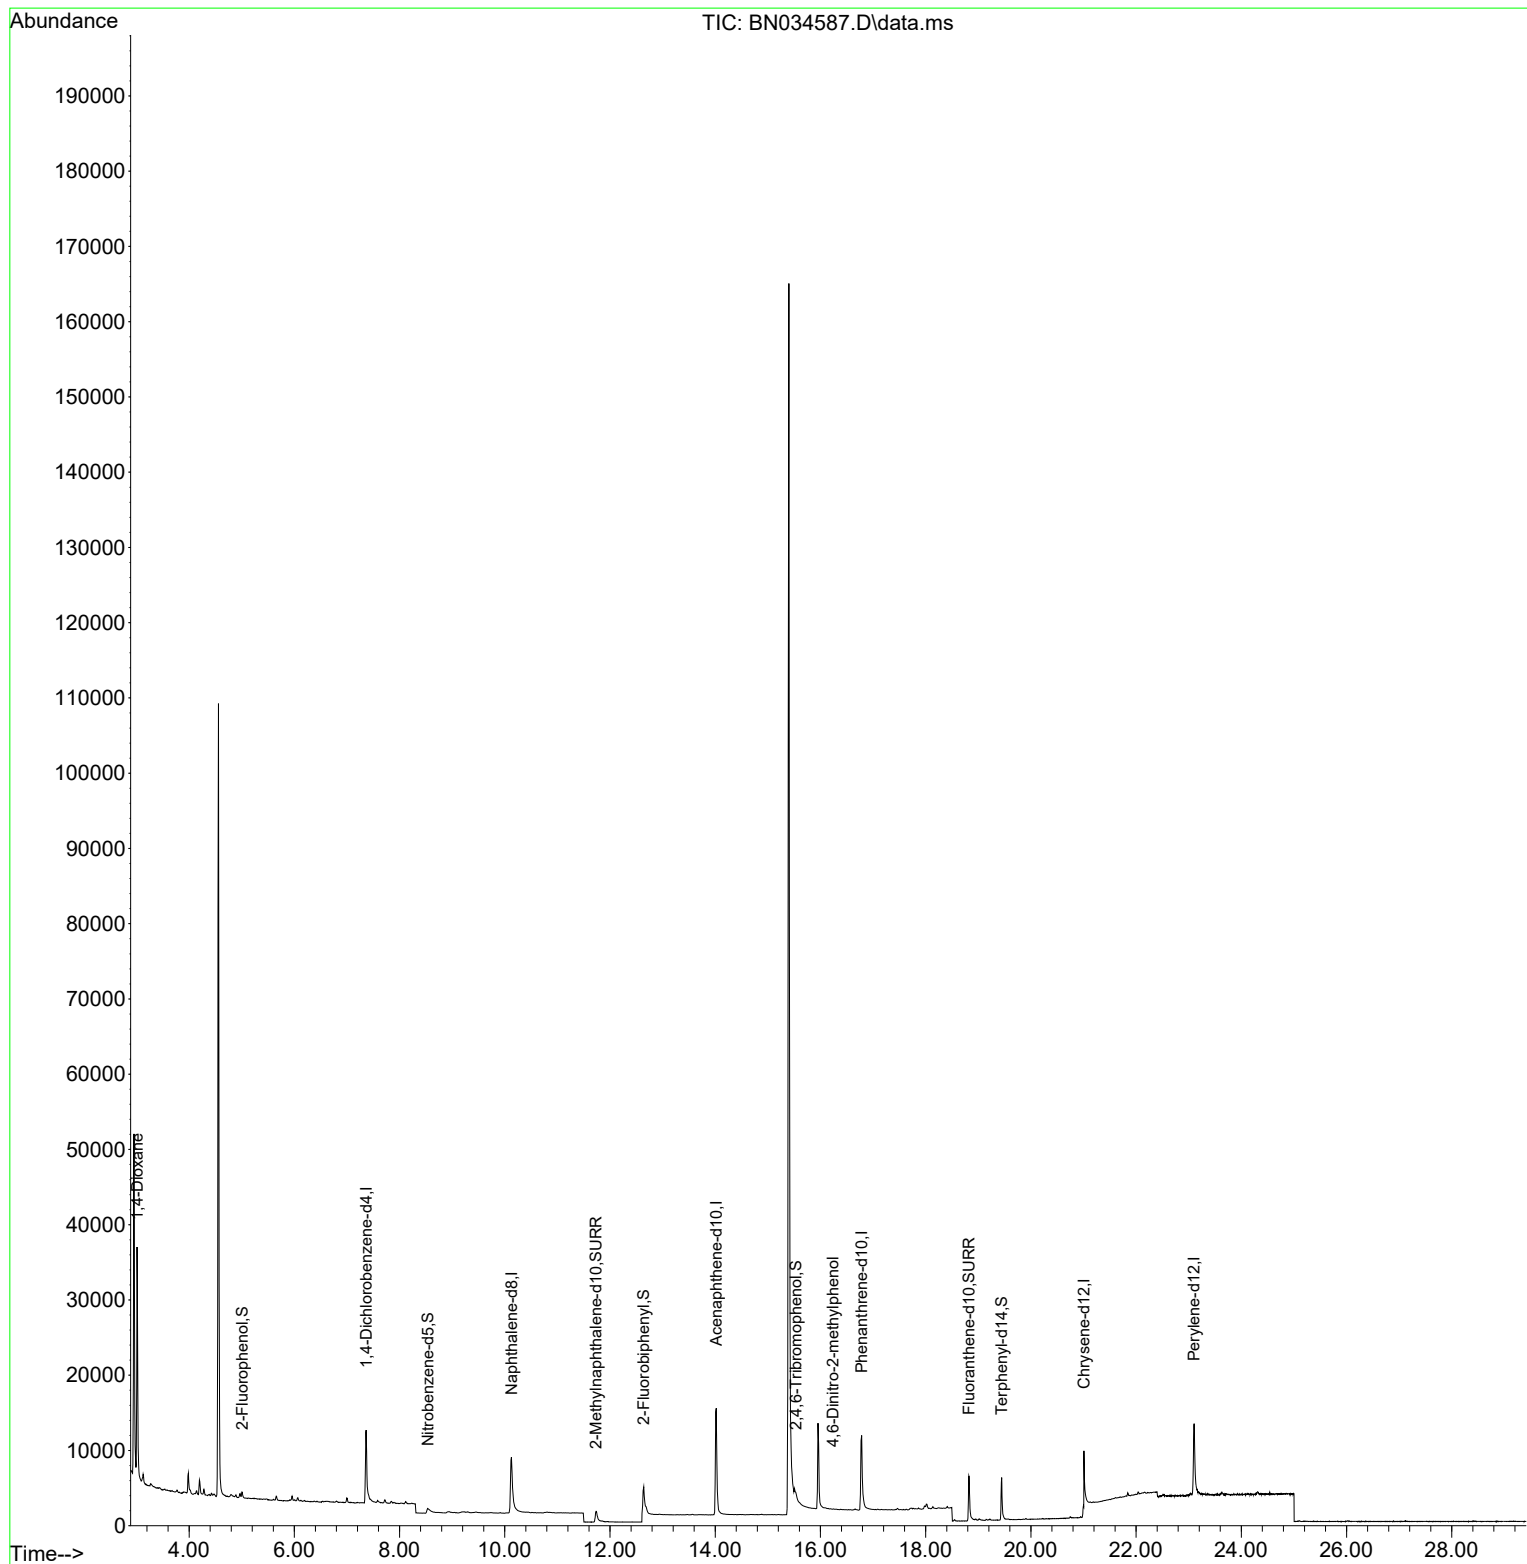






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.365 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN034587.D
 Acq: 15 Oct 2024 00:44


Instrument :
 BNA_N
 ClientSampleId :
 BP-TT189D2-GW-20240926DL

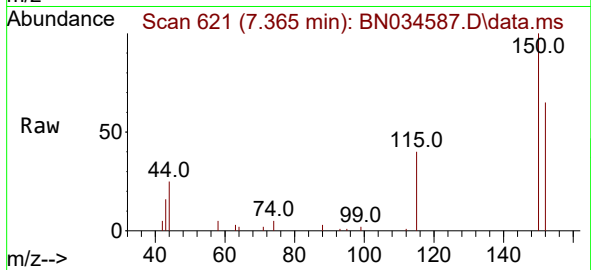



Tgt Ion:152 Resp: 5957
 Ion Ratio Lower Upper
 152 100
 150 154.3 122.0 183.0
 115 61.1 48.3 72.5

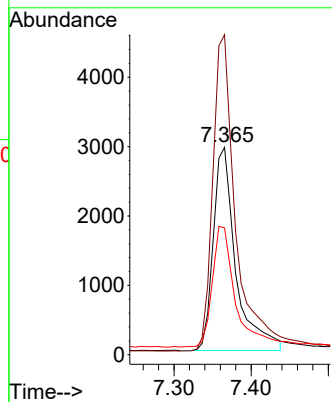


#2
 1,4-Dioxane
 Concen: 2.481 ng
 RT: 3.018 min Scan# 19
 Delta R.T. -0.007 min
 Lab File: BN034587.D
 Acq: 15 Oct 2024 00:44

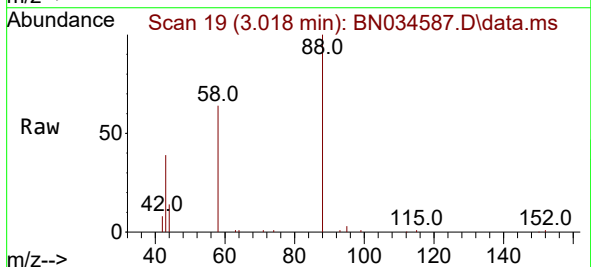

Tgt Ion: 88 Resp: 17829
 Ion Ratio Lower Upper
 88 100
 43 32.6 22.8 34.2
 58 73.3 56.4 84.6



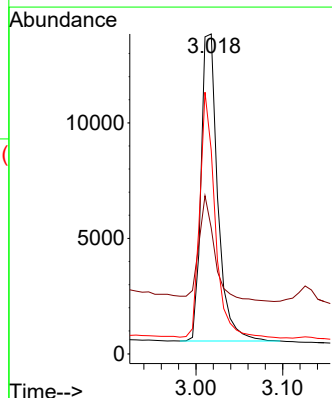





#4
2-Fluorophenol
Concen: 0.042 ng
RT: 5.011 min Scan# 294
Delta R.T. 0.007 min
Lab File: BN034587.D
Acq: 15 Oct 2024 00:44




Instrument :
BNA_N
ClientSampleId :
BP-TT189D2-GW-20240926DL


Tgt Ion:112 Resp: 683
Ion Ratio Lower Upper
112 100
64 56.1 44.6 66.8
63 28.3 23.8 35.6

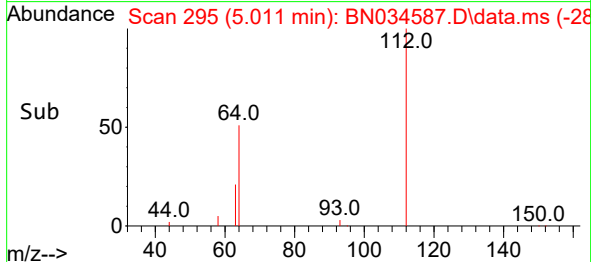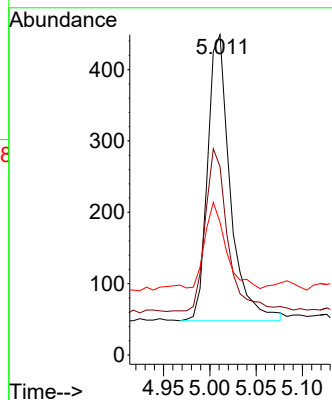

#5
Phenol-d6
Concen: 0.017 ng
RT: 6.621 min Scan# 518
Delta R.T. 0.058 min
Lab File: BN034587.D
Acq: 15 Oct 2024 00:44

Tgt Ion: 99 Resp: 291
Ion Ratio Lower Upper
99 100
42 0.0 15.0 22.6#
71 26.8 28.0 42.0#


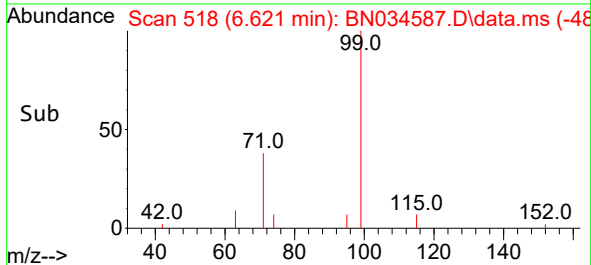
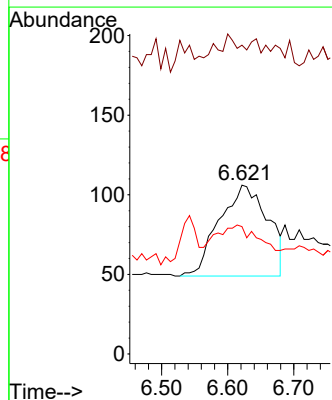
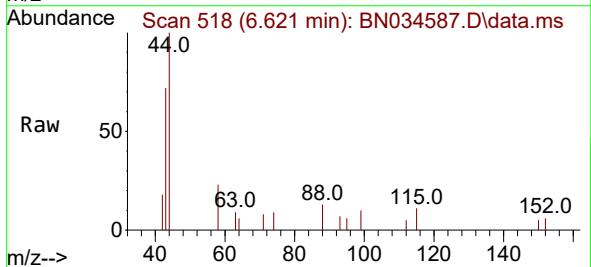




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.127 min Scan# 91
Delta R.T. 0.011 min
Lab File: BN034587.D
Acq: 15 Oct 2024 00:44




Instrument :
BNA_N
ClientSampleId :
BP-TT189D2-GW-20240926DL


Tgt Ion:	136	Resp:	17679
Ion	Ratio	Lower	Upper
136	100		
137	11.6	9.4	14.0
54	7.6	6.2	9.4
68	5.7	4.6	6.8

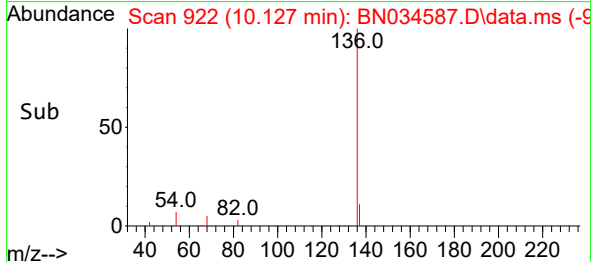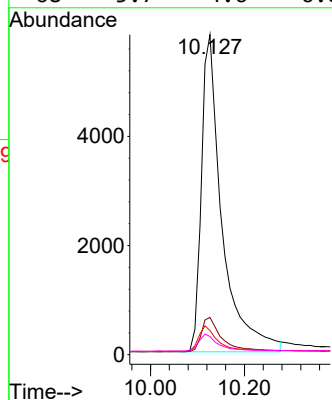

#8
Nitrobenzene-d5
Concen: 0.123 ng
RT: 8.536 min Scan# 773
Delta R.T. 0.021 min
Lab File: BN034587.D
Acq: 15 Oct 2024 00:44

Tgt Ion:	82	Resp:	1413
Ion	Ratio	Lower	Upper
82	100		
128	55.0	38.0	57.0
54	60.1	40.6	60.8


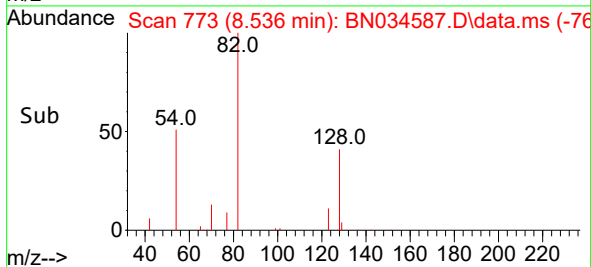
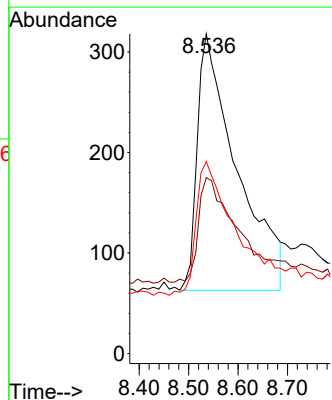
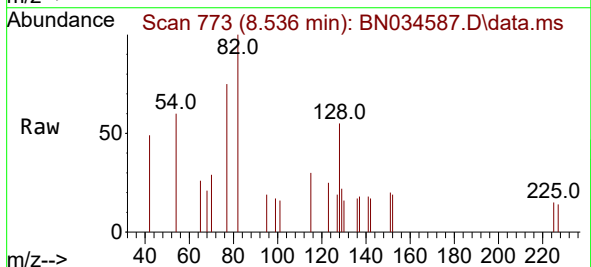




#11
2-Methylnaphthalene-d10
Concen: 0.143 ng
RT: 11.734 min Scan# 1112
Delta R.T. 0.011 min
Lab File: BN034587.D
Acq: 15 Oct 2024 00:44




Instrument :
BNA_N
ClientSampleId :
BP-TT189D2-GW-20240926DL


Tgt Ion:152 Resp: 3790
Ion Ratio Lower Upper
152 100
151 20.1 16.7 25.1

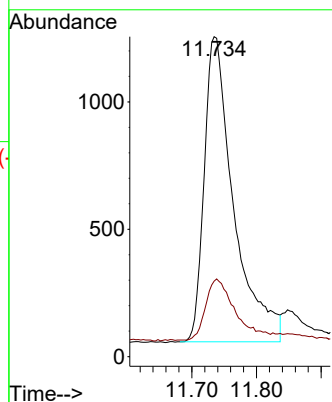

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.019 min Scan# 1475
Delta R.T. -0.000 min
Lab File: BN034587.D
Acq: 15 Oct 2024 00:44

Tgt Ion:164 Resp: 11244
Ion Ratio Lower Upper
164 100
162 102.0 79.7 119.5
160 48.3 37.9 56.9


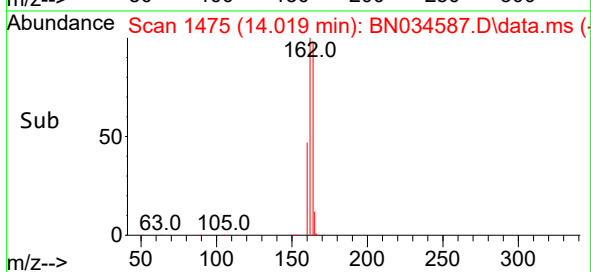
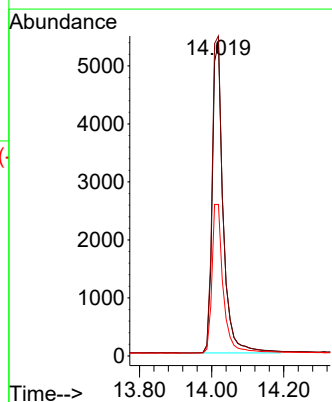





#14
2,4,6-Tribromophenol
Concen: 0.107 ng
RT: 15.530 min Scan# 1616
Delta R.T. -0.000 min
Lab File: BN034587.D
Acq: 15 Oct 2024 00:44




Instrument :
BNA_N
ClientSampleId :
BP-TT189D2-GW-20240926DL


Tgt Ion:330 Resp: 532
Ion Ratio Lower Upper
330 100
332 160.3 104.3 156.5#
141 38.3 29.4 44.0

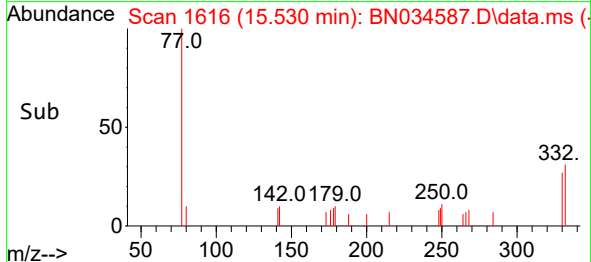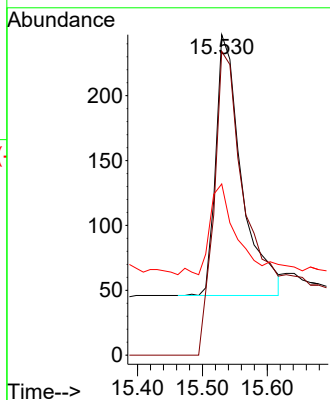

#15
2-Fluorobiphenyl
Concen: 0.152 ng
RT: 12.640 min Scan# 1346
Delta R.T. -0.000 min
Lab File: BN034587.D
Acq: 15 Oct 2024 00:44

Tgt Ion:172 Resp: 5902
Ion Ratio Lower Upper
172 100
171 36.1 27.1 40.7
170 24.6 18.5 27.7

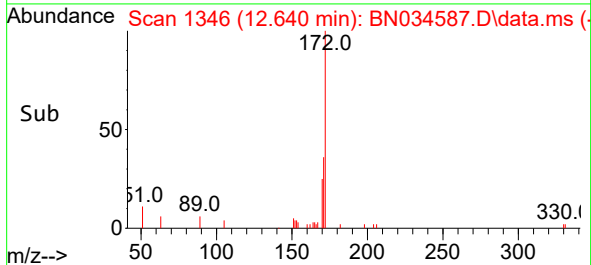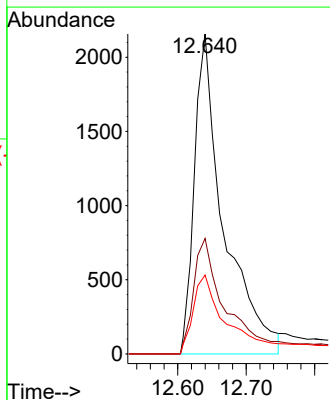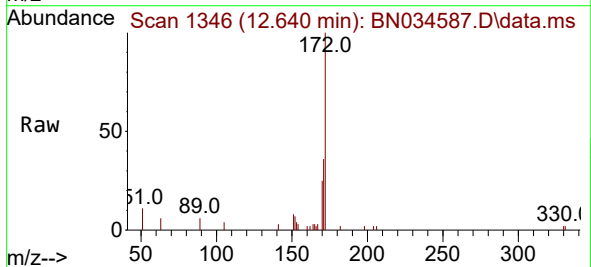



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.783 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN034587.D

Acq: 15 Oct 2024 00:44

Instrument :

BNA_N

ClientSampleId :

BP-TT189D2-GW-20240926DL





Tgt Ion:188 Resp: 21118

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 8.1 6.3 9.5

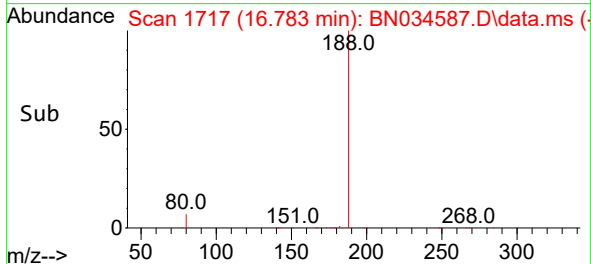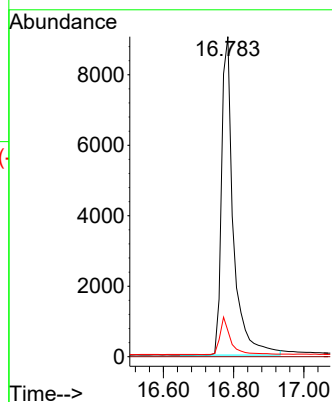

#20

4,6-Dinitro-2-methylphenol

Concen: 0.055 ng

RT: 16.237 min Scan# 1673

Delta R.T. -0.038 min

Lab File: BN034587.D

Acq: 15 Oct 2024 00:44




Tgt Ion:198 Resp: 16


Ion Ratio Lower Upper

198 100

51 350.0 174.8 262.2#

105 403.7 167.9 251.9#

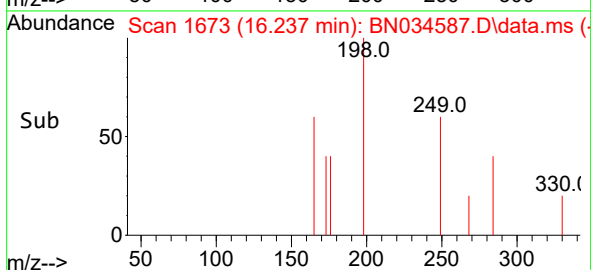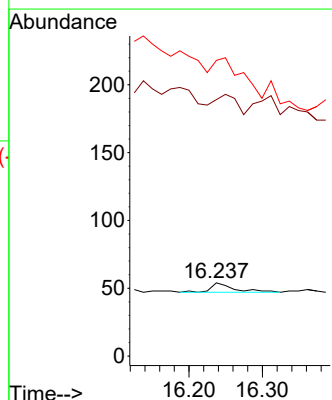



#27

Fluoranthene-d10

Concen: 0.178 ng

RT: 18.825 min Scan# 1924

Delta R.T. -0.000 min

Lab File: BN034587.D

Acq: 15 Oct 2024 00:44

Instrument :

BNA_N

ClientSampleId :

BP-TT189D2-GW-20240926DL





Tgt Ion:212 Resp: 9123

Ion Ratio Lower Upper

212 100

106 13.4 11.1 16.7

104 7.8 6.5 9.7

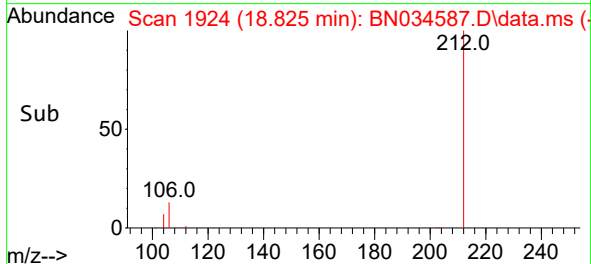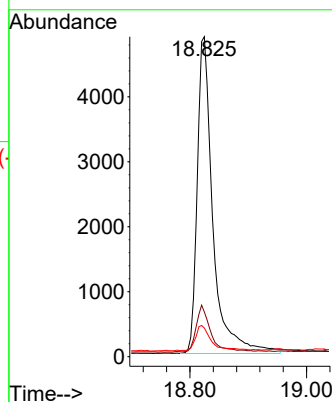

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.008 min Scan# 2394

Delta R.T. -0.000 min

Lab File: BN034587.D

Acq: 15 Oct 2024 00:44




Tgt Ion:240 Resp: 7258


Ion Ratio Lower Upper

240 100

120 12.3 10.1 15.1


236 27.9 22.6 34.0

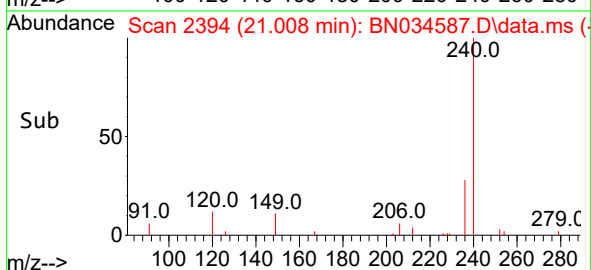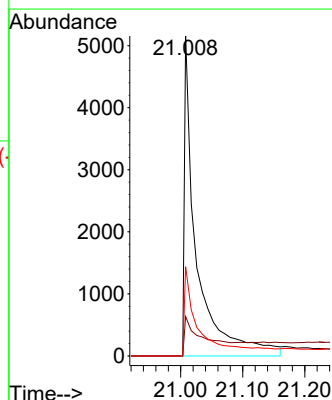






#31
Terphenyl-d14
Concen: 0.329 ng
RT: 19.442 min Scan# 2057
Delta R.T. -0.010 min
Lab File: BN034587.D
Acq: 15 Oct 2024 00:44

Instrument :
BNA_N
ClientSampleId :
BP-TT189D2-GW-20240926DL

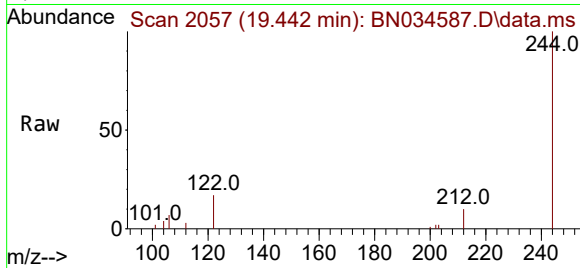

Tgt Ion:244 Resp: 6896
Ion Ratio Lower Upper
244 100
212 10.1 7.7 11.5
122 17.0 12.6 19.0

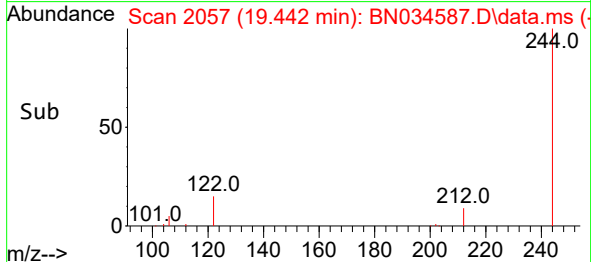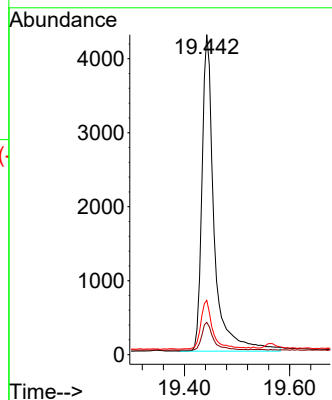

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.101 min Scan# 2788
Delta R.T. -0.009 min
Lab File: BN034587.D
Acq: 15 Oct 2024 00:44

Tgt Ion:264 Resp: 15100
Ion Ratio Lower Upper
264 100
260 26.3 20.9 31.3
265 59.4 61.6 92.4#

