
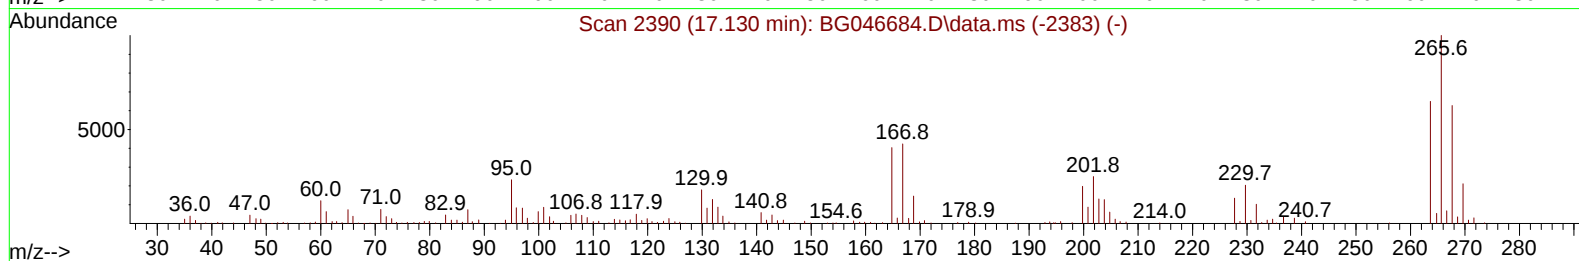
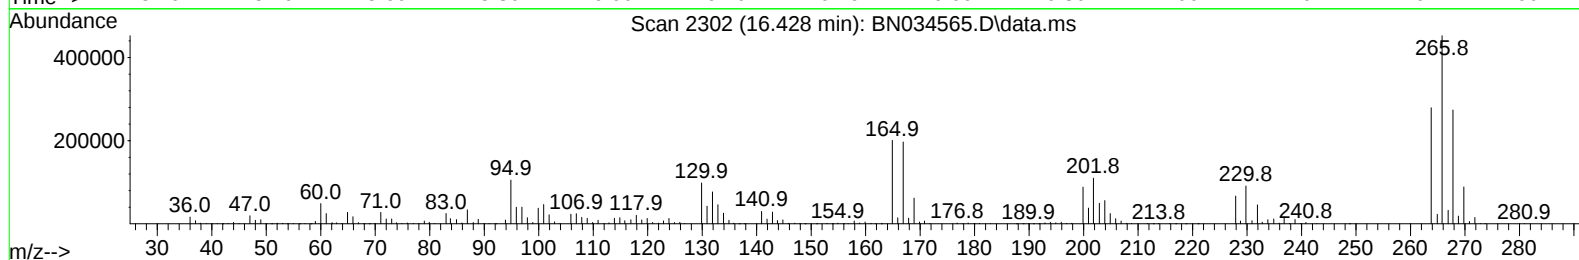


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
Data File : BN034565.D
Acq On : 14 Oct 2024 10:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 11:36:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 02:51:59 2024
Response via : Initial Calibration

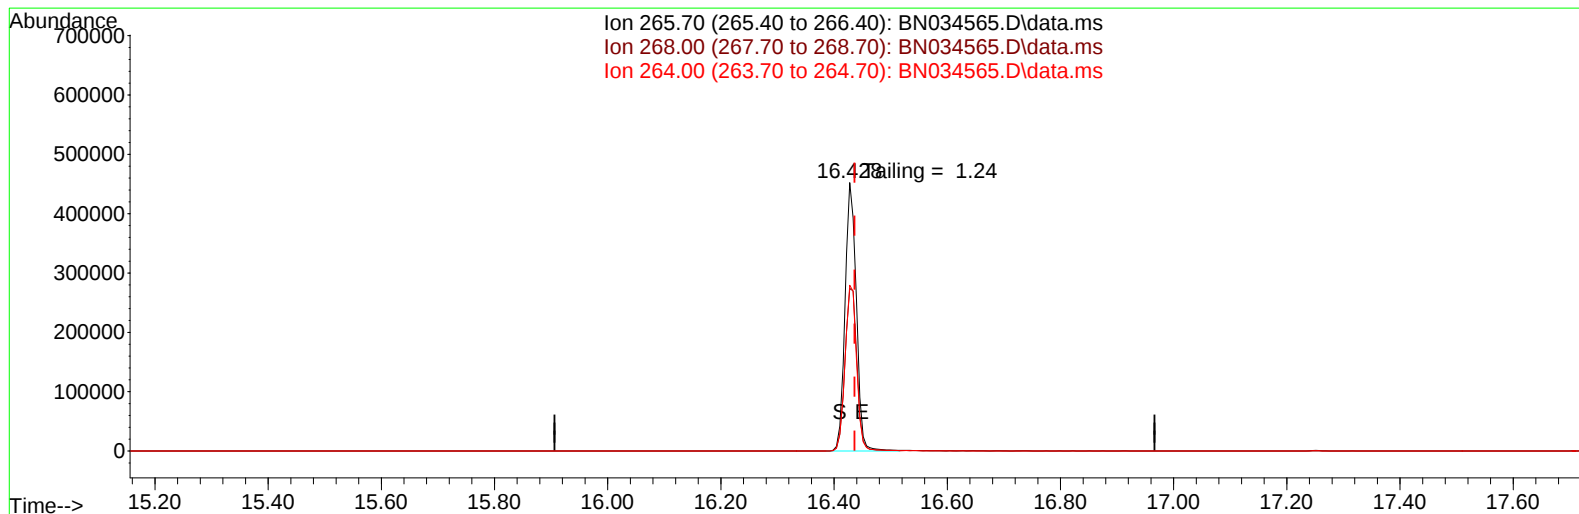

TIC: BN034565.D\data.ms

(70) Pentachlorophenol (C)




16.428min (-0.008) 27287.04 ng

response 628078

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.55
264.00	61.60	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
Data File : BN034565.D
Acq On : 14 Oct 2024 10:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 11:36:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 02:51:59 2024
Response via : Initial Calibration

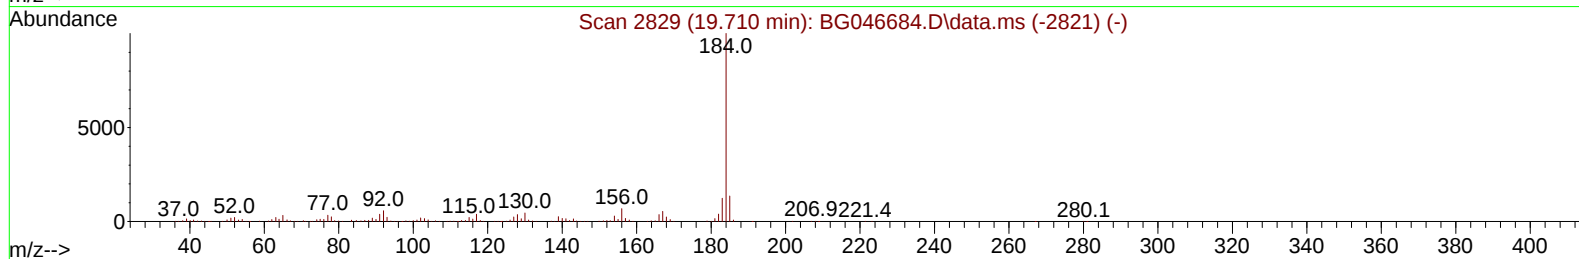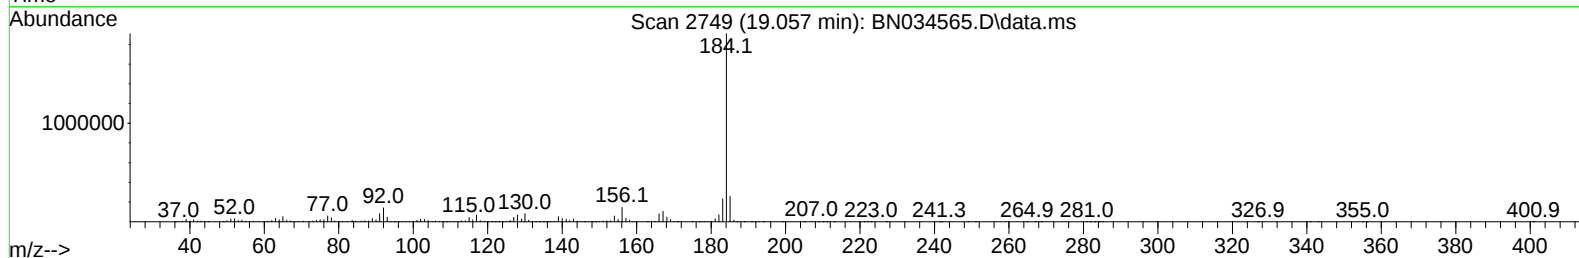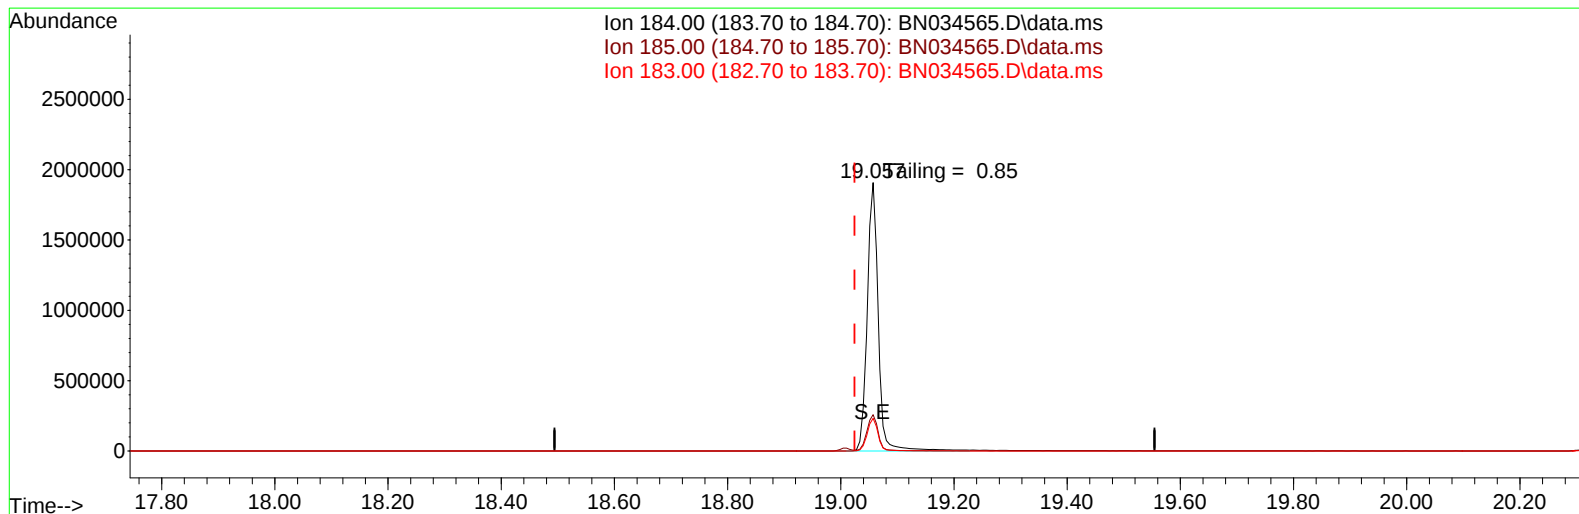

TIC: BN034565.D\data.ms

(77) Benzidine

19.057min (+ 0.033) 0.00 ng

response 2580788

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.57
183.00	13.20	12.18
0.00	0.00	0.00