
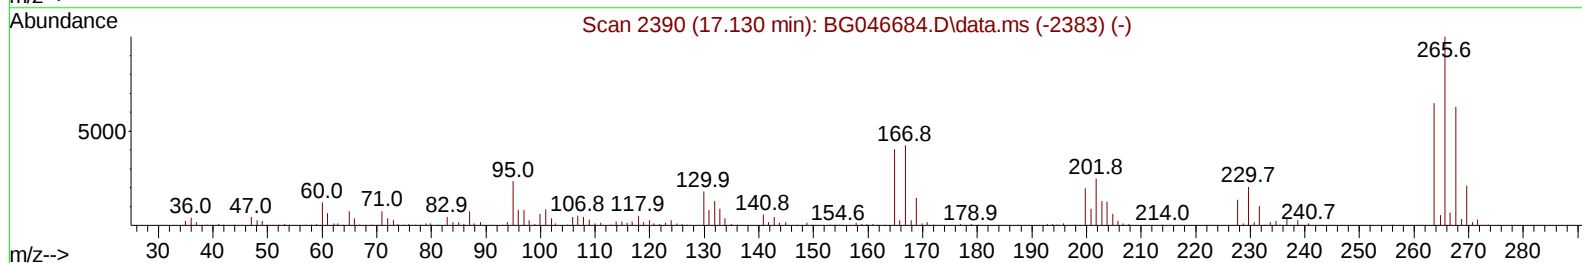
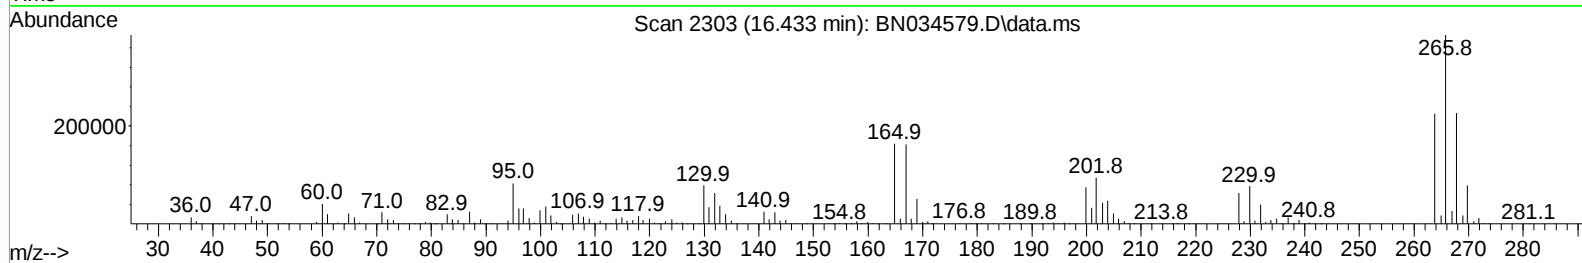


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
Data File : BN034579.D
Acq On : 14 Oct 2024 19:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 00:48:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 15 00:48:16 2024
Response via : Initial Calibration

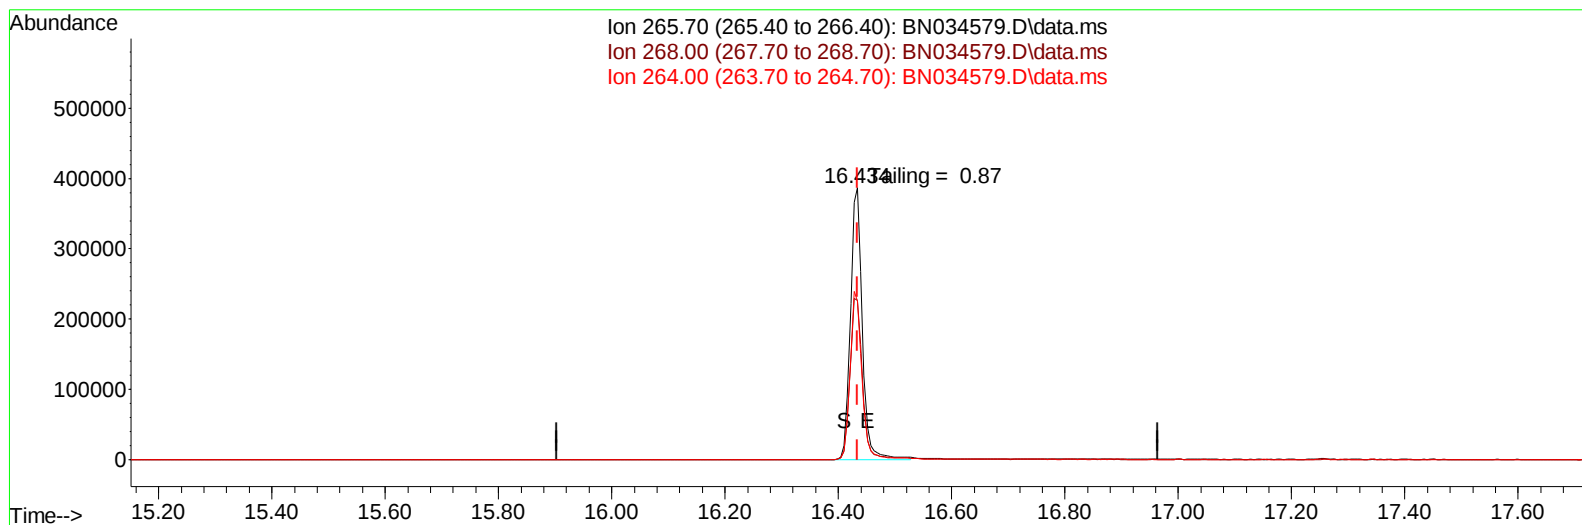

TIC: BN034579.D\data.ms

(70) Pentachlorophenol (C)




16.433min (0.000) 26821.50 ng

response 571476

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.52
264.00	61.60	58.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
Data File : BN034579.D
Acq On : 14 Oct 2024 19:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 00:48:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 15 00:48:16 2024
Response via : Initial Calibration

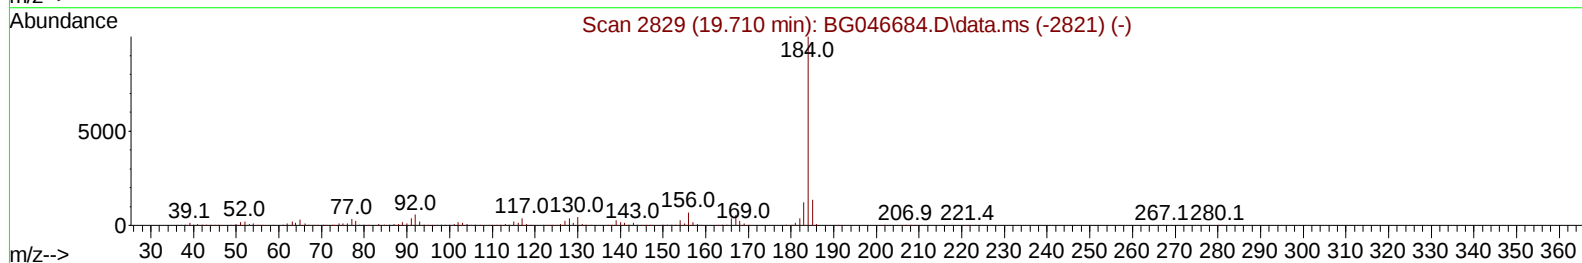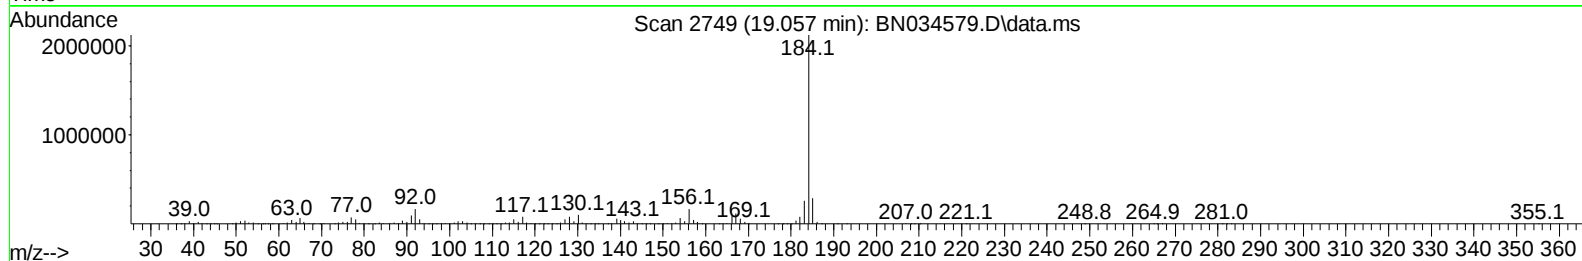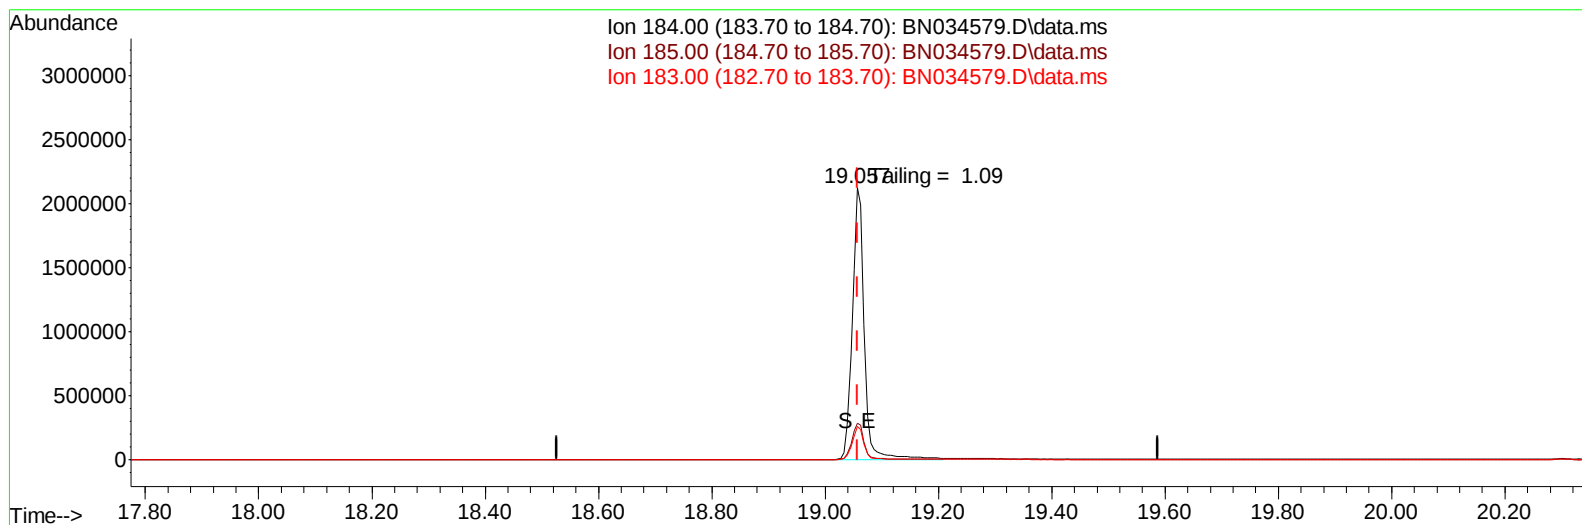

TIC: BN034579.D\data.ms

(77) Benzidine

19.057min (0.000) 0.00 ng

response 3146886

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.44
183.00	13.20	12.17
0.00	0.00	0.00