

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
 Data File : BN034573.D
 Acq On : 14 Oct 2024 16:13
 Operator : RC/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Oct 14 17:39:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 14 16:58:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.358	152	5343	0.400	ng	0.00
7) Naphthalene-d8	10.116	136	15688	0.400	ng	# 0.00
13) Acenaphthene-d10	14.008	164	9488	0.400	ng	-0.01
19) Phenanthrene-d10	16.771	188	20373	0.400	ng	-0.01
29) Chrysene-d12	21.008	240	3865	0.400	ng	# 0.00
35) Perylene-d12	23.104	264	12249	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.004	112	69455	4.795	ng	0.00
5) Phenol-d6	6.564	99	87872	5.853	ng	0.00
8) Nitrobenzene-d5	8.493	82	57986	5.668	ng	-0.02
11) 2-Methylnaphthalene-d10	11.712	152	122004	5.189	ng	-0.01
14) 2,4,6-Tribromophenol	15.517	330	29679	7.058	ng	-0.01
15) 2-Fluorobiphenyl	12.618	172	157382	4.810	ng	-0.02
27) Fluoranthene-d10	18.820	212	256499	5.178	ng	0.00
31) Terphenyl-d14	0.000	244	0d	0.000	ng	
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.018	88	26990	4.188	ng	98
3) n-Nitrosodimethylamine	3.314	42	28302	4.822	ng	# 97
6) bis(2-Chloroethyl)ether	6.809	93	66318	5.401	ng	95
9) Naphthalene	10.159	128	200654	4.889	ng	99
10) Hexachlorobutadiene	10.458	225	41506	4.637	ng	# 100
12) 2-Methylnaphthalene	11.787	142	137789	5.210	ng	99
16) Acenaphthylene	13.720	152	213808	5.543	ng	100
17) Acenaphthene	14.072	154	138183	5.059	ng	99
18) Fluorene	15.077	166	181240	5.193	ng	99
20) 4,6-Dinitro-2-methylph...	16.262	198	1440	5.145	ng	# 14
21) 4-Bromophenyl-phenylether	15.977	248	57947	5.240	ng	99
22) Hexachlorobenzene	16.076	284	71798	4.810	ng	97
23) Atrazine	16.262	200	48966	5.560	ng	93
24) Pentachlorophenol	16.436	266	32007	7.495	ng	96
25) Phenanthrene	16.808	178	275276	5.121	ng	100
26) Anthracene	16.908	178	259020	5.553	ng	99
28) Fluoranthene	18.848	202	315099	5.147	ng	99
30) Pyrene	19.215	202	320399	8.448	ng	100
33) Chrysene	21.035	228	254990	7.363	ng	98
36) Indeno(1,2,3-cd)pyrene	25.151	276	238548	5.014	ng	99
37) Benzo(b)fluoranthene	22.481	252	231677	5.658	ng	# 90
38) Benzo(k)fluoranthene	22.522	252	239725	5.139	ng	# 90
39) Benzo(a)pyrene	23.010	252	189742	5.338	ng	# 84
40) Dibenzo(a,h)anthracene	25.168	278	188016	5.164	ng	93
41) Benzo(g,h,i)perylene	25.773	276	207886	4.776	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
Data File : BN034573.D
Acq On : 14 Oct 2024 16:13
Operator : RC/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Oct 14 17:39:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 16:58:38 2024
Response via : Initial Calibration




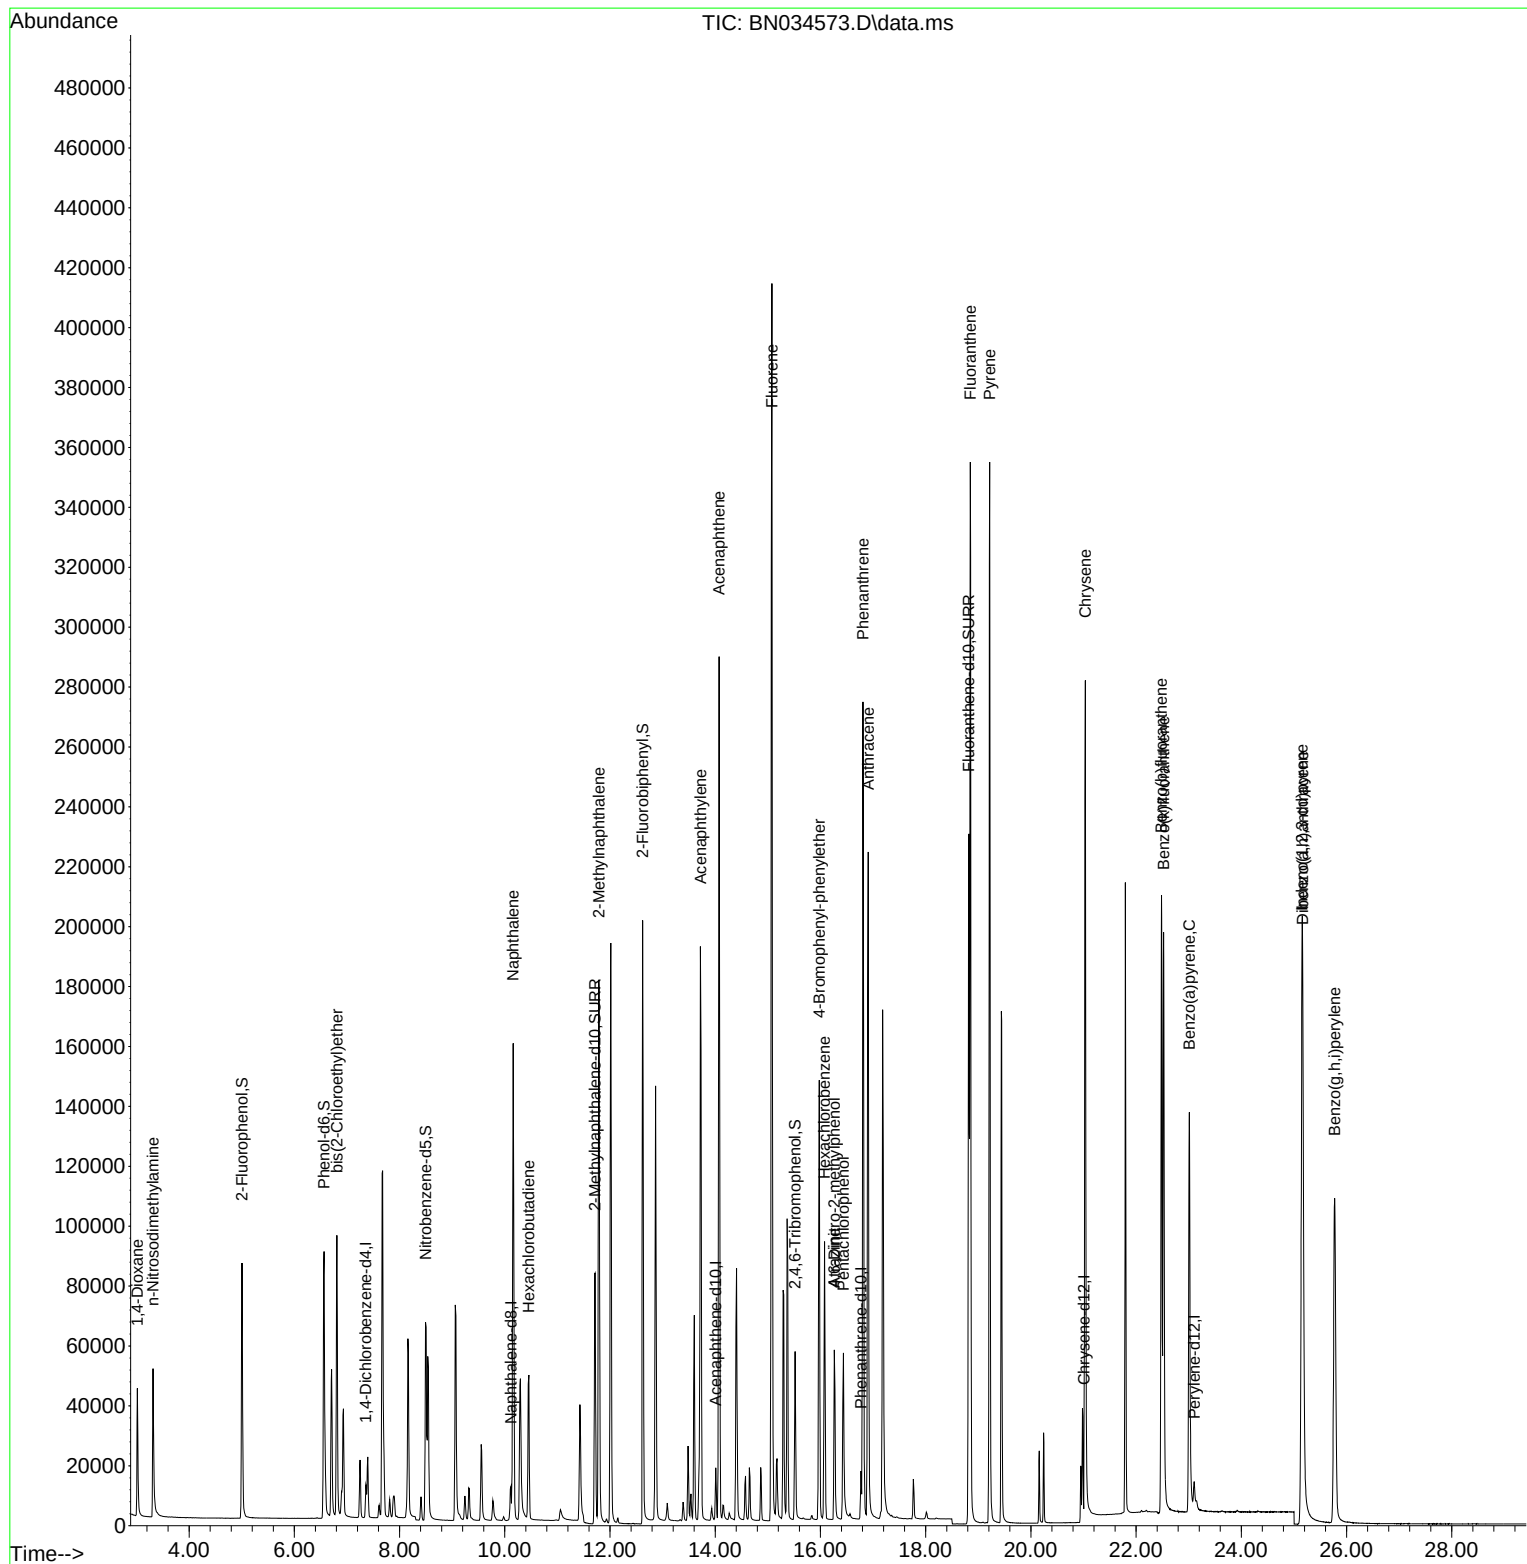




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.358 min Scan# 61
Delta R.T. -0.007 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 5343
Ion Ratio Lower Upper
152 100
150 158.8 122.0 183.0
115 63.0 48.3 72.5

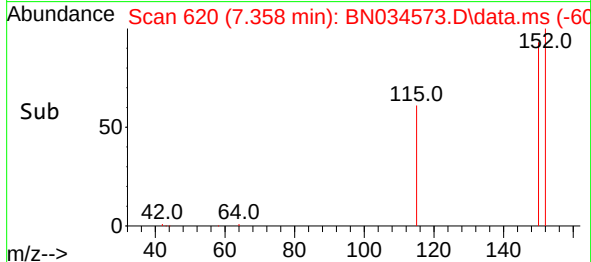

#2
1,4-Dioxane
Concen: 4.188 ng
RT: 3.018 min Scan# 19
Delta R.T. -0.007 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion: 88 Resp: 26990
Ion Ratio Lower Upper
88 100
43 28.2 22.8 34.2
58 73.0 56.4 84.6

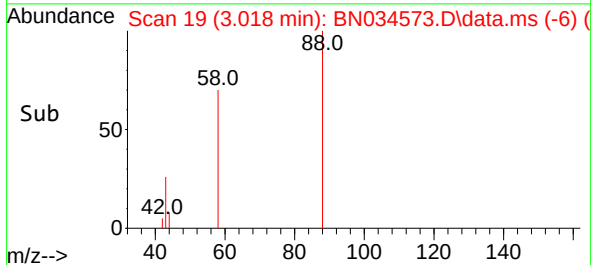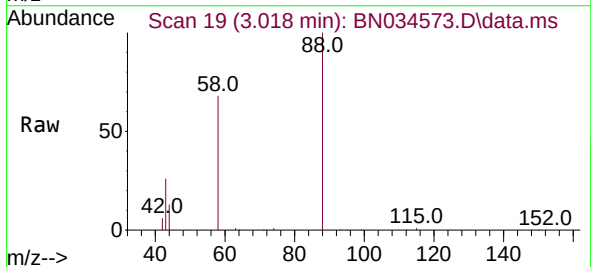

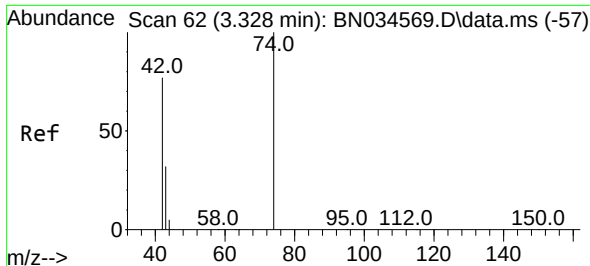

#3

n-Nitrosodimethylamine

Concen: 4.822 ng

RT: 3.314 min Scan# 60

Delta R.T. -0.015 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion: 42 Resp: 28302

Ion Ratio Lower Upper

42 100

74 127.4 99.0 148.6

44 6.1 6.6 9.8#

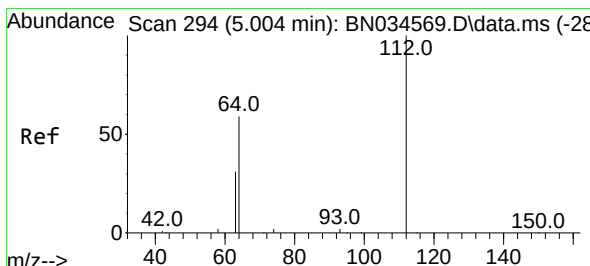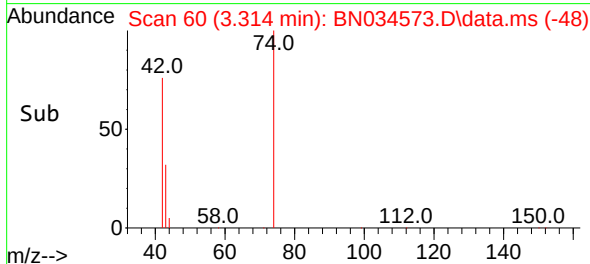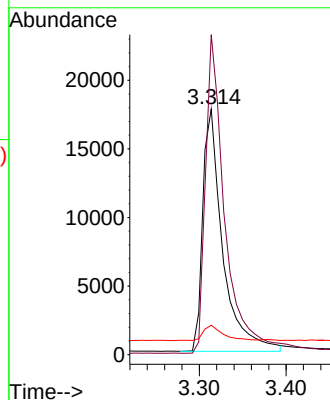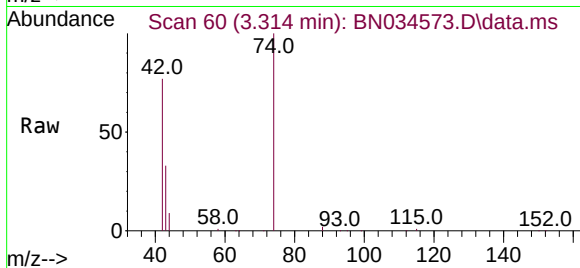

#4

2-Fluorophenol

Concen: 4.795 ng

RT: 5.004 min Scan# 294

Delta R.T. -0.000 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13




Tgt Ion: 112 Resp: 69455


Ion Ratio Lower Upper

112 100

64 55.3 44.6 66.8

63 29.0 23.8 35.6


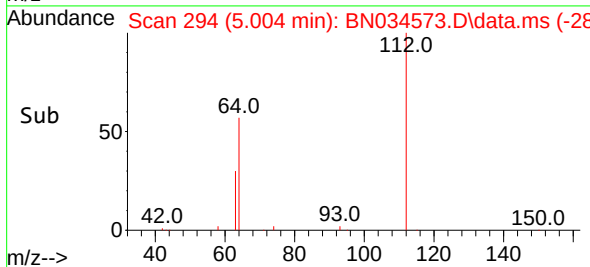
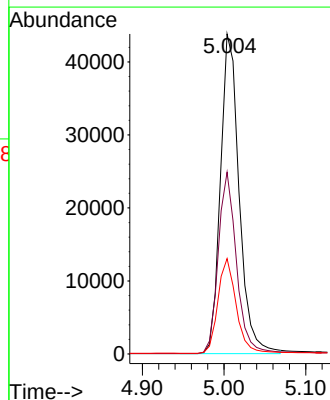
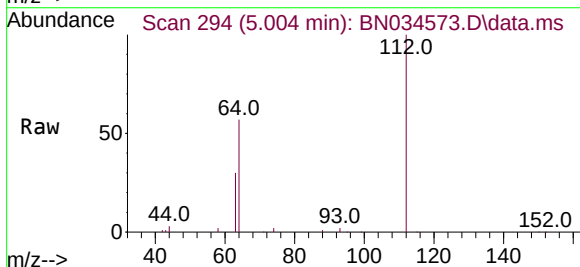




#5
Phenol-d6
Concen: 5.853 ng
RT: 6.564 min Scan# 510
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 87872
Ion Ratio Lower Upper
99 100
42 18.6 15.0 22.6
71 33.9 28.0 42.0

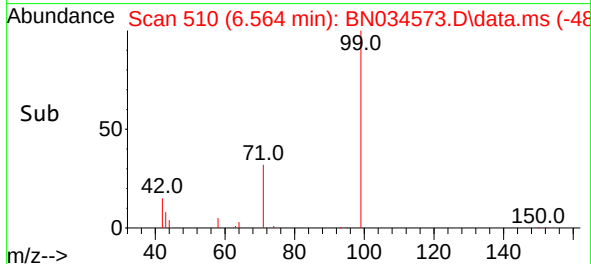

#6
bis(2-Chloroethyl)ether
Concen: 5.401 ng
RT: 6.809 min Scan# 544
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion: 93 Resp: 66318
Ion Ratio Lower Upper
93 100
63 75.3 64.6 96.8
95 33.2 27.9 41.9


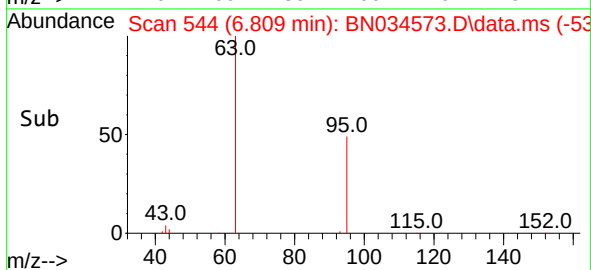

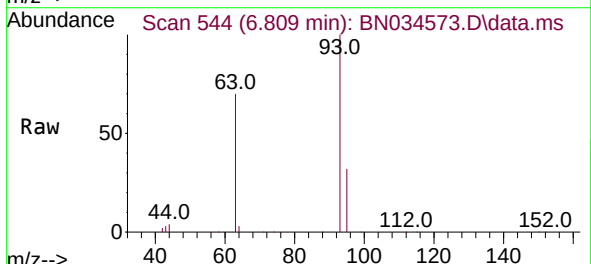




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.116 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	15688
Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.4	14.0
54	6.0	6.2	9.4#
68	4.6	4.6	6.8

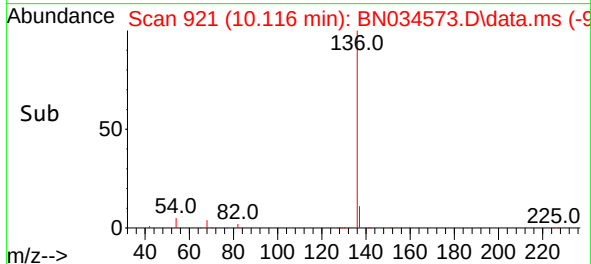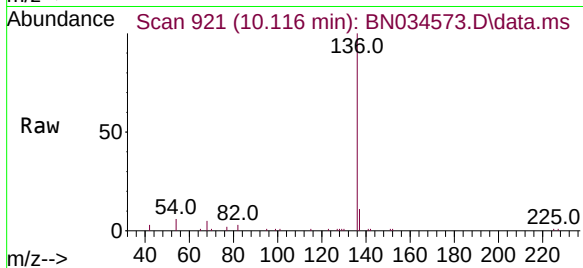

#8
Nitrobenzene-d5
Concen: 5.668 ng
RT: 8.493 min Scan# 769
Delta R.T. -0.021 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:	82	Resp:	57986
Ion	Ratio	Lower	Upper
82	100		
128	37.3	38.0	57.0#
54	55.6	40.6	60.8


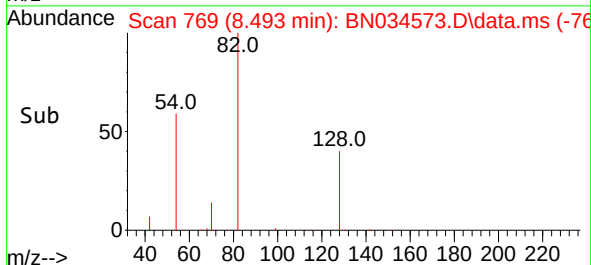
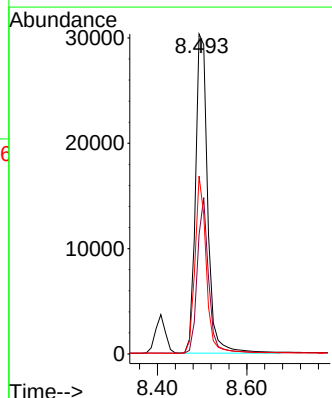
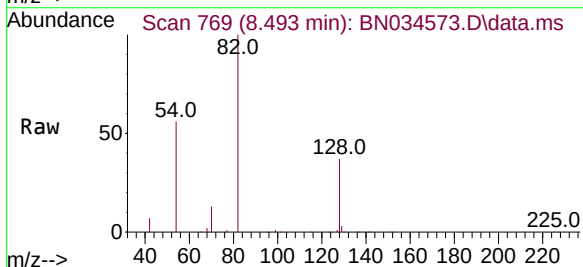


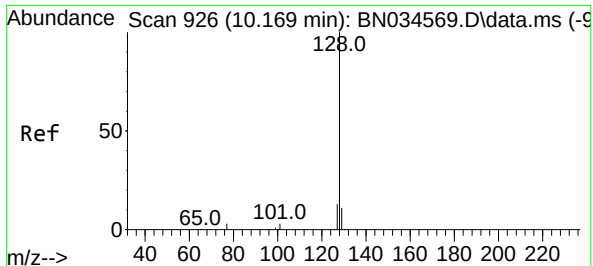

#9
Naphthalene
Concen: 4.889 ng
RT: 10.159 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 200654
Ion Ratio Lower Upper
128 100
129 10.9 9.3 13.9
127 13.1 10.8 16.2

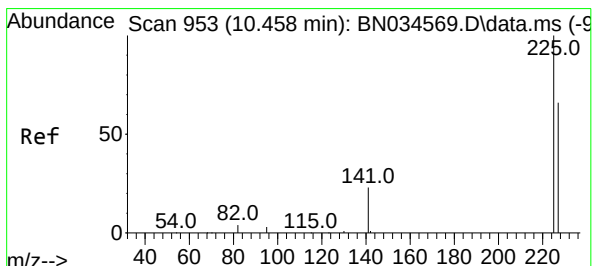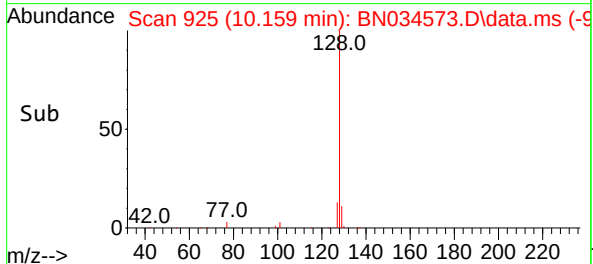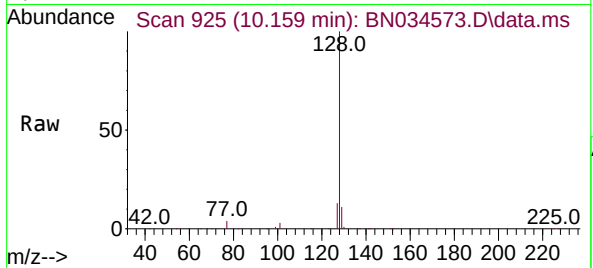

#10
Hexachlorobutadiene
Concen: 4.637 ng
RT: 10.458 min Scan# 953
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:225 Resp: 41506
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.0 51.4 77.0


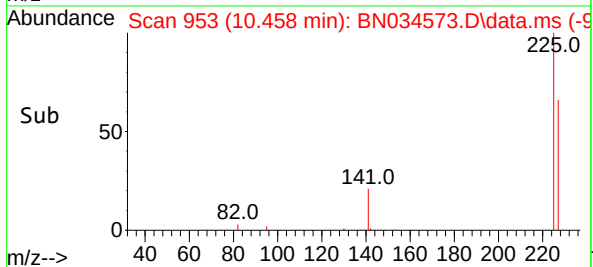

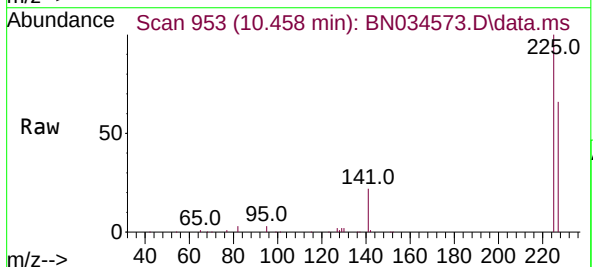




#11
2-Methylnaphthalene-d10
Concen: 5.189 ng
RT: 11.712 min Scan# 1106
Delta R.T. -0.011 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 122004
Ion Ratio Lower Upper
152 100
151 20.6 16.7 25.1

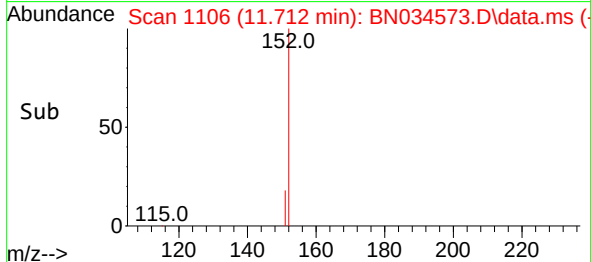

#12
2-Methylnaphthalene
Concen: 5.210 ng
RT: 11.787 min Scan# 1126
Delta R.T. -0.011 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:142 Resp: 137789
Ion Ratio Lower Upper
142 100
141 89.2 70.6 105.8
115 35.1 29.2 43.8


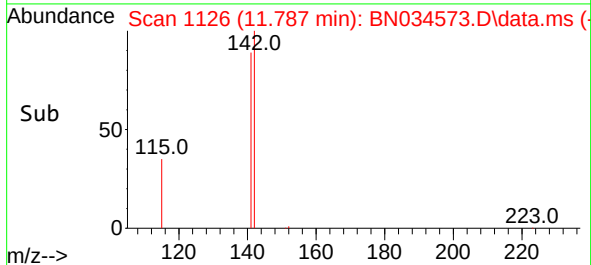

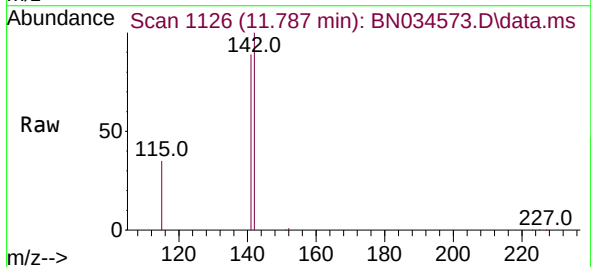




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.008 min Scan# 14
Delta R.T. -0.011 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 9488
Ion Ratio Lower Upper
164 100
162 103.8 79.7 119.5
160 48.7 37.9 56.9

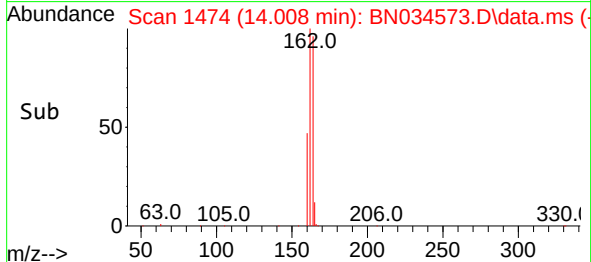

#14
2,4,6-Tribromophenol
Concen: 7.058 ng
RT: 15.517 min Scan# 1615
Delta R.T. -0.012 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:330 Resp: 29679
Ion Ratio Lower Upper
330 100
332 98.5 104.3 156.5#
141 34.0 29.4 44.0


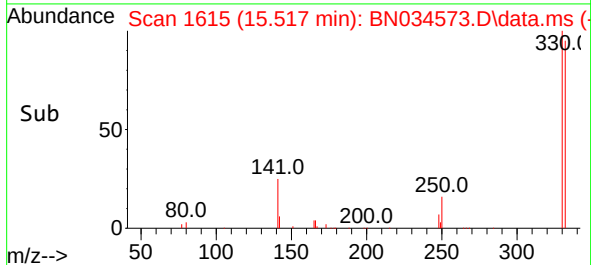

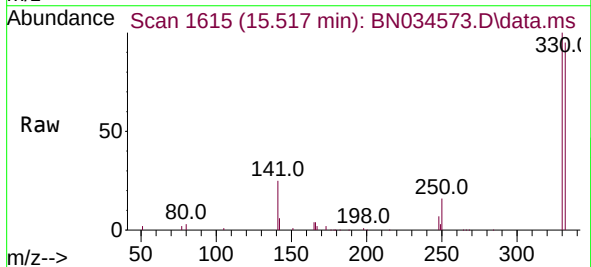


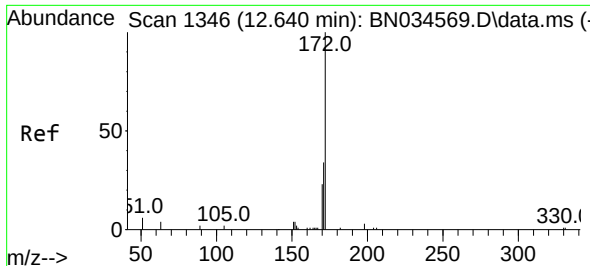

#15
2-Fluorobiphenyl
Concen: 4.810 ng
RT: 12.618 min Scan# 1344
Delta R.T. -0.021 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:172 Resp: 157382
Ion Ratio Lower Upper
172 100
171 35.6 27.1 40.7
170 23.6 18.5 27.7

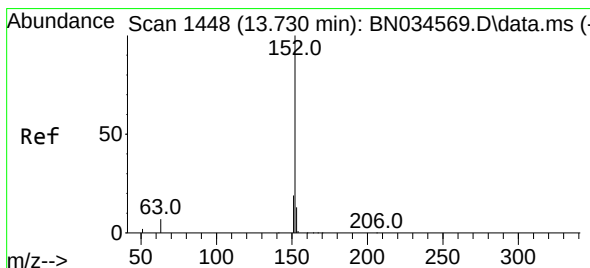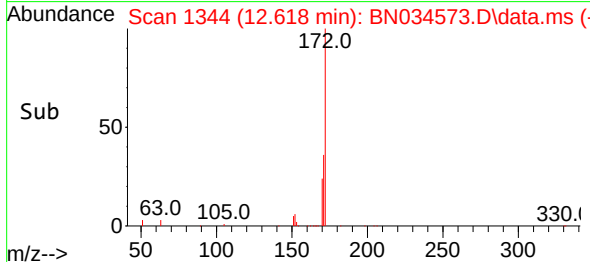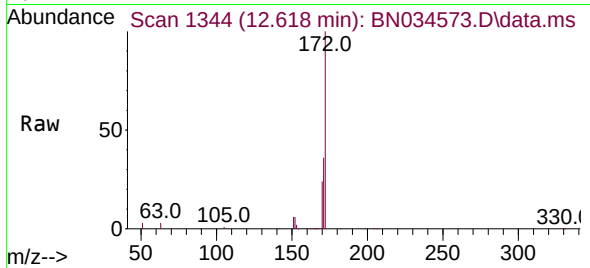

#16
Acenaphthylene
Concen: 5.543 ng
RT: 13.720 min Scan# 1447
Delta R.T. -0.011 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:152 Resp: 213808
Ion Ratio Lower Upper
152 100
151 19.5 15.5 23.3
153 13.0 10.4 15.6


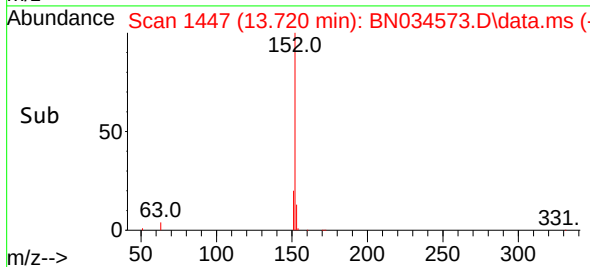

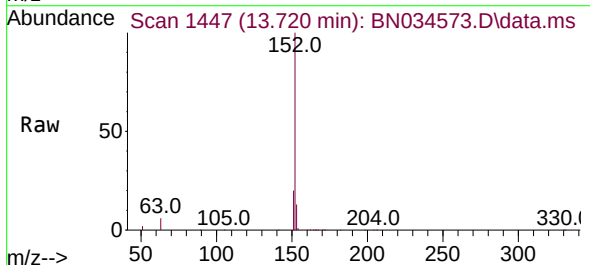




#17
Acenaphthene
Concen: 5.059 ng
RT: 14.072 min Scan# 1480
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 138183
Ion Ratio Lower Upper
154 100
153 113.8 91.5 137.3
152 55.1 45.8 68.8

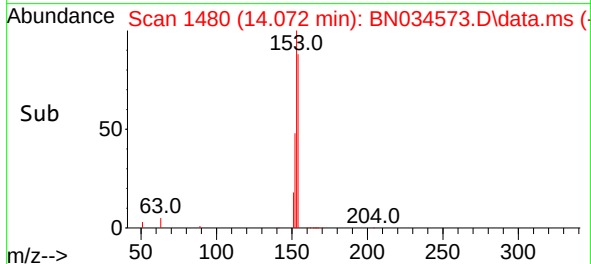

#18
Fluorene
Concen: 5.193 ng
RT: 15.077 min Scan# 1574
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:166 Resp: 181240
Ion Ratio Lower Upper
166 100
165 97.4 78.6 118.0
167 13.4 10.8 16.2


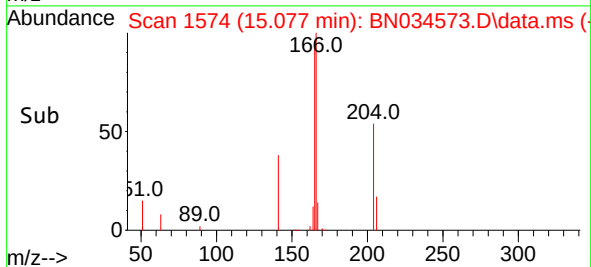

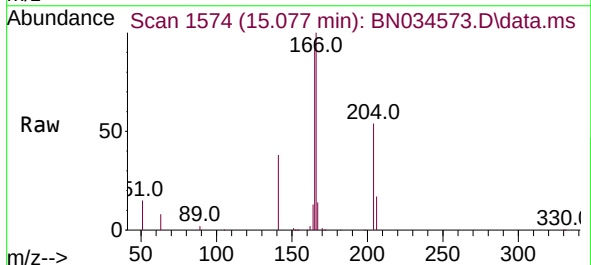


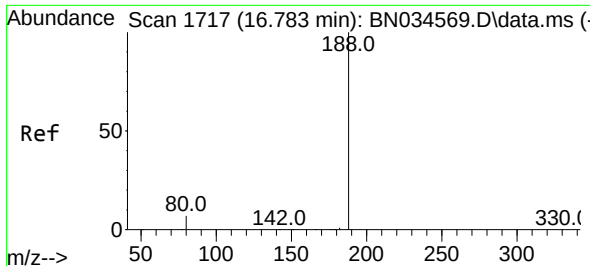

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.771 min Scan# 1716
Delta R.T. -0.012 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 20373
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.4 6.3 9.5

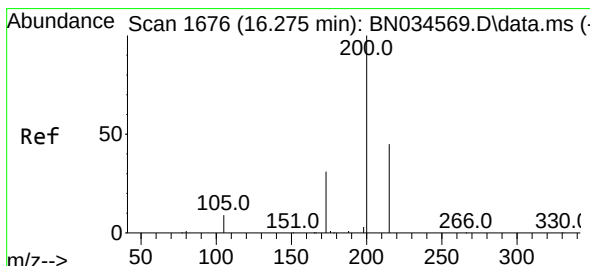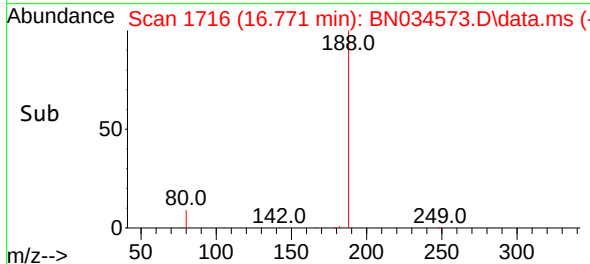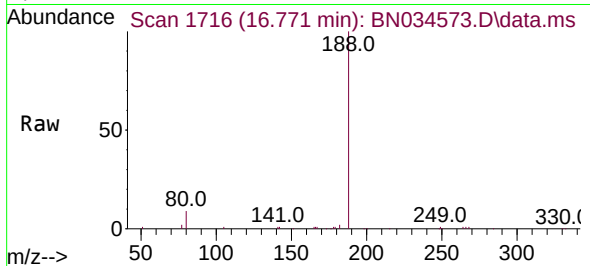

#20
4,6-Dinitro-2-methylphenol
Concen: 5.145 ng
RT: 16.262 min Scan# 1675
Delta R.T. -0.013 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:198 Resp: 1440
Ion Ratio Lower Upper
198 100
51 26.0 174.8 262.2#
105 287.5 167.9 251.9#


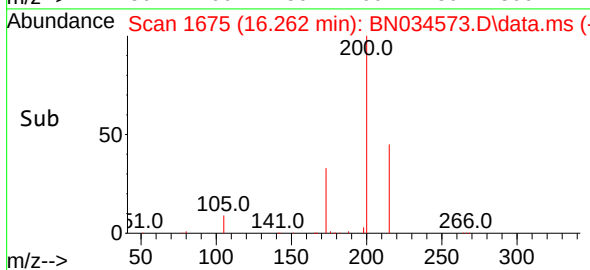

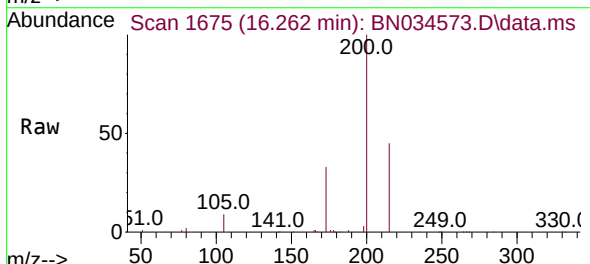


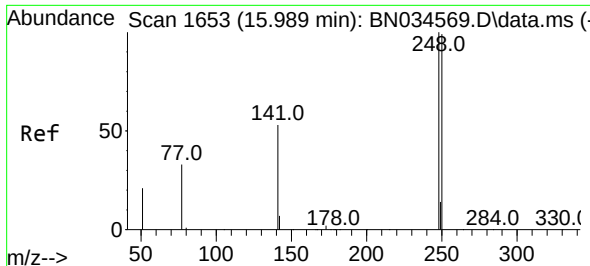

#21
4-Bromophenyl-phenylether
Concen: 5.240 ng
RT: 15.977 min Scan# 1652
Delta R.T. -0.012 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 57947
Ion Ratio Lower Upper
248 100
250 98.3 79.8 119.6
141 56.3 44.3 66.5

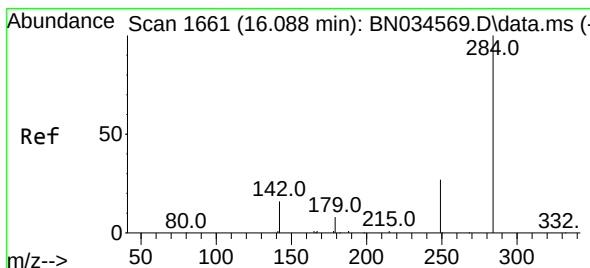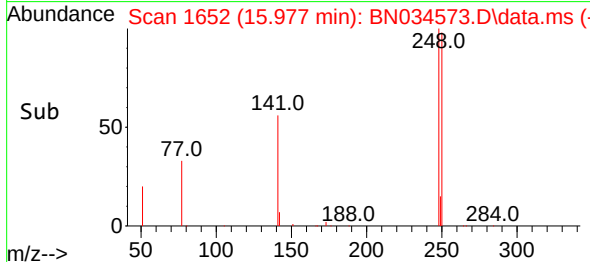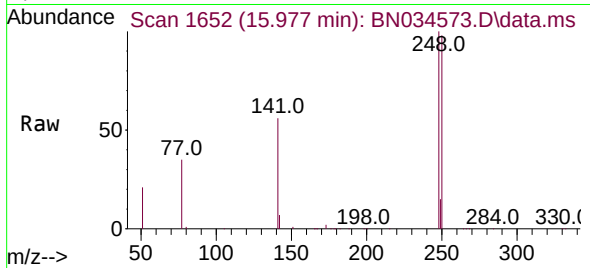

#22
Hexachlorobenzene
Concen: 4.810 ng
RT: 16.076 min Scan# 1660
Delta R.T. -0.012 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:284 Resp: 71798
Ion Ratio Lower Upper
284 100
142 33.2 28.4 42.6
249 30.4 25.0 37.4

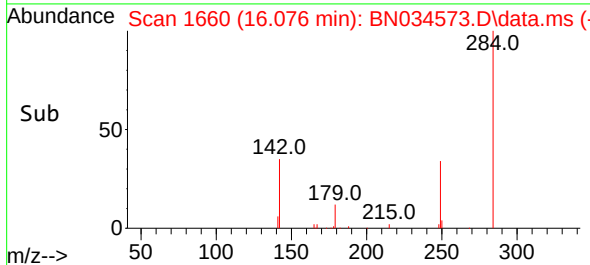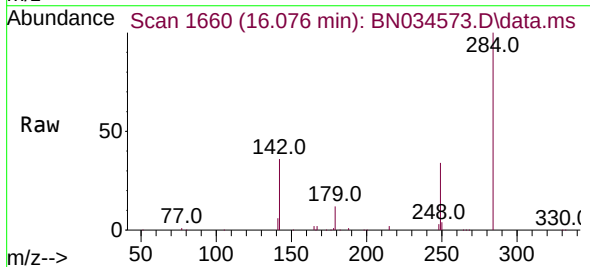

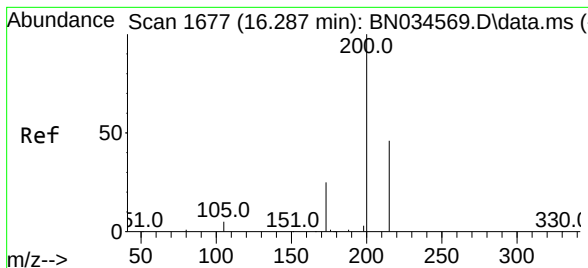

#23

Atrazine

Concen: 5.560 ng

RT: 16.262 min Scan# 1675

Delta R.T. -0.025 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:200 Resp: 48966

Ion Ratio Lower Upper

200 100

173 33.4 22.9 34.3

215 44.8 38.8 58.2

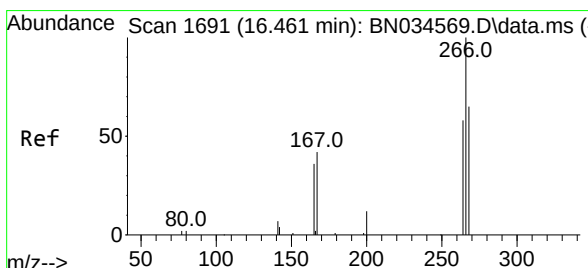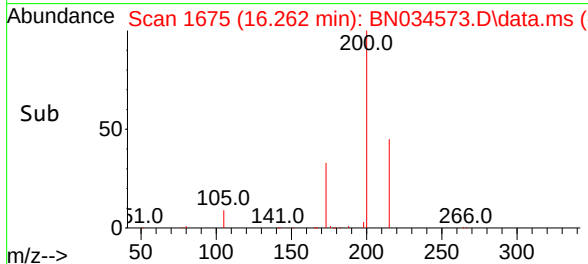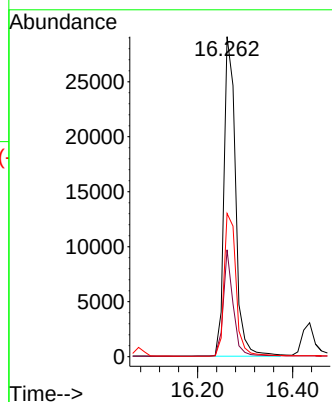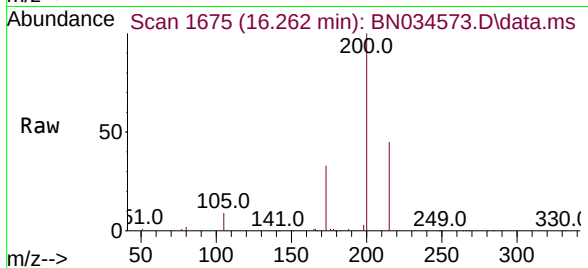

#24

Pentachlorophenol

Concen: 7.495 ng

RT: 16.436 min Scan# 1689

Delta R.T. -0.025 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13




Tgt Ion:266 Resp: 32007


Ion Ratio Lower Upper

266 100

264 62.7 46.6 69.8

268 63.6 52.0 78.0


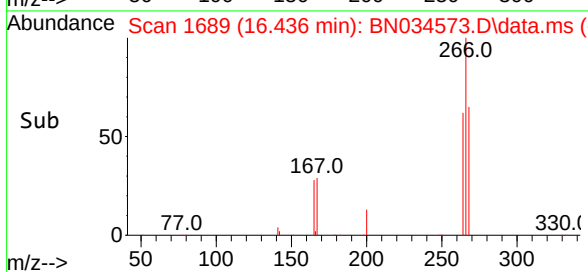
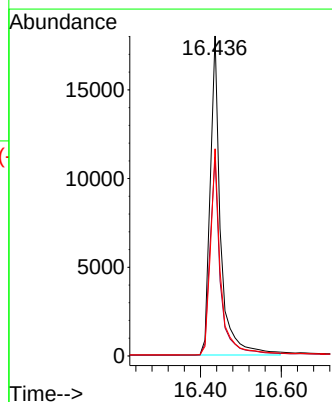
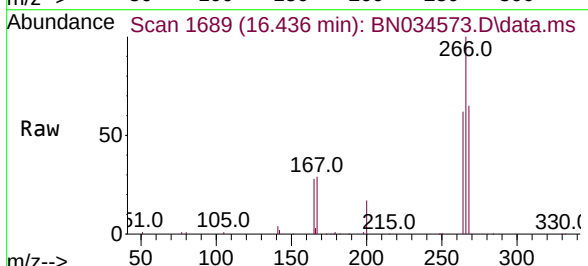


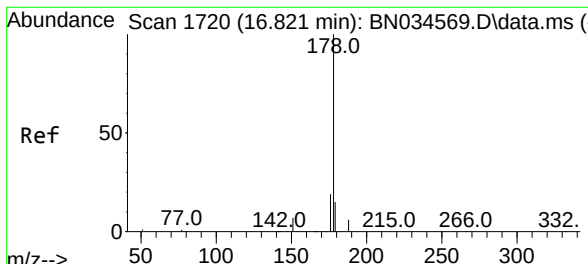

#25
Phenanthrene
Concen: 5.121 ng
RT: 16.808 min Scan# 1719
Delta R.T. -0.012 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 275276
Ion Ratio Lower Upper
178 100
176 19.0 15.3 22.9
179 15.2 12.2 18.4

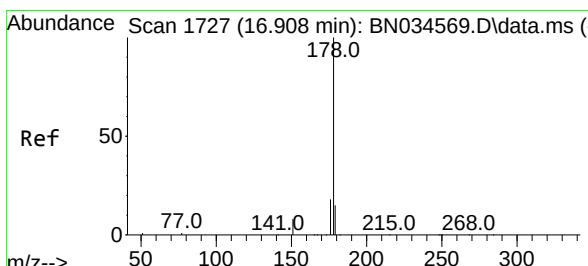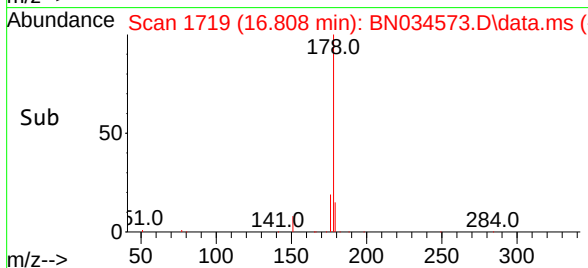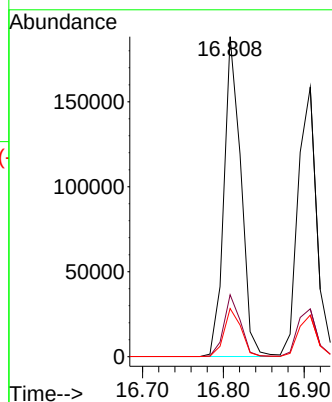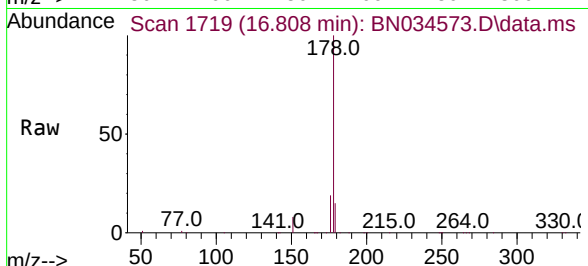

#26
Anthracene
Concen: 5.553 ng
RT: 16.908 min Scan# 1727
Delta R.T. -0.000 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:178 Resp: 259020
Ion Ratio Lower Upper
178 100
176 18.2 14.3 21.5
179 15.2 12.0 18.0


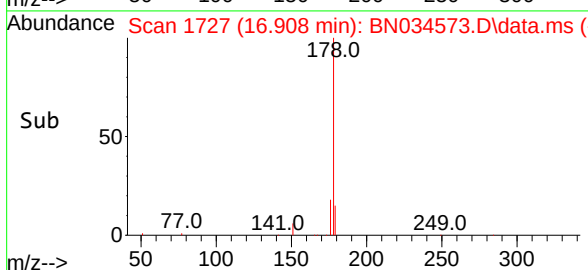

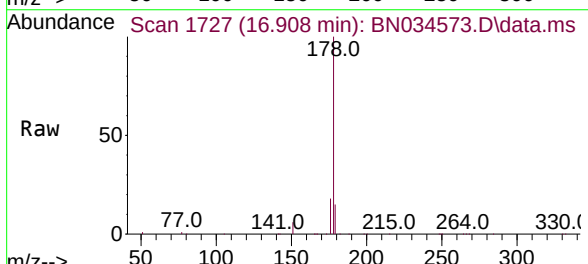


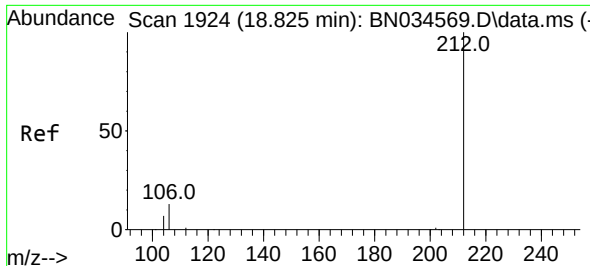

#27
Fluoranthene-d10
Concen: 5.178 ng
RT: 18.820 min Scan# 1923
Delta R.T. -0.005 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 256499
Ion Ratio Lower Upper
212 100
106 14.2 11.1 16.7
104 8.0 6.5 9.7

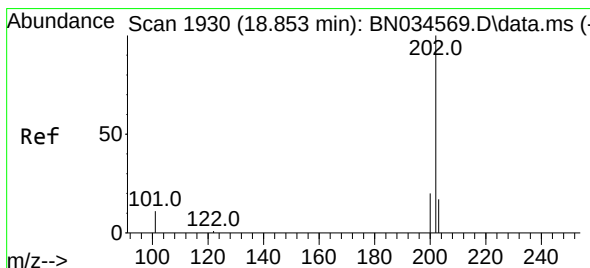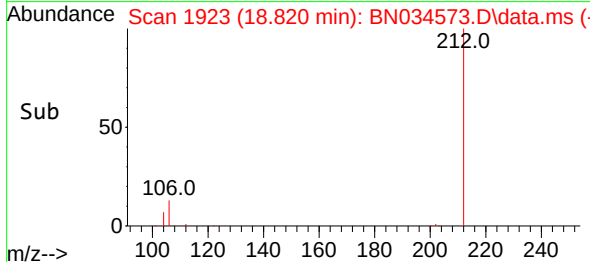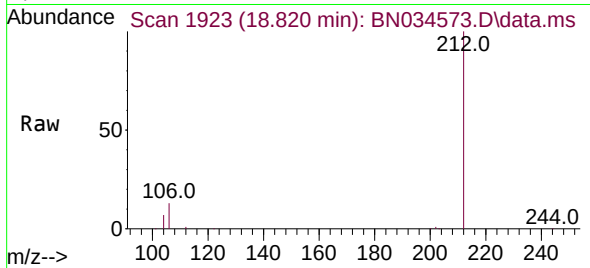

#28
Fluoranthene
Concen: 5.147 ng
RT: 18.848 min Scan# 1929
Delta R.T. -0.005 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:202 Resp: 315099
Ion Ratio Lower Upper
202 100
101 11.2 8.8 13.2
203 17.3 13.4 20.0

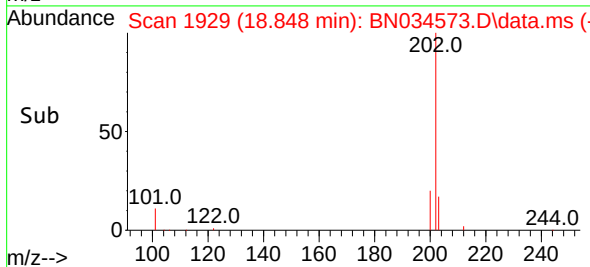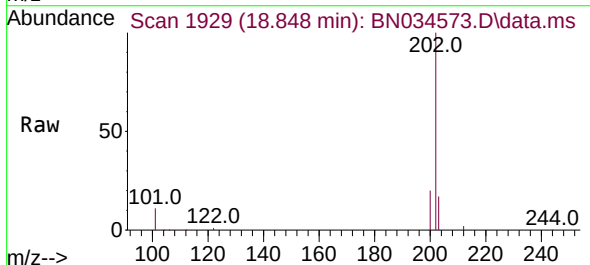

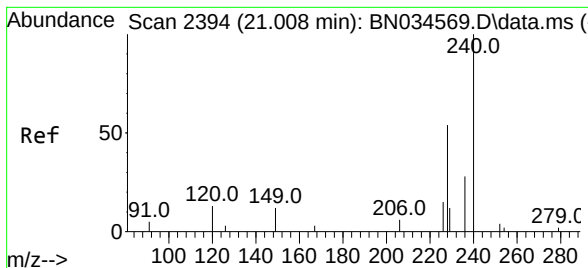

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.008 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:240 Resp: 3865

Ion Ratio Lower Upper

240 100

120 9.8 10.1 15.1#

236 27.8 22.6 34.0

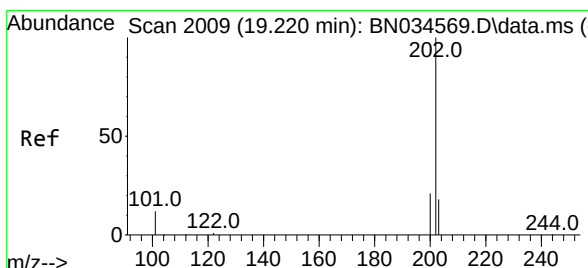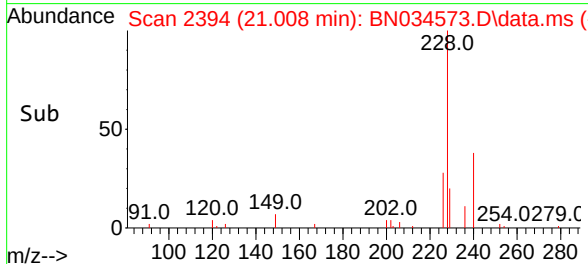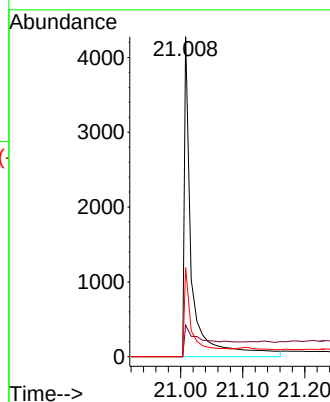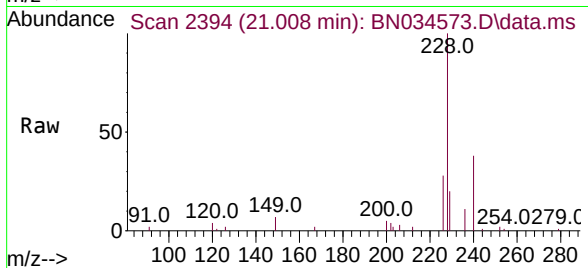

#30

Pyrene

Concen: 8.448 ng

RT: 19.215 min Scan# 2008

Delta R.T. -0.005 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13




Tgt Ion:202 Resp: 320399


Ion Ratio Lower Upper

202 100

200 20.7 16.6 24.8

203 17.9 14.3 21.5

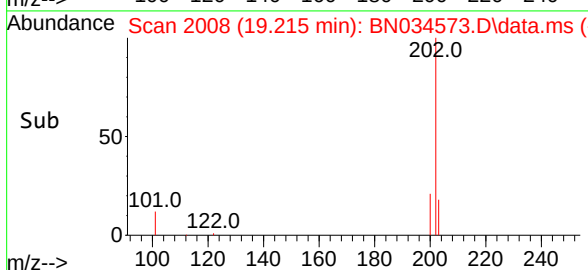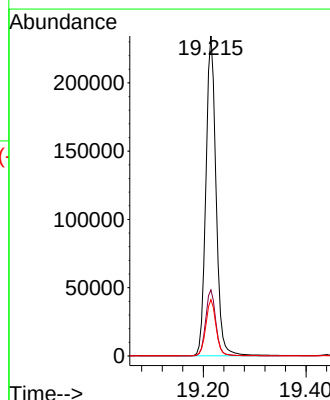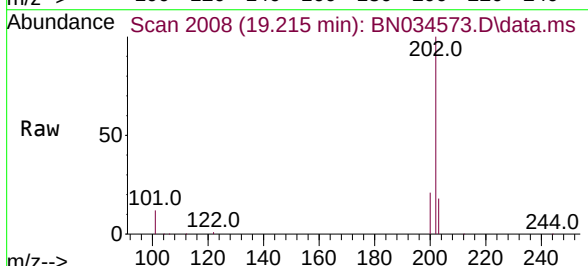


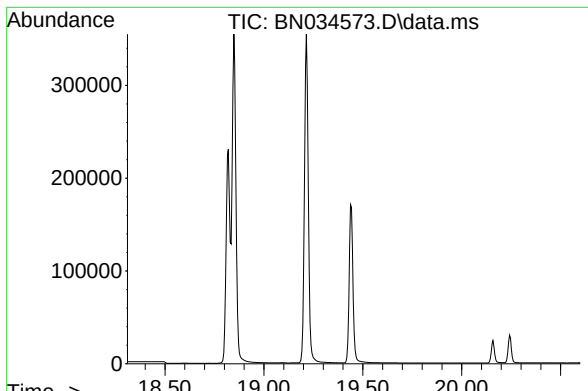


#31
 Terphenyl-d14
 Concen: 0.000 ng
 Expected RT: 19.45 min
 Lab File: BN034573.D
 Acq: 14 Oct 2024 16:13

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion: 244




Sig	Exp Ratio
244	100
212	9.6
122	15.8

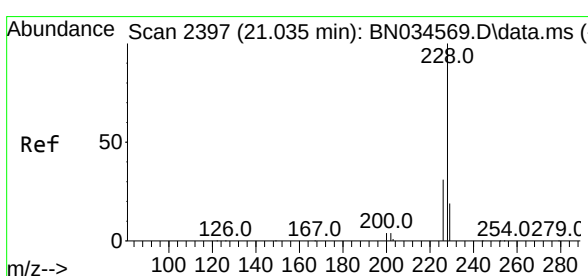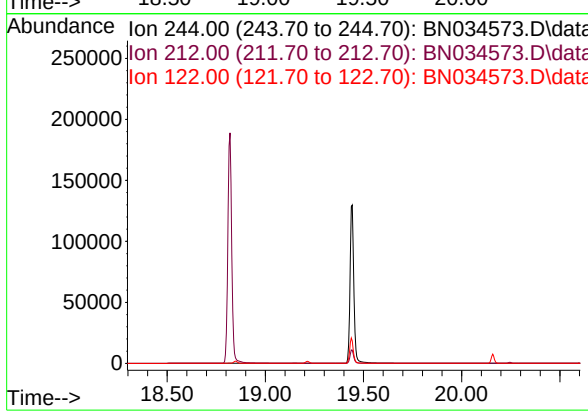


#33
 Chrysene
 Concen: 7.363 ng
 RT: 21.035 min Scan# 2397
 Delta R.T. -0.000 min
 Lab File: BN034573.D
 Acq: 14 Oct 2024 16:13

Tgt Ion: 228 Resp: 254990


Ion	Ratio	Lower	Upper
228	100		
226	29.1	24.4	36.6
229	19.8	15.8	23.6

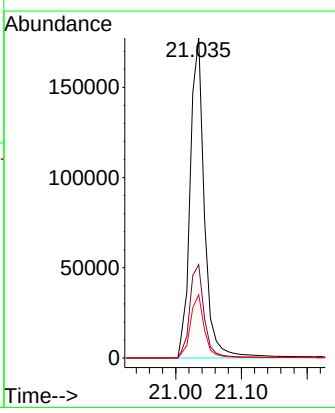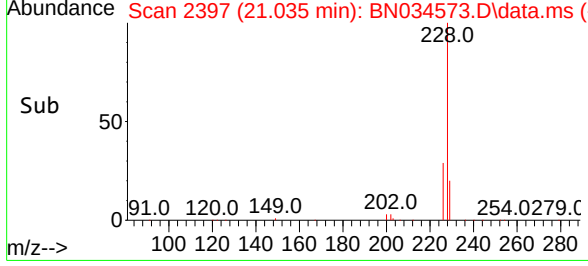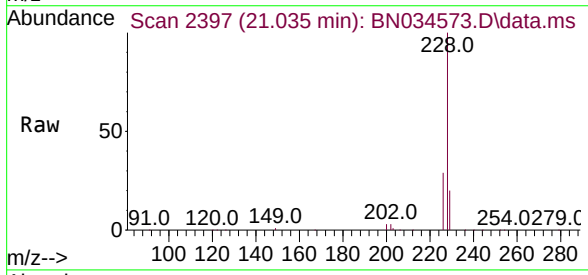






#35
Perylene-d12
Concen: 0.400 ng
RT: 23.104 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



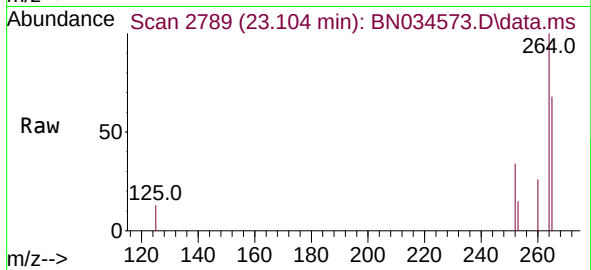



Tgt Ion:264 Resp: 12249
Ion Ratio Lower Upper
264 100
260 25.8 20.9 31.3
265 68.3 61.6 92.4

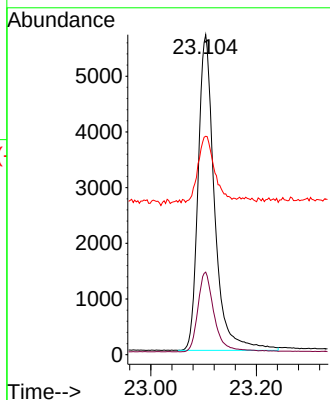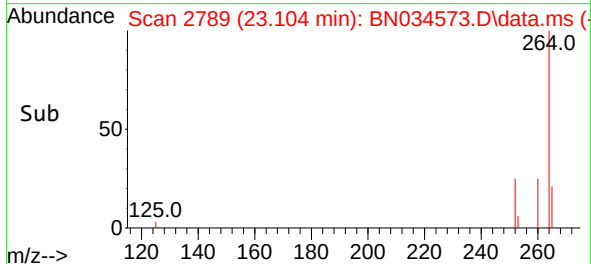

#36
Indeno(1,2,3-cd)pyrene
Concen: 5.014 ng
RT: 25.151 min Scan# 3489
Delta R.T. -0.015 min
Lab File: BN034573.D
Acq: 14 Oct 2024 16:13

Tgt Ion:276 Resp: 238548
Ion Ratio Lower Upper
276 100
138 28.0 22.0 33.0
277 25.0 20.1 30.1

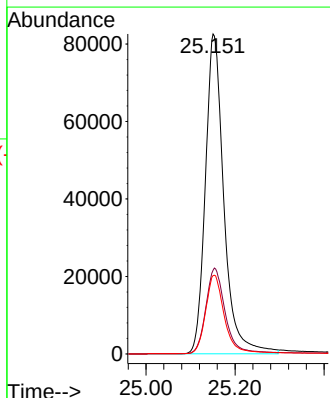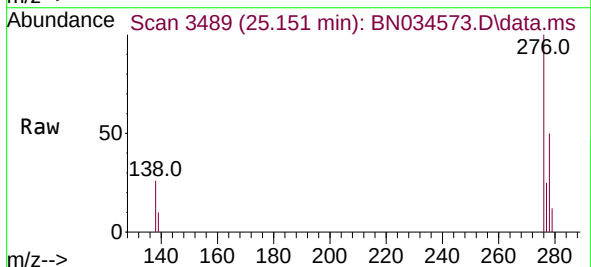



#37

Benzo(b)fluoranthene

Concen: 5.658 ng

RT: 22.481 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:252 Resp: 231677

Ion Ratio Lower Upper

252 100

253 22.0 21.3 31.9

125 11.3 12.7 19.1#

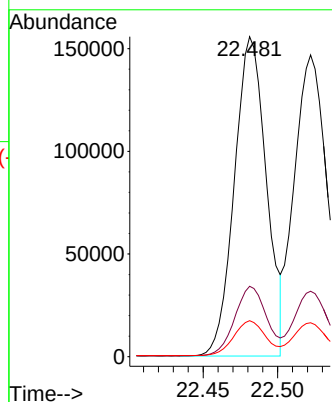

#38

Benzo(k)fluoranthene

Concen: 5.139 ng

RT: 22.522 min Scan# 2590

Delta R.T. -0.009 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13




Tgt Ion:252 Resp: 239725


Ion Ratio Lower Upper

252 100

253 21.7 21.0 31.6

125 11.2 13.3 19.9#

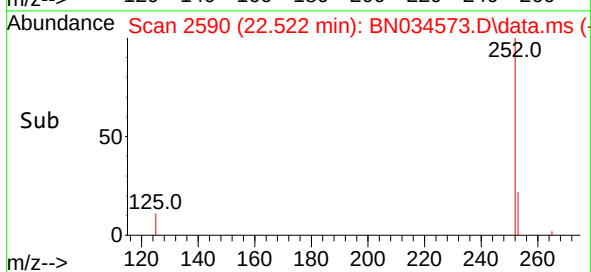



#39

Benzo(a)pyrene

Concen: 5.338 ng

RT: 23.010 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN034573.D


Acq: 14 Oct 2024 16:13

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0






Tgt Ion:252 Resp: 189742

Ion	Ratio	Lower	Upper
-----	-------	-------	-------

252	100		
-----	-----	--	--

253	22.1	23.8	35.8#
-----	------	------	-------

125	12.6	17.2	25.8#
-----	------	------	-------

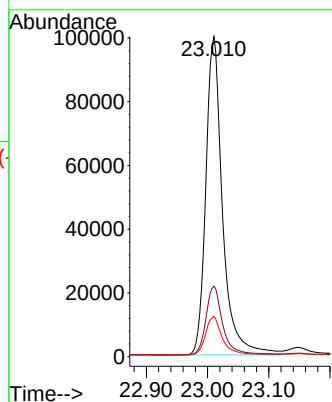

#40

Dibenzo(a,h)anthracene

Concen: 5.164 ng

RT: 25.168 min Scan# 3495

Delta R.T. -0.012 min

Lab File: BN034573.D

Acq: 14 Oct 2024 16:13




Tgt Ion:278 Resp: 188016


Ion	Ratio	Lower	Upper
-----	-------	-------	-------

278	100		
-----	-----	--	--

139	18.6	16.0	24.0
-----	------	------	------

279	23.7	23.4	35.0
-----	------	------	------

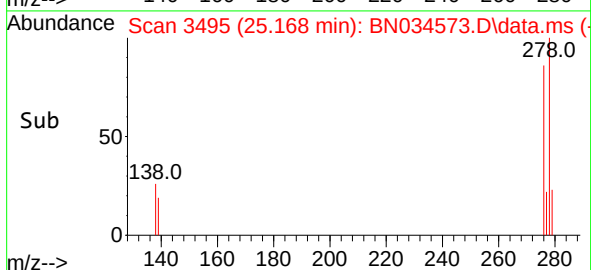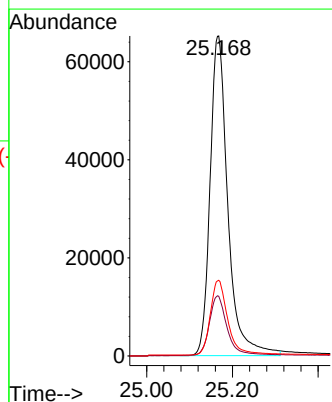

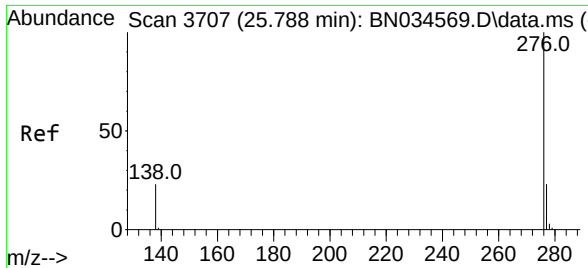

#41
 Benzo(g,h,i)perylene
 Concen: 4.776 ng
 RT: 25.773 min Scan# 31
 Delta R.T. -0.015 min
 Lab File: BN034573.D
 Acq: 14 Oct 2024 16:13

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:	276	Resp:	207886
Ion	Ratio	Lower	Upper
276	100		
277	23.7	19.8	29.8
138	24.1	19.2	28.8

