


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
Data File : BN034565.D
Acq On : 14 Oct 2024 10:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 14 17:52:02 2024

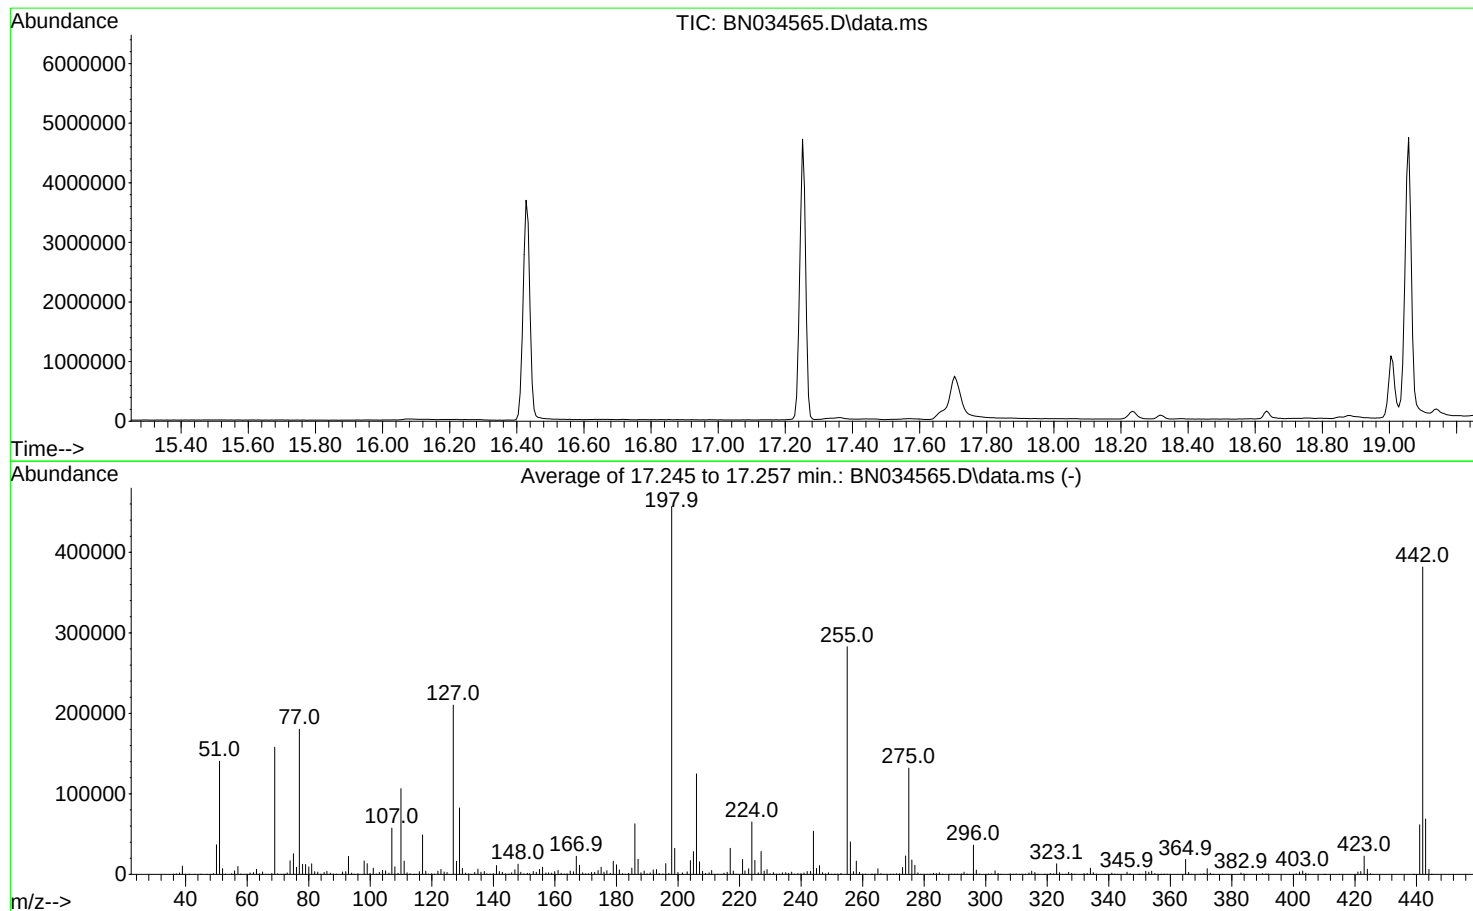

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.7	140433	PASS
68	69	0.00	2	0.6	989	PASS
69	198	0.00	100	34.6	158064	PASS
70	69	0.00	2	0.5	820	PASS
127	198	10	80	46.0	210357	PASS
197	198	0.00	2	0.3	1306	PASS
198	198	100	100	100.0	456917	PASS
199	198	5	9	7.1	32467	PASS
275	198	10	60	28.9	132061	PASS
365	198	1	100	4.1	18555	PASS
441	198	0.01	100	13.5	61563	PASS
442	442	50	100	100.0	381867	PASS
443	442	15	24	18.0	68723	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/14/2024	BNA_N	<u>BN034565.D</u>
Compound Name	Response	Retention Time
DDT	1446193	20.403
DDD	33527	19.863
DDE	1043	19.351
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34570	1480763	2.33

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
Data File : BN034565.D
Acq On : 14 Oct 2024 10:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 14 11:36:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 02:51:59 2024
Response via : Initial Calibration

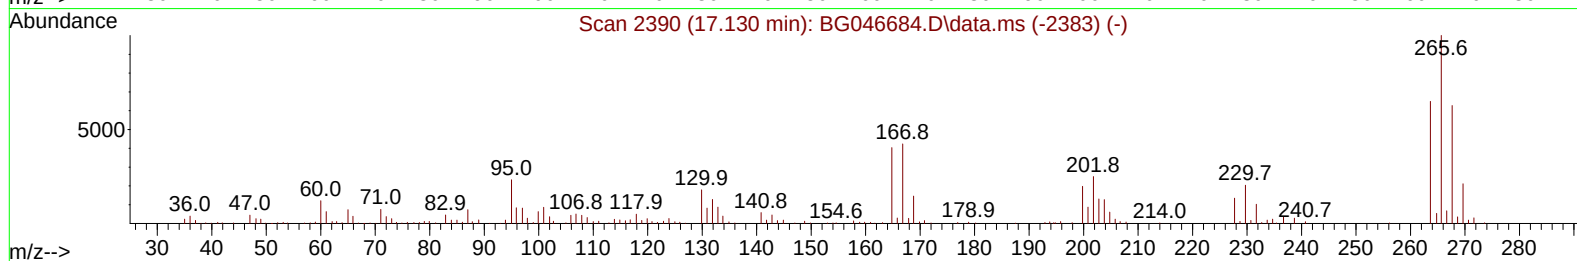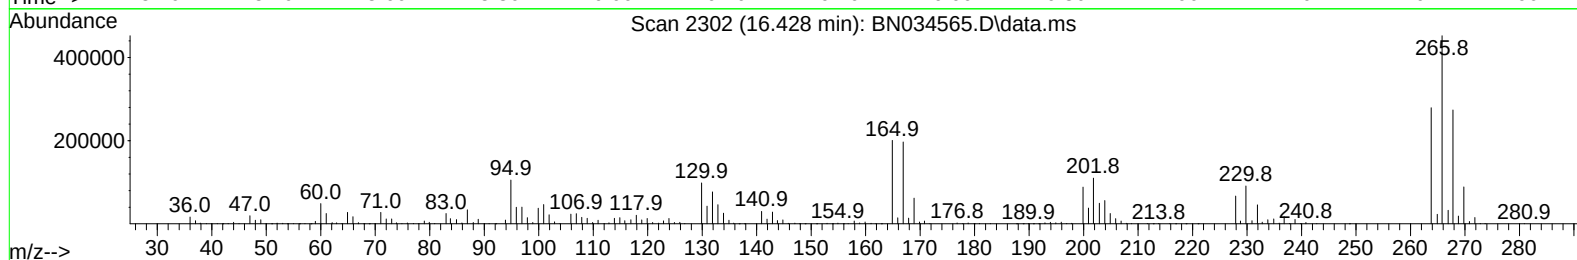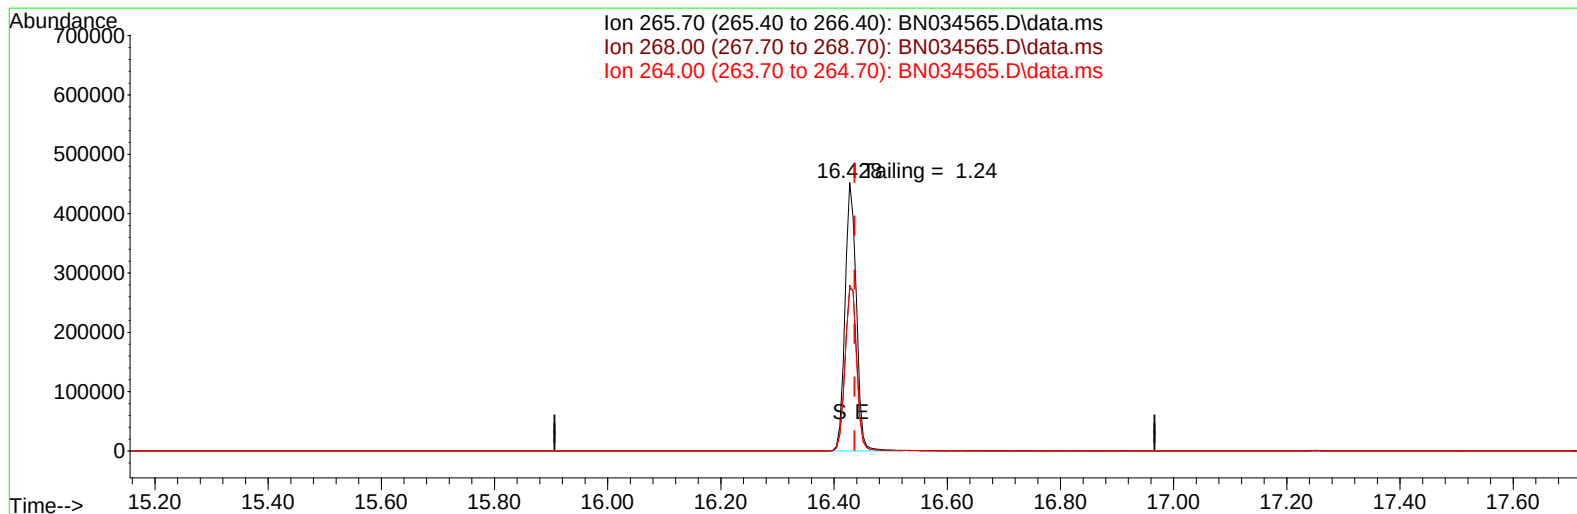

TIC: BN034565.D\data.ms

(70) Pentachlorophenol (C)

16.428min (-0.008) 27287.04 ng




response 628078

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.55
264.00	61.60	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101424\
Data File : BN034565.D
Acq On : 14 Oct 2024 10:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 14 11:36:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 02:51:59 2024
Response via : Initial Calibration

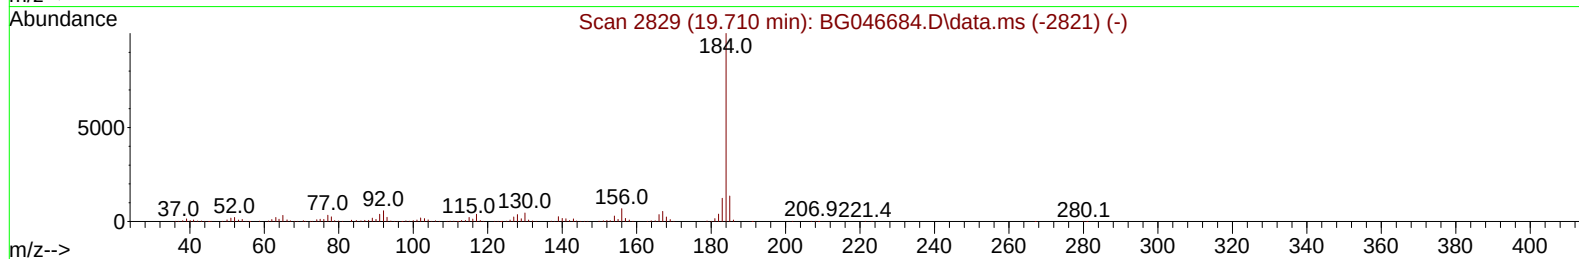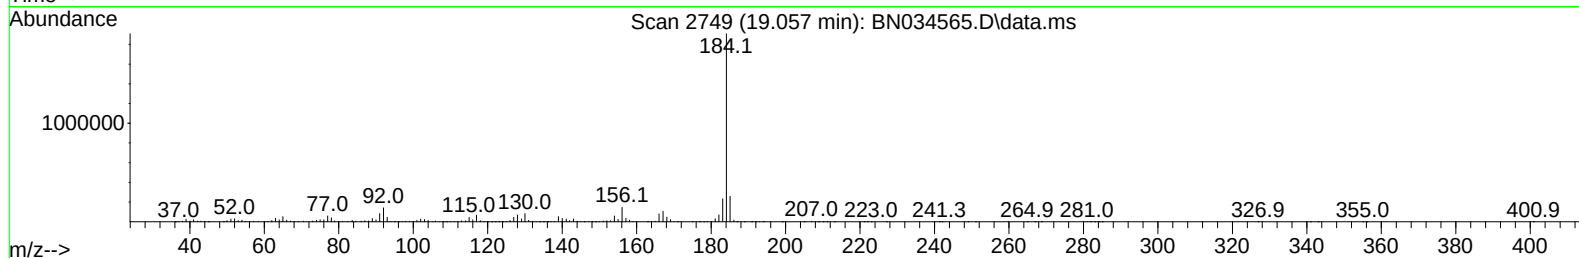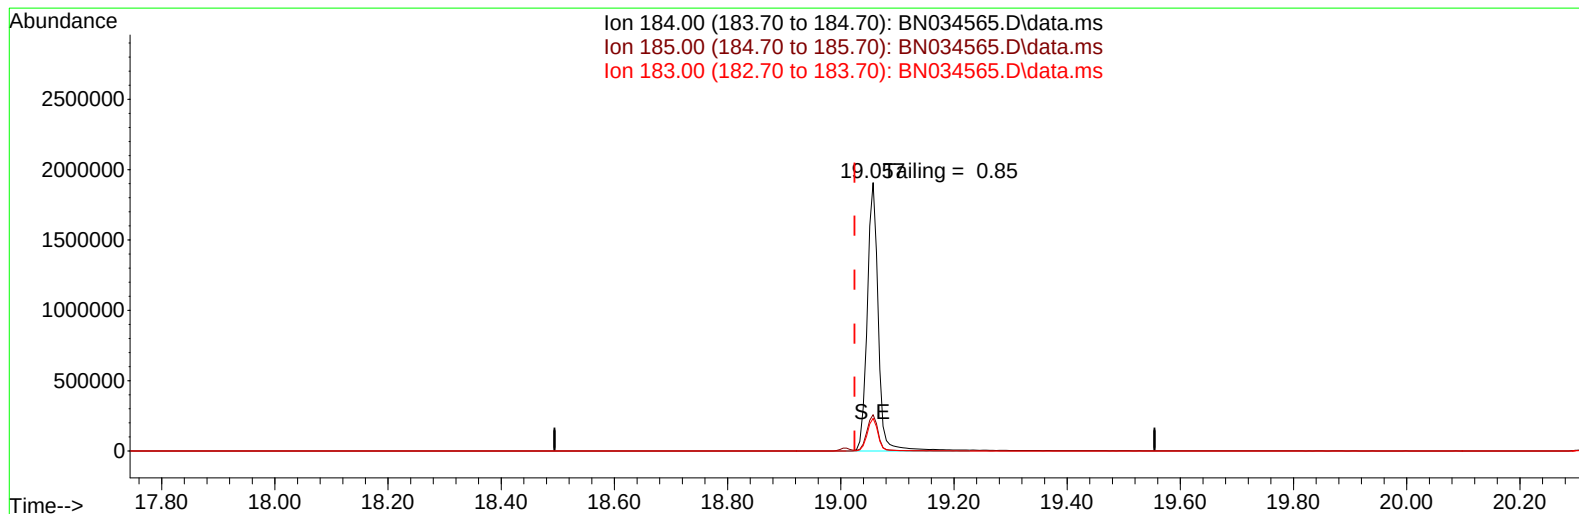

TIC: BN034565.D\data.ms

(77) Benzidine

19.057min (+ 0.033) 0.00 ng

response 2580788

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.57
183.00	13.20	12.18
0.00	0.00	0.00