


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN101424\  
Data File : BN034579.D  
Acq On : 14 Oct 2024 19:51  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN101424.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Mon Oct 14 17:52:02 2024

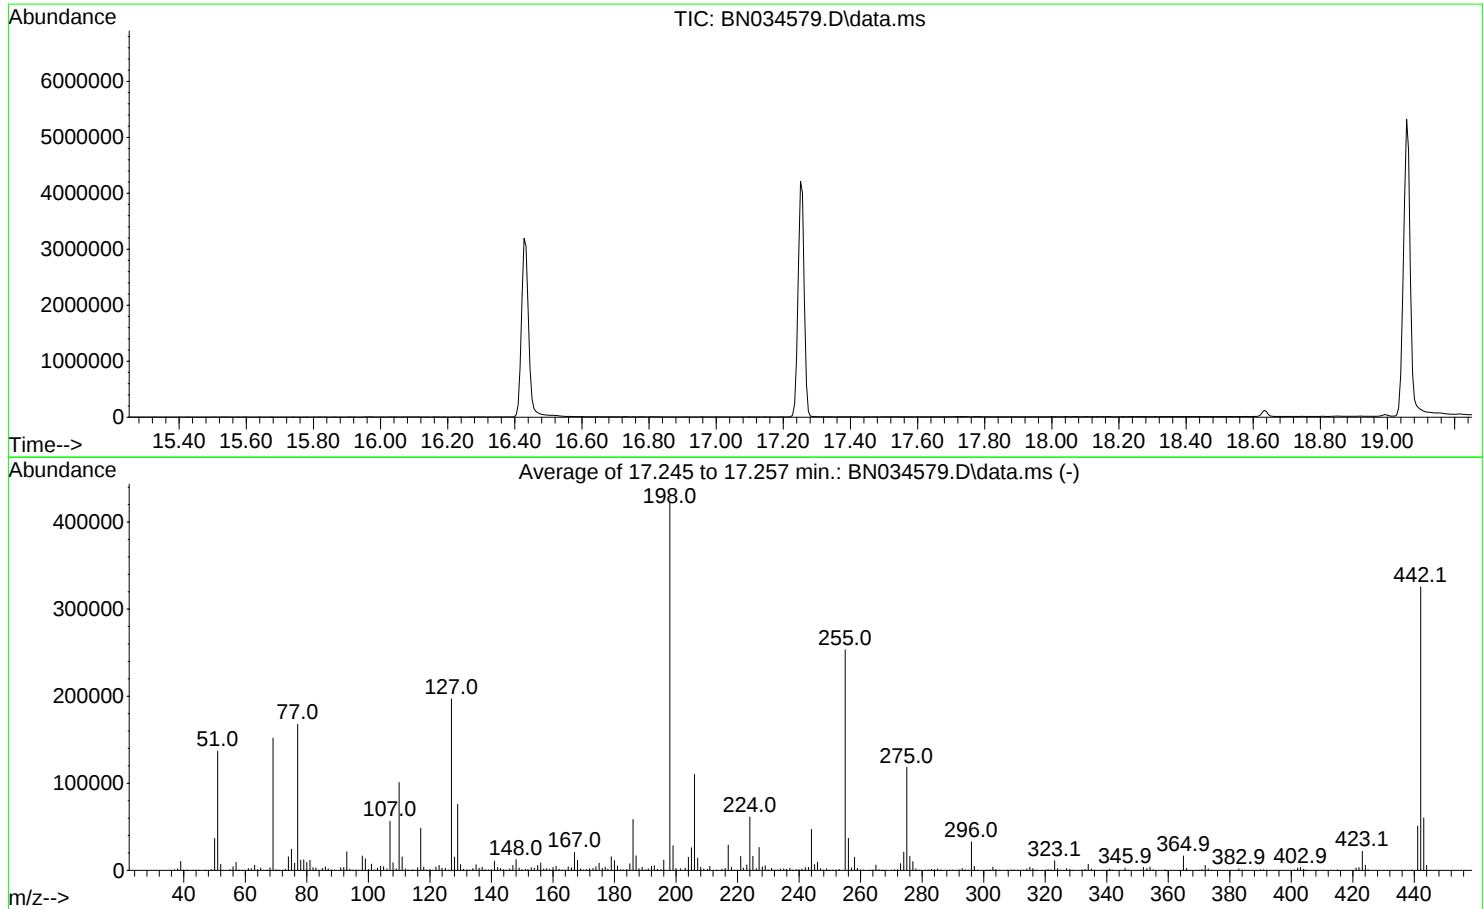

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2434

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 32.4         | 136928     | PASS                |
| 68             | 69              | 0.00            | 2               | 2.0          | 2970       | PASS                |
| 69             | 198             | 0.00            | 100             | 36.0         | 151952     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 844        | PASS                |
| 127            | 198             | 10              | 80              | 46.6         | 196949     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 422485     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 28237      | PASS                |
| 275            | 198             | 10              | 60              | 28.0         | 118312     | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 16638      | PASS                |
| 441            | 198             | 0.01            | 100             | 12.0         | 50904      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 325376     | PASS                |
| 443            | 442             | 15              | 24              | 18.5         | 60315      | PASS                |

### DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 10/14/2024    | BNA_N            | <u>BN034579.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1564746          | 20.304             |
| DDD           | 40693            | 19.861             |
| DDE           | 1091             | 19.345             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 41784         | 1606530          | 2.60               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN101424\  
Data File : BN034579.D  
Acq On : 14 Oct 2024 19:51  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Oct 15 00:48:20 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 15 00:48:16 2024  
Response via : Initial Calibration

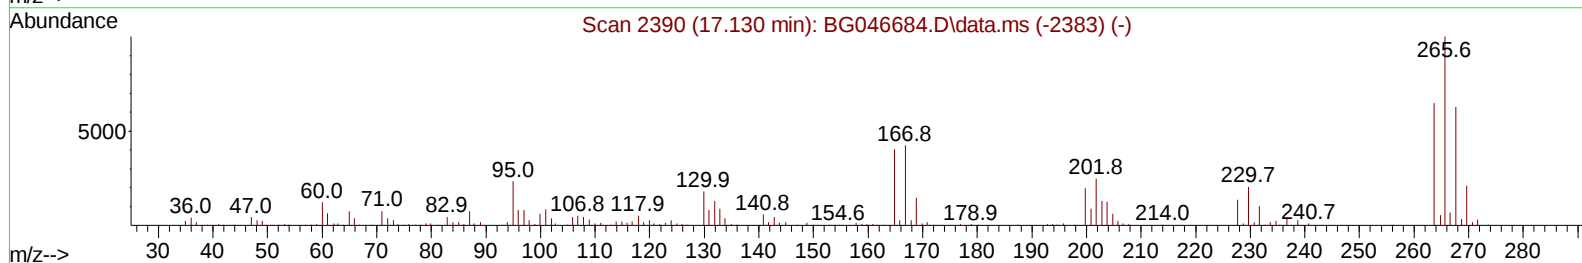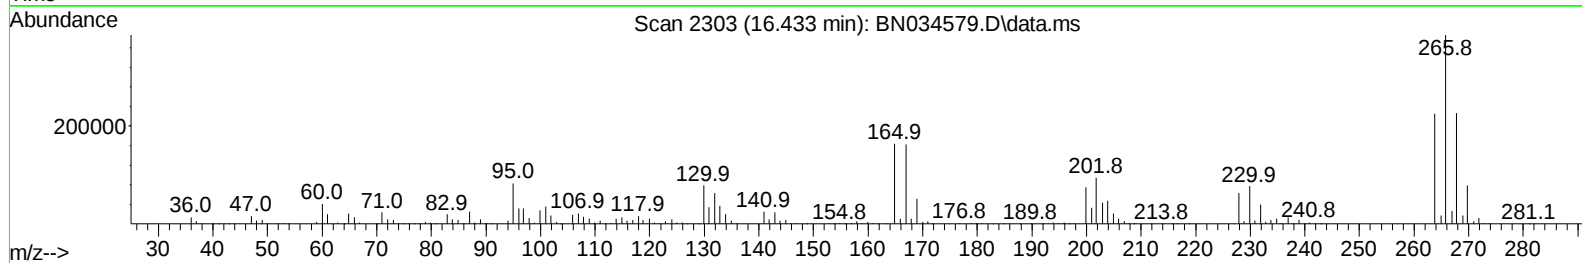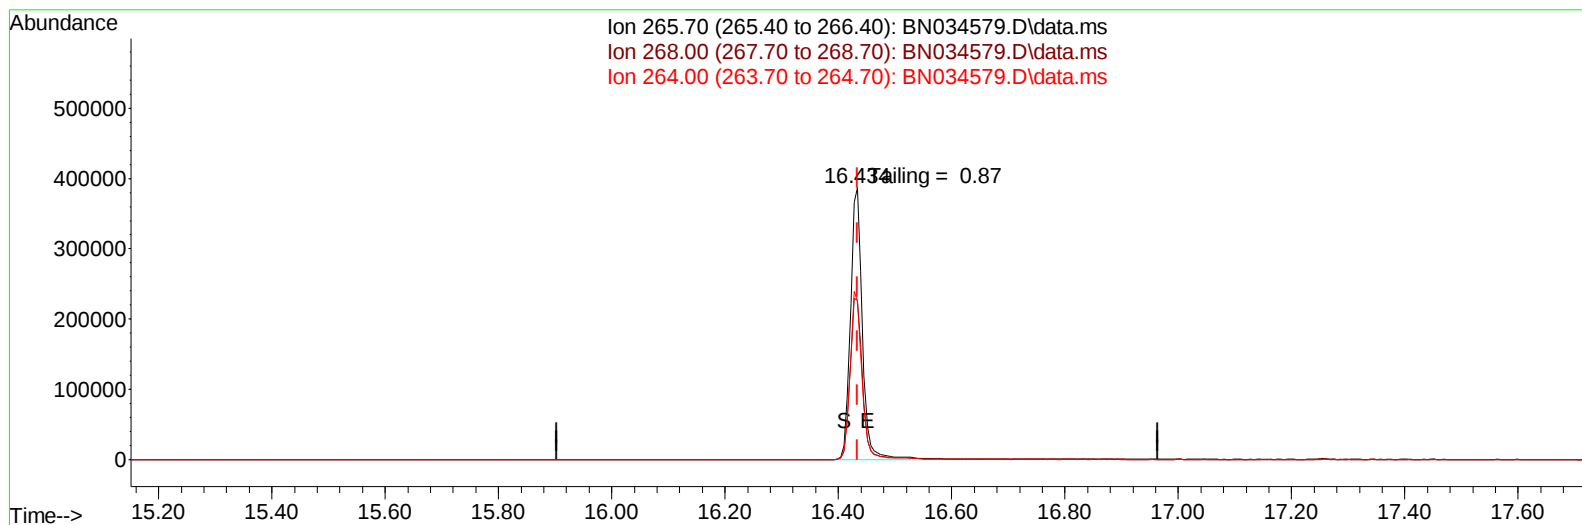

TIC: BN034579.D\data.ms

**(70) Pentachloropheno1 (C)**

**16.433min ( 0.000) 26821.50 ng**




**response 571476**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 58.52  |
| 264.00 | 61.60  | 58.29  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN101424\  
Data File : BN034579.D  
Acq On : 14 Oct 2024 19:51  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Oct 15 00:48:20 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 15 00:48:16 2024  
Response via : Initial Calibration

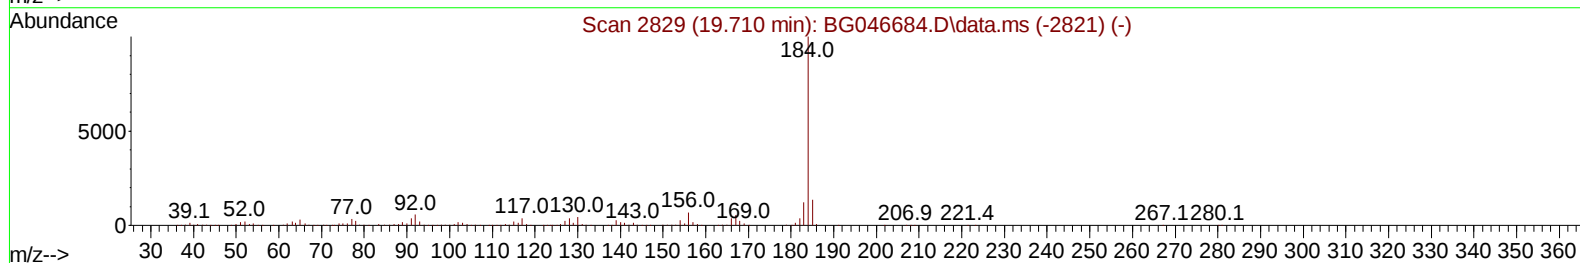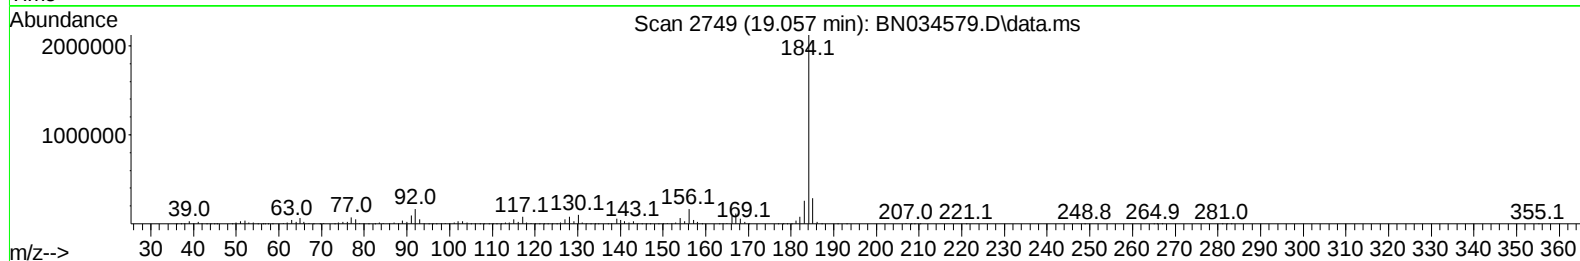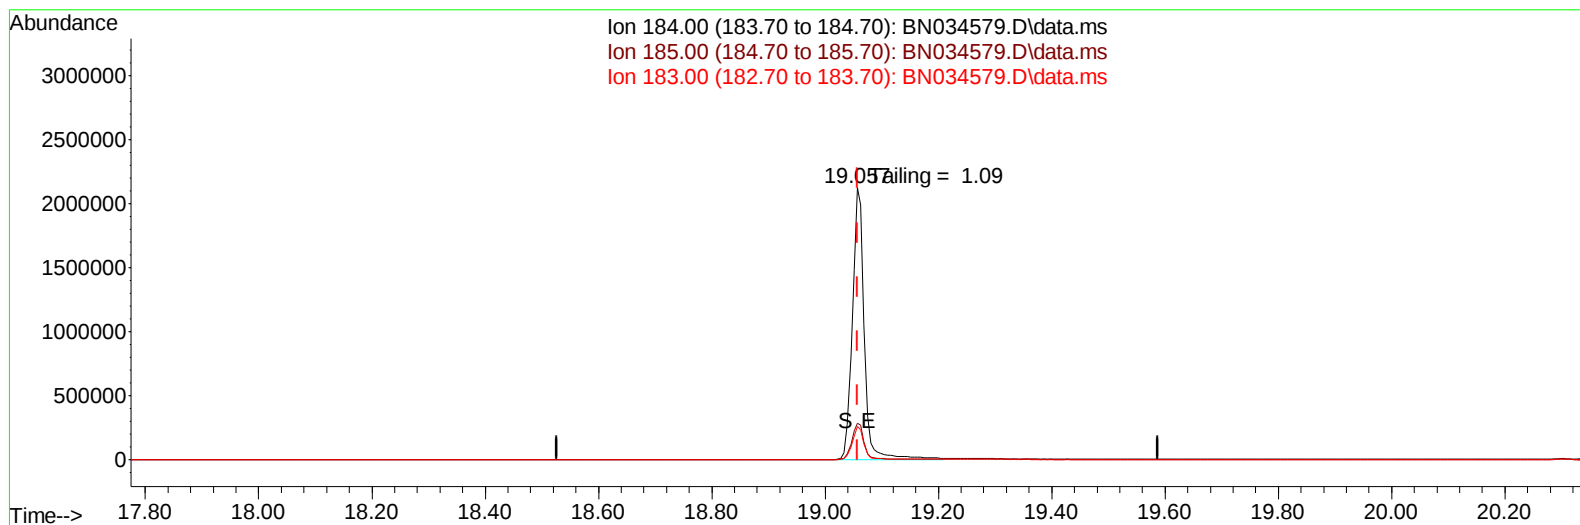

TIC: BN034579.D\data.ms

(77) Benzidine

19.057min ( 0.000) 0.00 ng

response 3146886

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.44  |
| 183.00 | 13.20  | 12.17  |
| 0.00   | 0.00   | 0.00   |