

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101524\
 Data File : BN034595.D
 Acq On : 15 Oct 2024 19:01
 Operator : RC/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Quant Time: Oct 16 00:02:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 15 23:53:04 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.669	152	5291	0.400	ng	0.00
7) Naphthalene-d8	10.447	136	14949	0.400	ng	0.00
13) Acenaphthene-d10	14.297	164	7763	0.400	ng	0.00
19) Phenanthrene-d10	17.044	188	16058	0.400	ng	0.00
29) Chrysene-d12	21.232	240	13358	0.400	ng	0.00
35) Perylene-d12	23.443	264	15063	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.278	112	14818	1.014	ng	0.00
5) Phenol-d6	6.831	99	18760	0.950	ng	0.00
8) Nitrobenzene-d5	8.803	82	9883	0.877	ng	0.00
11) 2-Methylnaphthalene-d10	12.041	152	18627	0.810	ng	0.00
14) 2,4,6-Tribromophenol	15.791	330	3264	0.820	ng	0.00
15) 2-Fluorobiphenyl	12.929	172	24868	0.781	ng	0.00
27) Fluoranthene-d10	19.076	212	34310	0.799	ng	0.00
31) Terphenyl-d14	19.689	244	22506	0.892	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.249	88	5218	0.888	ng	93
3) n-Nitrosodimethylamine	3.538	42	5549	0.733	ng	# 99
6) bis(2-Chloroethyl)ether	7.106	93	13010	0.814	ng	98
9) Naphthalene	10.490	128	34802	0.844	ng	96
10) Hexachlorobutadiene	10.799	225	6006	0.764	ng	# 99
12) 2-Methylnaphthalene	12.113	142	21962	0.789	ng	99
16) Acenaphthylene	14.019	152	32529	0.898	ng	99
17) Acenaphthene	14.361	154	20436	0.822	ng	100
18) Fluorene	15.355	166	25125	0.766	ng	100
20) 4,6-Dinitro-2-methylph...	15.420	198	1001	0.514	ng	# 42
21) 4-Bromophenyl-phenylether	16.250	248	7302	0.760	ng	96
22) Hexachlorobenzene	16.349	284	8466	0.786	ng	99
23) Atrazine	16.523	200	6989	0.917	ng	96
24) Pentachlorophenol	16.697	266	3625	0.832	ng	100
25) Phenanthrene	17.081	178	37429	0.807	ng	100
26) Anthracene	17.168	178	36637	0.892	ng	99
28) Fluoranthene	19.108	202	43002	0.753	ng	100
30) Pyrene	19.466	202	45035	0.847	ng	100
32) Benzo(a)anthracene	21.214	228	40874	0.819	ng	98
33) Chrysene	21.268	228	38664	0.770	ng	99
34) Bis(2-ethylhexyl)phtha...	21.196	149	26466	1.167	ng	100
36) Indeno(1,2,3-cd)pyrene	25.665	276	49168	0.790	ng	100
37) Benzo(b)fluoranthene	22.782	252	43113	0.761	ng	95
38) Benzo(k)fluoranthene	22.826	252	41189	0.712	ng	95
39) Benzo(a)pyrene	23.347	252	38079	0.798	ng	# 94
40) Dibenzo(a,h)anthracene	25.692	278	39322	0.800	ng	97
41) Benzo(g,h,i)perylene	26.338	276	41874	0.768	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101524\
Data File : BN034595.D
Acq On : 15 Oct 2024 19:01
Operator : RC/JU
Sample : SSTDICC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Quant Time: Oct 16 00:02:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 15 23:53:04 2024
Response via : Initial Calibration




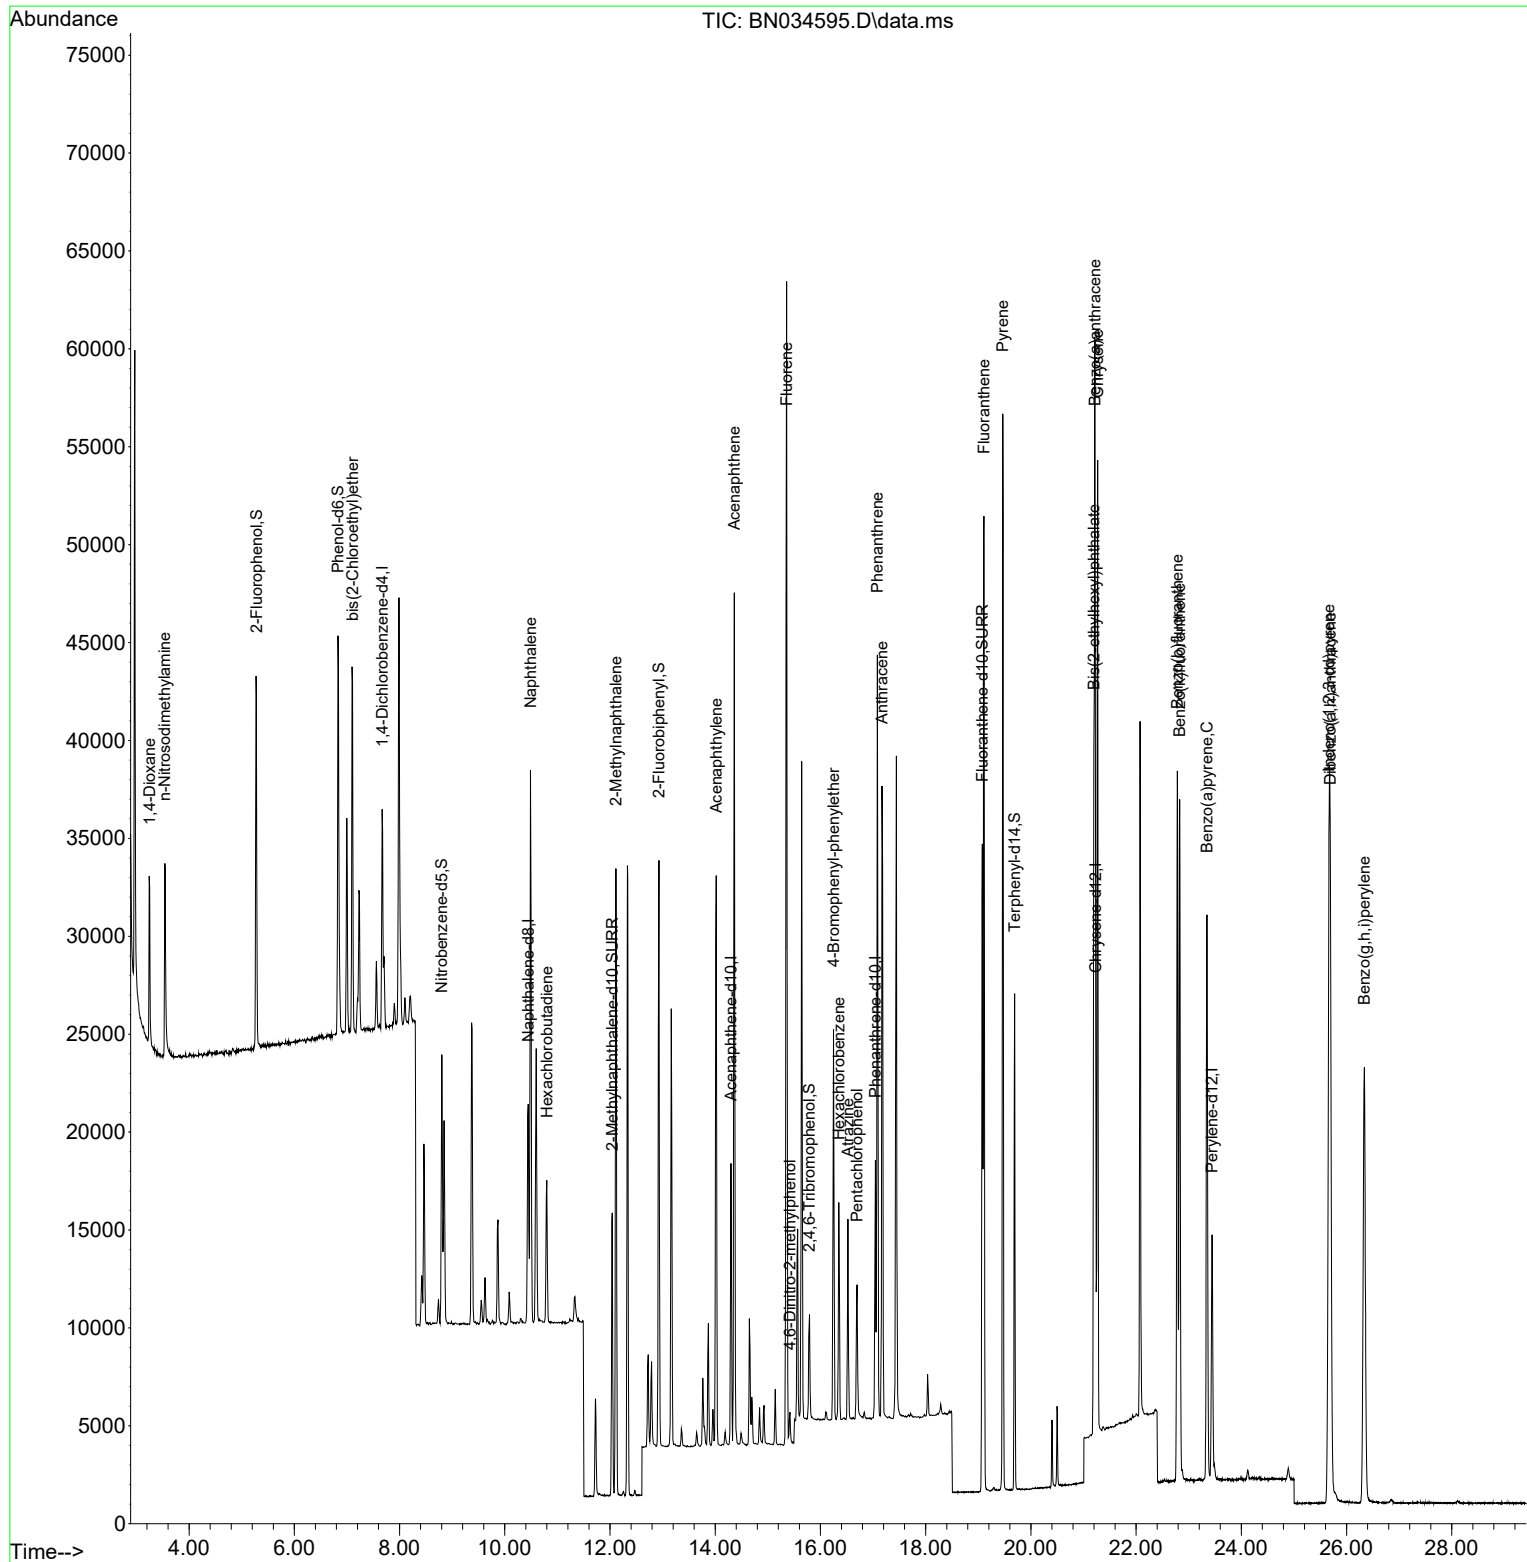




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.669 min Scan# 663
 Delta R.T. -0.000 min
 Lab File: BN034595.D
 Acq: 15 Oct 2024 19:01




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:152 Resp: 5291
 Ion Ratio Lower Upper
 152 100
 150 149.8 119.8 179.6
 115 67.9 55.8 83.6

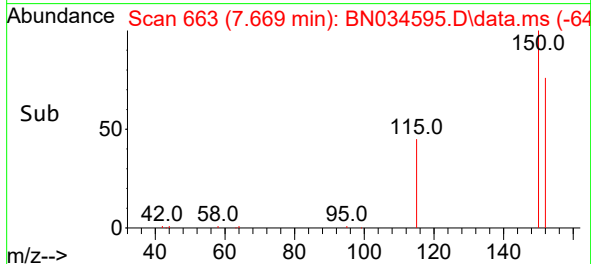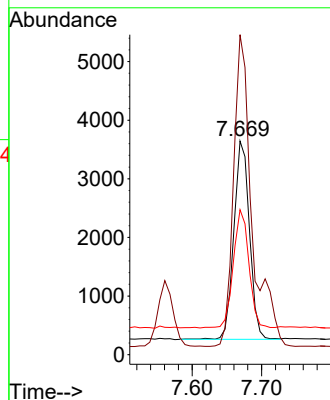

#2
 1,4-Dioxane
 Concen: 0.888 ng
 RT: 3.249 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BN034595.D
 Acq: 15 Oct 2024 19:01

Tgt Ion: 88 Resp: 5218
 Ion Ratio Lower Upper
 88 100
 43 28.5 27.7 41.5
 58 80.4 68.4 102.6



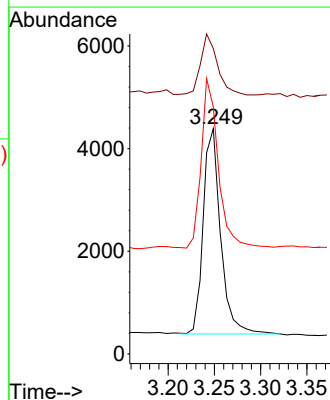
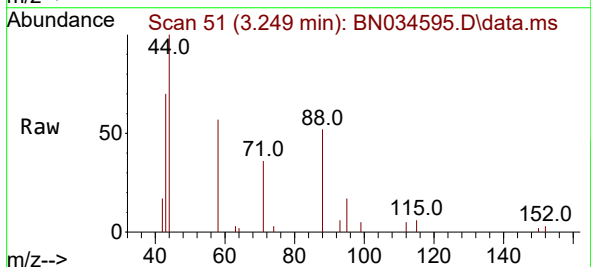




#3
n-Nitrosodimethylamine
Concen: 0.733 ng
RT: 3.538 min Scan# 91
Delta R.T. -0.007 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion: 42 Resp: 5549
Ion Ratio Lower Upper
42 100
74 140.3 112.0 168.0
44 12.5 7.1 10.7#

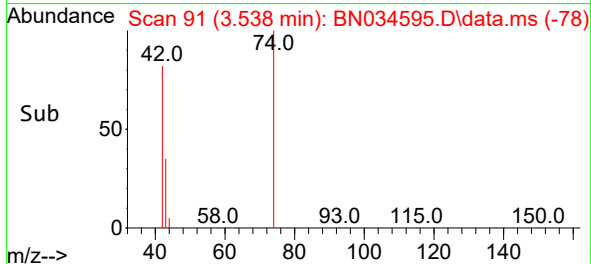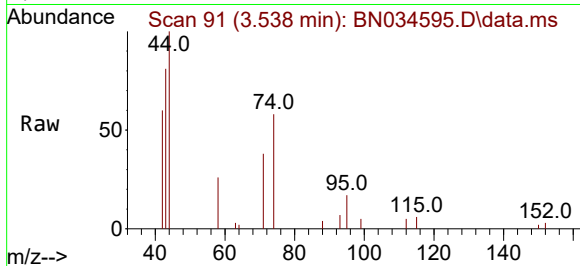

#4
2-Fluorophenol
Concen: 1.014 ng
RT: 5.278 min Scan# 332
Delta R.T. 0.000 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01

Tgt Ion: 112 Resp: 14818
Ion Ratio Lower Upper
112 100
64 58.6 46.6 70.0
63 28.6 23.0 34.6




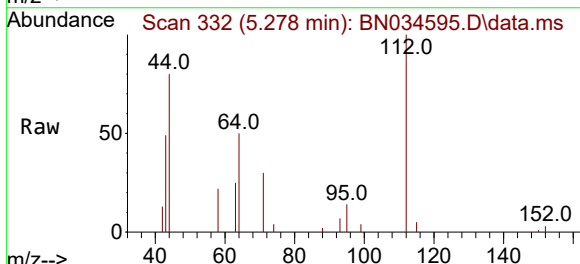




#5
Phenol-d6
Concen: 0.950 ng
RT: 6.831 min Scan# 54
Delta R.T. -0.007 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion: 99 Resp: 18760
Ion Ratio Lower Upper
99 100
42 17.9 15.0 22.4
71 30.0 25.4 38.0

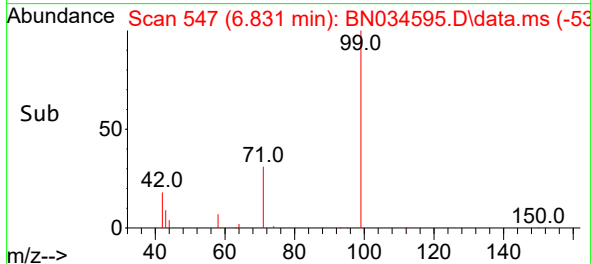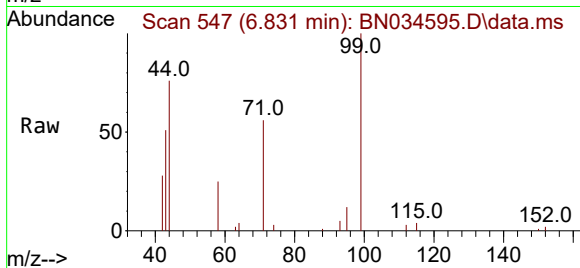

#6
bis(2-Chloroethyl)ether
Concen: 0.814 ng
RT: 7.106 min Scan# 585
Delta R.T. 0.000 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01

Tgt Ion: 93 Resp: 13010
Ion Ratio Lower Upper
93 100
63 80.2 63.0 94.4
95 33.7 27.7 41.5

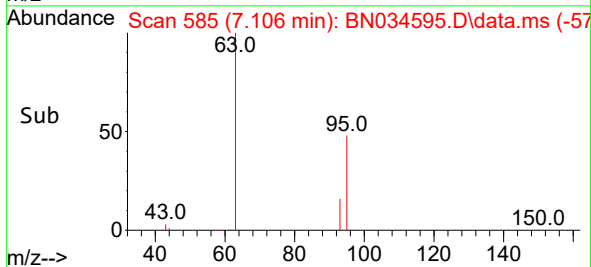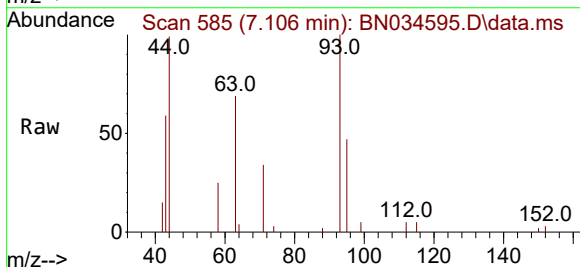



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.447 min Scan# 91

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8

Tgt Ion:136 Resp: 14949





Ion Ratio Lower Upper

136 100

137 13.6 10.7 16.1

54 13.8 11.6 17.4

68 13.5 11.4 17.0

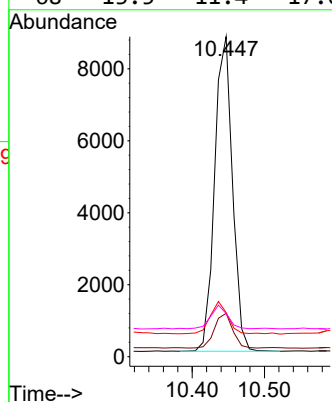

#8

Nitrobenzene-d5

Concen: 0.877 ng

RT: 8.803 min Scan# 798

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01




Tgt Ion: 82 Resp: 9883


Ion Ratio Lower Upper

82 100

128 37.4 27.0 40.4

54 53.9 43.7 65.5





#9

Naphthalene

Concen: 0.844 ng

RT: 10.490 min Scan# 956

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:128 Resp: 34802

Ion Ratio Lower Upper

128 100

129 11.8 10.6 15.8

127 14.3 12.8 19.2

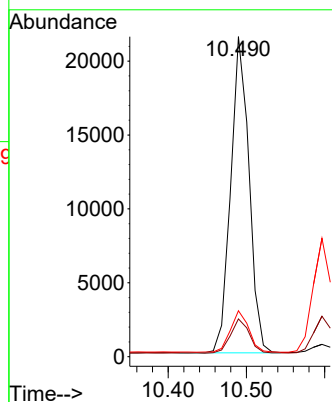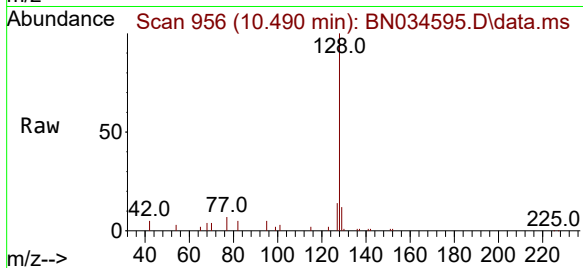

#10

Hexachlorobutadiene

Concen: 0.764 ng

RT: 10.799 min Scan# 985

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01




Tgt Ion:225 Resp: 6006


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.9 51.5 77.3

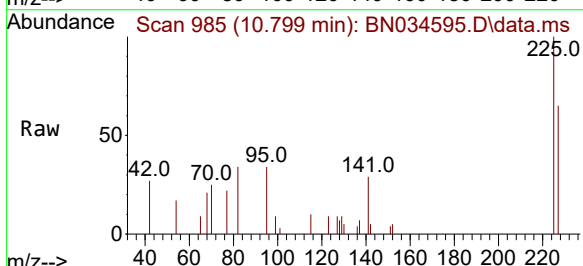



#11

2-Methylnaphthalene-d10

Concen: 0.810 ng

RT: 12.041 min Scan# 1193

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01

Instrument :

BNA_N

ClientSampleId :





SSTDICC0.8

Tgt Ion:152 Resp: 18627

Ion Ratio Lower Upper

152 100

151 20.6 17.0 25.4

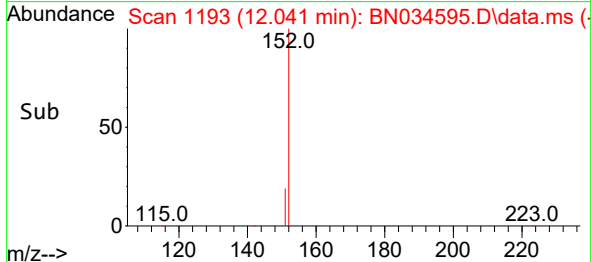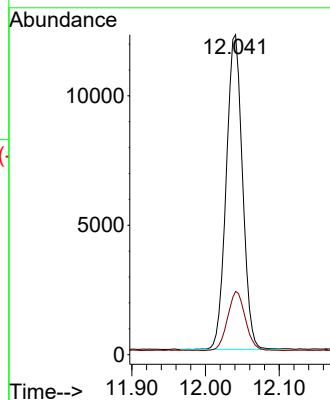

#12

2-Methylnaphthalene

Concen: 0.789 ng

RT: 12.113 min Scan# 1212

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01




Tgt Ion:142 Resp: 21962


Ion Ratio Lower Upper

142 100

141 89.5 72.1 108.1

115 35.3 30.0 45.0

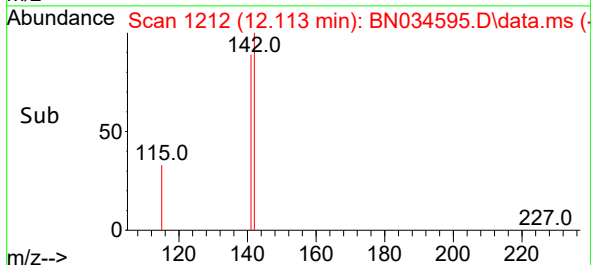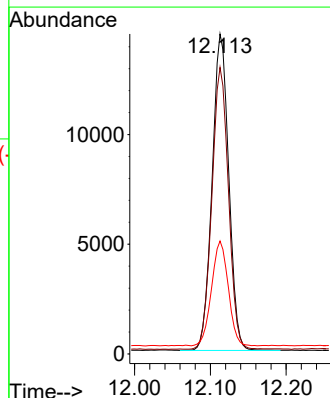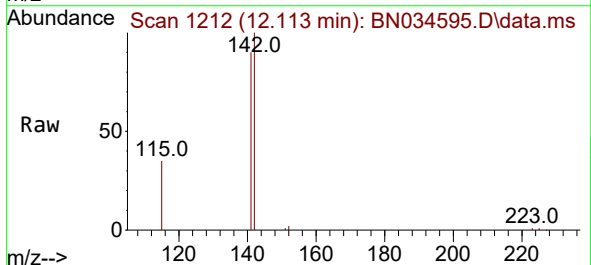



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.297 min Scan# 1501

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:164 Resp: 7763

Ion Ratio Lower Upper

164 100

162 103.8 82.5 123.7

160 48.5 37.8 56.6

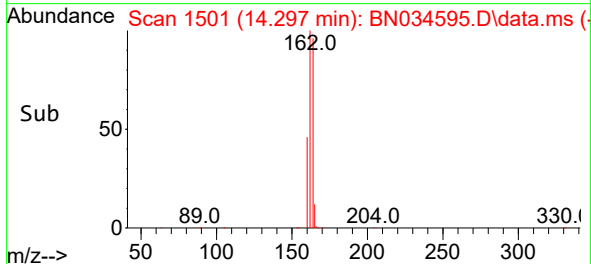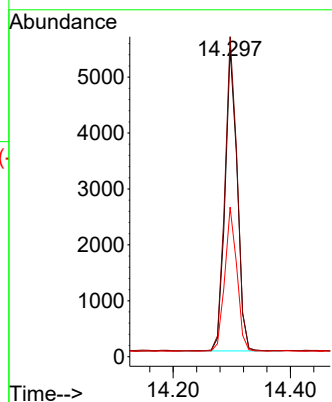

#14

2,4,6-Tribromophenol

Concen: 0.820 ng

RT: 15.791 min Scan# 1637

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01




Tgt Ion:330 Resp: 3264


Ion Ratio Lower Upper

330 100

332 94.4 76.8 115.2

141 39.8 31.5 47.3




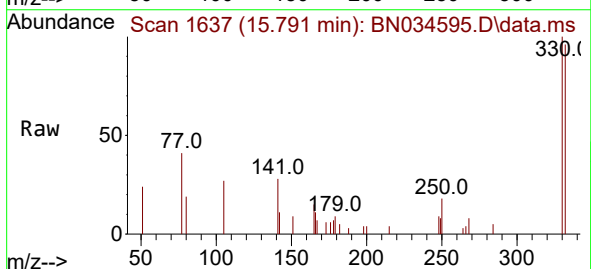




#15
2-Fluorobiphenyl
Concen: 0.781 ng
RT: 12.929 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:172 Resp: 24868
Ion Ratio Lower Upper
172 100
171 34.6 28.6 43.0
170 22.7 19.1 28.7

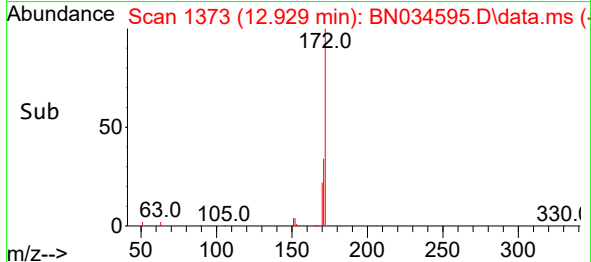

#16
Acenaphthylene
Concen: 0.898 ng
RT: 14.019 min Scan# 1475
Delta R.T. 0.000 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01

Tgt Ion:152 Resp: 32529
Ion Ratio Lower Upper
152 100
151 19.5 15.8 23.8
153 13.0 10.6 15.8

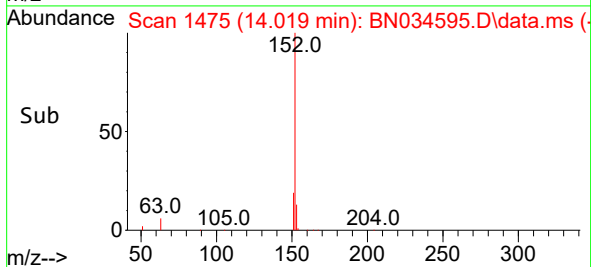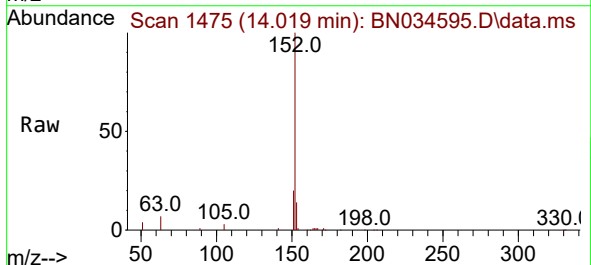



#17

Acenaphthene

Concen: 0.822 ng

RT: 14.361 min Scan# 1507

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:154 Resp: 20436

Ion Ratio Lower Upper

154 100

153 111.2 89.0 133.6

152 52.4 41.8 62.6

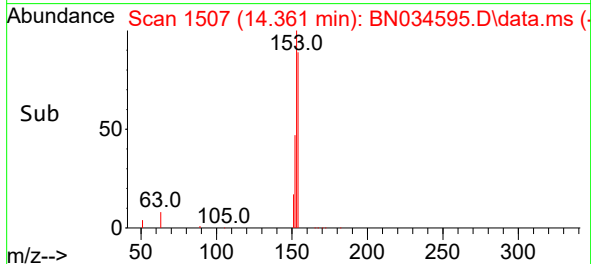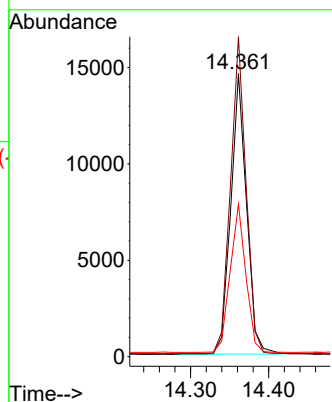

#18

Fluorene

Concen: 0.766 ng

RT: 15.355 min Scan# 1600

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01




Tgt Ion:166 Resp: 25125


Ion Ratio Lower Upper

166 100

165 98.0 78.7 118.1

167 13.6 10.9 16.3



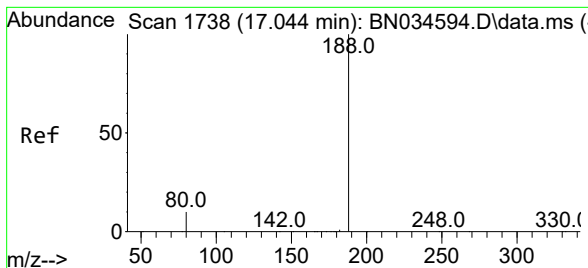

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.044 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:188 Resp: 16058

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 13.9 11.0 16.6

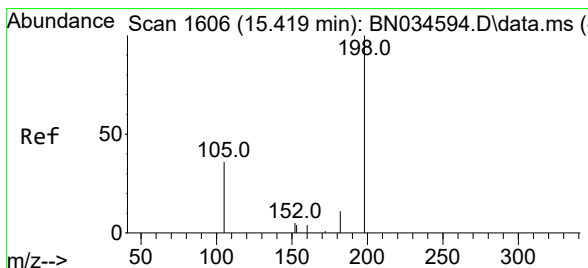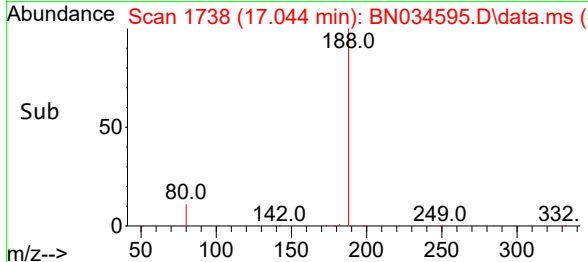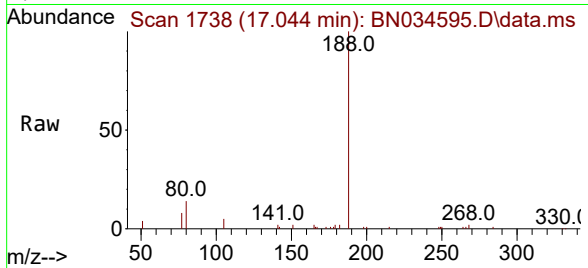

#20

4,6-Dinitro-2-methylphenol

Concen: 0.514 ng

RT: 15.420 min Scan# 1606

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01




Tgt Ion:198 Resp: 1001


Ion Ratio Lower Upper

198 100

51 100.5 138.6 208.0#

105 109.1 163.8 245.8#


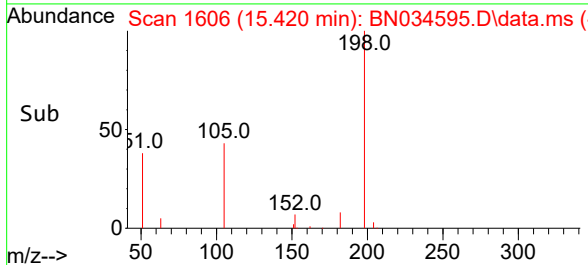

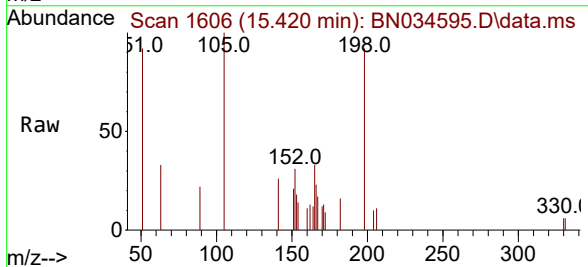


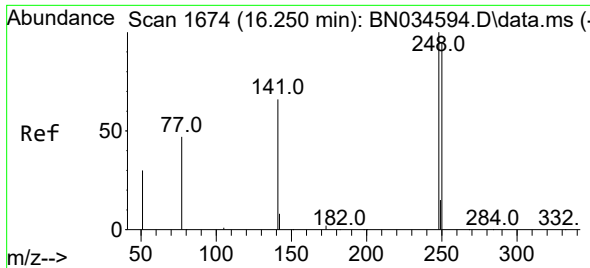

#21
4-Bromophenyl-phenylether
Concen: 0.760 ng
RT: 16.250 min Scan# 1674
Delta R.T. 0.000 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:248 Resp: 7302
Ion Ratio Lower Upper
248 100
250 97.5 76.9 115.3
141 67.3 58.7 88.1

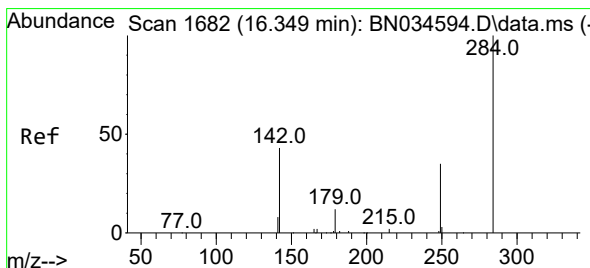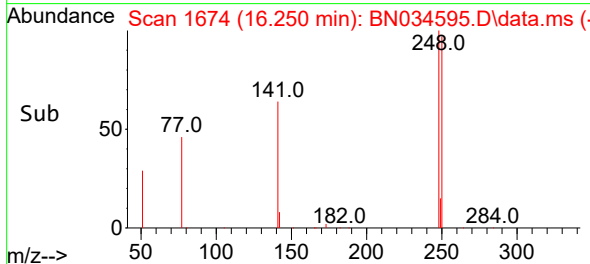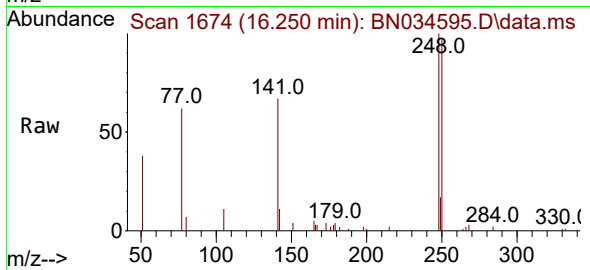

#22
Hexachlorobenzene
Concen: 0.786 ng
RT: 16.349 min Scan# 1682
Delta R.T. 0.000 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01

Tgt Ion:284 Resp: 8466
Ion Ratio Lower Upper
284 100
142 37.3 29.1 43.7
249 30.7 24.6 36.8

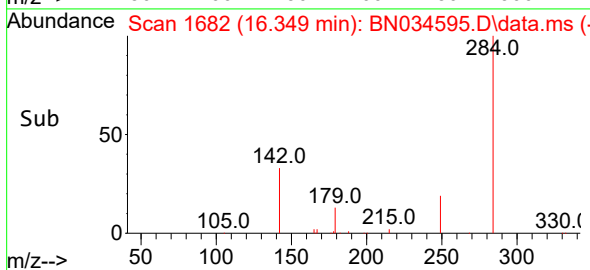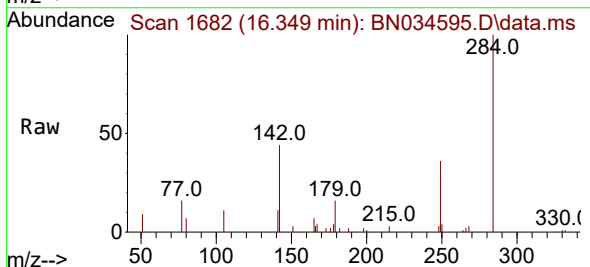



#23

Atrazine

Concen: 0.917 ng

RT: 16.523 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:200 Resp: 6989

Ion Ratio Lower Upper

200 100

173 29.4 26.0 39.0

215 45.9 37.9 56.9

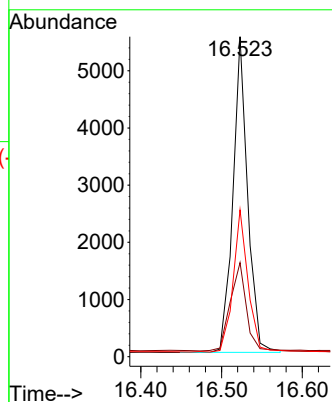

#24

Pentachlorophenol

Concen: 0.832 ng

RT: 16.697 min Scan# 1710

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01




Tgt Ion:266 Resp: 3625


Ion Ratio Lower Upper

266 100

264 62.1 49.9 74.9

268 62.3 49.7 74.5





#25

Phenanthrene

Concen: 0.807 ng

RT: 17.081 min Scan# 1741

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:178 Resp: 37429

Ion Ratio Lower Upper

178 100

176 18.8 15.1 22.7

179 15.1 12.2 18.2

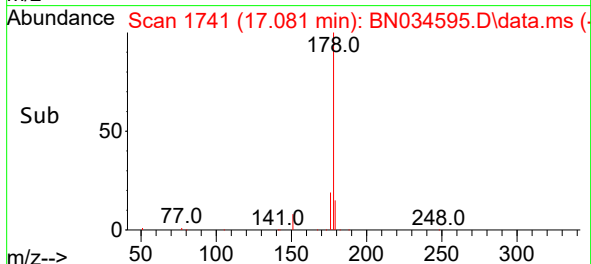

#26

Anthracene

Concen: 0.892 ng

RT: 17.168 min Scan# 1748

Delta R.T. -0.012 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01




Tgt Ion:178 Resp: 36637


Ion Ratio Lower Upper

178 100

176 18.1 14.6 22.0

179 15.1 11.8 17.6





#27

Fluoranthene-d10

Concen: 0.799 ng

RT: 19.076 min Scan# 1978

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:212 Resp: 34310

Ion Ratio Lower Upper

212 100

106 18.4 14.7 22.1

104 10.4 8.3 12.5

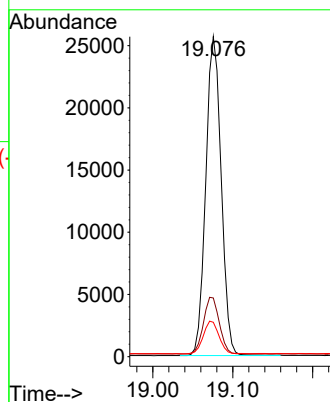

#28

Fluoranthene

Concen: 0.753 ng

RT: 19.108 min Scan# 1985

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01




Tgt Ion:202 Resp: 43002


Ion Ratio Lower Upper

202 100

101 14.0 11.2 16.8

203 17.3 13.7 20.5



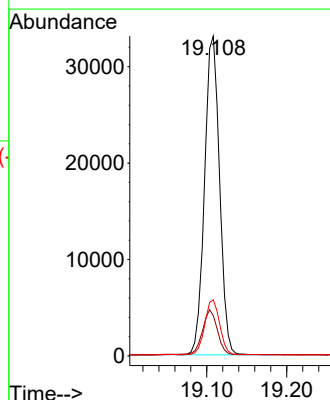



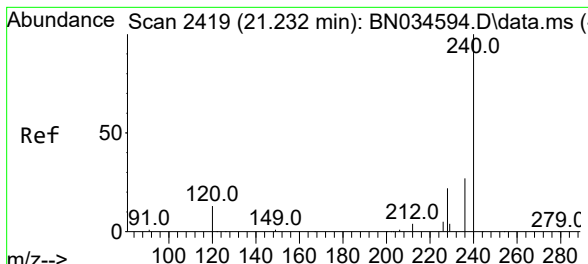

#29
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.232 min Scan# 2419
 Delta R.T. 0.000 min
 Lab File: BN034595.D
 Acq: 15 Oct 2024 19:01




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:	240	Resp:	13358
Ion Ratio	Lower	Upper	
240	100		
120	14.0	12.7	19.1
236	27.5	21.9	32.9

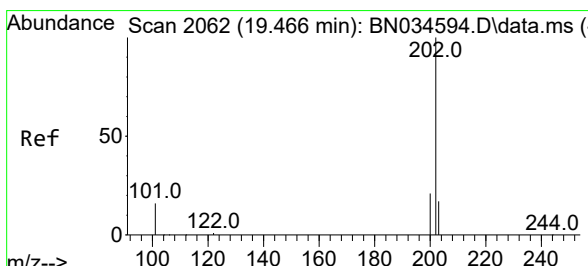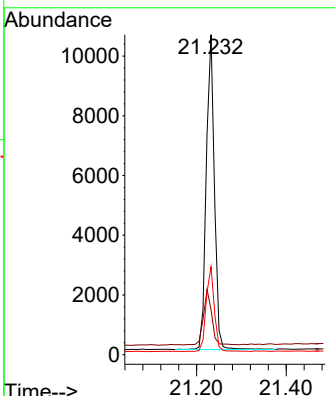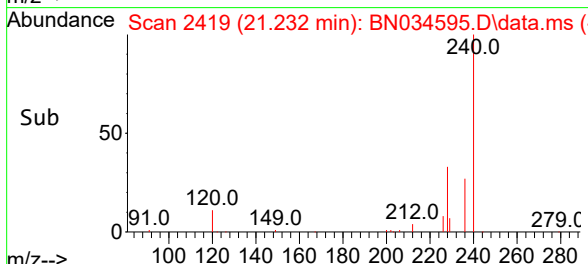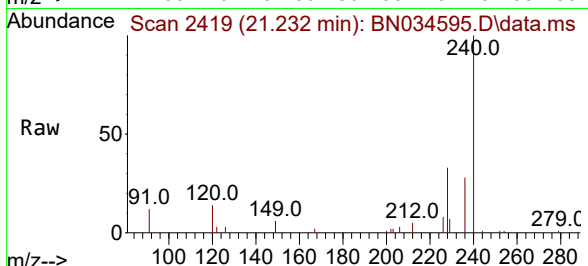

#30
 Pyrene
 Concen: 0.847 ng
 RT: 19.466 min Scan# 2062
 Delta R.T. 0.000 min
 Lab File: BN034595.D
 Acq: 15 Oct 2024 19:01

Tgt Ion:	202	Resp:	45035
Ion Ratio	Lower	Upper	
202	100		
200	20.6	16.6	24.8
203	17.8	14.2	21.4


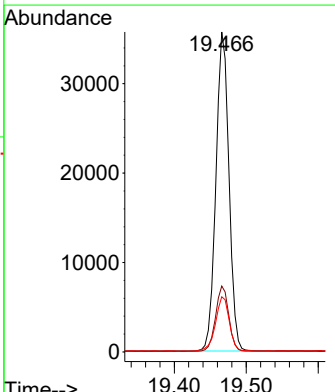
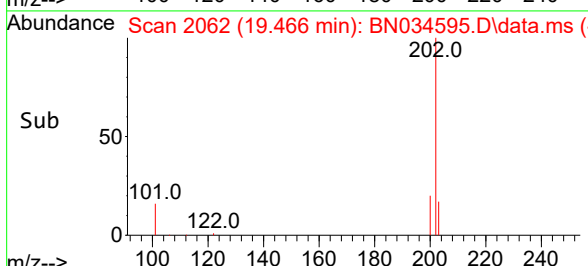
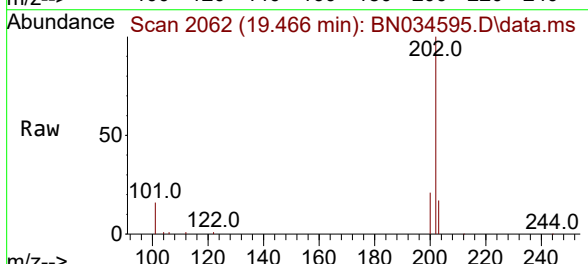




#31
 Terphenyl-d14
 Concen: 0.892 ng
 RT: 19.689 min Scan# 2110
 Delta R.T. 0.000 min
 Lab File: BN034595.D
 Acq: 15 Oct 2024 19:01




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:244 Resp: 22506
 Ion Ratio Lower Upper
 244 100
 212 8.7 7.1 10.7
 122 19.9 17.2 25.8

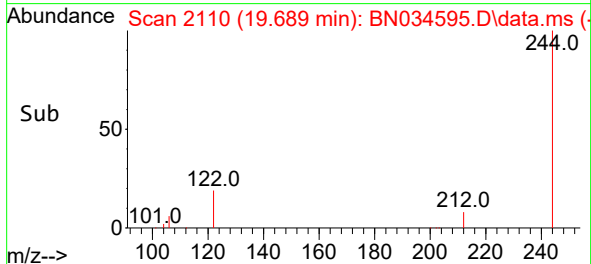

#32
 Benzo(a)anthracene
 Concen: 0.819 ng
 RT: 21.214 min Scan# 2417
 Delta R.T. 0.000 min
 Lab File: BN034595.D
 Acq: 15 Oct 2024 19:01

Tgt Ion:228 Resp: 40874
 Ion Ratio Lower Upper
 228 100
 226 26.9 22.4 33.6
 229 19.2 15.8 23.8

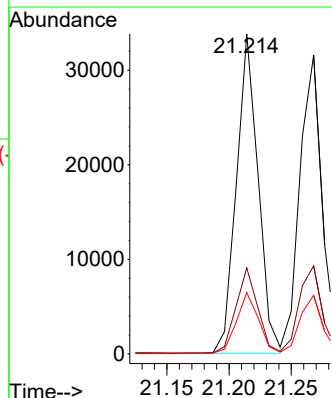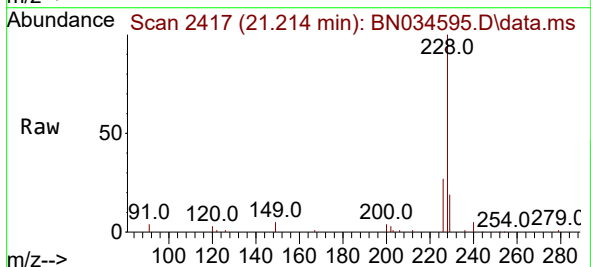

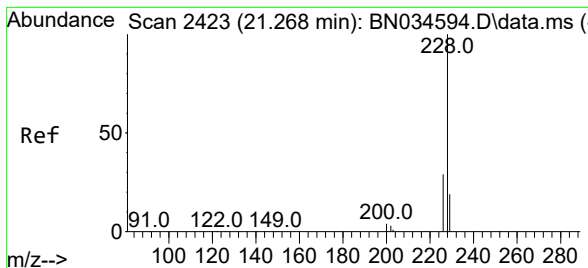

#33

Chrysene

Concen: 0.770 ng

RT: 21.268 min Scan# 2423

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:228 Resp: 38664

Ion Ratio Lower Upper

228 100

226 29.5 23.8 35.8

229 19.6 15.4 23.2

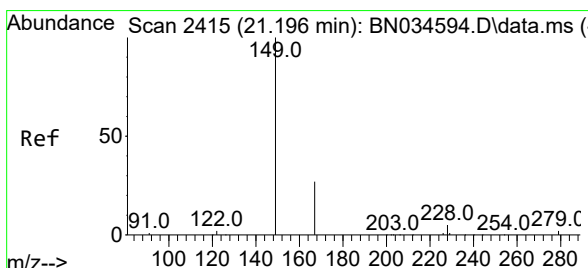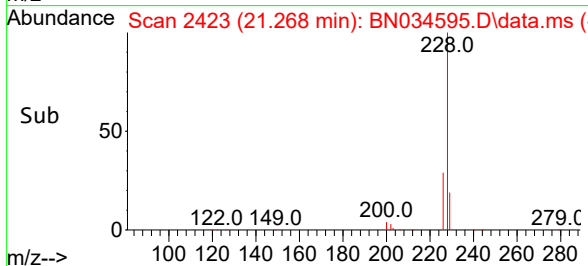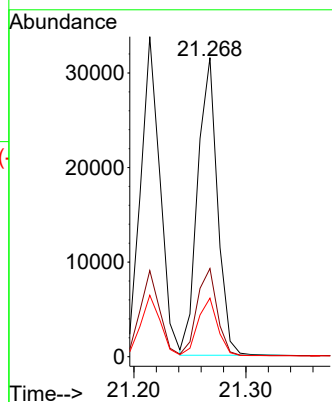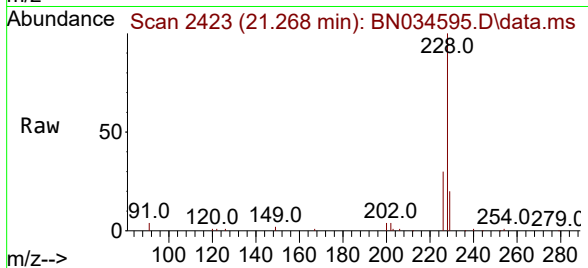

#34

Bis(2-ethylhexyl)phthalate

Concen: 1.167 ng

RT: 21.196 min Scan# 2415

Delta R.T. 0.000 min

Lab File: BN034595.D

Acq: 15 Oct 2024 19:01




Tgt Ion:149 Resp: 26466


Ion Ratio Lower Upper

149 100

167 27.1 21.7 32.5

279 2.8 2.3 3.5


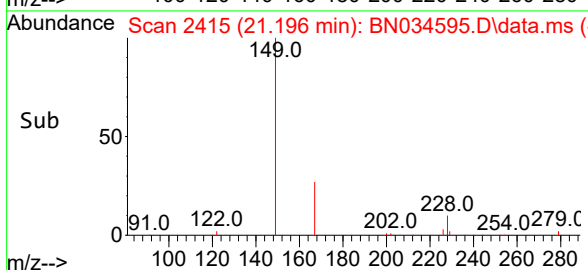

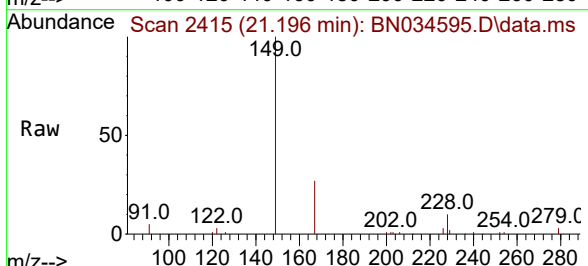




#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.443 min Scan# 2905
 Delta R.T. 0.000 min
 Lab File: BN034595.D
 Acq: 15 Oct 2024 19:01




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:264 Resp: 15063
 Ion Ratio Lower Upper
 264 100
 260 24.9 20.9 31.3
 265 31.0 26.6 40.0

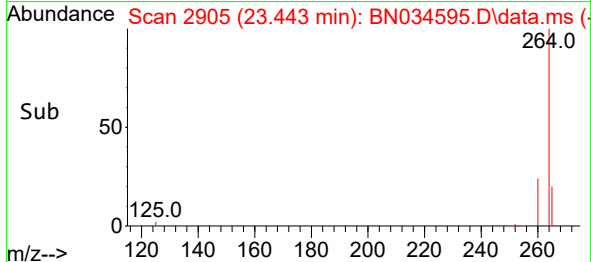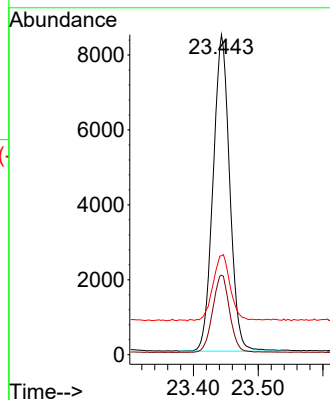

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.790 ng
 RT: 25.665 min Scan# 3665
 Delta R.T. -0.003 min
 Lab File: BN034595.D
 Acq: 15 Oct 2024 19:01

Tgt Ion:276 Resp: 49168
 Ion Ratio Lower Upper
 276 100
 138 34.1 27.2 40.8
 277 24.9 20.1 30.1


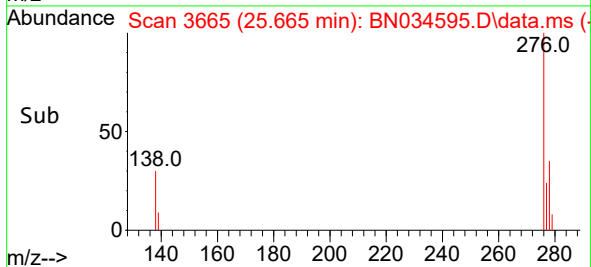
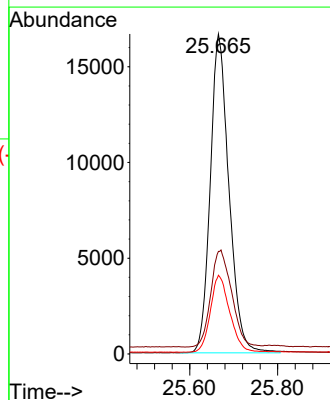
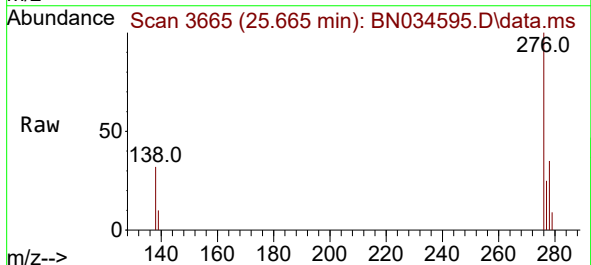




#37
Benzo(b)fluoranthene
Concen: 0.761 ng
RT: 22.782 min Scan# 2679
Delta R.T. -0.003 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:252 Resp: 43113
Ion Ratio Lower Upper
252 100
253 22.3 18.8 28.2
125 15.5 15.2 22.8

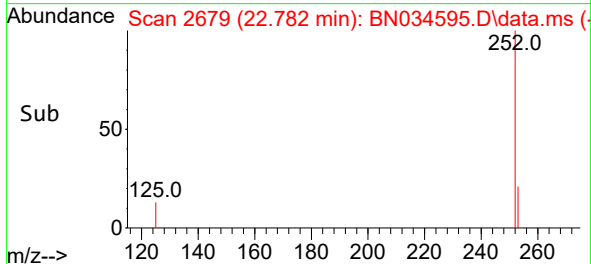

#38
Benzo(k)fluoranthene
Concen: 0.712 ng
RT: 22.826 min Scan# 2694
Delta R.T. -0.003 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01


Tgt Ion:252 Resp: 41189
Ion Ratio Lower Upper
252 100
253 22.6 19.1 28.7
125 15.7 15.4 23.0

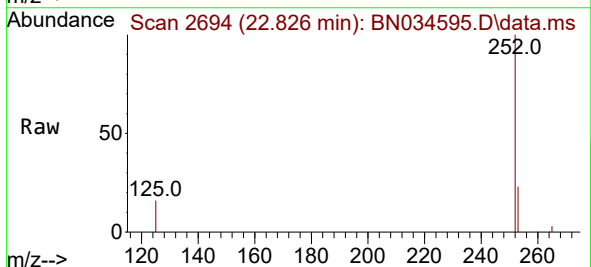






#39
Benzo(a)pyrene
Concen: 0.798 ng
RT: 23.347 min Scan# 2872
Delta R.T. -0.003 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8







Tgt Ion:252 Resp: 38079
Ion Ratio Lower Upper
252 100
253 22.8 19.4 29.0
125 17.5 17.6 26.4#

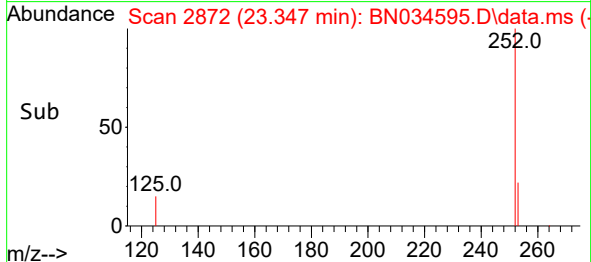

#40
Dibenzo(a,h)anthracene
Concen: 0.800 ng
RT: 25.692 min Scan# 3674
Delta R.T. 0.000 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01


Tgt Ion:278 Resp: 39322
Ion Ratio Lower Upper
278 100
139 24.2 21.4 32.0
279 24.8 20.2 30.4

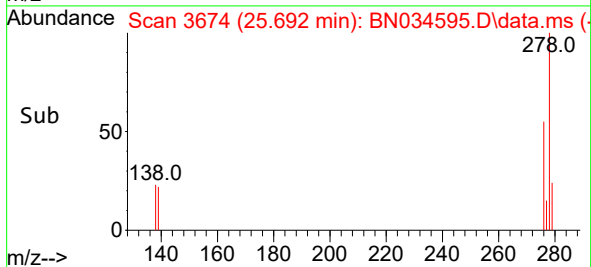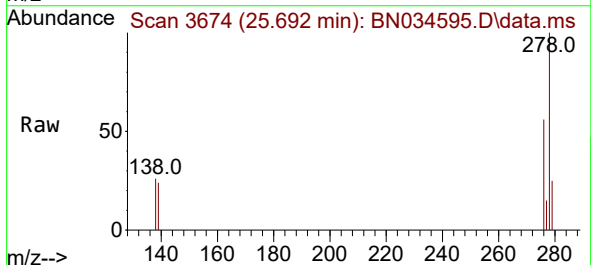

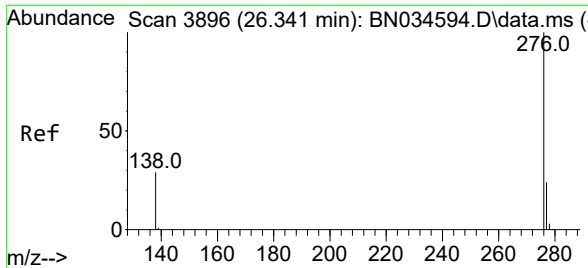

#41
Benzo(g,h,i)perylene
Concen: 0.768 ng
RT: 26.338 min Scan# 3895
Delta R.T. -0.003 min
Lab File: BN034595.D
Acq: 15 Oct 2024 19:01

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

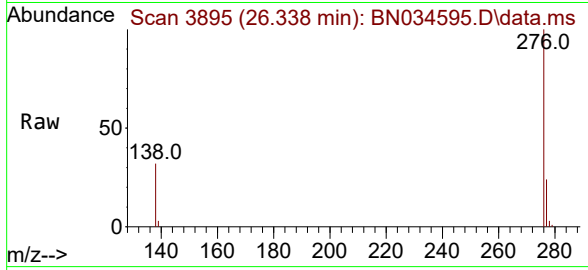

Tgt Ion:276 Resp: 41874
Ion Ratio Lower Upper
276 100
277 24.3 19.9 29.9
138 31.6 28.3 42.5

