
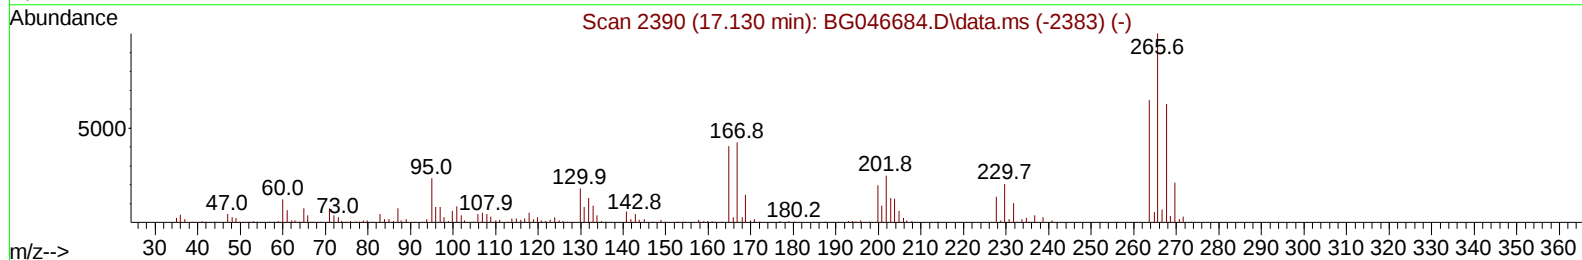
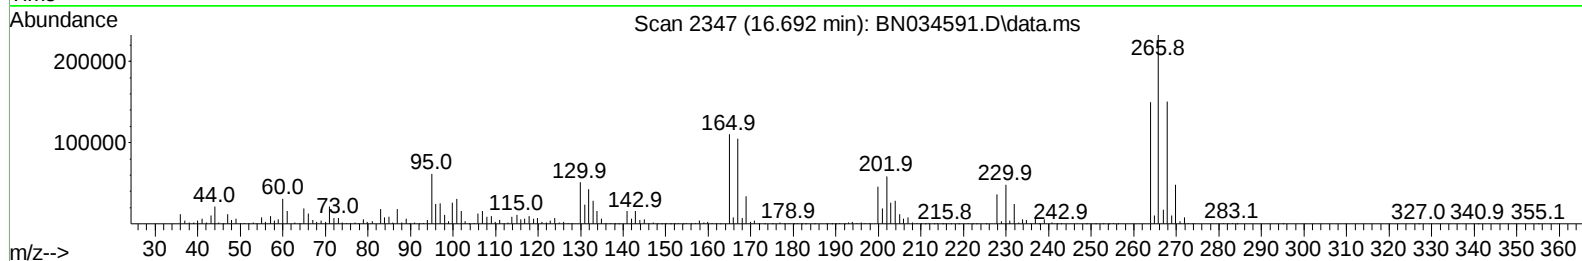


Quant Time: Oct 16 02:02:22 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 16 02:02:16 2024  
Response via : Initial Calibration

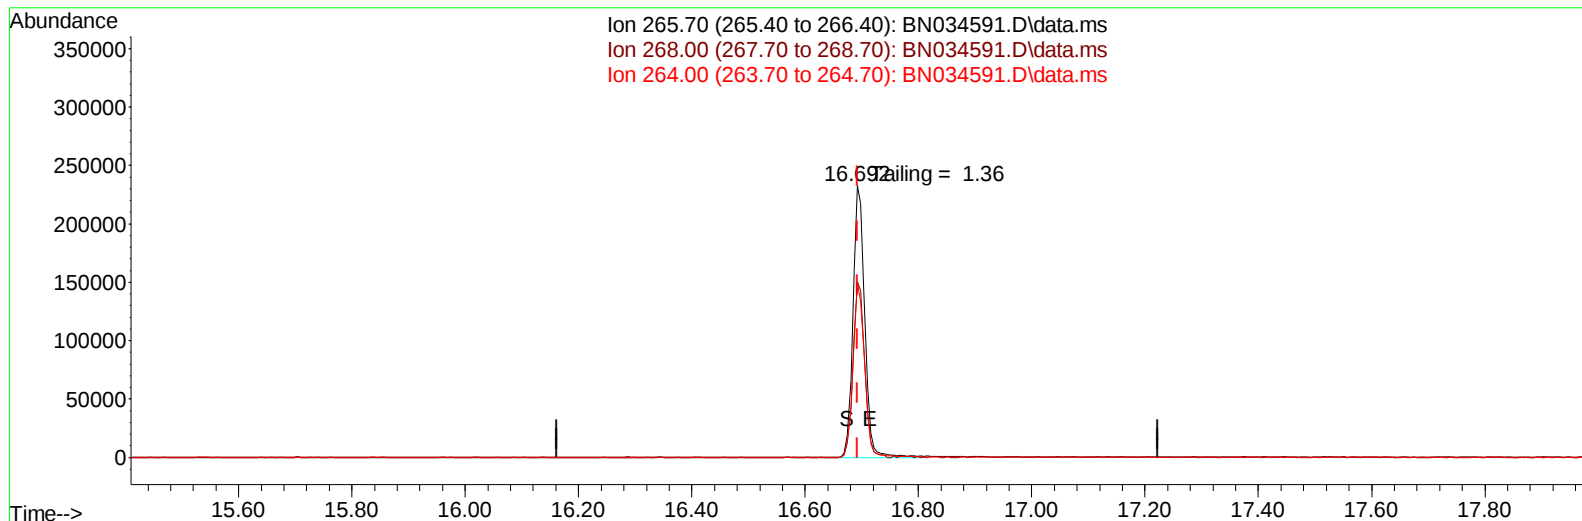

TIC: BN034591.D\data.ms




16.692min ( 0.000) 807423.05 ng

**response**      **335832**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 64.63  |
| 264.00 | 61.60  | 64.60  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN101524\  
Data File : BN034591.D  
Acq On : 15 Oct 2024 16:33  
Operator : RC/JU  
Sample : DFTTP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 02:02:22 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 16 02:02:16 2024  
Response via : Initial Calibration

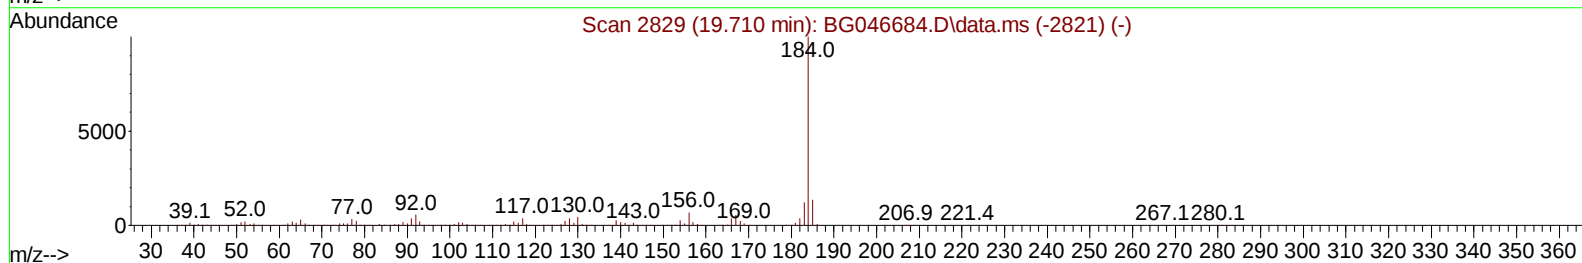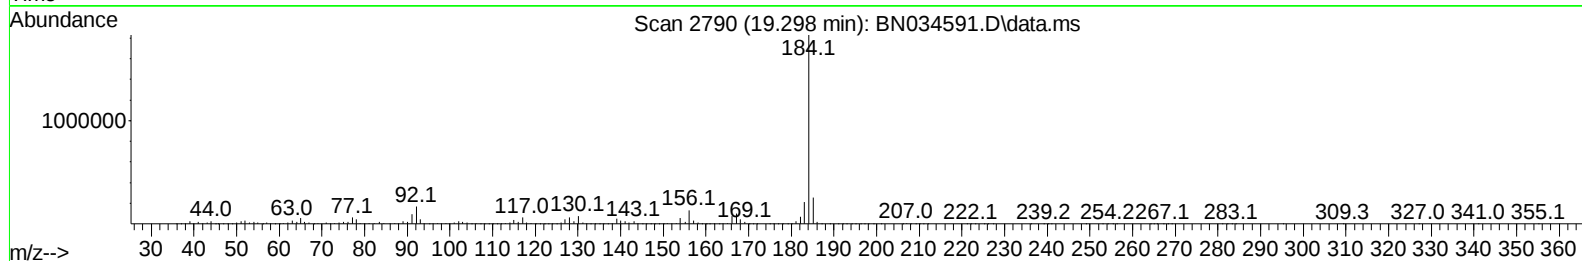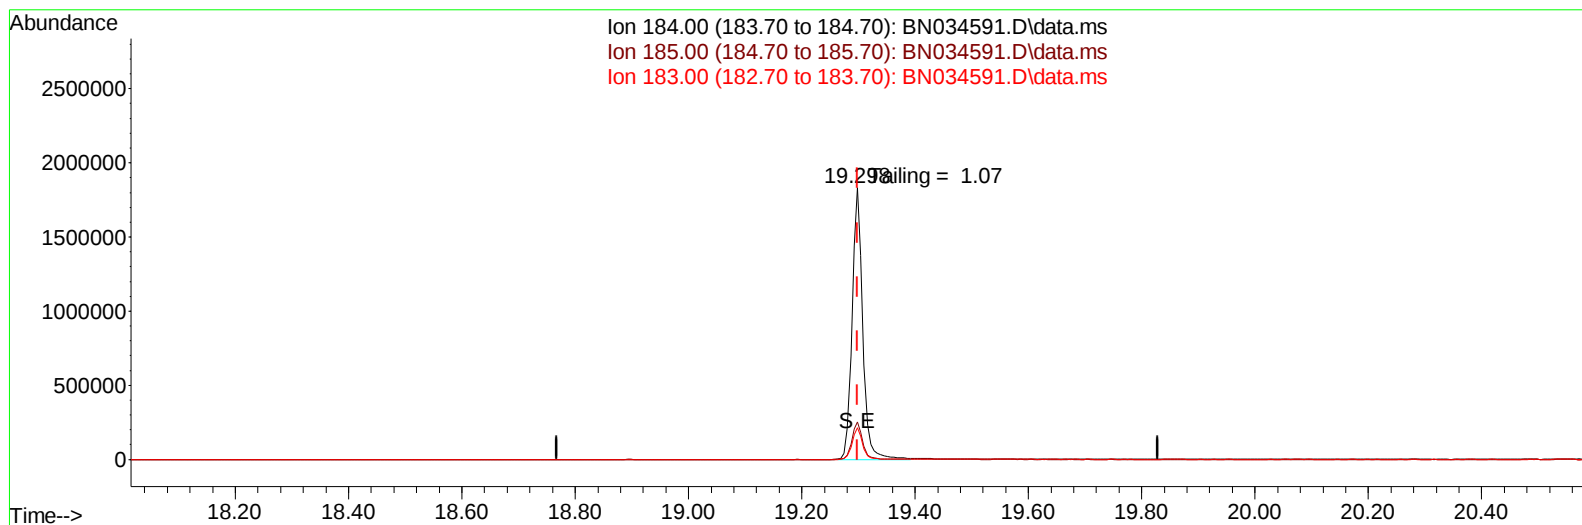

TIC: BN034591.D\data.ms

**(77) Benzidine****19.298min ( 0.000) 428024.92 ng****response 2427701**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.88  |
| 183.00 | 13.20  | 11.68  |
| 0.00   | 0.00   | 0.00   |