
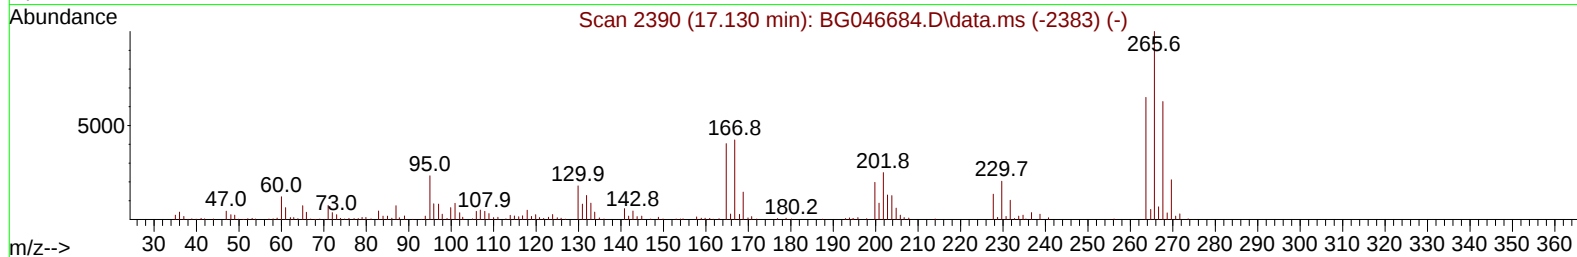
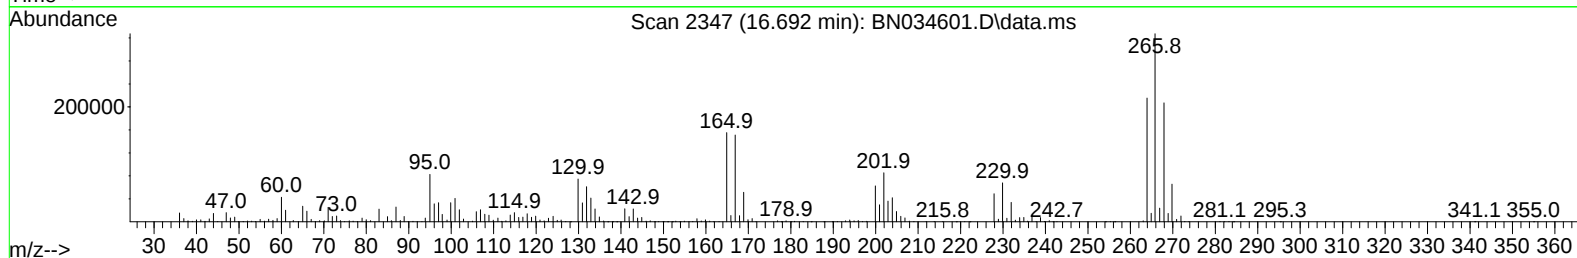


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101524\
Data File : BN034601.D
Acq On : 16 Oct 2024 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 17:05:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 16 02:02:16 2024
Response via : Initial Calibration

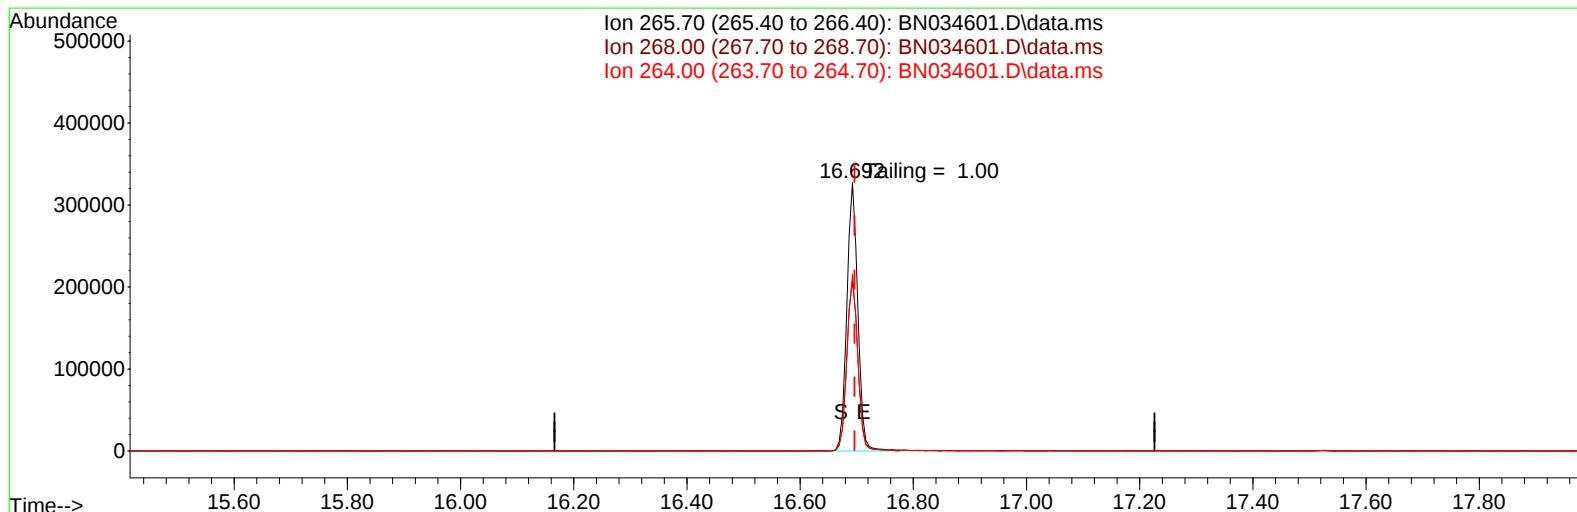

TIC: BN034601.D\data.ms

(70) Pentachlorophenol (C)




16.692min (-0.003) 206159.16 ng m

response 436829

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.24
264.00	61.60	65.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101524\
Data File : BN034601.D
Acq On : 16 Oct 2024 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 17:05:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 16 02:02:16 2024
Response via : Initial Calibration

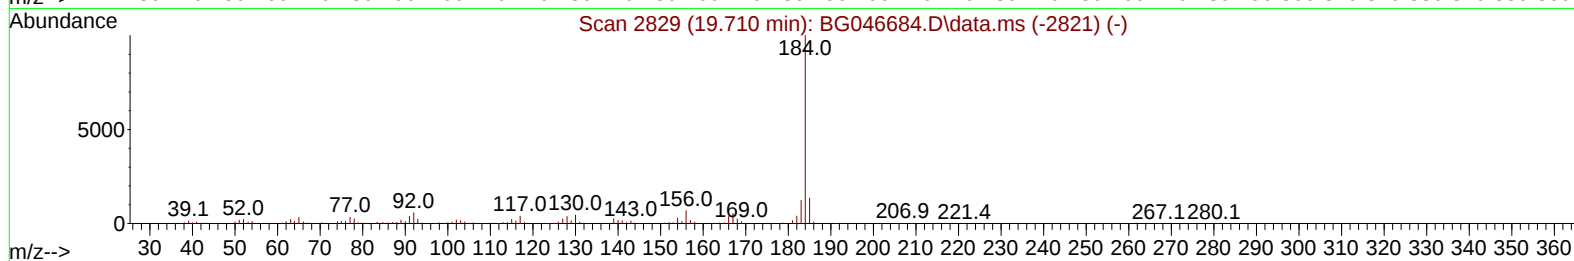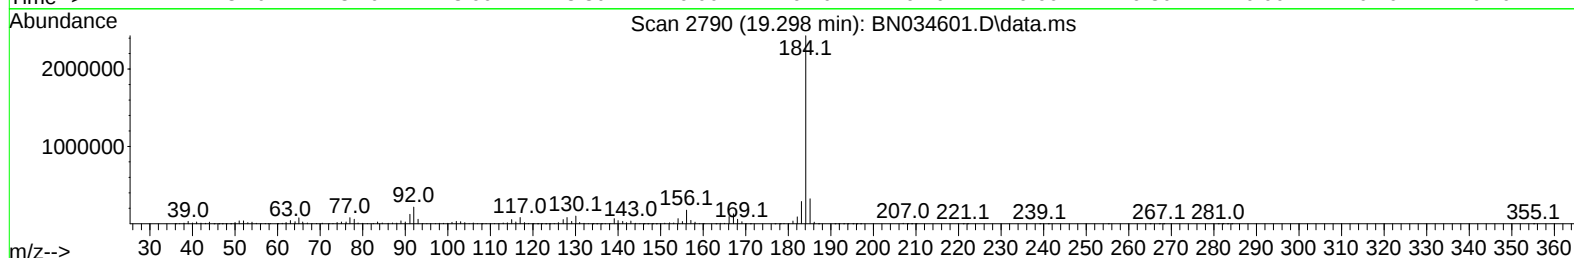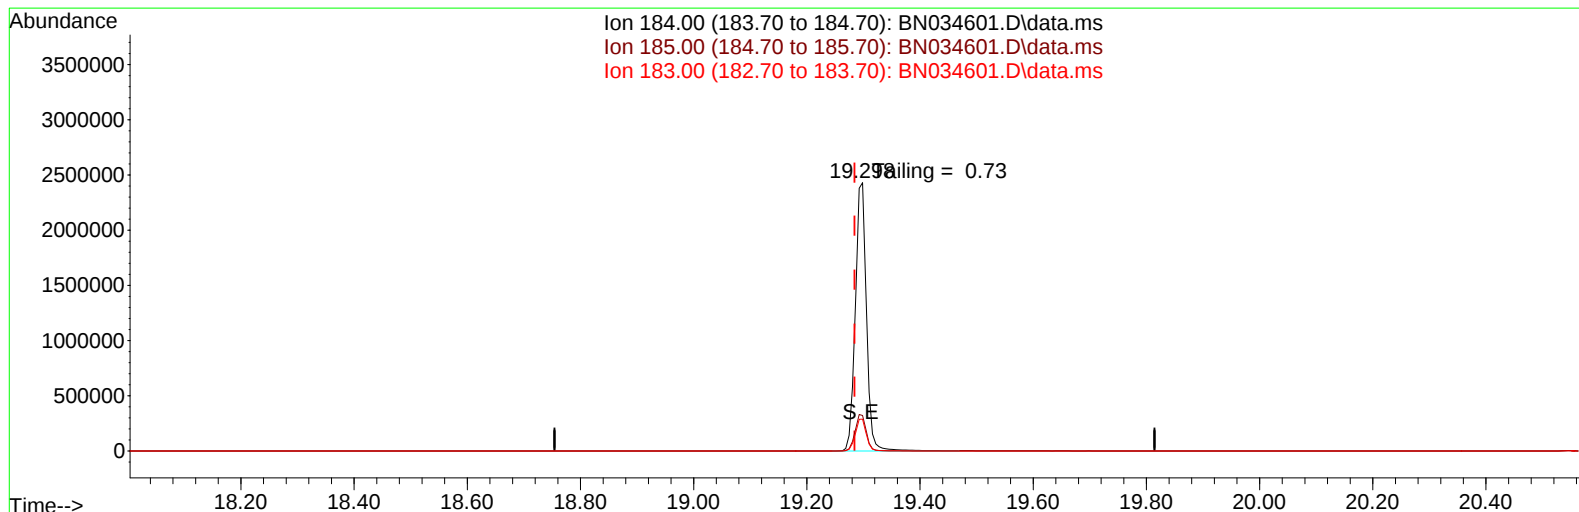

TIC: BN034601.D\data.ms

(77) Benzidine

19.298min (+ 0.014) 51127.30 ng m

response 3331702

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.28
183.00	13.20	11.86
0.00	0.00	0.00