
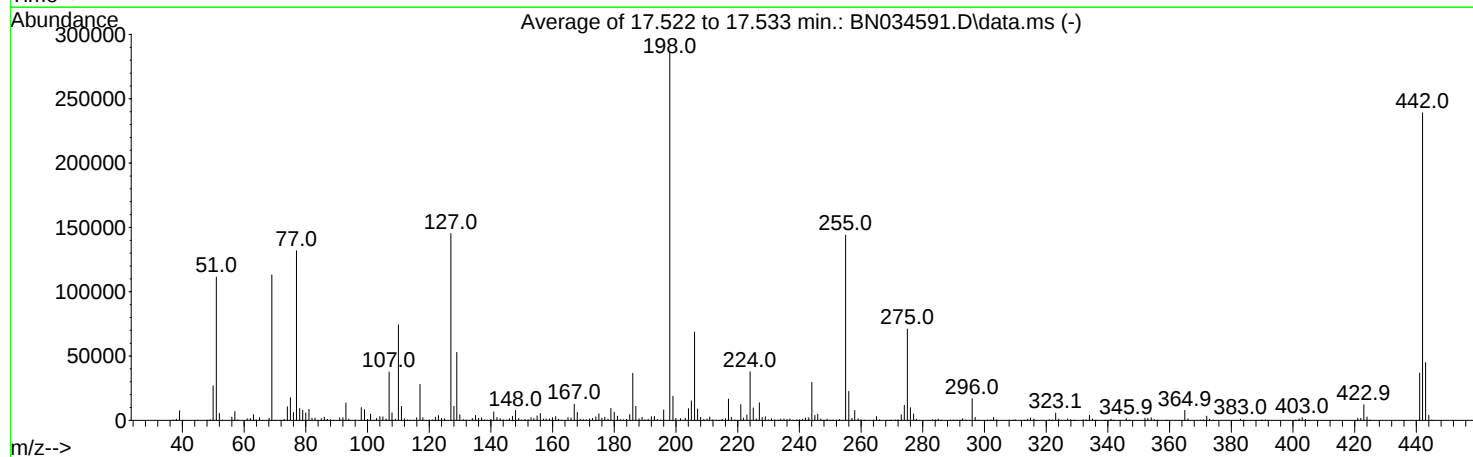


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101524\
Data File : BN034591.D
Acq On : 15 Oct 2024 16:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 16 00:09:32 2024

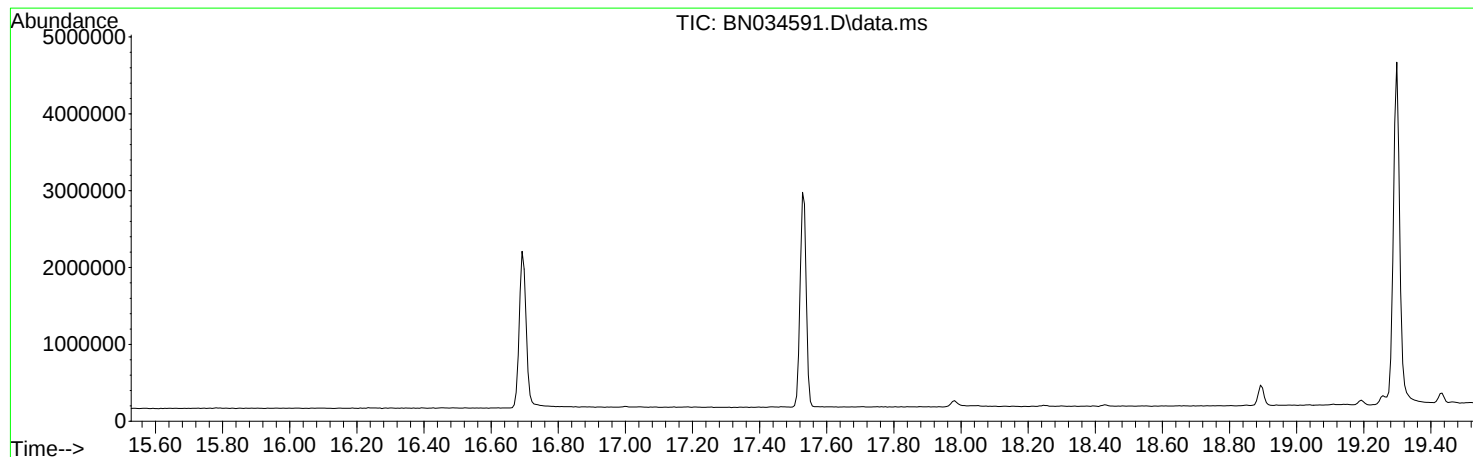




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2479

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	39.0	111409	PASS
68	69	0.00	2	1.5	1678	PASS
69	198	0.00	100	39.5	113113	PASS
70	69	0.00	2	0.1	100	PASS
127	198	10	80	50.8	145295	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	286011	PASS
199	198	5	9	6.6	18838	PASS
275	198	10	60	24.8	71040	PASS
365	198	1	100	2.7	7704	PASS
441	198	0.01	100	12.9	36773	PASS
442	442	50	100	100.0	239152	PASS
443	442	15	24	18.8	44888	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101524\
Data File : BN034591.D
Acq On : 15 Oct 2024 16:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 16 02:02:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 16 02:02:16 2024
Response via : Initial Calibration

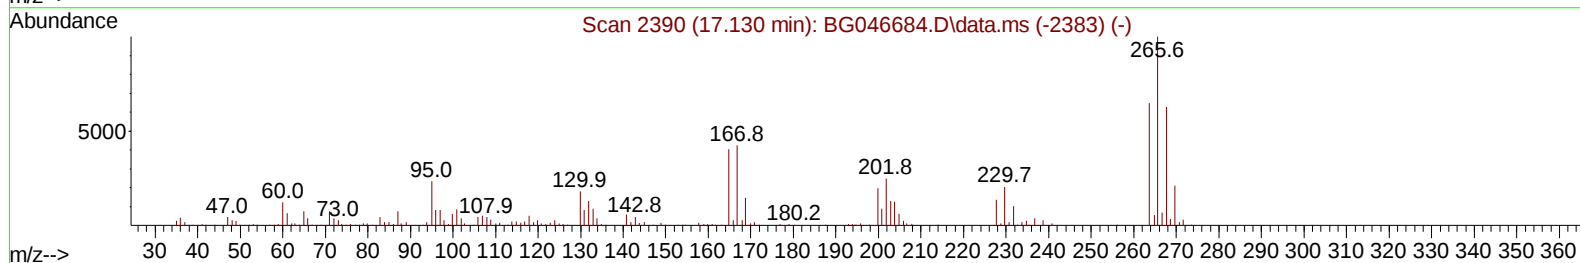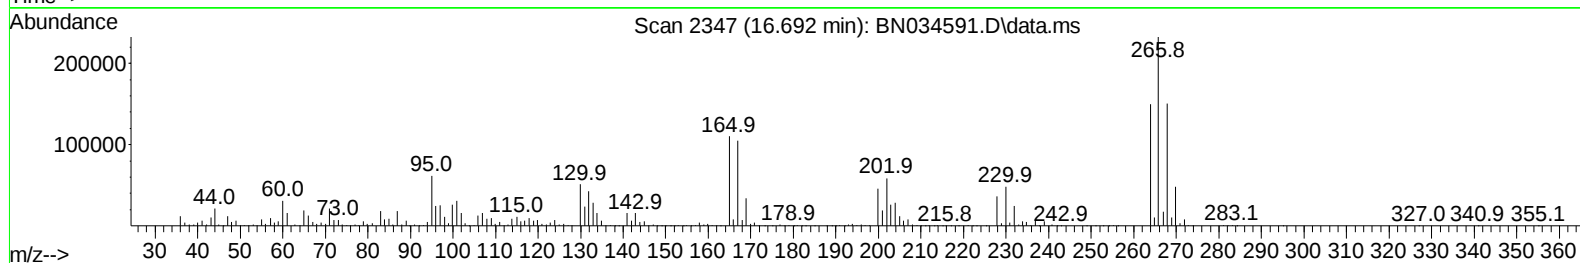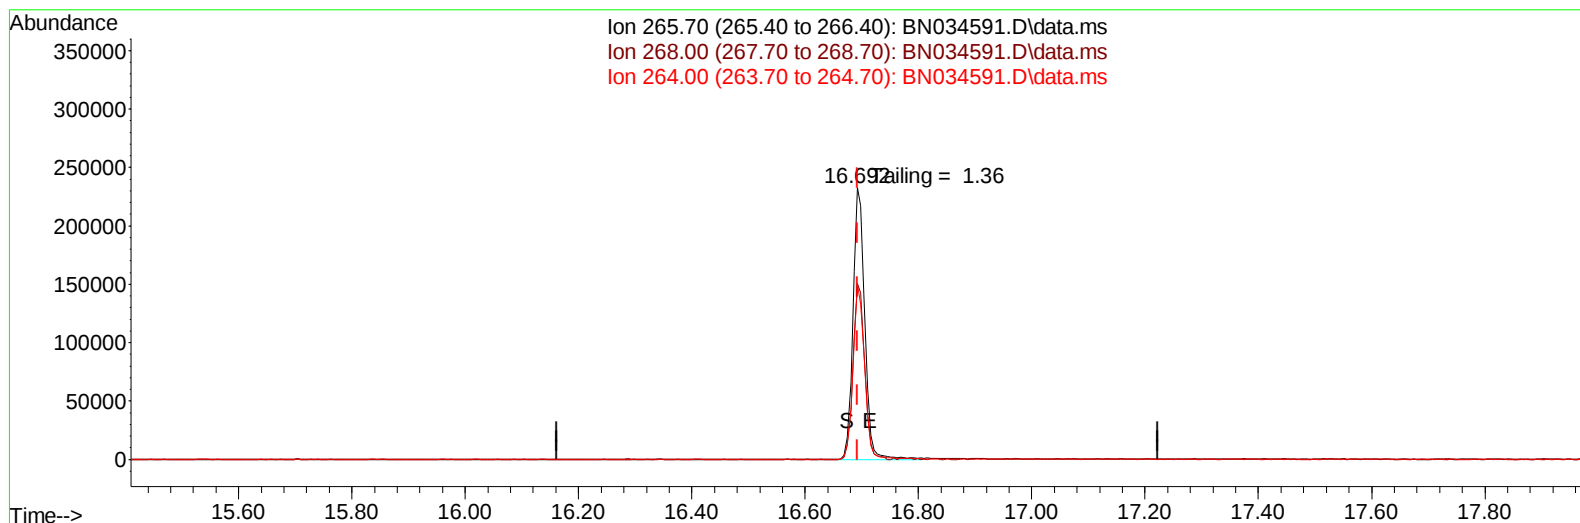

TIC: BN034591.D\data.ms

(70) Pentachloropheno1 (C)

16.692min (0.000) 807423.05 ng




response 335832

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.63
264.00	61.60	64.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101524\
Data File : BN034591.D
Acq On : 15 Oct 2024 16:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 16 02:02:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 16 02:02:16 2024
Response via : Initial Calibration

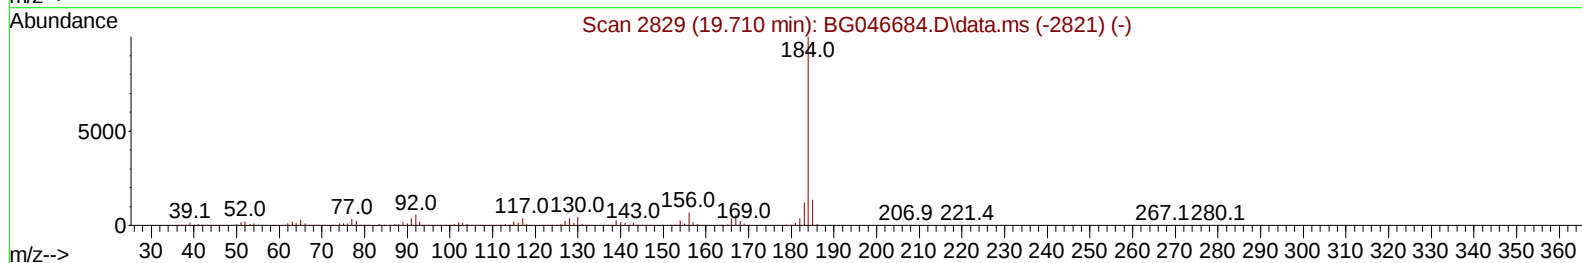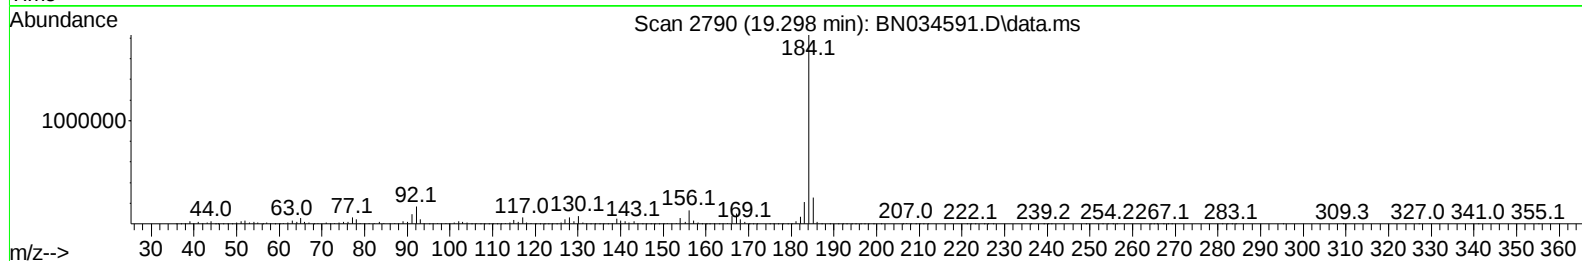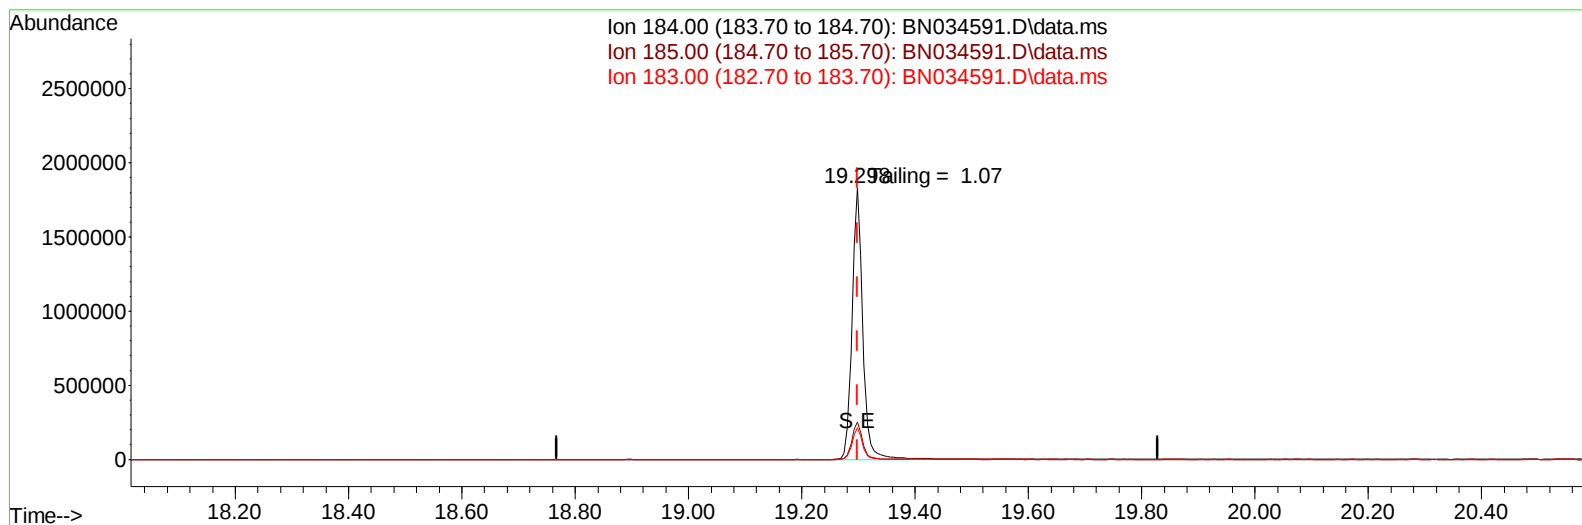

TIC: BN034591.D\data.ms

(77) Benzidine

19.298min (0.000) 428024.92 ng

response 2427701

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.88
183.00	13.20	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/15/2024	BNA_N	<u>BN034591.D</u>
Compound Name	Response	Retention Time
DDT	993177	20.551
DDD	26432	20.11
DDE	800	19.559
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27232	1020409	2.67

Instrument :
BNA_N
ClientSampleId :
DFTPP