
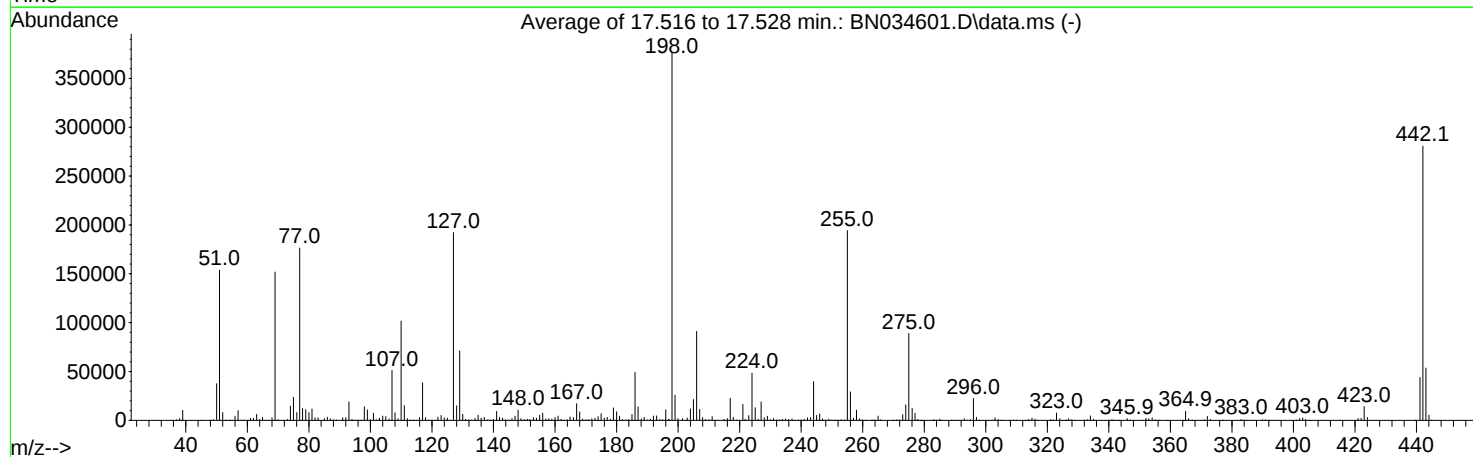


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101524\
Data File : BN034601.D
Acq On : 16 Oct 2024 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN101524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 16 00:09:32 2024

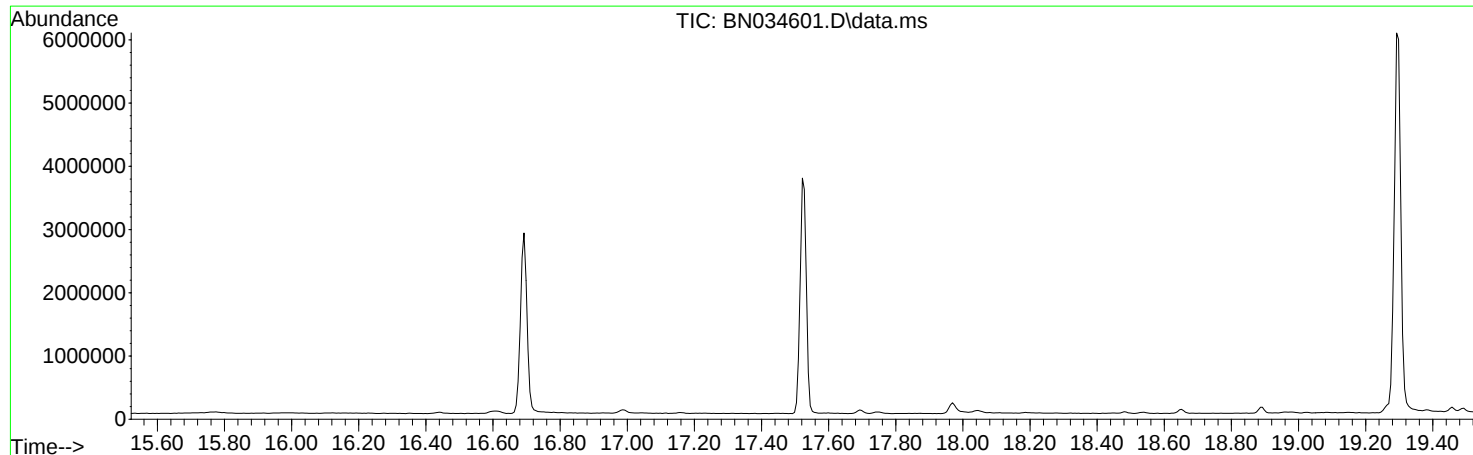




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	153837	PASS
68	69	0.00	2	1.8	2699	PASS
69	198	0.00	100	40.3	151835	PASS
70	69	0.00	2	0.4	632	PASS
127	198	10	80	51.0	192197	PASS
197	198	0.00	2	0.3	1099	PASS
198	198	100	100	100.0	376512	PASS
199	198	5	9	6.8	25789	PASS
275	198	10	60	23.6	88973	PASS
365	198	1	100	2.5	9348	PASS
441	198	0.01	100	11.7	43920	PASS
442	442	50	100	100.0	280704	PASS
443	442	15	24	19.1	53621	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101524\
Data File : BN034601.D
Acq On : 16 Oct 2024 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 16 17:05:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 16 02:02:16 2024
Response via : Initial Calibration

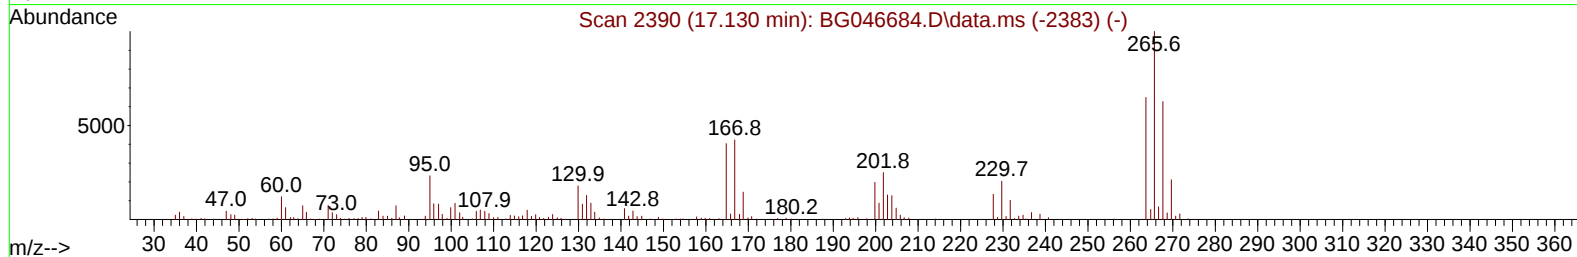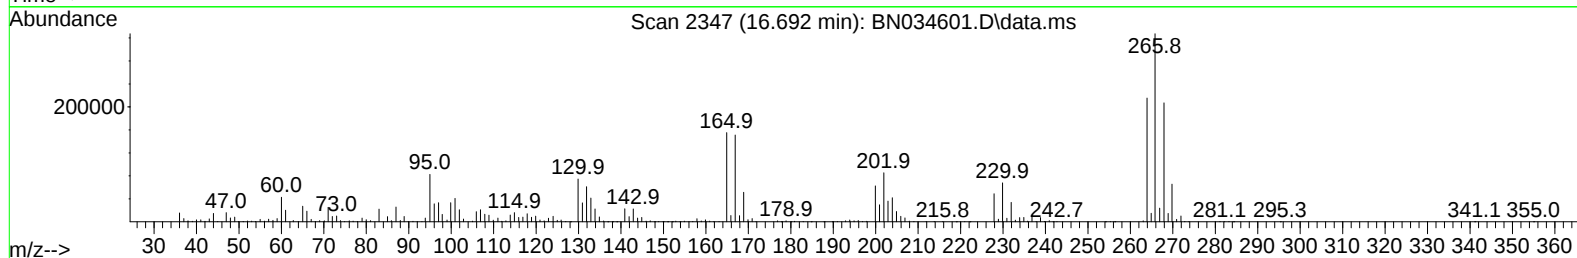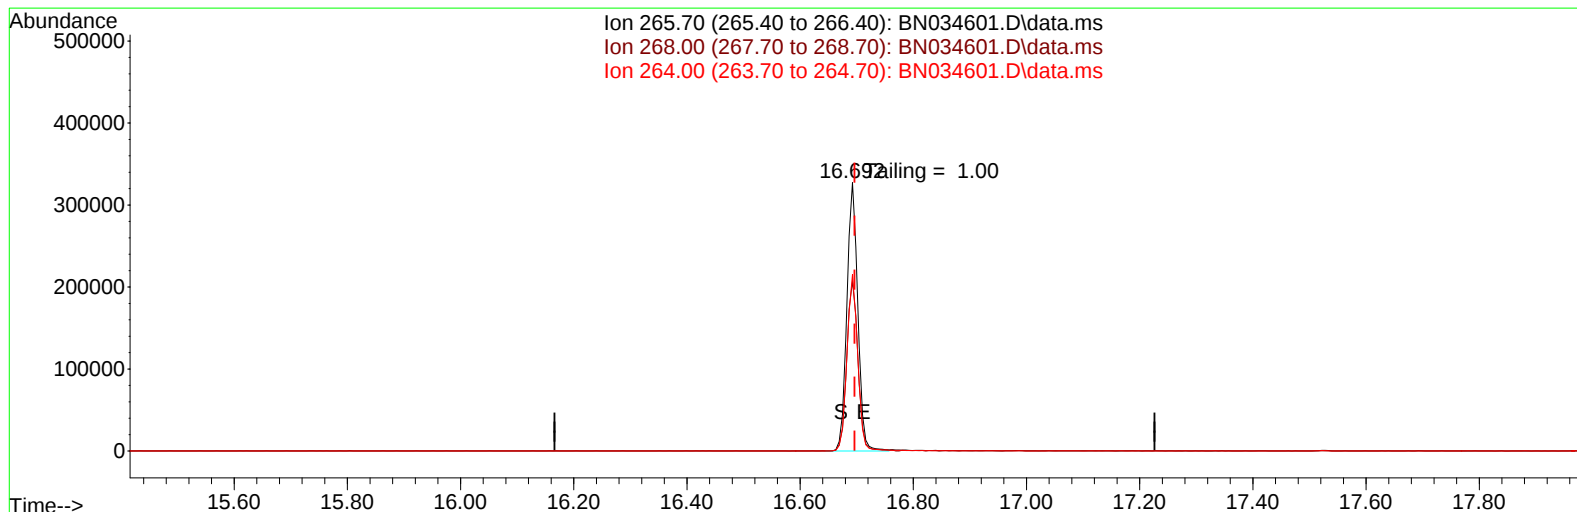

TIC: BN034601.D\data.ms

(70) Pentachlorophenol (C)

16.692min (-0.003) 206159.16 ng m




response 436829

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.24
264.00	61.60	65.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101524\
Data File : BN034601.D
Acq On : 16 Oct 2024 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 16 17:05:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 16 02:02:16 2024
Response via : Initial Calibration

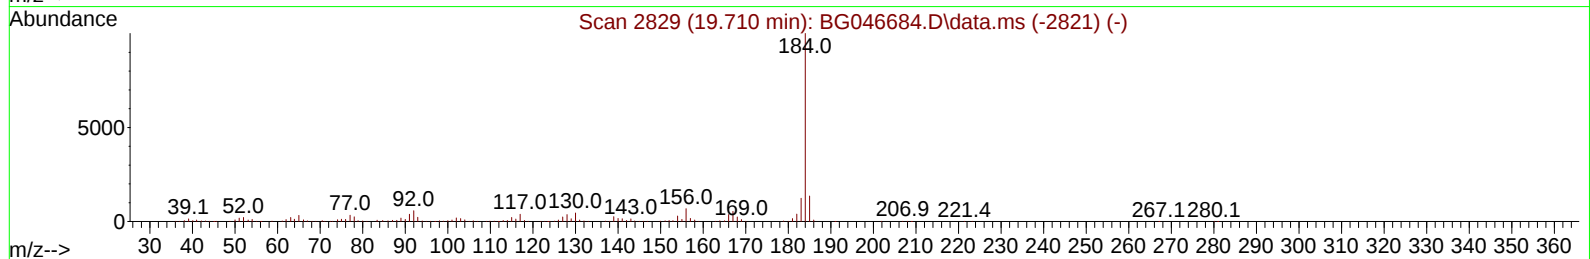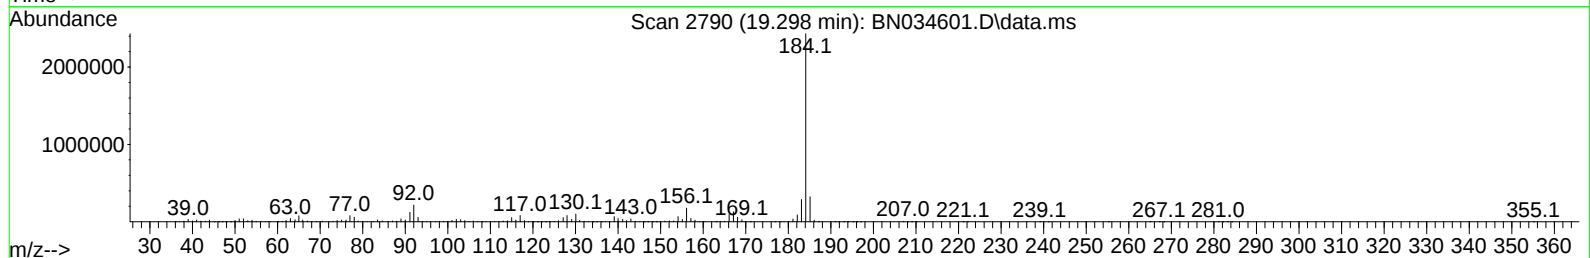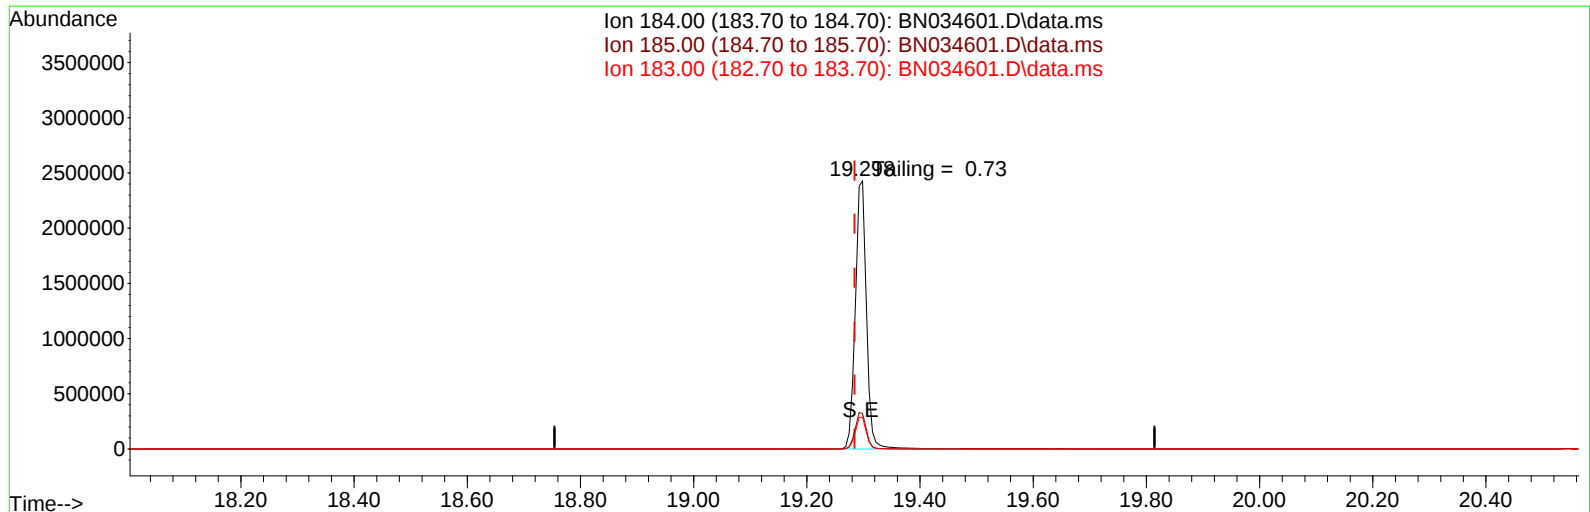

TIC: BN034601.D\data.ms

(77) Benzidine

19.298min (+ 0.014) 51127.30 ng m

response 3331702

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.28
183.00	13.20	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/16/2024	BNA_N	<u>BN034601.D</u>
Compound Name	Response	Retention Time
DDT	1230050	20.545
DDD	24457	20.104
DDE	1290	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25747	1255797	2.05

Instrument :
BNA_N
ClientSampleId :
DFTPP