

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101720\
 Data File : BN012295.D
 Acq On : 17 Oct 2020 16:32
 Operator : CG/JU
 Sample : PB132241BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK41

Quant Time: Oct 19 00:33:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 17 15:47:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	265470	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	1114399	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.25	164	695997	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	1469790	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	1391544	20.00	ng/ul	0.00
86) Perylene-d12	23.37	264	1400390	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	39143	6.79	ng/uL	0.00
5) Phenol-d5	6.78	99	722143	30.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	446513	31.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	594353	31.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	579334	30.22	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	286403	30.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	336150	31.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	555264	29.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	794237	33.94	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	1906947	33.76	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	2225437	32.83	ng/ul	0.00
52) 4-Nitrophenol-d4	14.45	143	311329	28.87	ng/ul	0.00
58) Fluorene-d10	15.24	176	1516468	31.41	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.37	200	301302	29.26	ng/ul	0.00
71) Anthracene-d10	17.09	188	2357443	32.64	ng/ul	0.00
79) Pyrene-d10	19.39	212	2541138	33.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.23	264	2713928	33.57	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.30	70	15822	1.017	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101720\
Data File : BN012295.D
Acq On : 17 Oct 2020 16:32
Operator : CG/JU
Sample : PB132241BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK41

Quant Time: Oct 19 00:33:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 17 15:47:34 2020
Response via : Initial Calibration

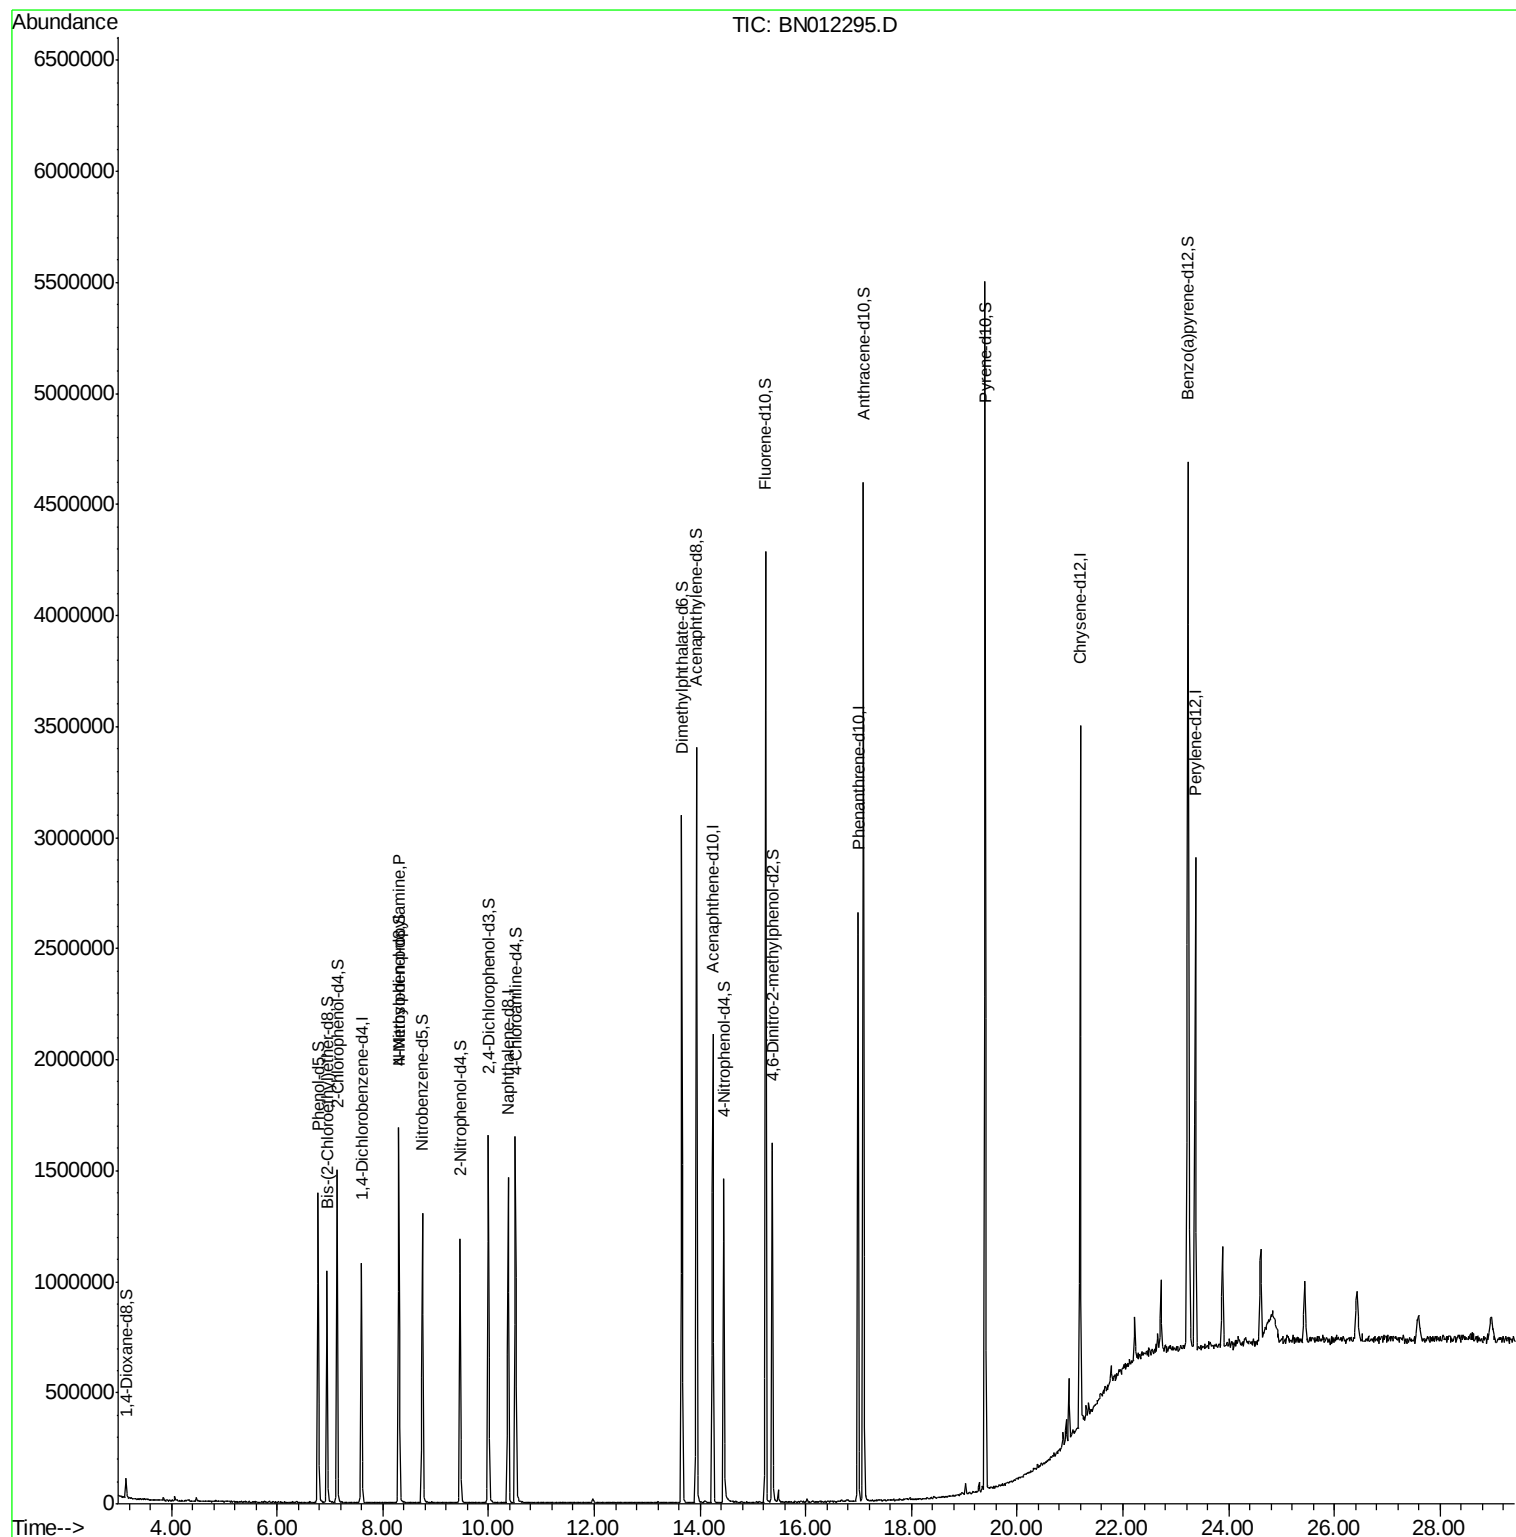

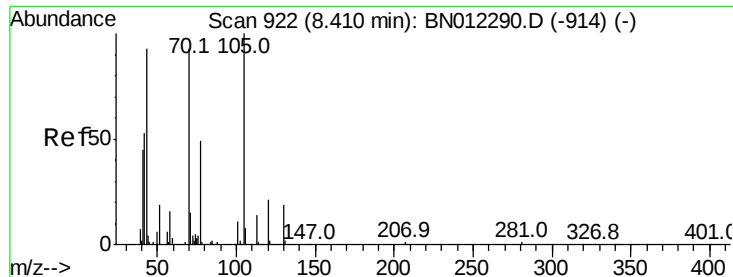

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.017 ng/ul
 RT: 8.30 min Scan# 904
 Delta R.T. -0.11 min
 Lab File: BN012295.D
 Acq: 17 Oct 2020 16:32

Instrument :
 BNA_N
 ClientSampleId :
 SBLK41

Tot Ion:	70	Resp:	15822
Ion	Ratio	Lower	Upper
70	100		
42	392.1	46.2	69.4#
101	0.0	9.0	13.6#
130	0.0	16.5	24.7#

