

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101720\
 Data File : BN012315.D
 Acq On : 18 Oct 2020 05:10
 Operator : CG/JU
 Sample : L4286-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AQ8

Quant Time: Oct 19 01:05:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 19 01:01:46 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	256509	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	1064962	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	640428	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	1305531	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	1258309	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	1279537	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	32827	5.90	ng/uL	0.00
5) Phenol-d5	6.78	99	136539	5.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	362792	26.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	399021	22.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	260228	14.05	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	239190	26.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	273753	26.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	463347	25.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	40190	1.80	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	1581341	30.43	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	1883255	30.19	ng/ul	0.00
52) 4-Nitrophenol-d4	14.45	143	53361	5.38	ng/ul	0.00
58) Fluorene-d10	15.24	176	1361734	30.66	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.36	200	255561	27.94	ng/ul	0.00
71) Anthracene-d10	17.09	188	2117135	33.00	ng/ul	0.00
79) Pyrene-d10	19.39	212	2328188	34.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.23	264	2453387	33.21	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.70	163	100673	1.859 ng/ul# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101720\
Data File : BN012315.D
Acq On : 18 Oct 2020 05:10
Operator : CG/JU
Sample : L4286-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AQ8

Quant Time: Oct 19 01:05:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 19 01:01:46 2020
Response via : Initial Calibration

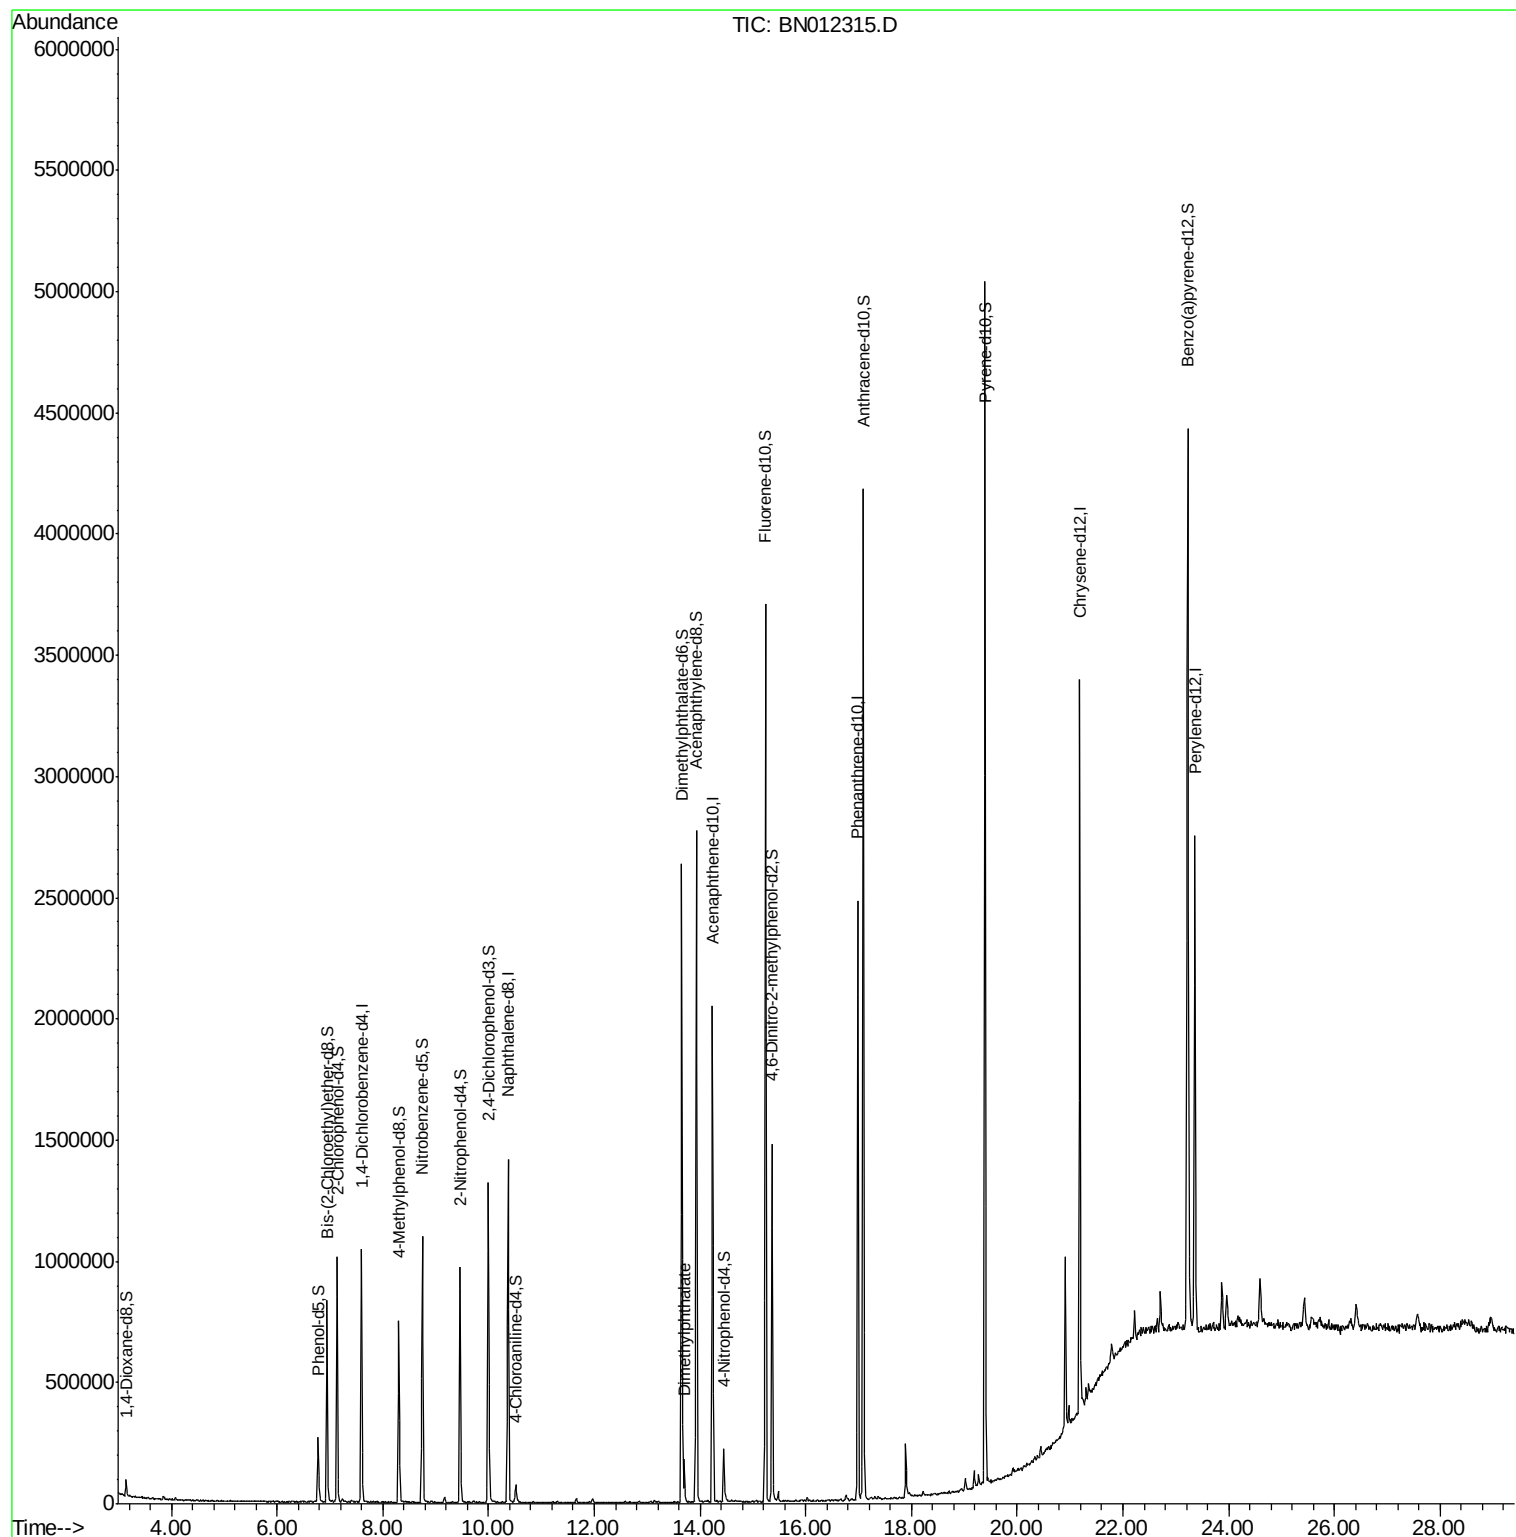

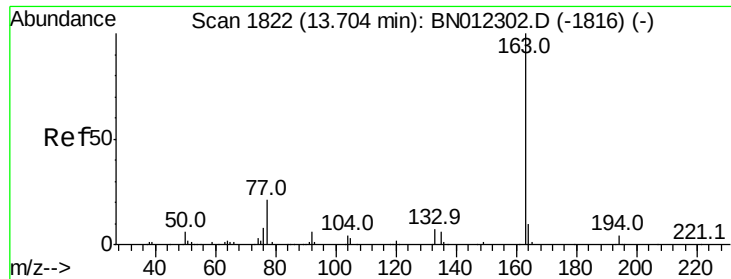

#45

Dimethylphthalate

Concen: 1.859 ng/ul

RT: 13.70 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BN012315.D

Acq: 18 Oct 2020 05:10

Instrument :

BNA_N

ClientSampleId :

C0AQ8


Tot Ion:163 Resp: 100673

Ion Ratio Lower Upper

163 100

194 3.2 3.3 4.9#

164 9.6 7.9 11.9

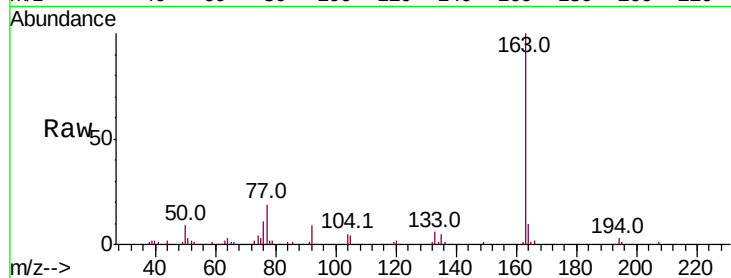

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

