

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101720\
 Data File : BN012323.D
 Acq On : 18 Oct 2020 10:34
 Operator : CG/JU
 Sample : L4286-09
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AQ9

Quant Time: Oct 19 02:24:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 19 02:21:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	231428	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	961165	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	600699	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	1256323	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	1204283	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	1283639	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	28651	5.70	ng/uL	0.00
5) Phenol-d5	6.78	99	115279	5.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	314974	25.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	347183	21.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	225037	13.47	ng/ul	-0.01
19) Nitrobenzene-d5	8.75	128	210169	25.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	247793	27.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	414274	25.23	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	32835	1.63	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	1519081	31.16	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	1718673	29.38	ng/ul	0.00
52) 4-Nitrophenol-d4	14.45	143	44320	4.76	ng/ul	0.00
58) Fluorene-d10	15.24	176	1262639	30.31	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.36	200	244647	27.79	ng/ul	0.00
71) Anthracene-d10	17.09	188	2026671	32.83	ng/ul	0.00
79) Pyrene-d10	19.39	212	2271964	34.89	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.23	264	2433260	32.83	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.70	163	80714	1.589	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101720\
Data File : BN012323.D
Acq On : 18 Oct 2020 10:34
Operator : CG/JU
Sample : L4286-09
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AQ9

Quant Time: Oct 19 02:24:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 19 02:21:59 2020
Response via : Initial Calibration

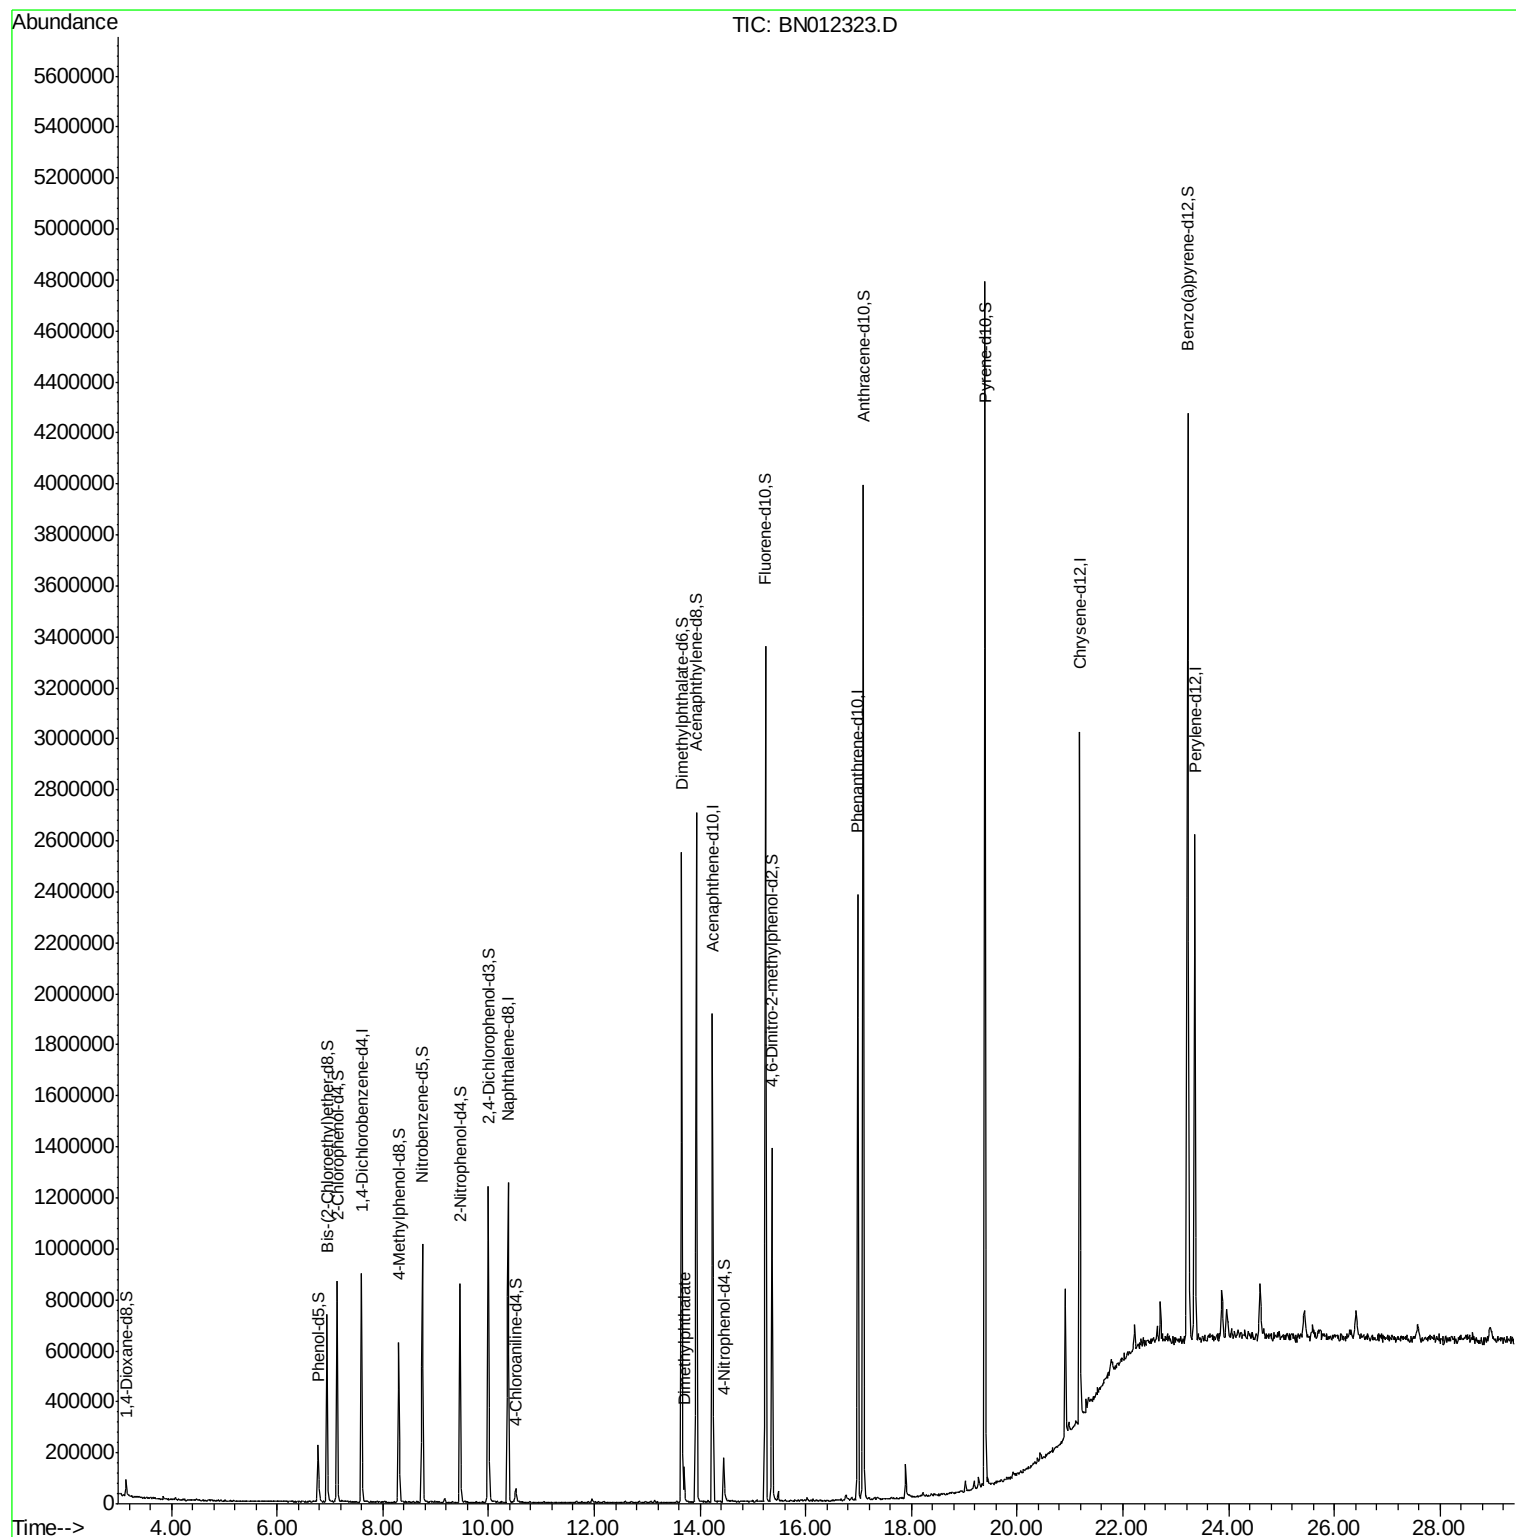

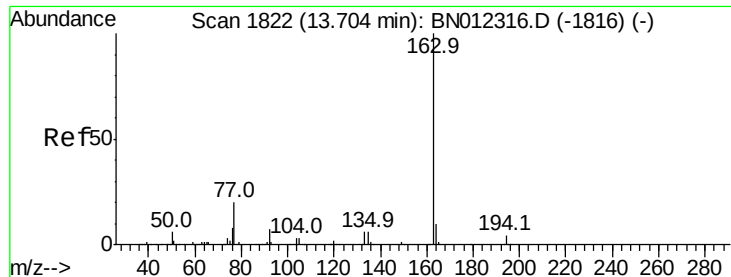

#45

Dimethylphthalate

Concen: 1.589 ng/ul

RT: 13.70 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BN012323.D

Acq: 18 Oct 2020 10:34

Instrument :

BNA_N

ClientSampleId :

C0AQ9


Tot Ion:163 Resp: 80714

Ion Ratio Lower Upper

163 100

194 3.6 3.3 4.9

164 10.5 7.9 11.9

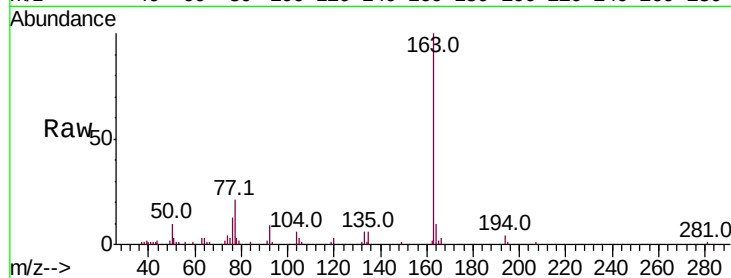

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

