

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101720\
 Data File : BN012301.D
 Acq On : 17 Oct 2020 20:09
 Operator : CG/JU
 Sample : L4235-19
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AT5

Quant Time: Oct 19 00:34:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 17 15:47:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	220275	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	892500	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	567065	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	1143405	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	1134134	20.00	ng/ul	0.00
86) Perylene-d12	23.37	264	1175237	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	14997	3.14	ng/uL	0.00
5) Phenol-d5	6.78	99	258978	13.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	182799	15.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	219891	14.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	216756	13.63	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	111825	14.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	126162	14.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	202070	13.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.51	131	287700	15.35	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	791734	17.21	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	815135	14.76	ng/ul	0.00
52) 4-Nitrophenol-d4	14.45	143	87420	9.95	ng/ul	0.00
58) Fluorene-d10	15.24	176	597891	15.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.36	200	97806	12.21	ng/ul	0.00
71) Anthracene-d10	17.09	188	868581	15.46	ng/ul	0.00
79) Pyrene-d10	19.39	212	968070	15.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.23	264	1022797	15.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.70	163	263568	5.495	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101720\
Data File : BN012301.D
Acq On : 17 Oct 2020 20:09
Operator : CG/JU
Sample : L4235-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AT5

Quant Time: Oct 19 00:34:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 17 15:47:34 2020
Response via : Initial Calibration

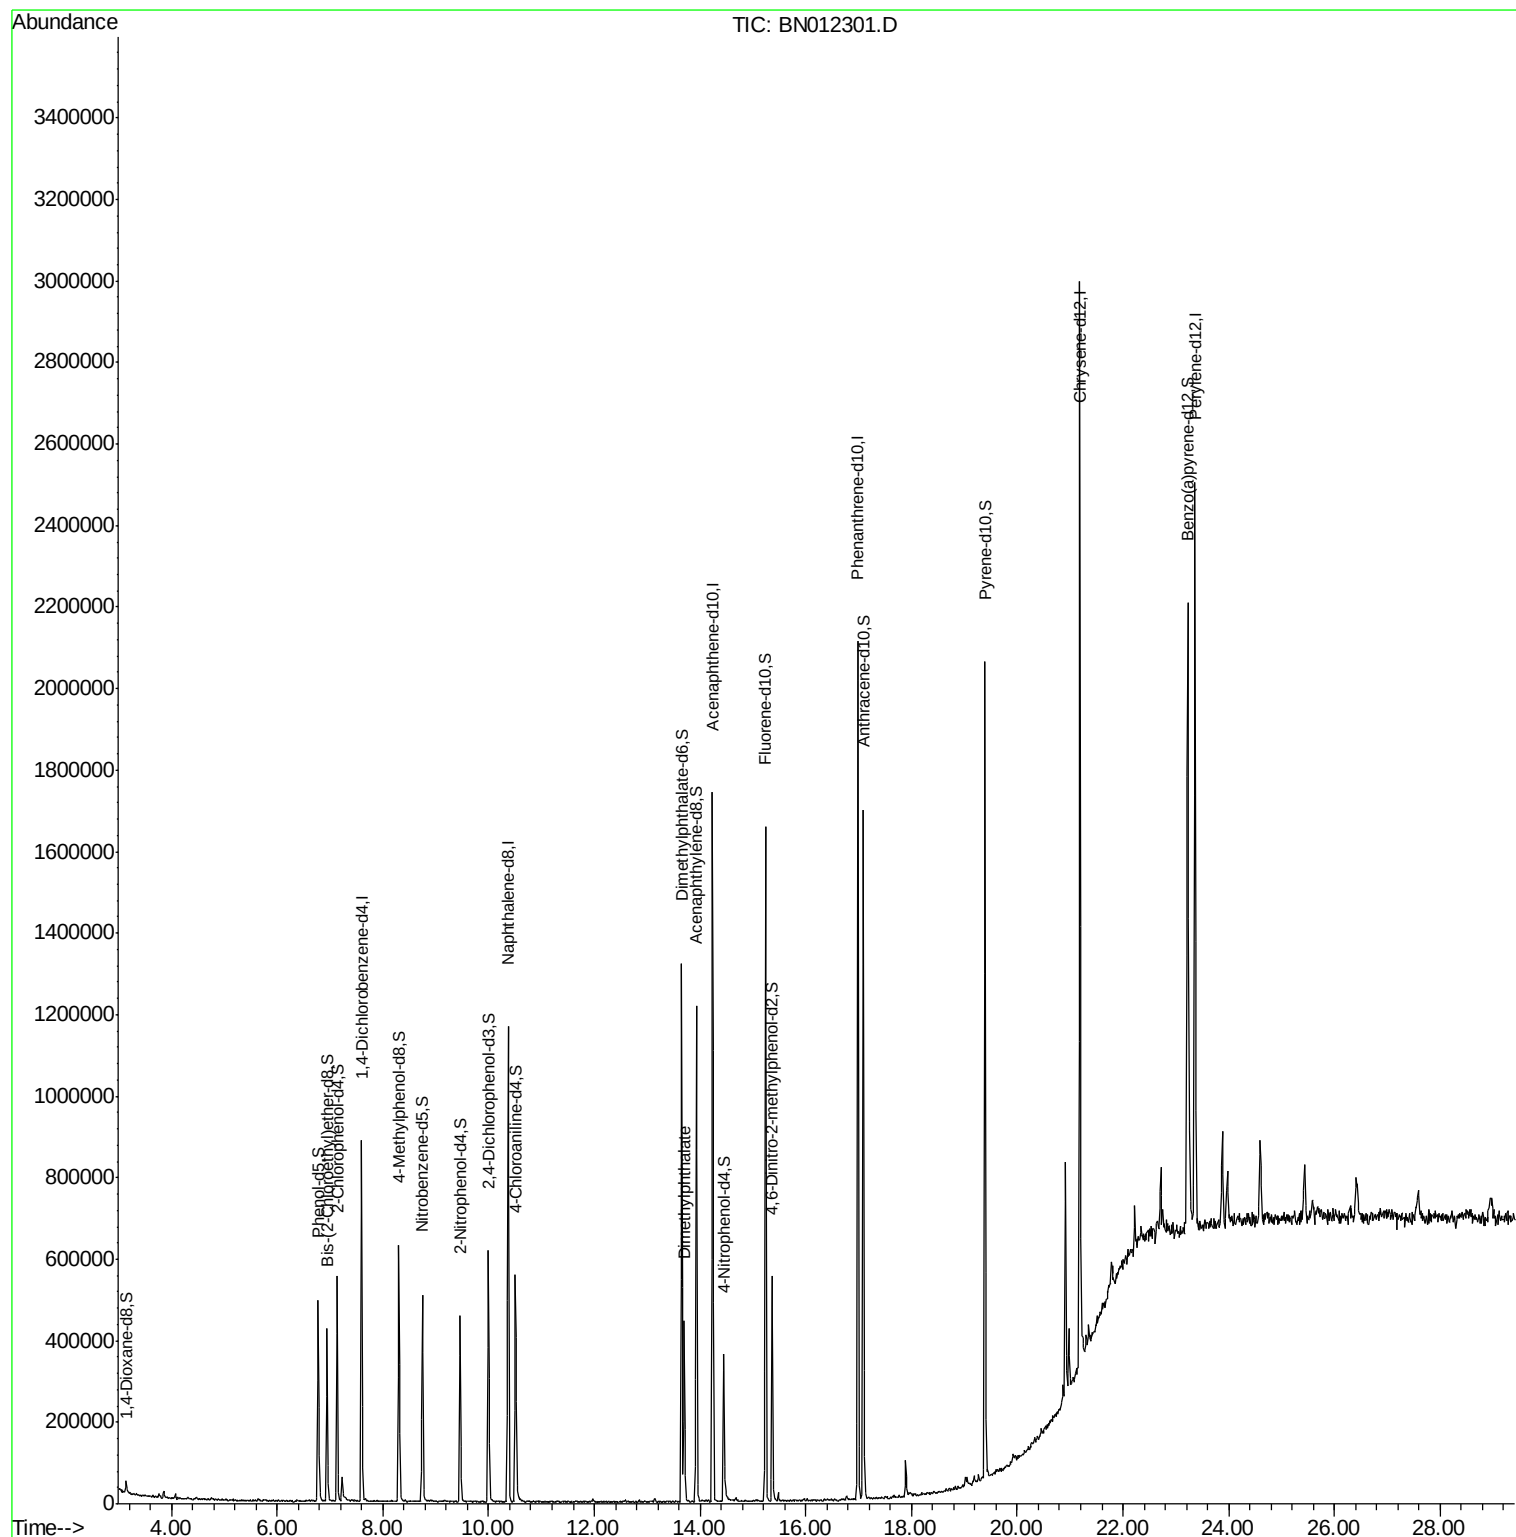

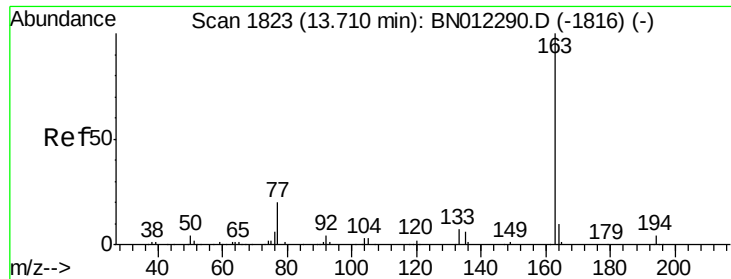

#45

Dimethylphthalate

Concen: 5.495 ng/ul

RT: 13.70 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BN012301.D

Acq: 17 Oct 2020 20:09

Instrument :

BNA_N

ClientSampleId :

C0AT5


Tot Ion:163 Resp: 263568

Ion Ratio Lower Upper

163 100

194 3.7 3.3 4.9

164 10.6 7.9 11.9

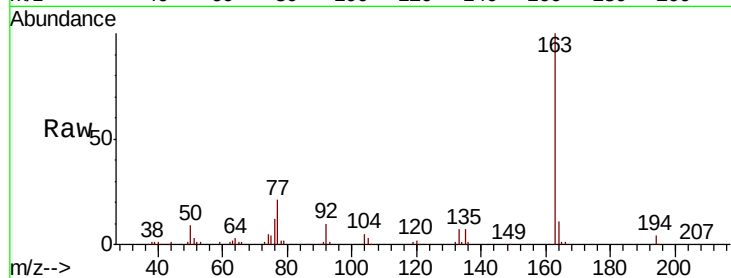

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

