

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101720\
 Data File : BN012321.D
 Acq On : 18 Oct 2020 09:22
 Operator : CG/JU
 Sample : L4286-02
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AR8

Quant Time: Oct 19 02:24:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 19 02:21:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	253880	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	1090007	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.24	164	689262	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	1383138	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	1359113	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	1372195	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	29899	5.42	ng/uL	0.00
5) Phenol-d5	6.78	99	131032	5.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	347267	25.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	382359	21.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	249398	13.61	ng/ul	-0.01
19) Nitrobenzene-d5	8.75	128	237002	25.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	269196	25.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	451431	24.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	45695	2.00	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	1680854	30.05	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	1967482	29.31	ng/ul	0.00
52) 4-Nitrophenol-d4	14.45	143	52863	4.95	ng/ul	0.00
58) Fluorene-d10	15.24	176	1401637	29.32	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.36	200	274637	28.34	ng/ul	0.00
71) Anthracene-d10	17.09	188	2375801	34.96	ng/ul	0.00
79) Pyrene-d10	19.39	212	2598945	35.37	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.23	264	2781027	35.11	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.70	163	113844	1.953	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101720\
Data File : BN012321.D
Acq On : 18 Oct 2020 09:22
Operator : CG/JU
Sample : L4286-02
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AR8

Quant Time: Oct 19 02:24:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 19 02:21:59 2020
Response via : Initial Calibration

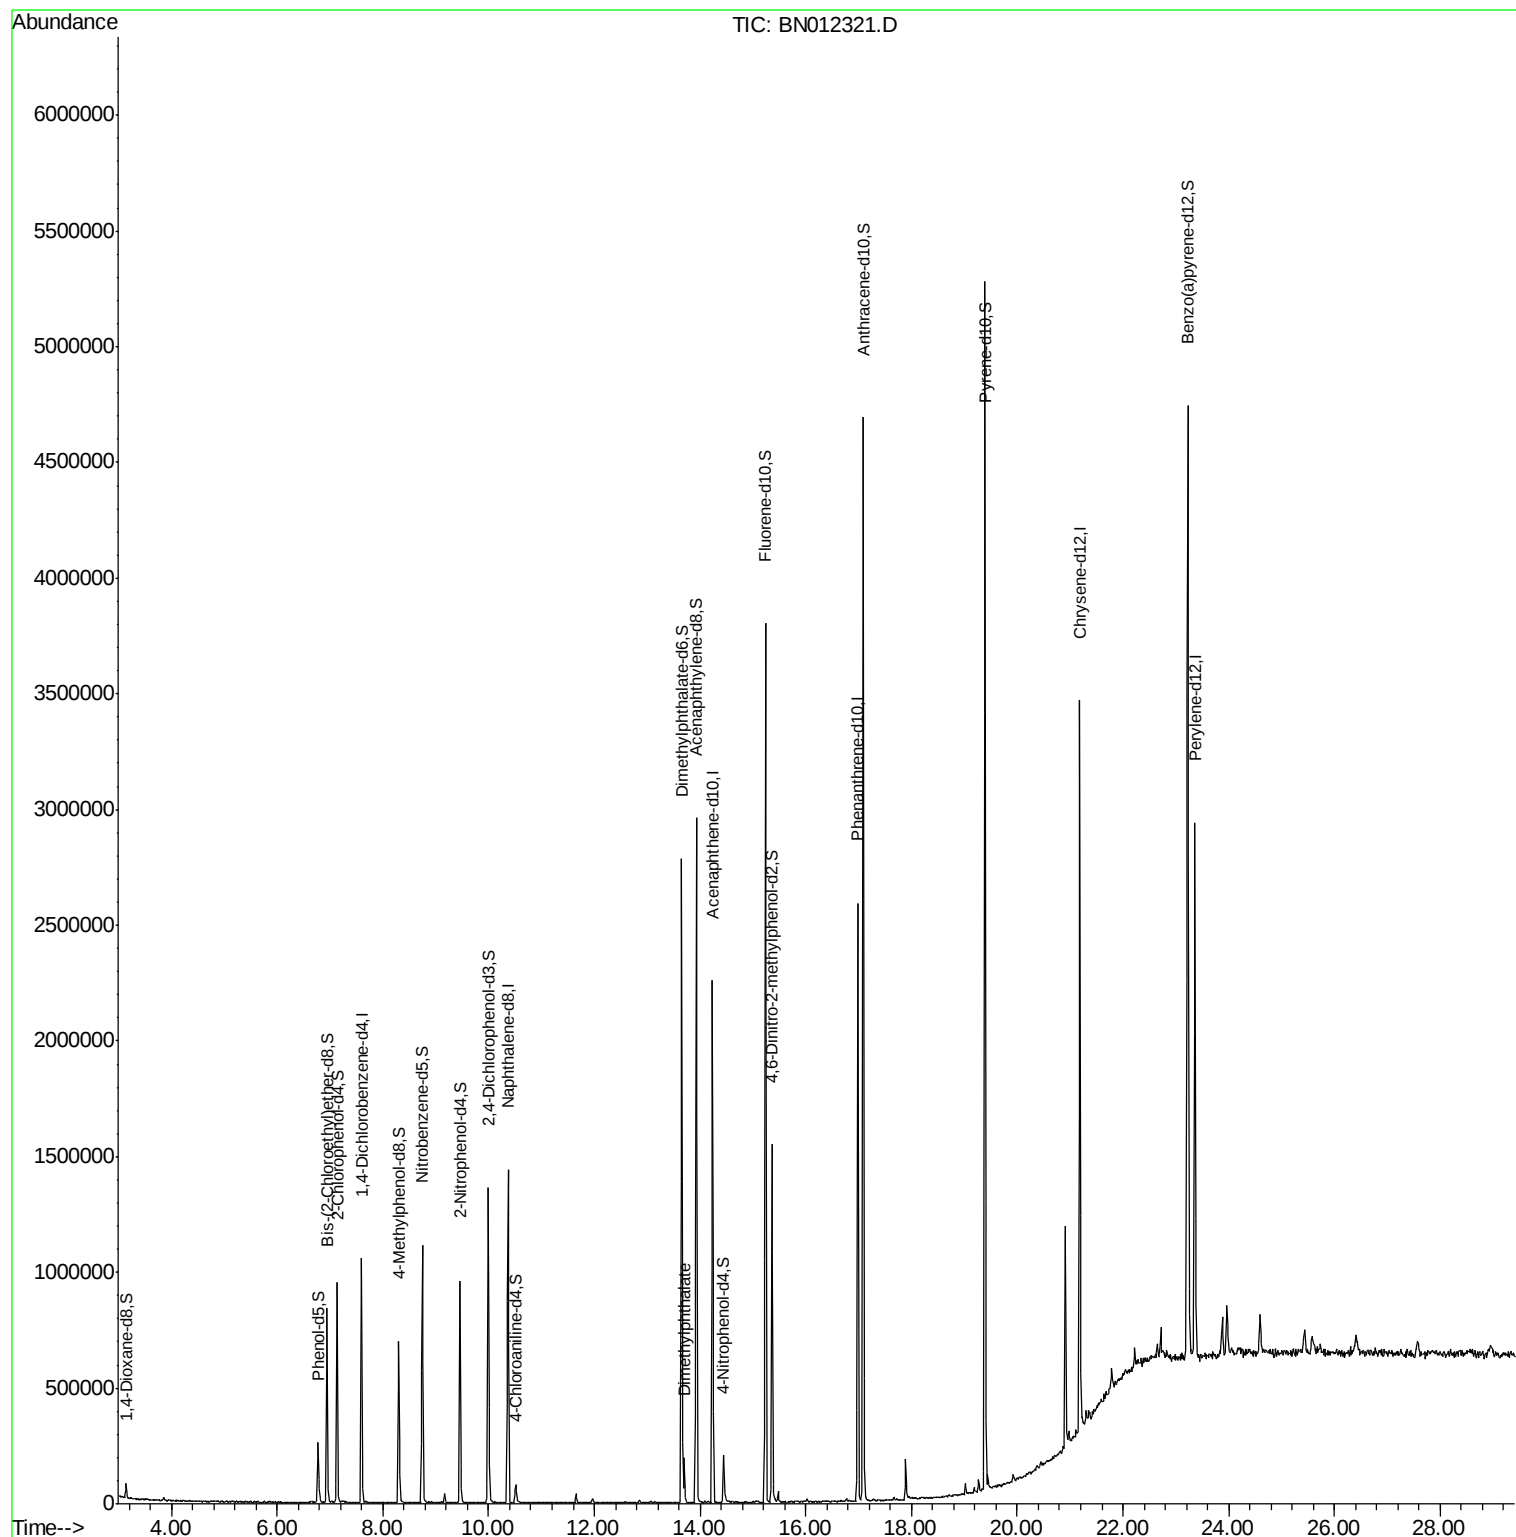

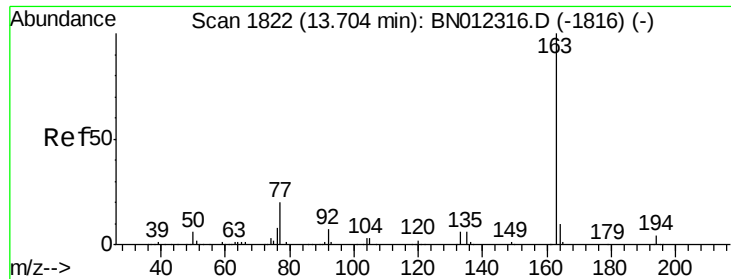

#45

Dimethylphthalate

Concen: 1.953 ng/ul

RT: 13.70 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BN012321.D

Acq: 18 Oct 2020 09:22

Instrument :

BNA_N

ClientSampleId :

C0AR8


Tot Ion:163 Resp: 113844

Ion Ratio Lower Upper

163 100

194 4.4 3.3 4.9

164 10.5 7.9 11.9

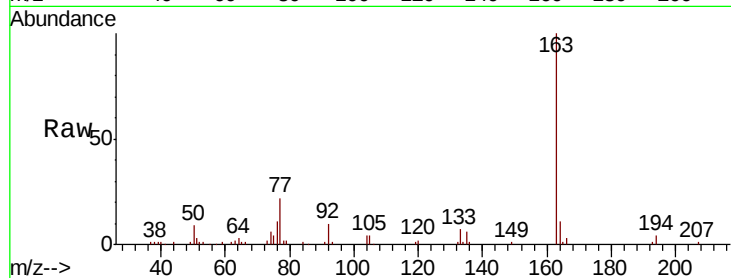

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

