

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101720\
 Data File : BN012313.D
 Acq On : 18 Oct 2020 03:58
 Operator : CG/JU
 Sample : L4235-14
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AP9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	37	rVB	84134	117257	1.78%	0.160%
2	3.858	145	148	153	rVB4	14073	19443	0.29%	0.026%
3	4.075	181	185	189	rBV3	20354	23641	0.36%	0.032%
4	4.323	221	227	229	rBV6	7845	12957	0.20%	0.018%
5	4.475	250	253	260	rVB5	13571	23216	0.35%	0.032%
6	4.846	314	316	320	rBV4	4901	6682	0.10%	0.009%
7	6.781	636	645	656	rBV	1360968	2113029	32.00%	2.876%
8	6.946	665	673	682	rBV	1048850	1590658	24.09%	2.165%
9	7.134	697	705	714	rBV	1447067	2228782	33.76%	3.033%
10	7.240	721	723	729	rVV4	6648	10889	0.16%	0.015%
11	7.599	777	784	793	rVB	1025603	1574553	23.85%	2.143%
12	8.305	897	904	919	rBV	1692940	2627594	39.80%	3.576%
13	8.752	972	980	990	rBV	1282645	2100597	31.82%	2.859%
14	9.463	1094	1101	1110	rBV	1176912	1865683	28.26%	2.539%
15	9.999	1184	1192	1203	rBV	1638866	2720637	41.21%	3.703%
16	10.369	1248	1255	1263	rBV	1351978	2249884	34.08%	3.062%
17	10.510	1272	1279	1298	rBV	1581345	2723527	41.25%	3.707%
18	11.975	1520	1528	1537	rBV3	18973	42113	0.64%	0.057%
19	13.140	1724	1726	1732	rVB3	8234	10418	0.16%	0.014%
20	13.657	1802	1814	1819	rBV	2989241	3932177	59.56%	5.352%
21	13.704	1819	1822	1828	rVB	186024	235291	3.56%	0.320%
22	13.934	1854	1861	1869	rBV	3339286	4758597	72.07%	6.476%
23	14.240	1906	1913	1921	rBV	2047717	3007962	45.56%	4.094%
24	14.451	1941	1949	1970	rBV	1298657	1984202	30.05%	2.700%
25	15.240	2076	2083	2095	rBV	4161538	5608232	84.94%	7.633%
26	15.363	2098	2104	2114	rBV	1417341	1907626	28.89%	2.596%
27	15.481	2119	2124	2129	rVB2	46870	70234	1.06%	0.096%
28	15.810	2174	2180	2183	rBV4	5955	10268	0.16%	0.014%
29	16.028	2213	2217	2220	rBV4	17371	23707	0.36%	0.032%
30	16.675	2325	2327	2333	rVB5	7326	10580	0.16%	0.014%
31	16.775	2341	2344	2352	rVB7	11382	20294	0.31%	0.028%
32	16.987	2374	2380	2387	rBV	2462362	3387007	51.30%	4.610%
33	17.087	2391	2397	2408	rVV2	4146699	5756021	87.18%	7.834%
34	17.251	2421	2425	2429	rBV7	9197	17349	0.26%	0.024%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101720\
Data File : BN012313.D
Acq On : 18 Oct 2020 03:58
Operator : CG/JU
Sample : L4235-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP9

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
Title : SVOA CALIBRATION

35	17.381	2442	2447	2448	rBV4	5376	7877	0.12%	0.011%
36	17.675	2492	2497	2499	rBV6	5393	8965	0.14%	0.012%
37	17.704	2499	2502	2506	rBV4	6248	9896	0.15%	0.013%
38	17.892	2530	2534	2540	rBV5	42087	61860	0.94%	0.084%
39	18.498	2635	2637	2640	rBV4	11221	11037	0.17%	0.015%
40	19.022	2722	2726	2729	rBV2	57893	84531	1.28%	0.115%
41	19.134	2743	2745	2748	rBV4	14742	14342	0.22%	0.020%
42	19.275	2766	2769	2774	rVB2	44242	59010	0.89%	0.080%
43	19.392	2783	2789	2796	rBV	4922904	6417191	97.20%	8.734%
44	20.910	3044	3047	3053	rVB4	246439	348370	5.28%	0.474%
45	21.186	3089	3094	3100	rBV	2814474	3538534	53.60%	4.816%
46	23.227	3434	3441	3451	rBV	3452735	6602330	100.00%	8.986%
47	23.363	3458	3464	3471	rVB2	1959481	3521830	53.34%	4.793%


Sum of corrected areas: 73476880

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101720\
Data File : BN012313.D
Acq On : 18 Oct 2020 03:58
Operator : CG/JU
Sample : L4235-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

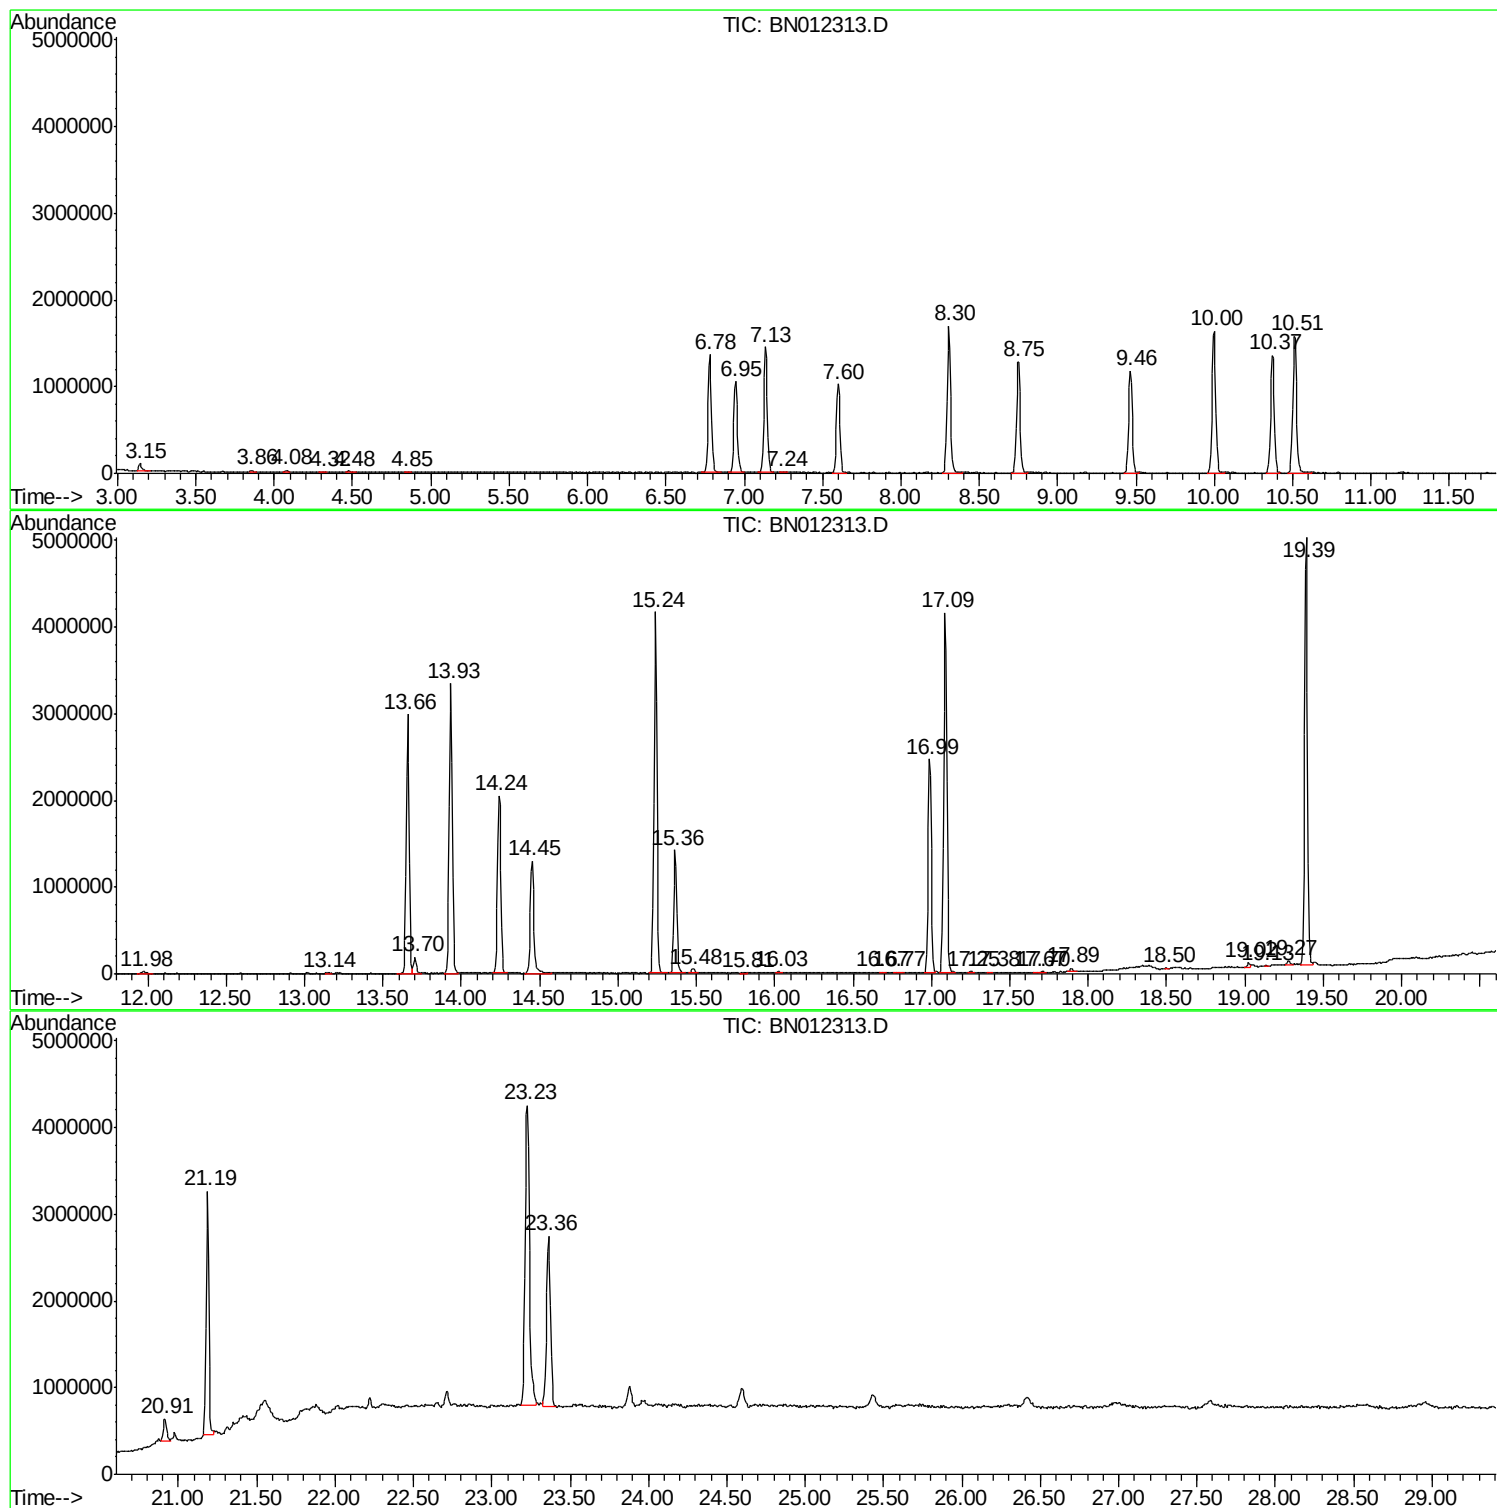

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101720\
Data File : BN012313.D
Acq On : 18 Oct 2020 03:58
Operator : CG/JU
Sample : L4235-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN101720\
Data File : BN012313.D
Acq On : 18 Oct 2020 03:58
Operator : CG/JU
Sample : L4235-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN101720.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc