




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034629.D
Acq On : 17 Oct 2024 19:56
Operator : RC/JU
Sample : P4360-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4FC8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :mohammad ahmed 10/21/2024

Quant Time: Oct 17 23:48:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 15:50:29 2024
Response via : Initial Calibration

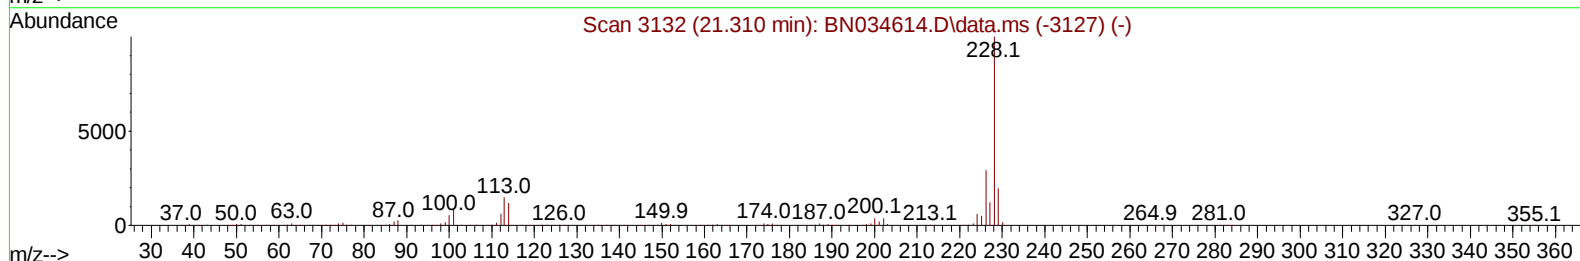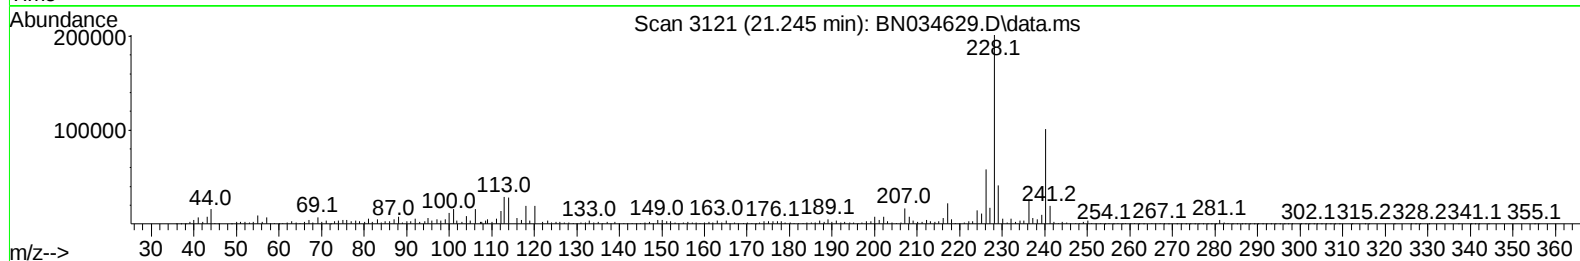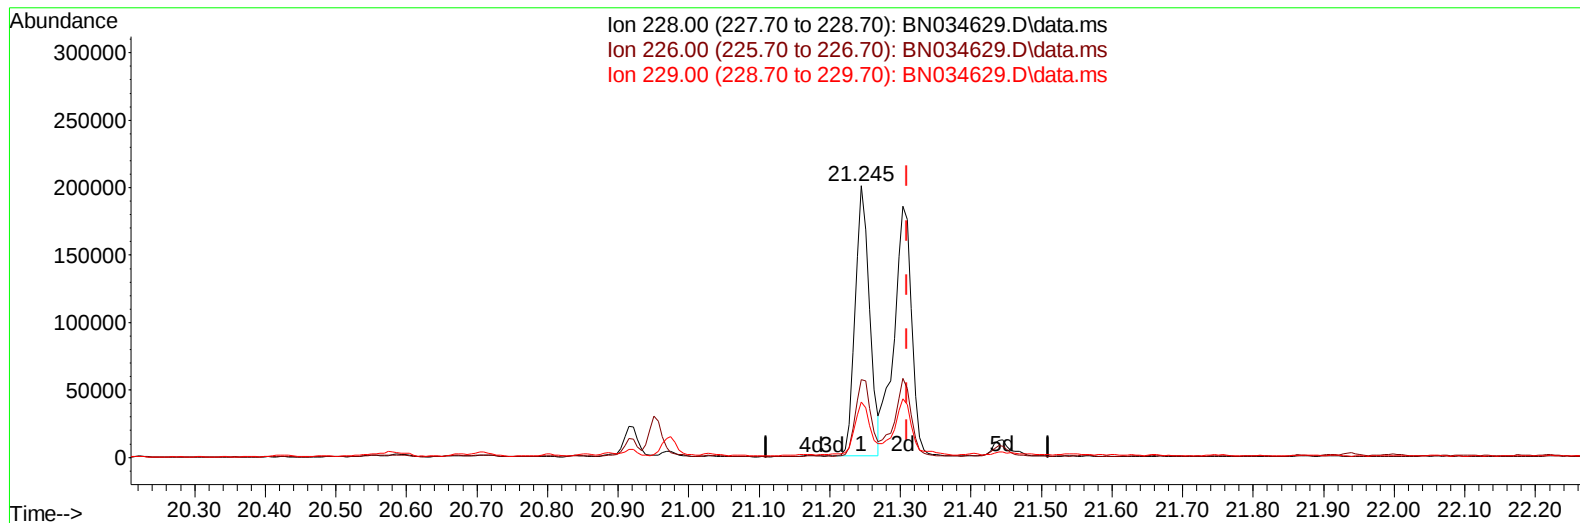

TIC: BN034629.D\data.ms

(87) Chrysene

21.245min (-0.065) 4.59 ng/u1

response 285508

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	28.30	28.76
229.00	19.00	20.49
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034629.D
Acq On : 17 Oct 2024 19:56
Operator : RC/JU
Sample : P4360-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4FC8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :mohammad ahmed 10/21/2024

Quant Time: Oct 17 23:48:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 15:50:29 2024
Response via : Initial Calibration

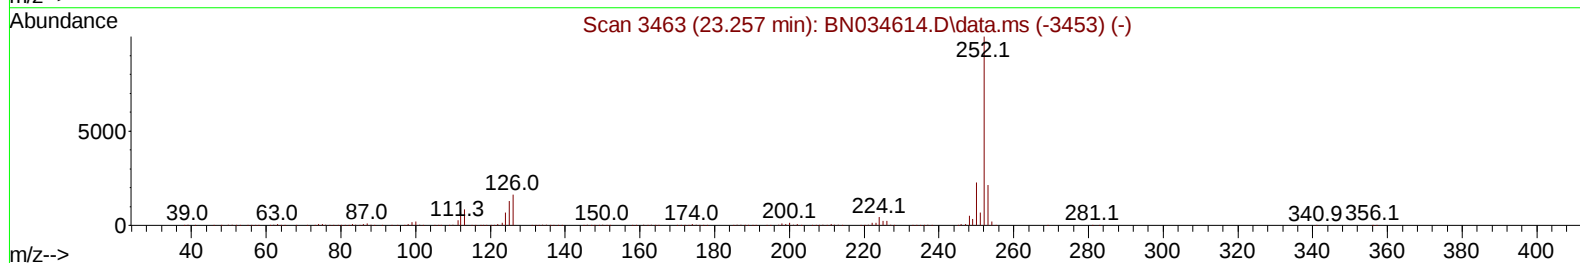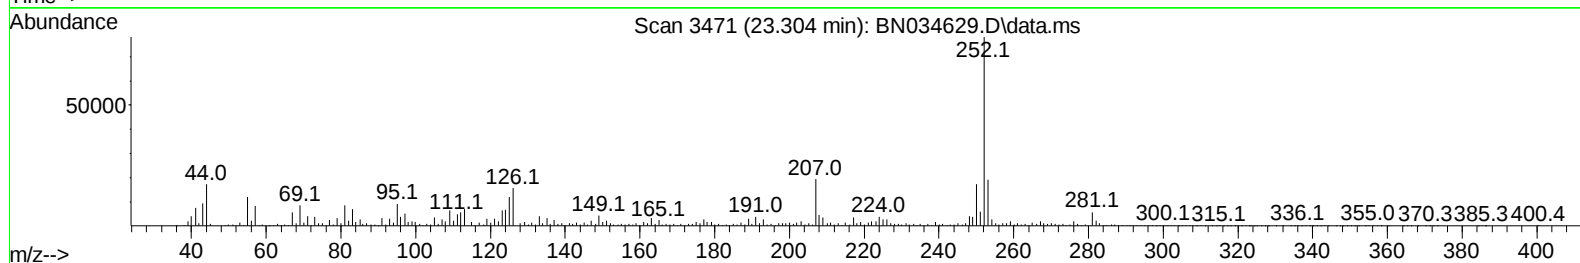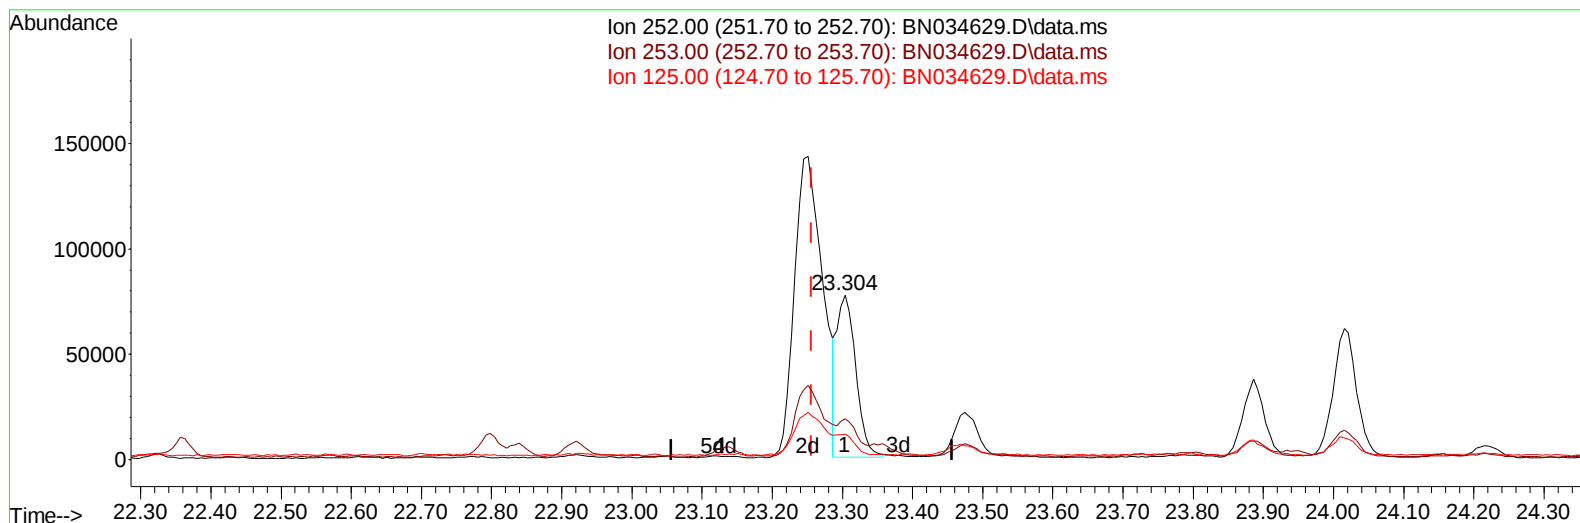

TIC: BN034629.D\data.ms

(90) Benzo(b)fluoranthene

23.304min (+ 0.047) 2.22 ng/u1

response 143853

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.60	24.65
125.00	12.90	15.32
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034629.D
 Acq On : 17 Oct 2024 19:56
 Operator : RC/JU
 Sample : P4360-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4FC8

Manual IntegrationsAPPROVED

Quant Time: Oct 17 23:48:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 16 15:50:29 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/18/2024
 Supervised By :mohammad ahmed 10/21/2024

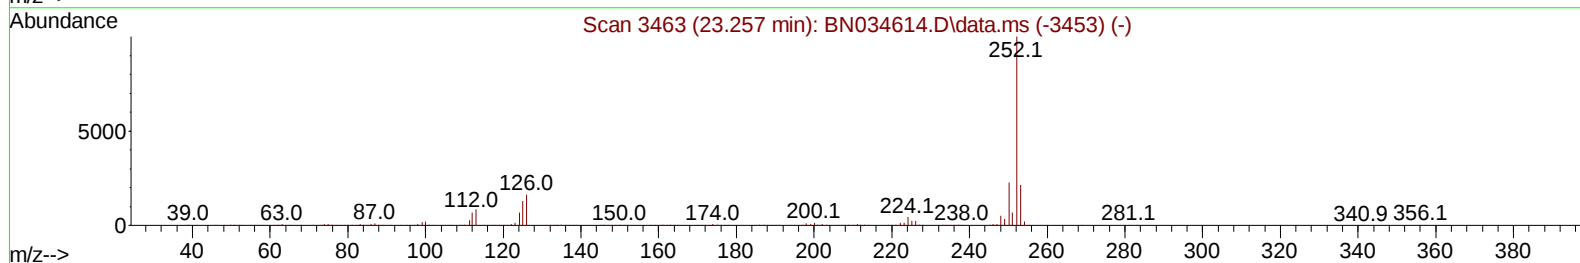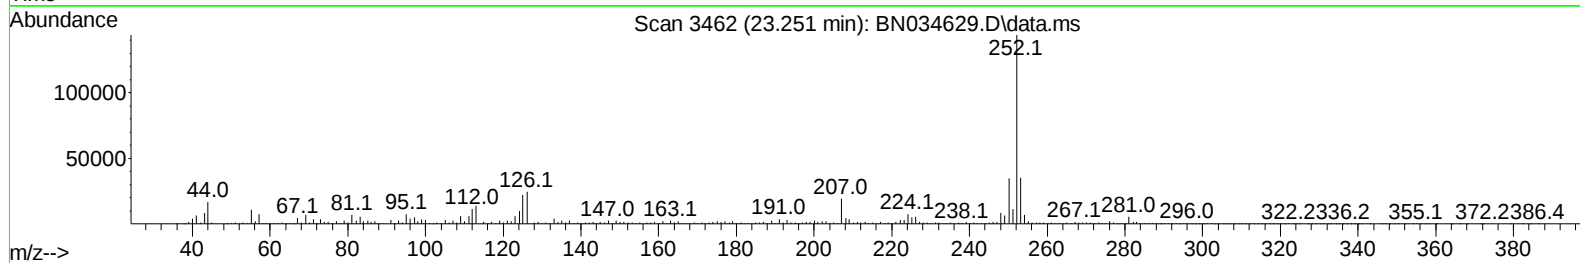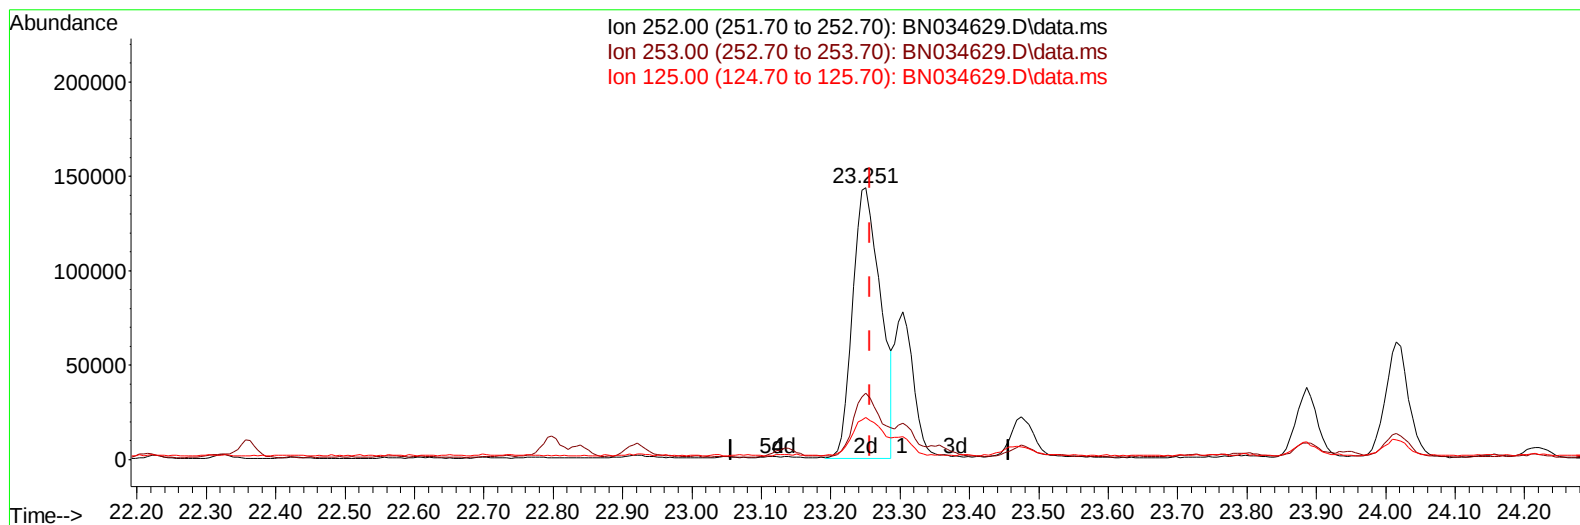

TIC: BN034629.D\data.ms

(90) Benzo(b)fluoranthene

23.251min (-0.006) 6.19 ng/u1 m

response 401583

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.60	24.35
125.00	12.90	15.52#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034629.D
 Acq On : 17 Oct 2024 19:56
 Operator : RC/JU
 Sample : P4360-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4FC8

Manual IntegrationsAPPROVED

Quant Time: Oct 17 23:58:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 16 15:50:29 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/18/2024
 Supervised By :mohammad ahmed 10/21/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.663	152		250708	20.000	ng/ul	0.00
20) Naphthalene-d8	10.440	136		1057467	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.298	164		604762	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.039	188		1153762	20.000	ng/ul	0.00
79) Chrysene-d12	21.263	240		1031370	20.000	ng/ul	0.00
88) Perylene-d12	24.157	264		1207181	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.211	96		12877	2.055	ng/uL	0.00
4) Pyridine-d5	3.605	84		46774	2.557	ng/ul	0.00
7) Phenol-d5	6.834	99		251574	12.227	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67		154650	12.185	ng/ul	0.00
11) 2-Chlorophenol-d4	7.199	132		194993	12.268	ng/ul	0.00
15) 4-Methylphenol-d8	8.357	113		185749	11.584	ng/ul	0.00
21) Nitrobenzene-d5	8.804	128		89662	12.184	ng/ul	0.00
24) 2-Nitrophenol-d4	9.522	143		65936	11.338	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.057	165		172949	12.903	ng/ul	0.00
31) 4-Chloroaniline-d4	10.569	131		109438	4.760	ng/ul	0.00
46) Dimethylphthalate-d6	13.716	166		532963	13.930	ng/ul	0.00
49) Acenaphthylene-d8	13.987	160		650432	13.687	ng/ul	0.00
54) 4-Nitrophenol-d4	14.481	143		66229	9.292	ng/ul	0.00
60) Fluorene-d10	15.292	176		491962	14.867	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200		20066	5.189	ng/ul	0.00
73) Anthracene-d10	17.133	188		730361	14.808	ng/ul	0.00
81) Pyrene-d10	19.433	212		709566	13.399	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.957	264		547664	9.846	ng/ul	-0.01
Target Compounds							
						Qvalue	
8) Phenol	6.858	94		30670	1.428	ng/ul	94
16) Acetophenone	8.475	105		127340	4.973	ng/ul	100
72) Phenanthrene	17.081	178		370561	6.435	ng/ul	98
74) Anthracene	17.169	178		71709	1.205	ng/ul	99
80) Fluoranthene	19.098	202		682364	10.741	ng/ul	97
82) Pyrene	19.457	202		488043	7.212	ng/ul	99
85) Benzo(a)anthracene	21.245	228		286567	4.373	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.221	149		55534	1.411	ng/ul	98
87) Chrysene	21.304	228		327176m	5.260	ng/ul	
90) Benzo(b)fluoranthene	23.251	252		401583m	6.191	ng/ul	
91) Benzo(k)fluoranthene	23.304	252		139147	2.099	ng/ul	93
93) Benzo(a)pyrene	24.015	252		143246	2.281	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	27.386	276		136999	1.748	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034629.D
Acq On : 17 Oct 2024 19:56
Operator : RC/JU
Sample : P4360-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4FC8

Manual IntegrationsAPPROVED

Quant Time: Oct 17 23:58:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 15:50:29 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :mohammad ahmed 10/21/2024

