




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034639.D
Acq On : 18 Oct 2024 02:29
Operator : RC/JU
Sample : P4346-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EOAX7

Manual IntegrationsAPPROVED

Quant Time: Oct 18 03:12:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 15:50:29 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :mohammad ahmed 10/21/2024

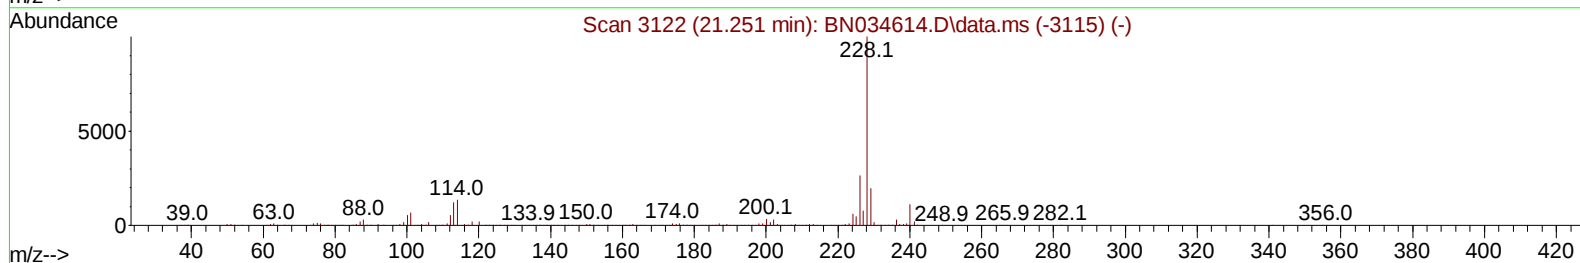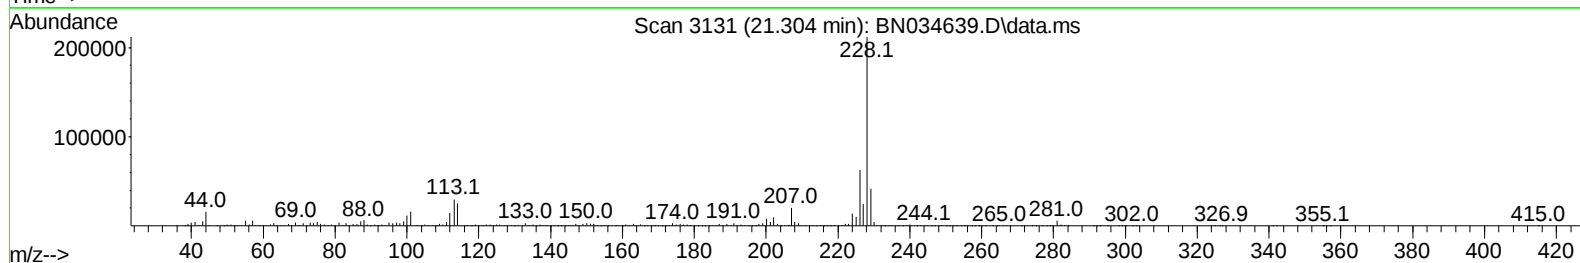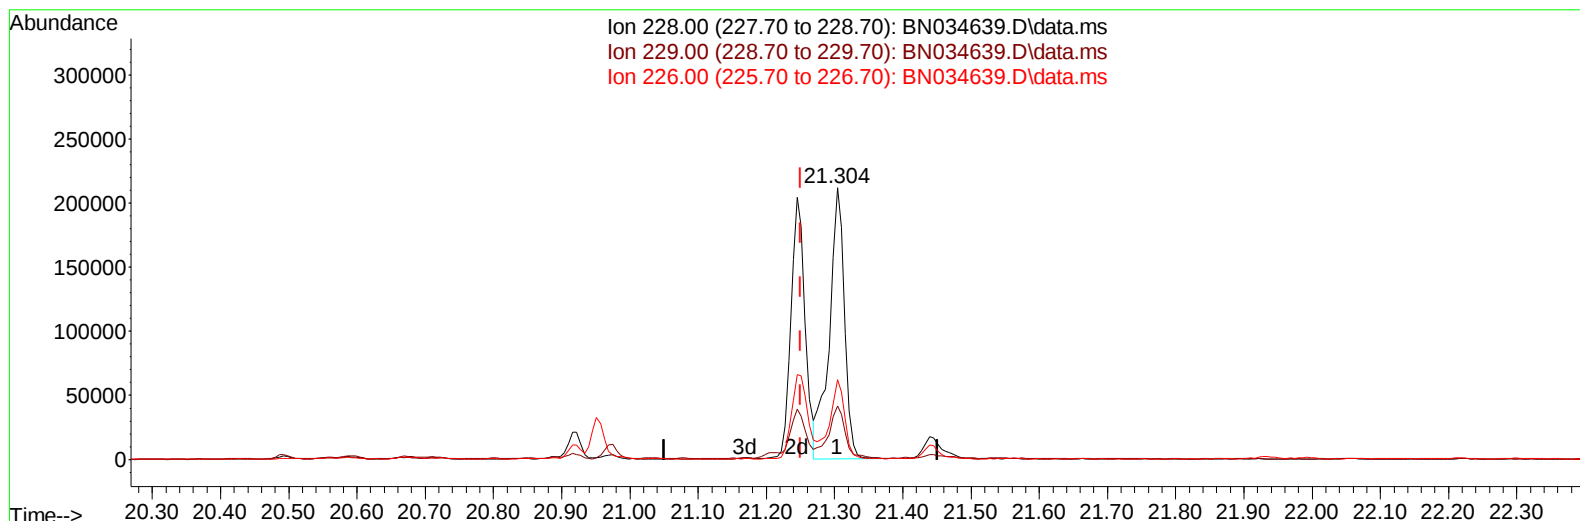

TIC: BN034639.D\data.ms

(85) Benzo(a)anthracene

21.304min (+ 0.053) 5.06 ng/u1

response 327597

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.60	19.82
226.00	26.60	29.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034639.D
Acq On : 18 Oct 2024 02:29
Operator : RC/JU
Sample : P4346-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EOAX7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :mohammad ahmed 10/21/2024

Quant Time: Oct 18 03:12:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 15:50:29 2024
Response via : Initial Calibration

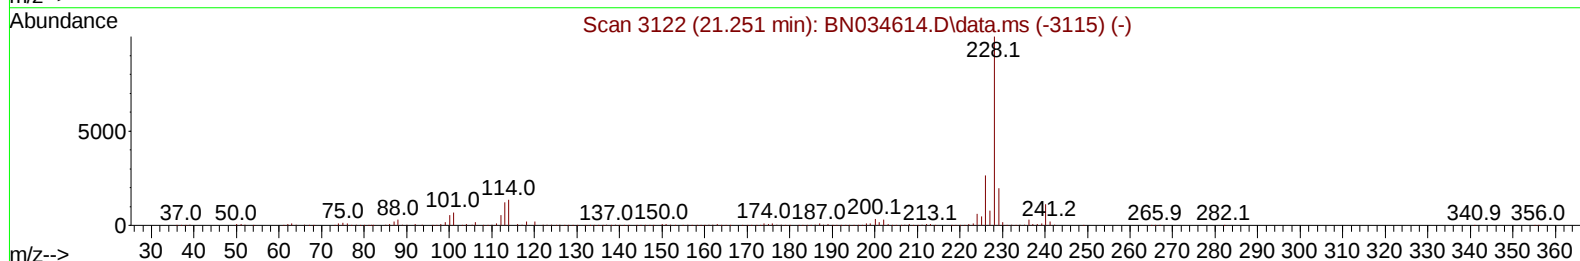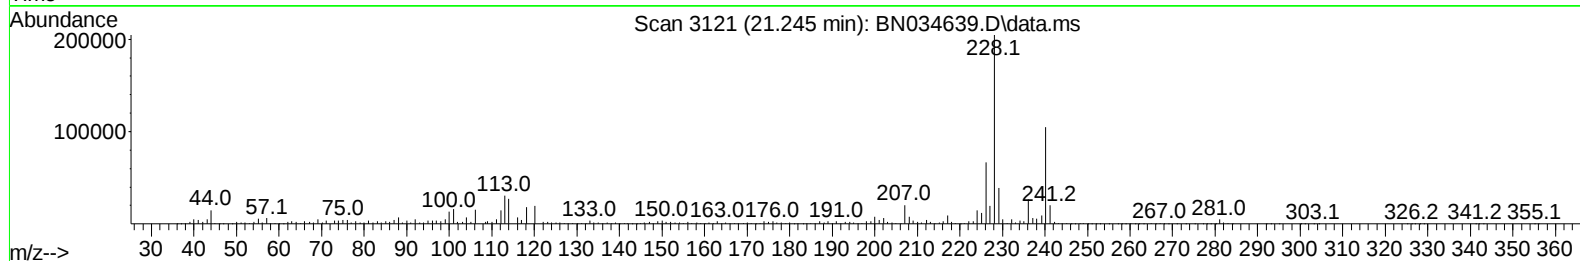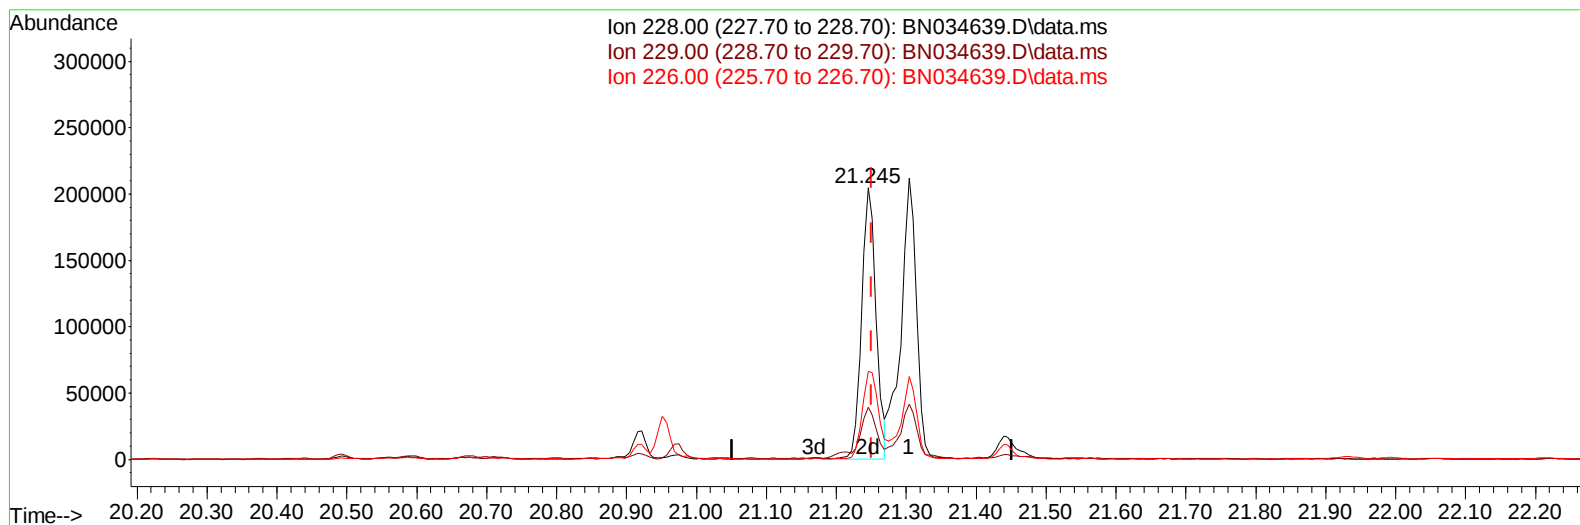

TIC: BN034639.D\data.ms

(85) Benzo(a)anthracene

21.245min (-0.006) 4.56 ng/u1 m

response 295518

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.60	19.15
226.00	26.60	32.47#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034639.D
Acq On : 18 Oct 2024 02:29
Operator : RC/JU
Sample : P4346-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EOAX7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :mohammad ahmed 10/21/2024

Quant Time: Oct 18 03:12:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 15:50:29 2024
Response via : Initial Calibration

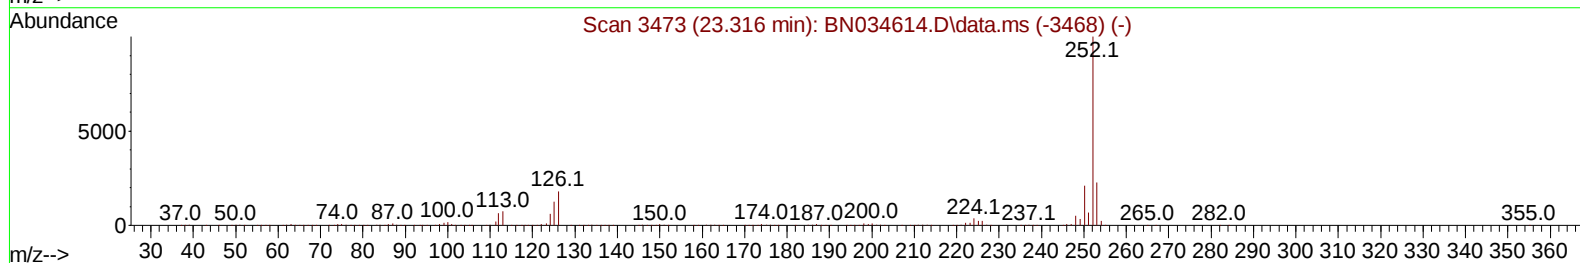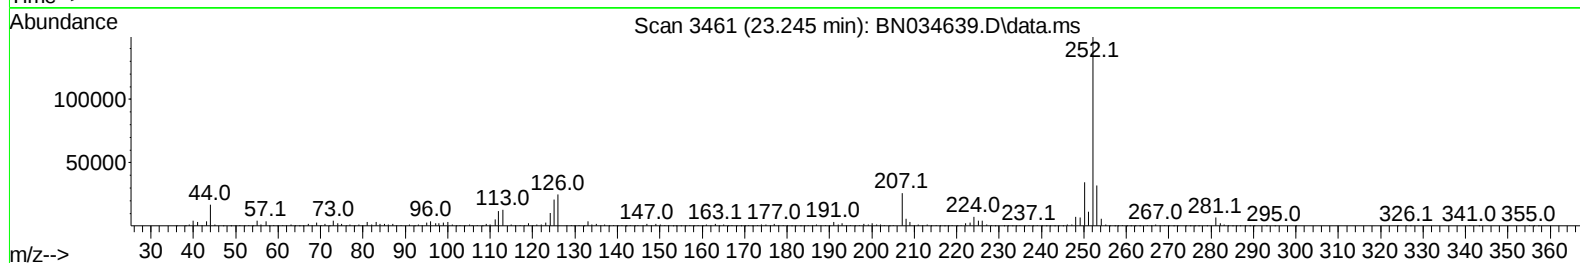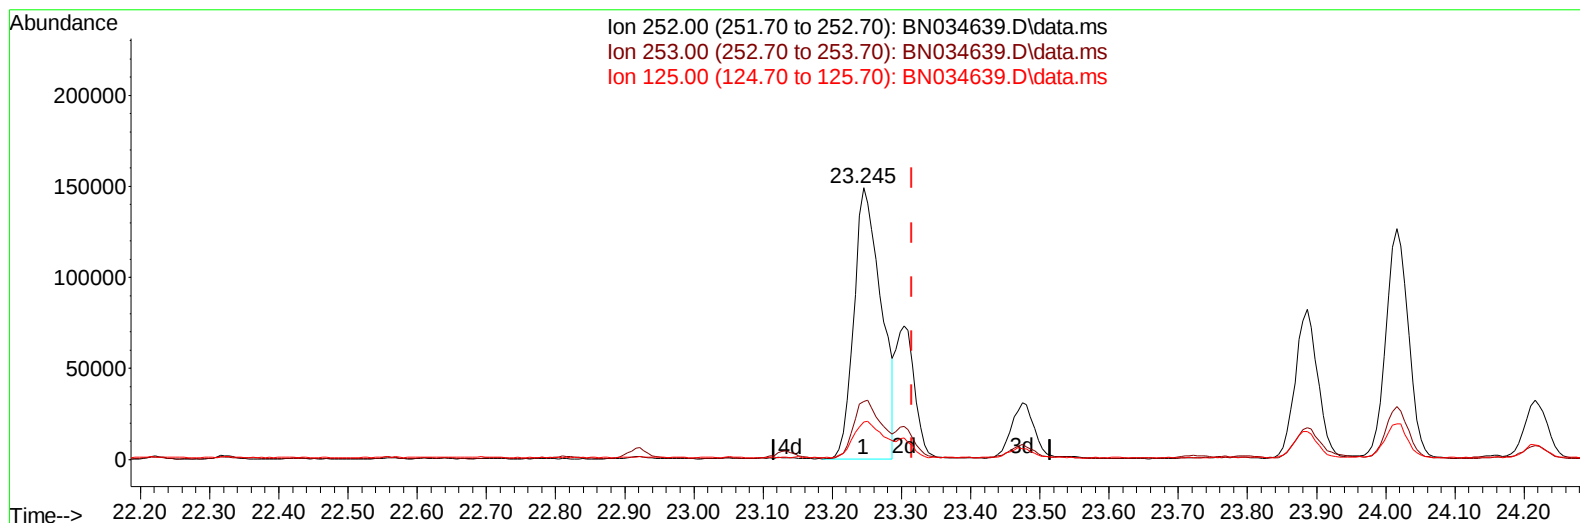

TIC: BN034639.D\data.ms

(91) Benzo(k)fluoranthene

23.245min (-0.070) 5.85 ng/u1

response 404928

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.40	21.30
125.00	12.90	13.89
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034639.D
Acq On : 18 Oct 2024 02:29
Operator : RC/JU
Sample : P4346-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EOAX7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :mohammad ahmed 10/21/2024

Quant Time: Oct 18 03:12:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 15:50:29 2024
Response via : Initial Calibration

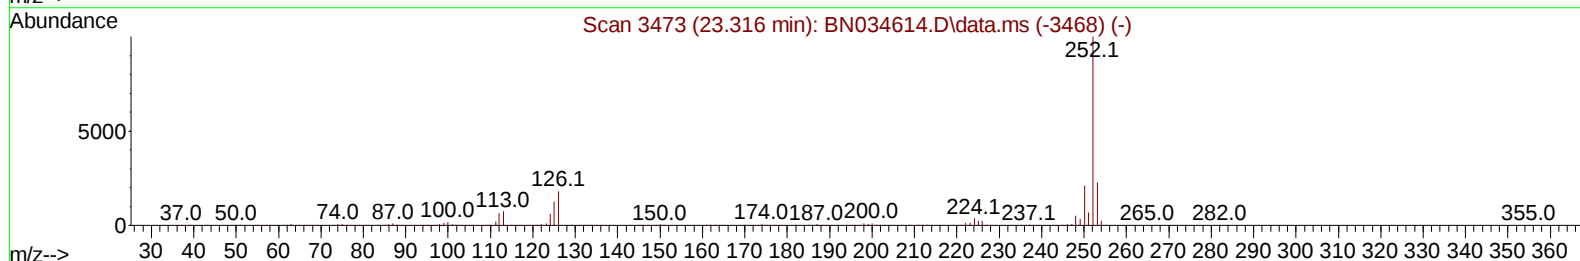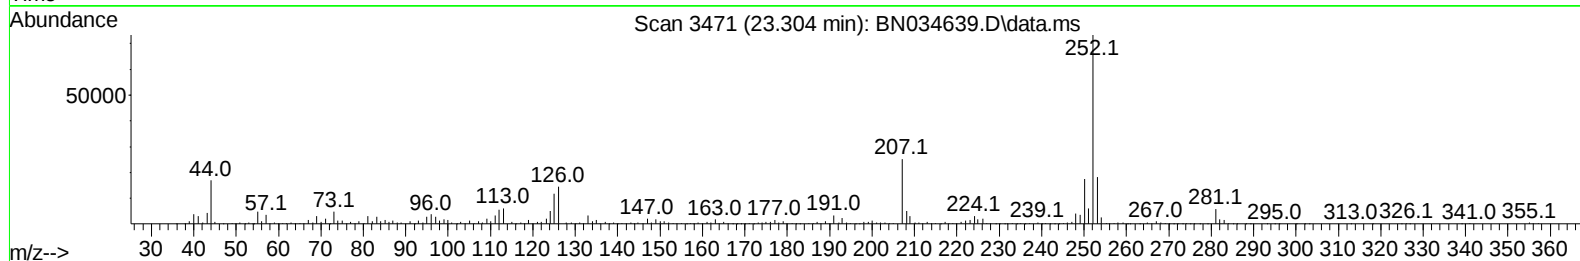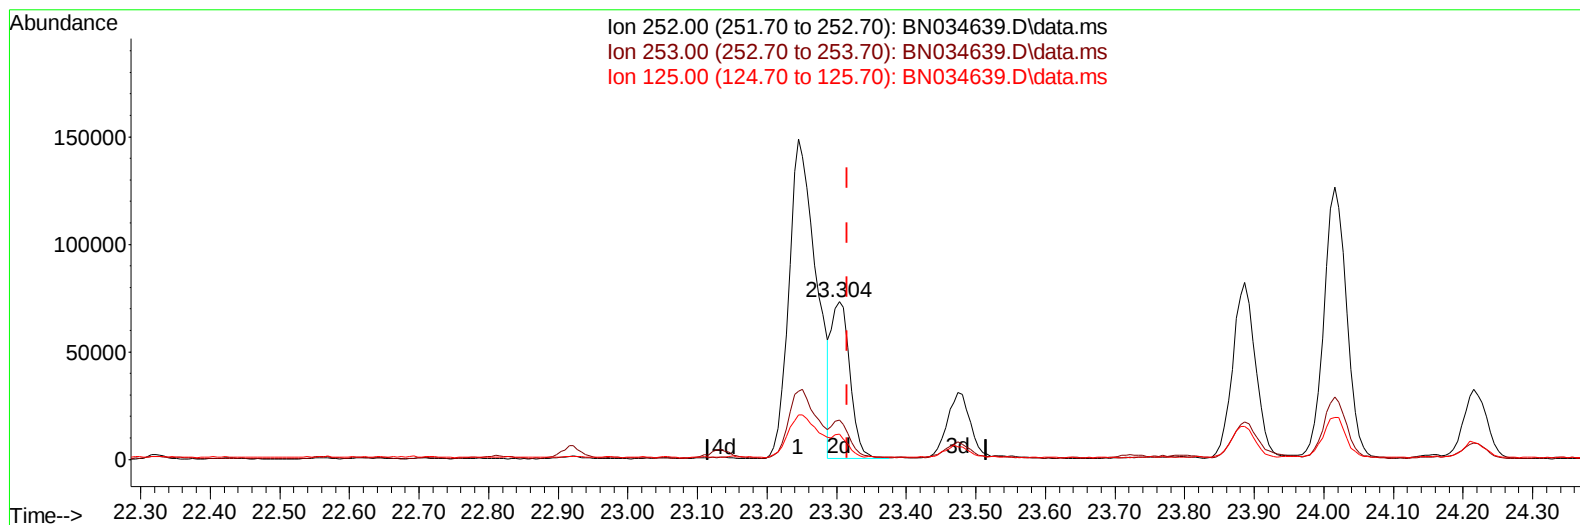

TIC: BN034639.D\data.ms

(91) Benzo(k)fluoranthene

23.304min (-0.011) 1.97 ng/u1 m

response 136527

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.40	24.97
125.00	12.90	16.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034639.D
 Acq On : 18 Oct 2024 02:29
 Operator : RC/JU
 Sample : P4346-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EOAX7

Manual IntegrationsAPPROVED

Quant Time: Oct 18 03:13:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 16 15:50:29 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/18/2024
 Supervised By :mohammad ahmed 10/21/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.664	152		303216	20.000	ng/ul	0.00
20) Naphthalene-d8	10.440	136		1164862	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.298	164		609547	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.040	188		1103039	20.000	ng/ul	0.00
79) Chrysene-d12	21.263	240		1019598	20.000	ng/ul	0.00
88) Perylene-d12	24.157	264		1261070	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.211	96		24631	3.251	ng/uL	0.00
4) Pyridine-d5	3.605	84		328750	14.859	ng/ul	0.00
7) Phenol-d5	6.834	99		417578	16.781	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67		261115	17.011	ng/ul	0.00
11) 2-Chlorophenol-d4	7.199	132		338988	17.635	ng/ul	0.00
15) 4-Methylphenol-d8	8.363	113		322714	16.641	ng/ul	0.00
21) Nitrobenzene-d5	8.805	128		155944	19.237	ng/ul	0.00
24) 2-Nitrophenol-d4	9.522	143		125360	19.570	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.058	165		256004	17.339	ng/ul	0.00
31) 4-Chloroaniline-d4	10.569	131		403629	15.936	ng/ul	0.00
46) Dimethylphthalate-d6	13.716	166		740327	19.198	ng/ul	0.00
49) Acenaphthylene-d8	13.987	160		914638	19.095	ng/ul	0.00
54) 4-Nitrophenol-d4	14.487	143		68762	9.572	ng/ul	0.00
60) Fluorene-d10	15.293	176		636797	19.093	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200		18574	5.024	ng/ul	0.00
73) Anthracene-d10	17.139	188		950394	20.156	ng/ul	0.00
81) Pyrene-d10	19.433	212		1053970	20.133	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.957	264		1185891	20.409	ng/ul	-0.01
Target Compounds							
						Qvalue	
50) Acenaphthylene	14.016	152		63250	1.219	ng/ul	97
52) Acenaphthene	14.363	153		56721	1.573	ng/ul	96
56) Dibenzofuran	14.698	168		59782	1.248	ng/ul	99
61) Fluorene	15.345	166		75783	1.963	ng/ul	93
72) Phenanthrene	17.081	178		307782	5.590	ng/ul	99
74) Anthracene	17.175	178		120144	2.112	ng/ul	97
80) Fluoranthene	19.098	202		667654	10.630	ng/ul	98
82) Pyrene	19.463	202		504067	7.534	ng/ul	98
85) Benzo(a)anthracene	21.245	228		295518m	4.562	ng/ul	
86) Bis(2-ethylhexyl)phtha...	21.222	149		101584	2.610	ng/ul	98
87) Chrysene	21.304	228		327042	5.319	ng/ul	98
90) Benzo(b)fluoranthene	23.245	252		404928	5.976	ng/ul	99
91) Benzo(k)fluoranthene	23.304	252		136527m	1.972	ng/ul	
93) Benzo(a)pyrene	24.016	252		285386	4.350	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	27.380	276		188889	2.308	ng/ul	94
96) Benzo(g,h,i)perylene	28.380	276		167343	2.634	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034639.D
Acq On : 18 Oct 2024 02:29
Operator : RC/JU
Sample : P4346-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EOAX7

Manual IntegrationsAPPROVED

Quant Time: Oct 18 03:13:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 15:50:29 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/18/2024
Supervised By :mohammad ahmed 10/21/2024

