

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034620.D
 Acq On : 17 Oct 2024 14:02
 Operator : RC/JU
 Sample : P4352-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4FD0

Quant Time: Oct 17 14:32:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 16 15:50:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	234660	20.000	ng/u1	0.00
20) Naphthalene-d8	10.434	136	923443	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.298	164	501328	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.039	188	906169	20.000	ng/u1	0.00
79) Chrysene-d12	21.269	240	776630	20.000	ng/u1	0.00
88) Perylene-d12	24.157	264	919246	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.205	96	30510	5.203	ng/uL	0.00
4) Pyridine-d5	3.593	84	414455	24.205	ng/u1	0.00
7) Phenol-d5	6.828	99	532974	27.675	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	333338	28.061	ng/u1	0.00
11) 2-Chlorophenol-d4	7.193	132	432043	29.042	ng/u1	0.00
15) 4-Methylphenol-d8	8.357	113	411515	27.419	ng/u1	0.00
21) Nitrobenzene-d5	8.804	128	198023	30.815	ng/u1	0.00
24) 2-Nitrophenol-d4	9.522	143	164865	32.465	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.057	165	336403	28.741	ng/u1	0.00
31) 4-Chloroaniline-d4	10.569	131	529023	26.347	ng/u1	0.00
46) Dimethylphthalate-d6	13.716	166	952741	30.040	ng/u1	0.00
49) Acenaphthylene-d8	13.987	160	1208316	30.672	ng/u1	0.00
54) 4-Nitrophenol-d4	14.481	143	115802	19.600	ng/u1	0.00
60) Fluorene-d10	15.292	176	825031	30.076	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200	46801	15.408	ng/u1	0.00
73) Anthracene-d10	17.139	188	1214212	31.345	ng/u1	0.00
81) Pyrene-d10	19.433	212	1300836	32.622	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.962	264	1376320	32.494	ng/u1	0.00
Target Compounds						Qvalue
8) Phenol	6.852	94	27948	1.390	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034620.D
Acq On : 17 Oct 2024 14:02
Operator : RC/JU
Sample : P4352-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4FD0

Quant Time: Oct 17 14:32:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 15:50:29 2024
Response via : Initial Calibration

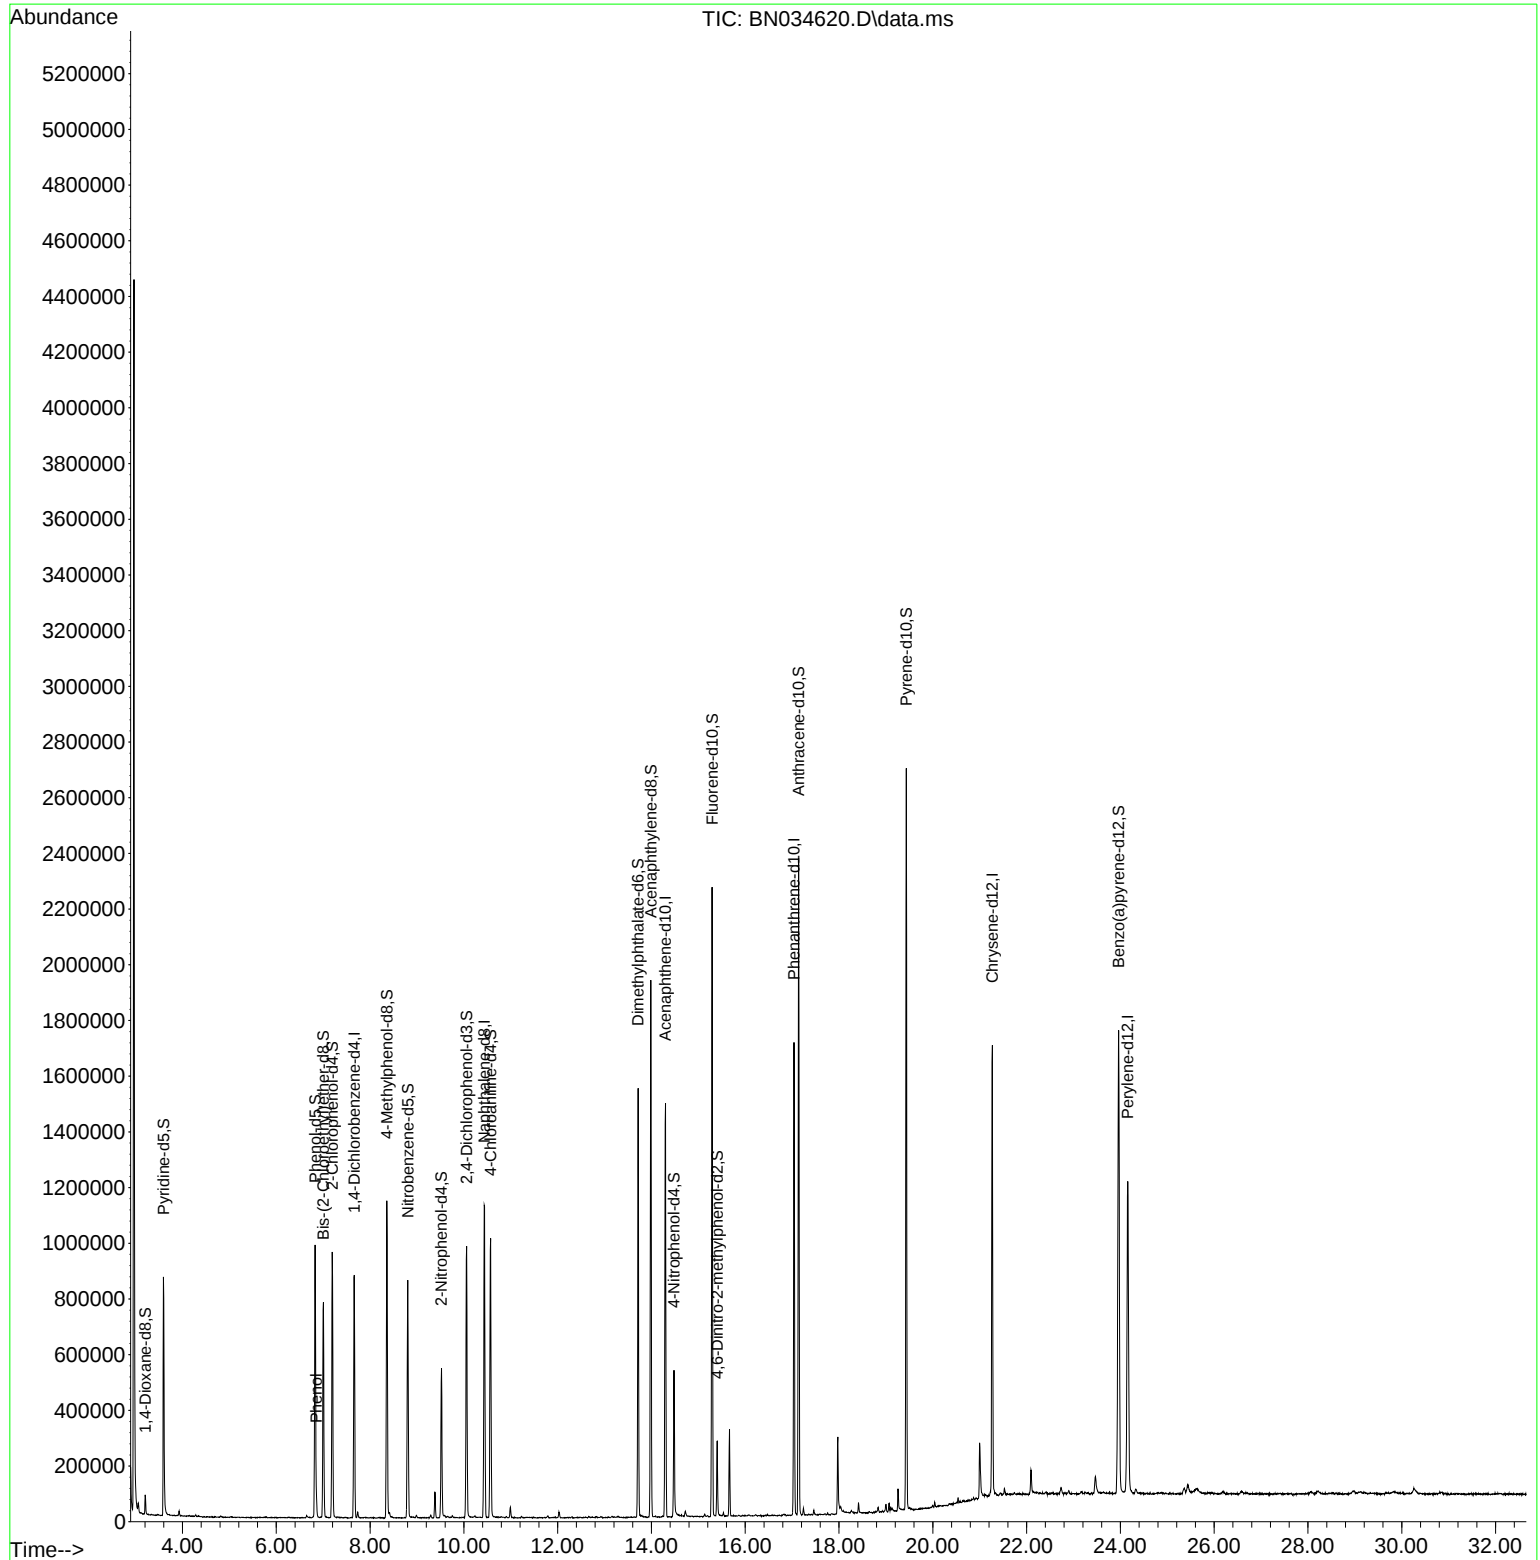

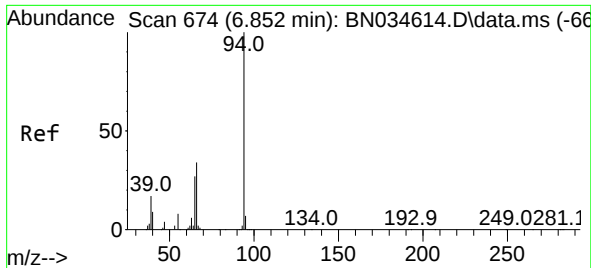

#8
Phenol
Concen: 1.390 ng/ul
RT: 6.852 min Scan# 61
Delta R.T. -0.006 min
Lab File: BN034620.D
Acq: 17 Oct 2024 14:02

Instrument :
BNA_N
ClientSampleId :
A4FD0

Tgt Ion: 94 Resp: 27948
Ion Ratio Lower Upper
94 100
65 26.2 22.2 33.4
66 38.0 27.4 41.0

