

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034666.D
 Acq On : 19 Oct 2024 02:26
 Operator : RC/JU
 Sample : P4380-06RXDL 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E27H7RXDL

Quant Time: Oct 19 03:54:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 16 15:50:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.664	152	312938	20.000	ng/u1	0.00
20) Naphthalene-d8	10.440	136	1267442	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.293	164	674786	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.039	188	1150299	20.000	ng/u1	0.00
79) Chrysene-d12	21.257	240	957540	20.000	ng/u1	-0.01
88) Perylene-d12	24.139	264	1121538	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	4469	0.571	ng/uL	0.00
4) Pyridine-d5	3.617	84	28414	1.244	ng/u1	0.02
7) Phenol-d5	6.834	99	29513	1.149	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	54351	3.431	ng/u1	0.00
11) 2-Chlorophenol-d4	7.199	132	67762	3.416	ng/u1	0.00
15) 4-Methylphenol-d8	8.363	113	48200	2.408	ng/u1	0.00
21) Nitrobenzene-d5	8.805	128	31887	3.615	ng/u1	0.00
24) 2-Nitrophenol-d4	9.522	143	30672	4.401	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.057	165	60610	3.773	ng/u1	0.00
31) 4-Chloroaniline-d4	10.569	131	77635	2.817	ng/u1	0.00
46) Dimethylphthalate-d6	13.716	166	131261	3.075	ng/u1	0.00
49) Acenaphthylene-d8	13.981	160	188895	3.562	ng/u1	0.00
54) 4-Nitrophenol-d4	14.487	143	7056	0.887	ng/u1	0.00
60) Fluorene-d10	15.287	176	134538	3.644	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	
73) Anthracene-d10	17.134	188	196512	3.996	ng/u1	0.00
81) Pyrene-d10	19.428	212	204006	4.149	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.945	264	206124	3.989	ng/u1	-0.02
Target Compounds						
					Qvalue	
8) Phenol	6.864	94	517182	19.286	ng/u1	99
30) Naphthalene	10.487	128	1163855	18.268	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034666.D
Acq On : 19 Oct 2024 02:26
Operator : RC/JU
Sample : P4380-06RXDL 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E27H7RXDL


Quant Time: Oct 19 03:54:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 16 15:50:29 2024
Response via : Initial Calibration

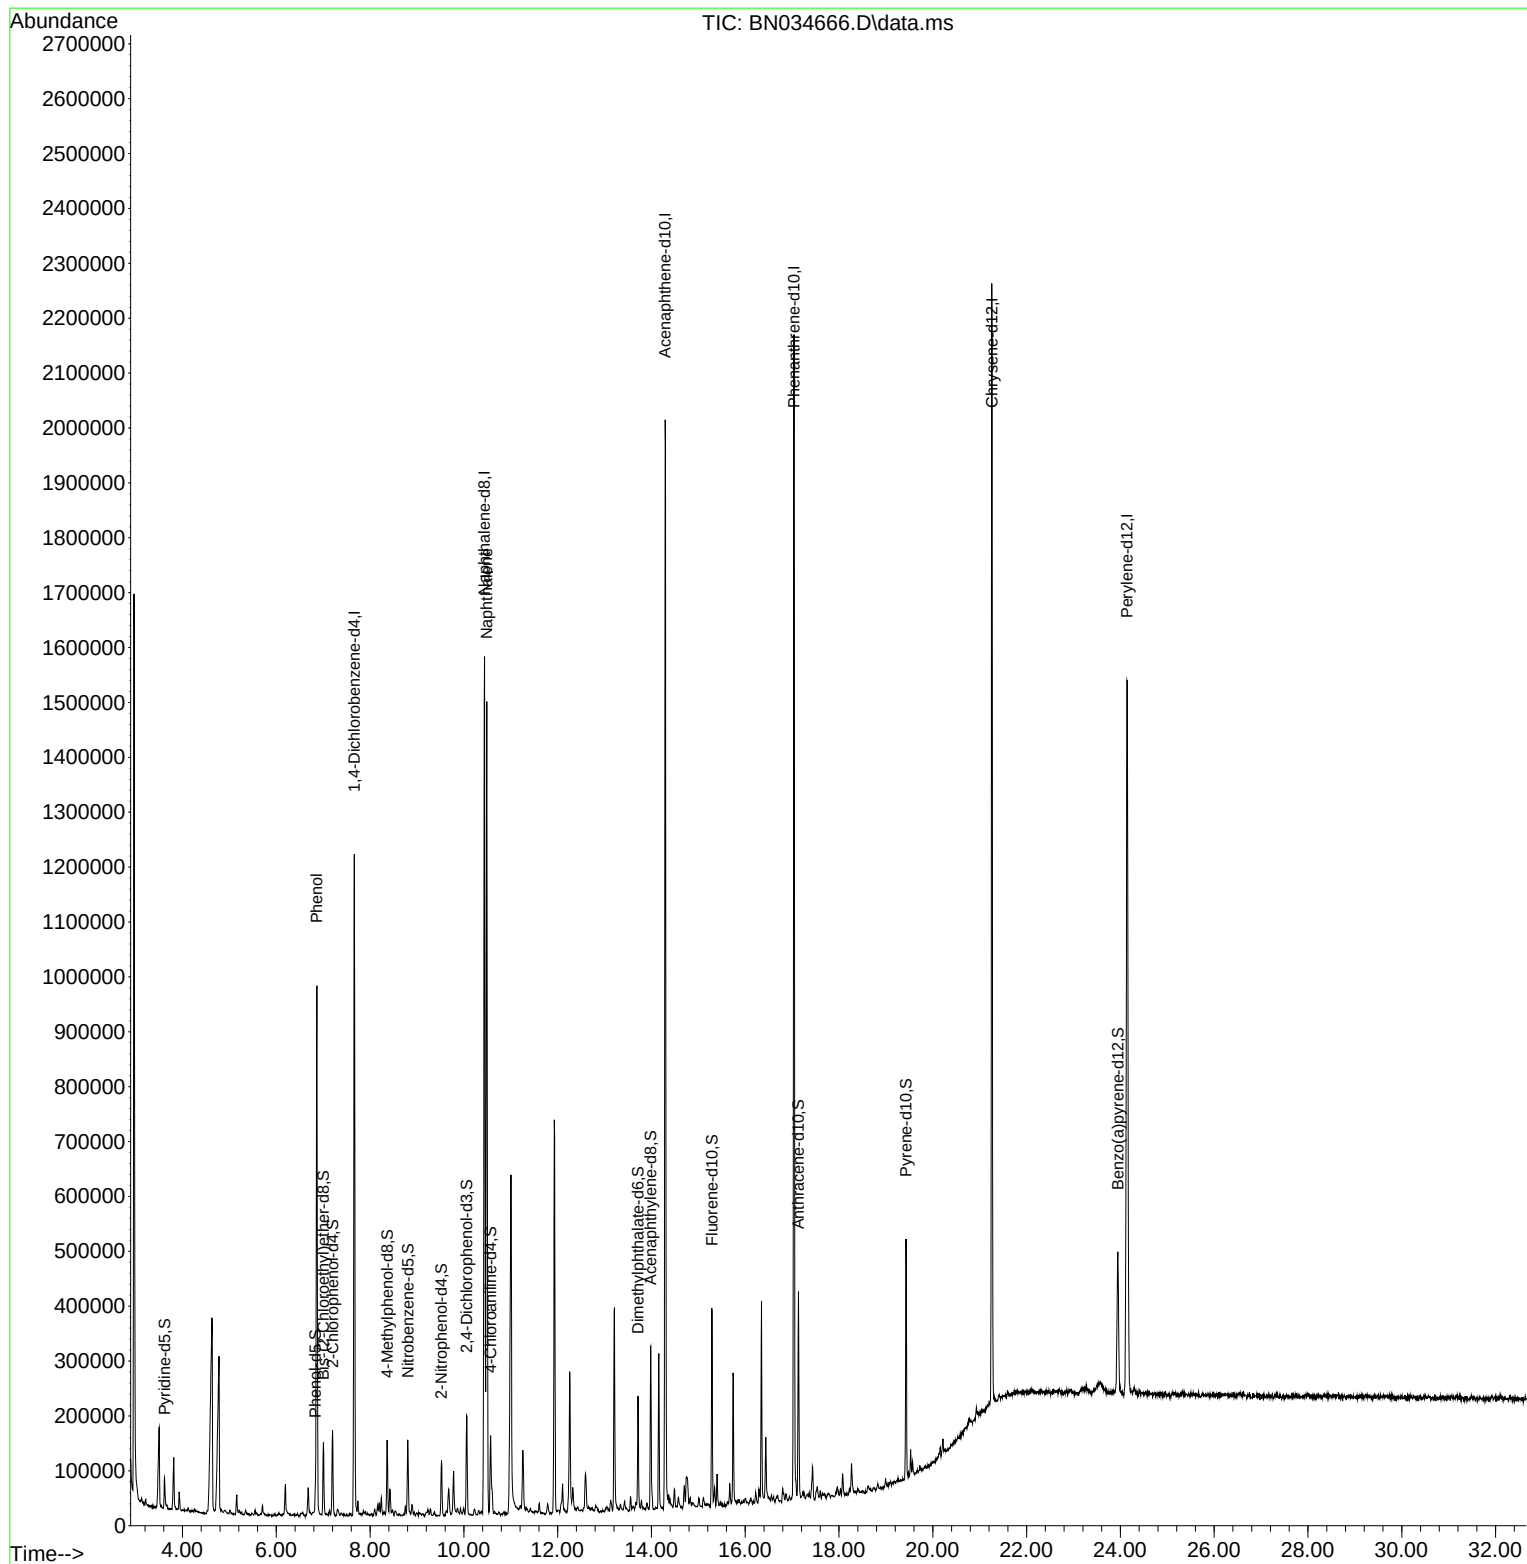



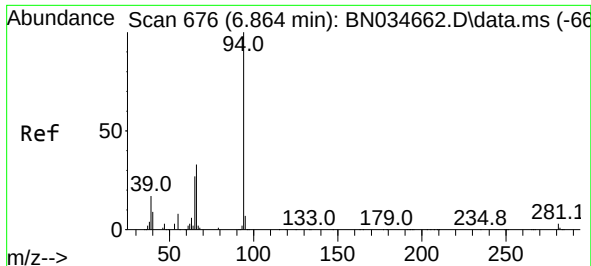


#8
Phenol
Concen: 19.286 ng/ul
RT: 6.864 min Scan# 61
Delta R.T. 0.006 min
Lab File: BN034666.D
Acq: 19 Oct 2024 02:26

Instrument :
BNA_N
ClientSampleId :
E27H7RXDL

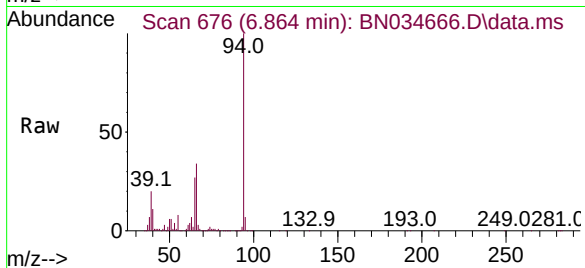

Tgt Ion: 94 Resp: 517182
Ion Ratio Lower Upper
94 100
65 27.0 22.2 33.4
66 34.2 27.4 41.0

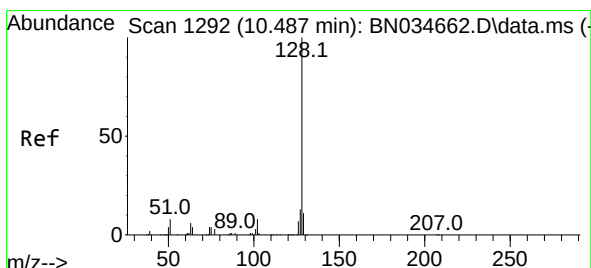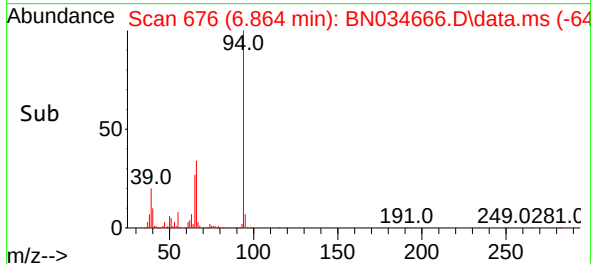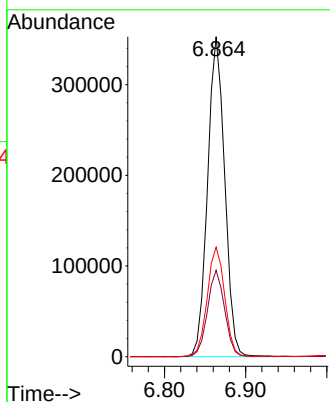

#30
Naphthalene
Concen: 18.268 ng/ul
RT: 10.487 min Scan# 1292
Delta R.T. -0.006 min
Lab File: BN034666.D
Acq: 19 Oct 2024 02:26

Tgt Ion: 128 Resp: 1163855
Ion Ratio Lower Upper
128 100
129 11.0 8.2 12.4
127 13.0 10.3 15.5

