

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034615.D
 Acq On : 17 Oct 2024 10:20
 Operator : RC/JU
 Sample : PB164147BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK147

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	25	rVB	321715	400324	9.66%	0.800%
2	3.058	26	29	36	rVB2	15313	24246	0.59%	0.048%
3	3.211	51	55	61	rVB	69802	85471	2.06%	0.171%
4	3.599	117	121	142	rBV	954860	1303625	31.46%	2.607%
5	3.928	173	177	184	rVB	16390	22738	0.55%	0.045%
6	6.828	663	670	679	rBV	918917	1407458	33.97%	2.814%
7	7.005	694	700	708	rVB	768744	1149996	27.76%	2.299%
8	7.199	726	733	741	rBV	920056	1418456	34.24%	2.836%
9	7.664	805	812	819	rBV	982176	1471952	35.53%	2.943%
10	8.358	923	930	941	rBV	1070762	1688161	40.75%	3.376%
11	8.805	999	1006	1016	rBV	850169	1336361	32.25%	2.672%
12	9.293	1085	1089	1094	rVB4	4505	6256	0.15%	0.013%
13	9.522	1121	1128	1137	rBV	534482	845097	20.40%	1.690%
14	10.057	1211	1219	1231	rBV	961793	1529035	36.91%	3.057%
15	10.440	1275	1284	1293	rBV	1268941	2070956	49.98%	4.141%
16	10.569	1297	1306	1317	rBV	1067583	1779149	42.94%	3.557%
17	12.034	1548	1555	1561	rBV	21057	35707	0.86%	0.071%
18	12.299	1596	1600	1606	rVB3	4481	7313	0.18%	0.015%
19	13.716	1833	1841	1851	rBV	1645782	2171086	52.40%	4.341%
20	13.987	1880	1887	1894	rBV	1983311	2848506	68.75%	5.696%
21	14.298	1932	1940	1947	rBV	1766135	2573277	62.11%	5.145%
22	14.481	1963	1971	1985	rBV	748439	1091243	26.34%	2.182%
23	14.722	2009	2012	2015	rVB5	4892	7406	0.18%	0.015%
24	15.293	2102	2109	2119	rBV	2433149	3283118	79.24%	6.565%
25	15.404	2122	2128	2136	rBV	401542	557464	13.46%	1.115%
26	15.534	2146	2150	2154	rVB3	12203	17259	0.42%	0.035%
27	16.087	2239	2244	2247	rVB6	5703	10181	0.25%	0.020%
28	16.822	2366	2369	2373	rVB3	4948	6586	0.16%	0.013%
29	17.039	2400	2406	2413	rBV	2072902	2831989	68.35%	5.663%
30	17.139	2417	2423	2431	rVV	2562646	3468408	83.71%	6.935%
31	17.404	2466	2468	2474	rVB7	4255	5417	0.13%	0.011%
32	18.998	2734	2739	2743	rBV3	32965	42988	1.04%	0.086%
33	19.069	2746	2751	2756	rBV	31853	46130	1.11%	0.092%
34	19.433	2806	2813	2819	rBV	2923254	3878069	93.60%	7.754%
35	21.263	3118	3124	3135	rBV2	2096088	3022106	72.94%	6.043%
36	23.957	3573	3582	3594	rBV	1790602	4143159	100.00%	8.284%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034615.D
Acq On : 17 Oct 2024 10:20
Operator : RC/JU
Sample : PB164147BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK147

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Title : SVOA CALIBRATION

37 24.157 3607 3616 3631 rVB 1482700 3424902 82.66% 6.848%




Sum of corrected areas: 50011595

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034615.D
Acq On : 17 Oct 2024 10:20
Operator : RC/JU
Sample : PB164147BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK147

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

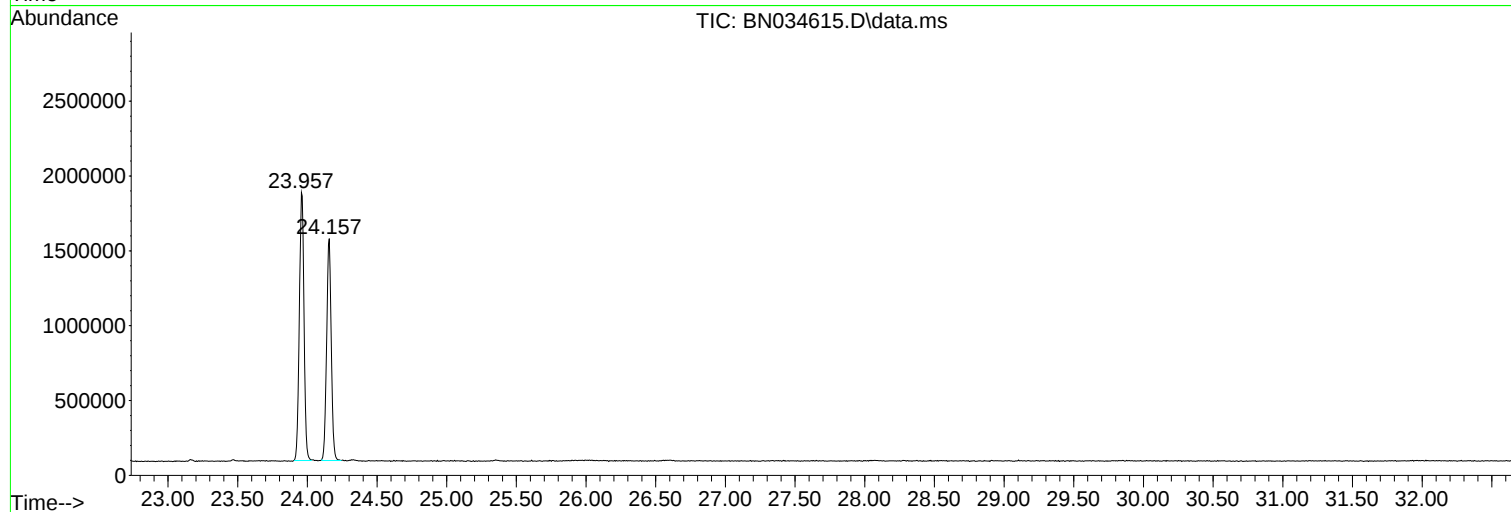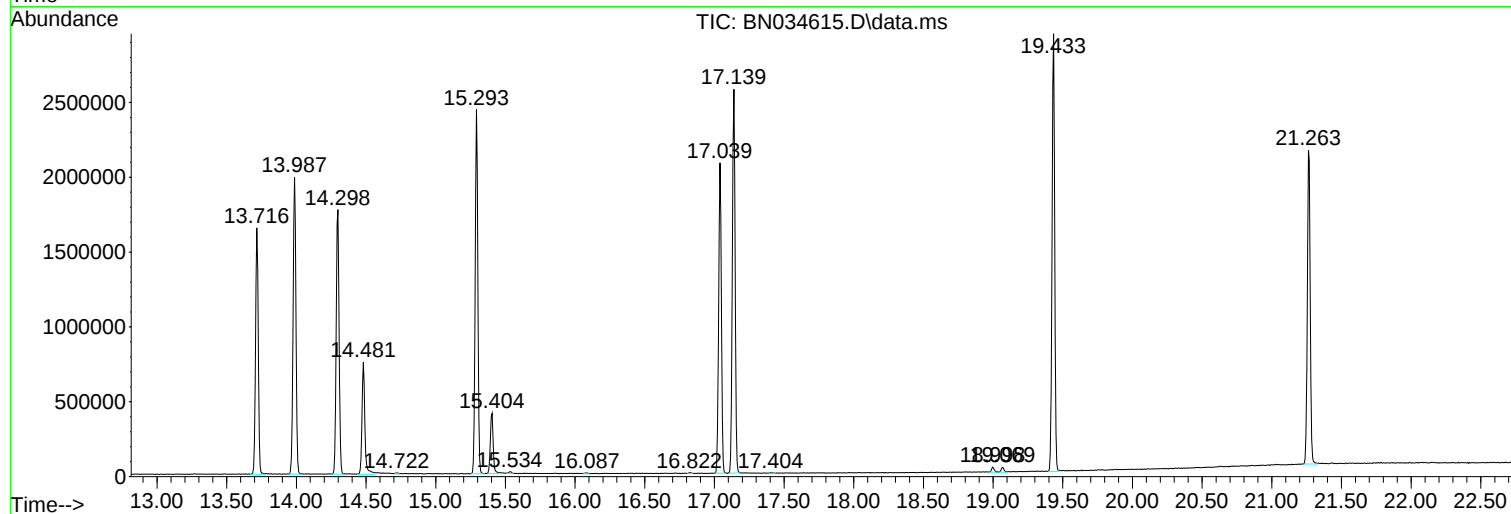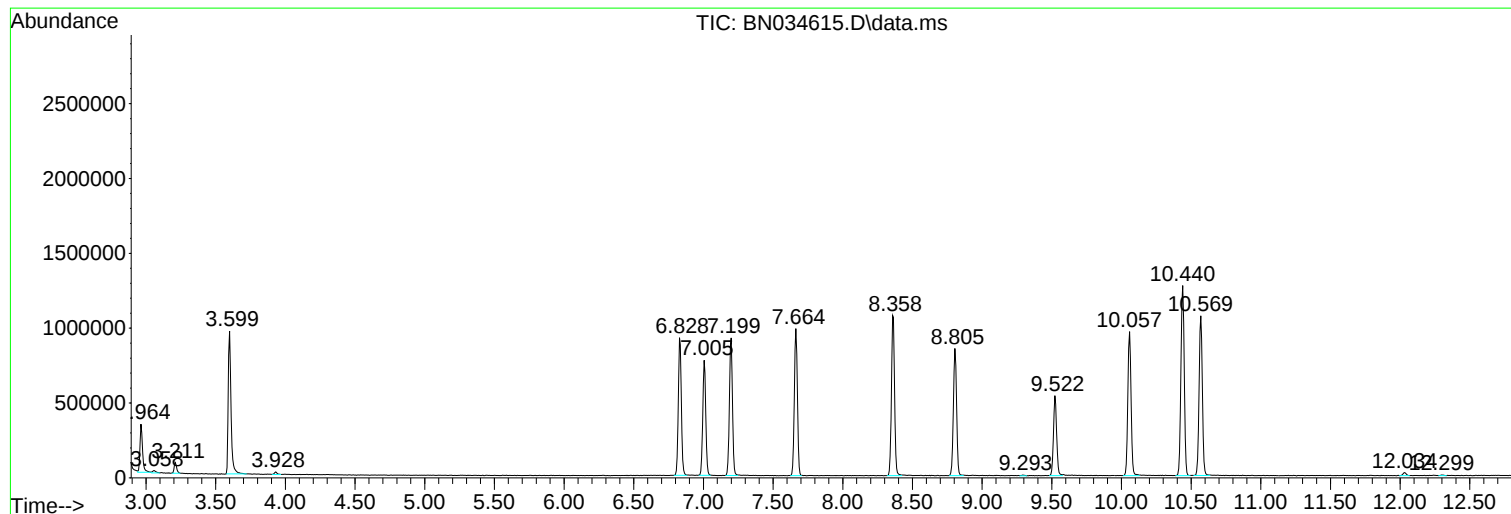

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034615.D
Acq On : 17 Oct 2024 10:20
Operator : RC/JU
Sample : PB164147BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK147

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034615.D
Acq On : 17 Oct 2024 10:20
Operator : RC/JU
Sample : PB164147BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK147

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc