

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034626.D
 Acq On : 17 Oct 2024 17:58
 Operator : RC/JU
 Sample : PB164165BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK165

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	24	rVB	324109	395242	12.26%	0.931%
2	3.058	25	29	37	rVB	18591	29899	0.93%	0.070%
3	3.211	51	55	65	rBV	73152	92889	2.88%	0.219%
4	3.428	89	92	95	rBV5	2914	3349	0.10%	0.008%
5	3.599	116	121	136	rBV	938682	1267230	39.31%	2.984%
6	3.928	173	177	183	rVB	16408	22073	0.68%	0.052%
7	4.140	208	213	217	rBV7	4166	6217	0.19%	0.015%
8	4.534	278	280	282	rBV2	3808	4324	0.13%	0.010%
9	6.128	546	551	555	rVB7	2510	4574	0.14%	0.011%
10	6.834	664	671	684	rBV	881892	1376280	42.69%	3.240%
11	7.005	694	700	708	rVB	736841	1099666	34.11%	2.589%
12	7.199	726	733	741	rBV	895594	1375308	42.66%	3.238%
13	7.663	805	812	822	rVB	895670	1370437	42.51%	3.227%
14	8.363	924	931	945	rBV	1012602	1600979	49.66%	3.769%
15	8.805	998	1006	1019	rBV	788519	1267796	39.32%	2.985%
16	9.293	1086	1089	1093	rVB4	9526	13032	0.40%	0.031%
17	9.522	1121	1128	1138	rBV	463096	768560	23.84%	1.810%
18	9.605	1141	1142	1150	rVB6	2630	5195	0.16%	0.012%
19	10.057	1211	1219	1233	rBV	890510	1444096	44.79%	3.400%
20	10.440	1276	1284	1294	rVB	1128193	1858350	57.64%	4.375%
21	10.569	1298	1306	1316	rBV	1018583	1625876	50.43%	3.828%
22	11.787	1508	1513	1519	rBV3	7822	13573	0.42%	0.032%
23	12.034	1550	1555	1562	rVV3	17932	28396	0.88%	0.067%
24	12.298	1594	1600	1605	rVB2	4798	7752	0.24%	0.018%
25	13.716	1834	1841	1851	rBV	1370566	1824888	56.60%	4.297%
26	13.793	1851	1854	1859	rVB5	5339	8188	0.25%	0.019%
27	13.987	1879	1887	1896	rBV	1719443	2511646	77.90%	5.913%
28	14.298	1933	1940	1948	rVB	1490678	2131637	66.12%	5.019%
29	14.481	1965	1971	1984	rBV	590252	858549	26.63%	2.021%
30	15.140	2078	2083	2088	rBV8	1842	3231	0.10%	0.008%
31	15.292	2102	2109	2119	rBV	1993149	2789152	86.51%	6.567%
32	15.398	2122	2127	2139	rVV	276582	397070	12.32%	0.935%
33	15.481	2139	2141	2145	rVV4	3723	5167	0.16%	0.012%
34	15.534	2145	2150	2154	rVB5	9976	14861	0.46%	0.035%
35	16.081	2238	2243	2250	rBV9	5266	9132	0.28%	0.022%
36	16.475	2307	2310	2314	rBV2	1641	3228	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034626.D
 Acq On : 17 Oct 2024 17:58
 Operator : RC/JU
 Sample : PB164165BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK165

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

37	16.775	2358	2361	2363	rBV3	2509	3291	0.10%	0.008%
38	16.822	2365	2369	2375	rVV5	4117	6700	0.21%	0.016%
39	17.039	2400	2406	2415	rVB	1683290	2226628	69.06%	5.242%
40	17.139	2415	2423	2432	rBV	2036799	2843343	88.19%	6.694%
41	17.686	2511	2516	2519	rBV6	3661	6439	0.20%	0.015%
42	18.069	2580	2581	2587	rBV5	2189	4298	0.13%	0.010%
43	18.545	2660	2662	2666	rVB4	3342	3851	0.12%	0.009%
44	18.828	2708	2710	2714	rBV5	2906	3500	0.11%	0.008%
45	18.998	2734	2739	2746	rVB3	24173	34034	1.06%	0.080%
46	19.069	2746	2751	2755	rBV2	23831	35016	1.09%	0.082%
47	19.433	2807	2813	2819	rBV	2211573	3055877	94.79%	7.195%
48	21.263	3118	3124	3135	rBV2	1601156	2244747	69.63%	5.285%
49	23.957	3573	3582	3597	rVB	1449980	3223986	100.00%	7.591%
50	24.151	3606	3615	3628	rBV	1062765	2543718	78.90%	5.989%




Sum of corrected areas: 42473270

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034626.D
Acq On : 17 Oct 2024 17:58
Operator : RC/JU
Sample : PB164165BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK165

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

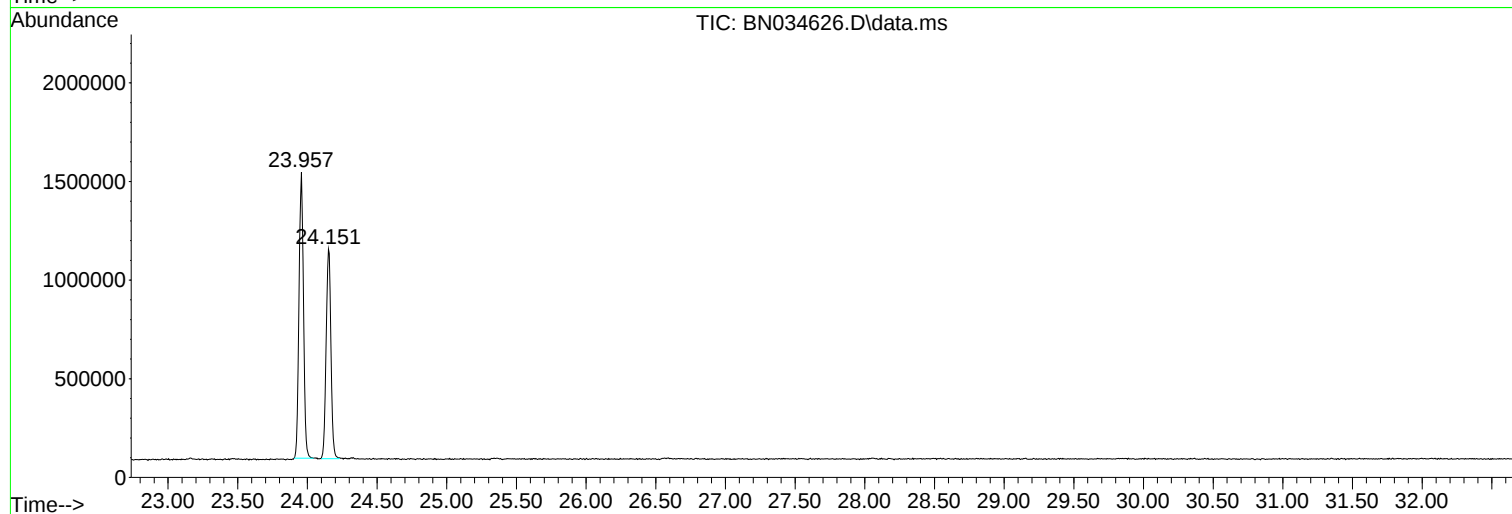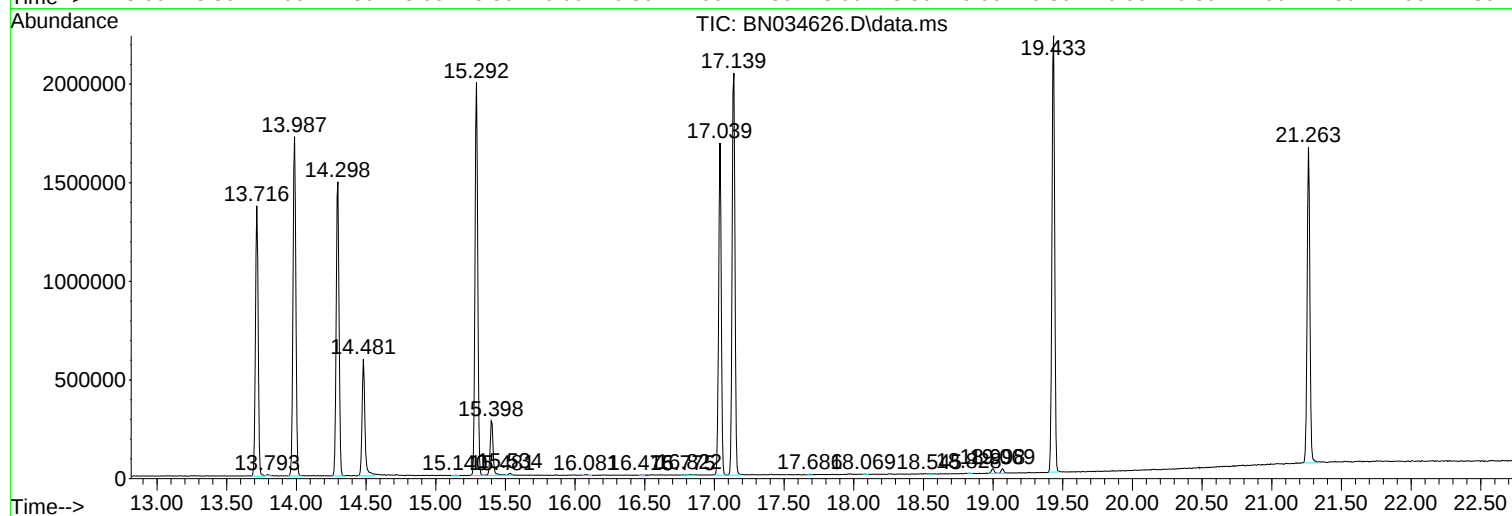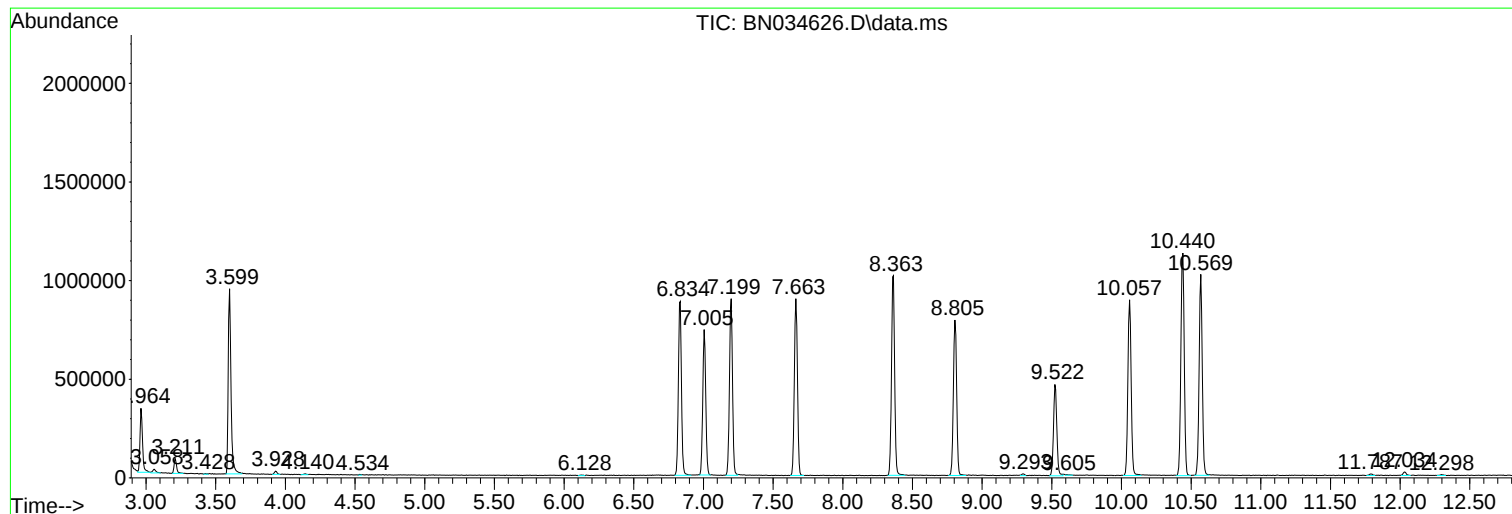

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034626.D
Acq On : 17 Oct 2024 17:58
Operator : RC/JU
Sample : PB164165BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK165

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034626.D
Acq On : 17 Oct 2024 17:58
Operator : RC/JU
Sample : PB164165BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK165

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------