

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034627.D
 Acq On : 17 Oct 2024 18:37
 Operator : RC/JU
 Sample : PB164170BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK170

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	24	rVB	304673	364340	11.43%	0.899%
2	3.211	51	55	61	rVB	68699	80897	2.54%	0.200%
3	3.599	117	121	139	rBV	906098	1218923	38.23%	3.008%
4	3.928	173	177	181	rBV	17664	21417	0.67%	0.053%
5	6.828	662	670	681	rBV	858004	1313051	41.18%	3.240%
6	7.005	693	700	708	rBV	706957	1055009	33.09%	2.604%
7	7.199	725	733	745	rBV	844740	1302602	40.85%	3.215%
8	7.663	805	812	819	rVB	851716	1287792	40.39%	3.178%
9	8.005	867	870	874	rBV5	1976	3437	0.11%	0.008%
10	8.105	885	887	892	rBV4	2222	3311	0.10%	0.008%
11	8.357	923	930	939	rBV	958556	1514860	47.51%	3.738%
12	8.804	998	1006	1017	rBV	746561	1197184	37.55%	2.954%
13	9.293	1084	1089	1094	rBV2	14246	20623	0.65%	0.051%
14	9.522	1120	1128	1137	rBV	441964	699359	21.93%	1.726%
15	9.587	1137	1139	1142	rVV4	4263	5560	0.17%	0.014%
16	10.057	1211	1219	1231	rBV	850902	1360002	42.65%	3.356%
17	10.440	1276	1284	1293	rBV	1062975	1750548	54.90%	4.320%
18	10.569	1298	1306	1315	rBV	957514	1551630	48.66%	3.829%
19	10.634	1315	1317	1322	rVB5	3416	4573	0.14%	0.011%
20	11.793	1508	1514	1517	rBV2	10546	15991	0.50%	0.039%
21	12.034	1547	1555	1562	rVV2	16749	28952	0.91%	0.071%
22	12.104	1562	1567	1573	rVB7	2319	5712	0.18%	0.014%
23	12.245	1589	1591	1596	rBV3	3116	4034	0.13%	0.010%
24	12.322	1601	1604	1607	rBV3	2376	3416	0.11%	0.008%
25	13.534	1808	1810	1815	rVB5	2464	3338	0.10%	0.008%
26	13.716	1834	1841	1850	rBV	1307187	1759393	55.18%	4.342%
27	13.798	1850	1855	1860	rVB3	7037	10668	0.33%	0.026%
28	13.987	1880	1887	1895	rBV2	1598206	2372334	74.40%	5.855%
29	14.292	1933	1939	1947	rBV	1391854	2001846	62.78%	4.940%
30	14.481	1962	1971	1989	rBV	562795	852551	26.74%	2.104%
31	14.928	2043	2047	2050	rBV5	2766	3958	0.12%	0.010%
32	15.134	2080	2082	2089	rVB7	3308	4638	0.15%	0.011%
33	15.292	2102	2109	2115	rBV	1977242	2679179	84.03%	6.612%
34	15.351	2115	2119	2121	rVV5	3179	4287	0.13%	0.011%
35	15.398	2122	2127	2138	rVV	281326	392486	12.31%	0.969%
36	15.534	2146	2150	2153	rVB4	8705	11603	0.36%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034627.D
Acq On : 17 Oct 2024 18:37
Operator : RC/JU
Sample : PB164170BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK170

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Title : SVOA CALIBRATION

37	15.851	2202	2204	2209	rVB4	2292	3316	0.10%	0.008%
38	16.616	2332	2334	2337	rVB4	3581	3741	0.12%	0.009%
39	16.828	2367	2370	2375	rVV6	4091	5465	0.17%	0.013%
40	17.039	2399	2406	2416	rVB	1535716	2070846	64.95%	5.111%
41	17.133	2416	2422	2432	rBV	1943609	2753370	86.35%	6.795%
42	18.998	2735	2739	2745	rVB3	21984	31391	0.98%	0.077%
43	19.063	2745	2750	2755	rBV	22381	35314	1.11%	0.087%
44	19.257	2780	2783	2785	rBV4	4594	5005	0.16%	0.012%
45	19.427	2806	2812	2823	rBV	2228181	2992280	93.84%	7.384%
46	21.263	3118	3124	3138	rBV	1548283	2121248	66.53%	5.235%
47	23.957	3573	3582	3598	rBV	1365675	3188540	100.00%	7.869%
48	24.151	3606	3615	3629	rVB2	981830	2401281	75.31%	5.926%




Sum of corrected areas: 40521301

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034627.D
Acq On : 17 Oct 2024 18:37
Operator : RC/JU
Sample : PB164170BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK170

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

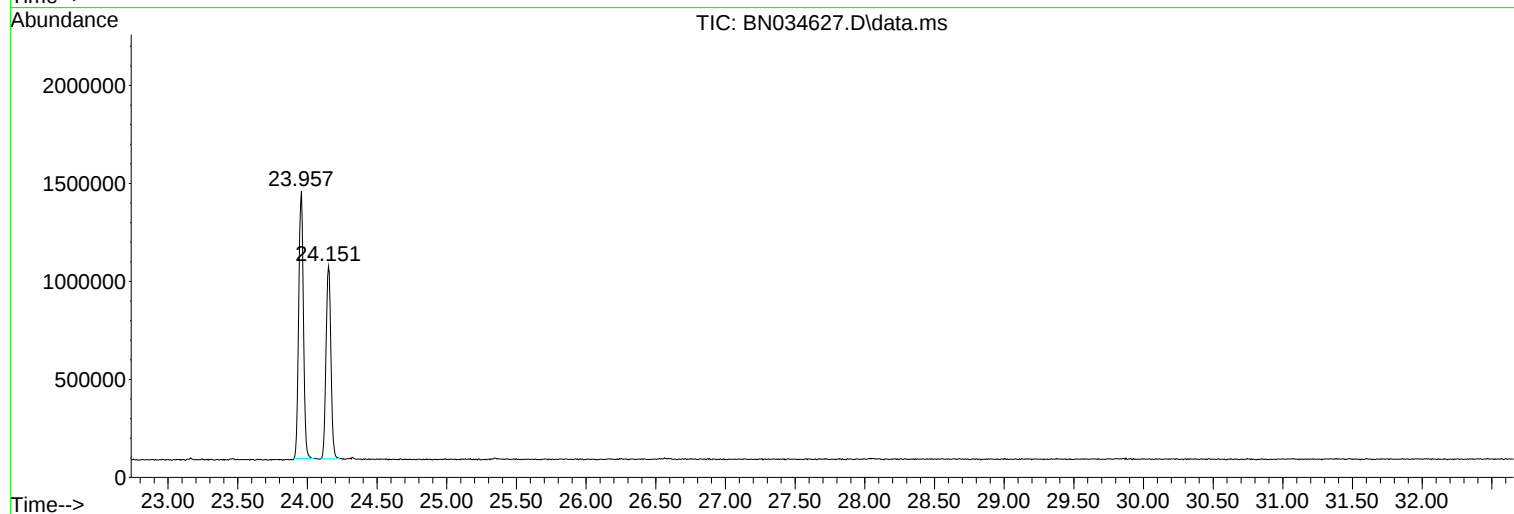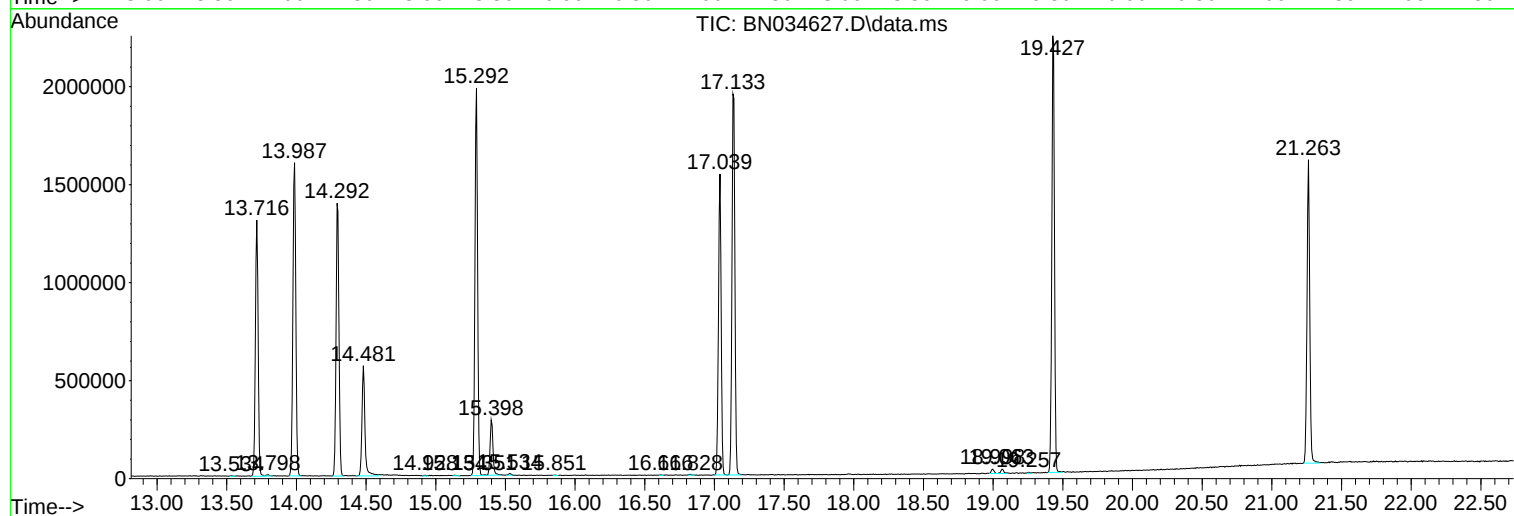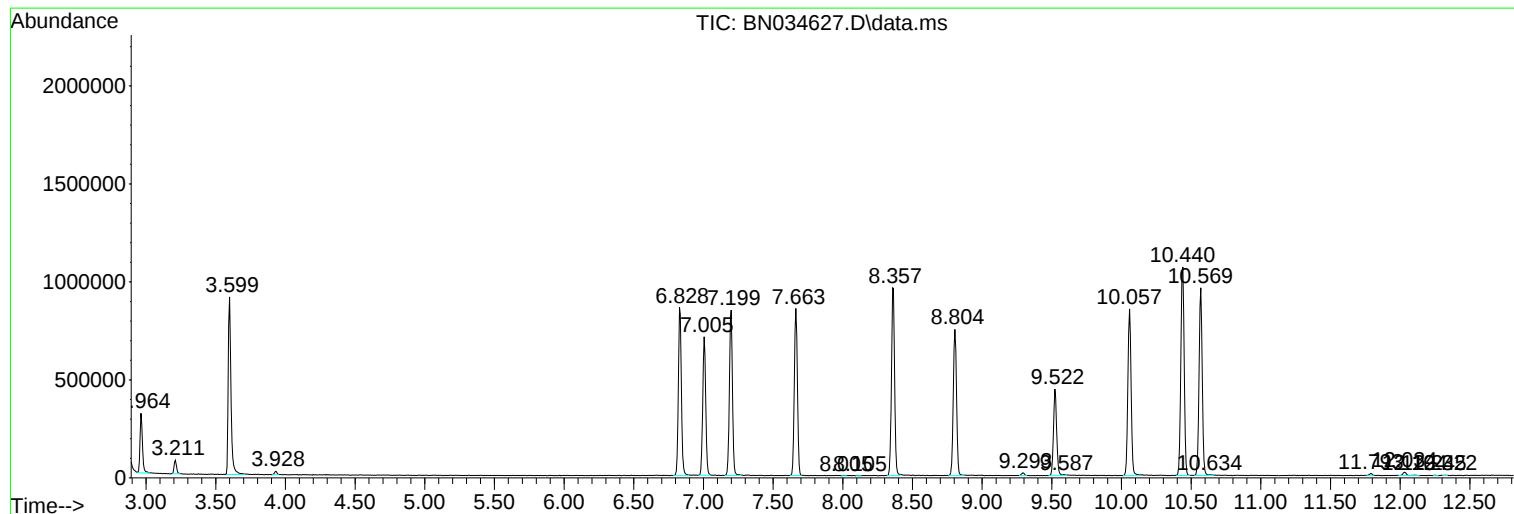

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034627.D
Acq On : 17 Oct 2024 18:37
Operator : RC/JU
Sample : PB164170BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK170

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034627.D
Acq On : 17 Oct 2024 18:37
Operator : RC/JU
Sample : PB164170BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK170

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------