

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034633.D
 Acq On : 17 Oct 2024 22:33
 Operator : RC/JU
 Sample : P4346-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EOAX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034633.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.970	9	14	29	rVB	1584915	2094549	66.77%	6.529%
2	3.217	51	56	62	rVB	32407	43004	1.37%	0.134%
3	3.605	118	122	138	rBV	413508	578611	18.44%	1.803%
4	3.793	150	154	158	rBV7	3940	7501	0.24%	0.023%
5	3.934	173	178	184	rVB	26185	36707	1.17%	0.114%
6	4.287	235	238	241	rVB4	3495	3400	0.11%	0.011%
7	4.822	325	329	334	rBV6	3910	7739	0.25%	0.024%
8	5.058	365	369	376	rVB8	6394	12826	0.41%	0.040%
9	5.640	465	468	470	rBV4	2594	3913	0.12%	0.012%
10	5.734	479	484	485	rBV5	2215	3566	0.11%	0.011%
11	6.605	628	632	637	rVB8	5187	7387	0.24%	0.023%
12	6.664	637	642	647	rBV9	3960	9618	0.31%	0.030%
13	6.769	653	660	664	rVB8	2529	4819	0.15%	0.015%
14	6.834	664	671	680	rBV	457077	723653	23.07%	2.256%
15	7.005	694	700	709	rVB	373820	563659	17.97%	1.757%
16	7.199	723	733	739	rBV	463514	705893	22.50%	2.200%
17	7.269	744	745	751	rVV5	2660	3605	0.11%	0.011%
18	7.316	751	753	756	rVV4	3251	3882	0.12%	0.012%
19	7.369	759	762	764	rBV4	2705	3736	0.12%	0.012%
20	7.664	806	812	820	rVV	1152523	1758077	56.04%	5.480%
21	7.746	822	826	829	rVV3	12006	17389	0.55%	0.054%
22	7.934	854	858	861	rVB6	2751	3531	0.11%	0.011%
23	8.363	924	931	938	rBV	525881	819126	26.11%	2.553%
24	8.805	999	1006	1018	rBV	390727	626607	19.97%	1.953%
25	8.987	1033	1037	1043	rBV8	4752	9214	0.29%	0.029%
26	9.293	1084	1089	1095	rVB	18606	29015	0.92%	0.090%
27	9.387	1099	1105	1110	rVB2	39932	60406	1.93%	0.188%
28	9.522	1121	1128	1136	rBV	218251	369280	11.77%	1.151%
29	9.587	1136	1139	1143	rVB6	2785	4749	0.15%	0.015%
30	10.058	1212	1219	1228	rBV	425258	709688	22.62%	2.212%
31	10.228	1246	1248	1253	rVV5	2617	4153	0.13%	0.013%
32	10.440	1275	1284	1292	rBV	1392755	2286034	72.87%	7.125%
33	10.569	1298	1306	1315	rBV	492503	809586	25.81%	2.523%
34	10.805	1344	1346	1349	rBV4	2774	3258	0.10%	0.010%
35	10.899	1359	1362	1365	rBV5	3063	3174	0.10%	0.010%
36	10.963	1369	1373	1375	rVV5	2224	3376	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034633.D
 Acq On : 17 Oct 2024 22:33
 Operator : RC/JU
 Sample : P4346-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EOAX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

37	10.993	1375	1378	1383	rVB4	11739	15854	0.51%	0.049%
38	11.240	1415	1420	1425	rBV7	3151	5329	0.17%	0.017%
39	11.510	1459	1466	1468	rVV5	3005	5196	0.17%	0.016%
40	11.528	1468	1469	1475	rVB4	2533	3476	0.11%	0.011%
41	11.793	1509	1514	1518	rVB2	8674	12192	0.39%	0.038%
42	11.834	1518	1521	1522	rVV3	3816	3792	0.12%	0.012%
43	11.852	1522	1524	1526	rVV3	3780	3539	0.11%	0.011%
44	11.887	1526	1530	1531	rVV4	2523	3670	0.12%	0.011%
45	11.899	1531	1532	1538	rVV6	3549	5312	0.17%	0.017%
46	12.034	1551	1555	1559	rVB3	9786	14162	0.45%	0.044%
47	12.116	1565	1569	1570	rBV3	2619	3173	0.10%	0.010%
48	12.299	1595	1600	1603	rBV2	9676	12354	0.39%	0.039%
49	12.393	1611	1616	1618	rBV6	2063	3424	0.11%	0.011%
50	12.810	1684	1687	1692	rBV6	2654	4994	0.16%	0.016%
51	12.875	1695	1698	1701	rVB4	2751	3609	0.12%	0.011%
52	13.075	1729	1732	1737	rVB4	2266	3610	0.12%	0.011%
53	13.134	1737	1742	1743	rBV4	2721	4860	0.15%	0.015%
54	13.163	1743	1747	1751	rVV4	5548	7916	0.25%	0.025%
55	13.222	1753	1757	1760	rBV6	2353	3474	0.11%	0.011%
56	13.716	1835	1841	1849	rBV	637190	873718	27.85%	2.723%
57	13.793	1852	1854	1858	rVV6	4861	7184	0.23%	0.022%
58	13.828	1858	1860	1864	rVB5	4006	4354	0.14%	0.014%
59	13.987	1880	1887	1900	rBV	837785	1197692	38.18%	3.733%
60	14.146	1909	1914	1915	rBV5	2357	3202	0.10%	0.010%
61	14.163	1915	1917	1923	rVB6	2217	3831	0.12%	0.012%
62	14.298	1933	1940	1949	rBV	1688731	2421921	77.20%	7.549%
63	14.363	1949	1951	1955	rVB5	3751	3450	0.11%	0.011%
64	14.487	1965	1972	1982	rBV	199725	322664	10.29%	1.006%
65	14.716	2009	2011	2019	rVB8	5650	9740	0.31%	0.030%
66	14.863	2034	2036	2040	rVV5	3899	3862	0.12%	0.012%
67	15.193	2090	2092	2097	rVB4	3392	3409	0.11%	0.011%
68	15.293	2103	2109	2116	rBV	950696	1318210	42.02%	4.109%
69	15.404	2123	2128	2134	rBV2	40010	55941	1.78%	0.174%
70	15.534	2144	2150	2154	rBV7	5798	8369	0.27%	0.026%
71	15.581	2156	2158	2160	rBV3	3398	3727	0.12%	0.012%
72	15.663	2167	2172	2177	rBV	229409	296224	9.44%	0.923%
73	15.757	2185	2188	2190	rBV4	2544	3233	0.10%	0.010%
74	15.987	2223	2227	2231	rBV2	8385	12202	0.39%	0.038%
75	16.057	2236	2239	2240	rVV3	2443	3264	0.10%	0.010%
76	16.087	2241	2244	2250	rVB4	6853	12121	0.39%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034633.D
 Acq On : 17 Oct 2024 22:33
 Operator : RC/JU
 Sample : P4346-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EOAX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

77	16.228	2265	2268	2271	rBV5	3541	3820	0.12%	0.012%
78	16.316	2281	2283	2288	rBV6	3263	4891	0.16%	0.015%
79	16.416	2296	2300	2302	rVB5	3431	3778	0.12%	0.012%
80	16.469	2305	2309	2315	rBV9	5256	11238	0.36%	0.035%
81	16.822	2367	2369	2372	rBV3	6378	7714	0.25%	0.024%
82	16.910	2381	2384	2387	rBV5	5058	5778	0.18%	0.018%
83	16.998	2394	2399	2400	rBV5	2655	4280	0.14%	0.013%
84	17.039	2400	2406	2412	rBV	1752213	2467738	78.67%	7.692%
85	17.081	2412	2413	2417	rVV	31891	33275	1.06%	0.104%
86	17.139	2417	2423	2435	rVB	926860	1320744	42.10%	4.117%
87	17.239	2435	2440	2443	rBV6	12275	19060	0.61%	0.059%
88	17.269	2443	2445	2453	rVB5	19026	30487	0.97%	0.095%
89	17.357	2458	2460	2462	rBV3	4738	4324	0.14%	0.013%
90	17.457	2475	2477	2482	rVB4	10353	13361	0.43%	0.042%
91	17.569	2495	2496	2499	rBV3	4550	4144	0.13%	0.013%
92	17.969	2560	2564	2569	rBV2	65375	91673	2.92%	0.286%
93	18.257	2611	2613	2619	rBV7	8633	11657	0.37%	0.036%
94	18.410	2637	2639	2644	rVB5	14430	17416	0.56%	0.054%
95	19.098	2752	2756	2762	rVB	86967	112610	3.59%	0.351%
96	19.257	2780	2783	2787	rBV4	29338	37626	1.20%	0.117%
97	19.433	2807	2813	2821	rBV	1135170	1562985	49.82%	4.872%
98	21.263	3119	3124	3130	rBV2	1865557	2608094	83.14%	8.129%
99	23.957	3575	3582	3590	rVB2	701150	1546038	49.28%	4.819%
100	24.151	3607	3615	3627	rBV	1311846	3137021	100.00%	9.778%




Sum of corrected areas: 32082737

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034633.D
Acq On : 17 Oct 2024 22:33
Operator : RC/JU
Sample : P4346-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EOAX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

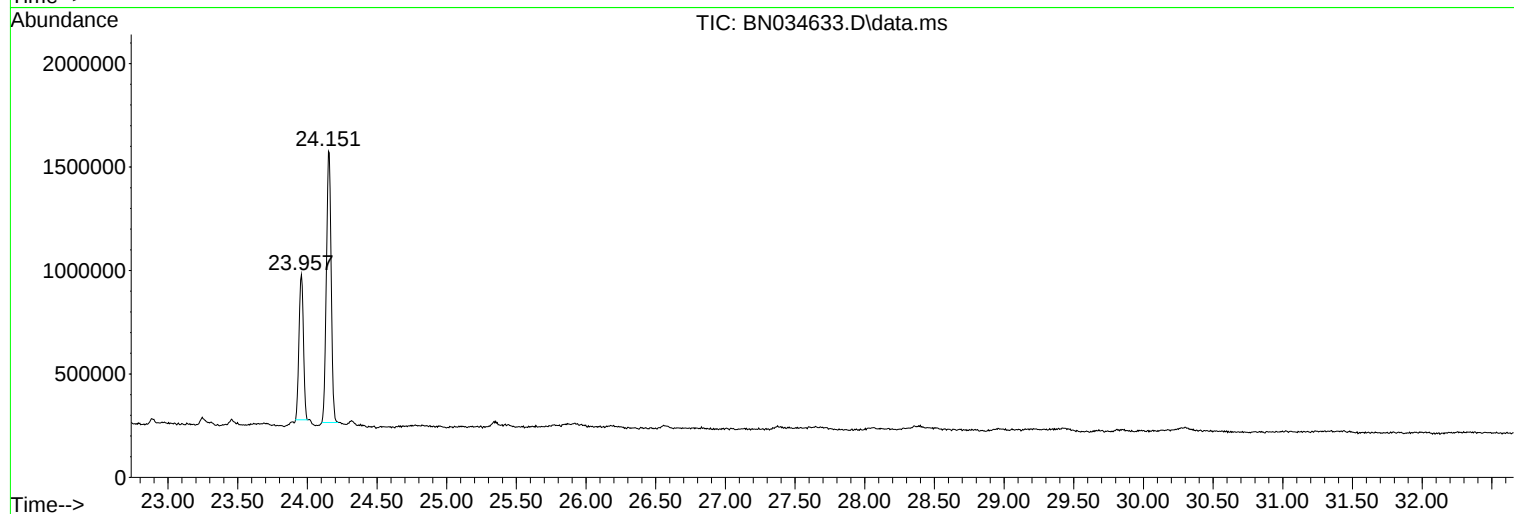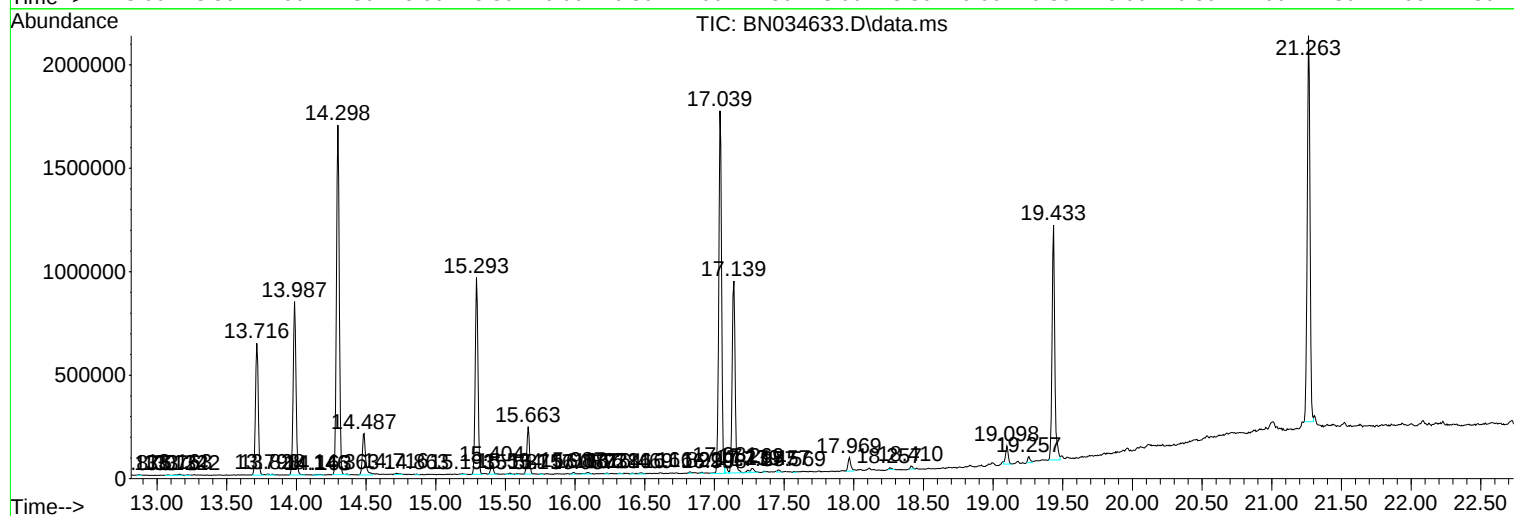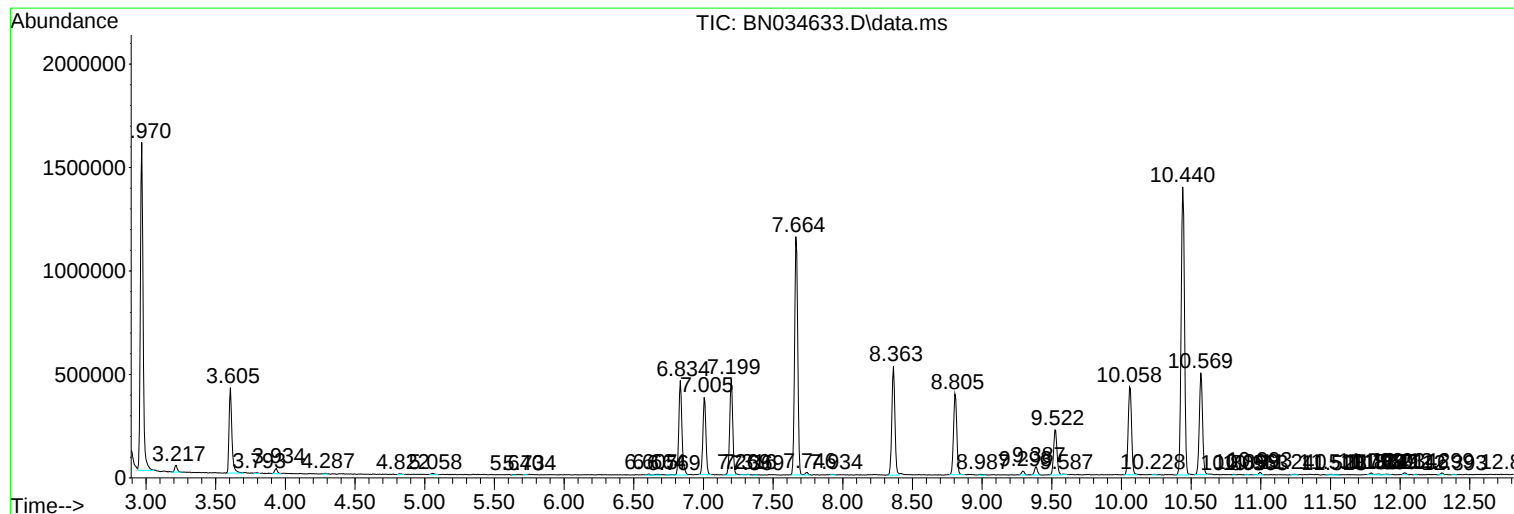

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034633.D
Acq On : 17 Oct 2024 22:33
Operator : RC/JU
Sample : P4346-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EOAX0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzophenone Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.663	2.45 ng/ul	296224	Acenaphthene-d10	14.299

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	95
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	91

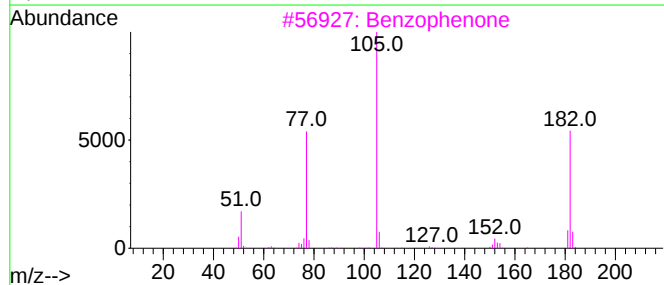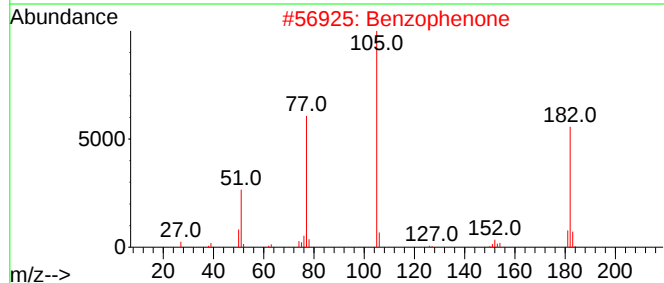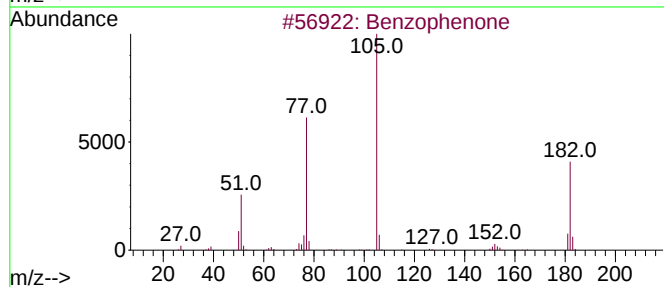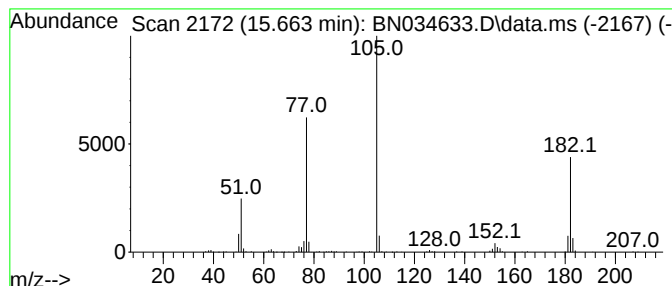

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034633.D
Acq On : 17 Oct 2024 22:33
Operator : RC/JU
Sample : P4346-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EOAX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.663	2.5	ng/u1	296224	3	14.299	2421920	20.0