

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034644.D
 Acq On : 18 Oct 2024 10:25
 Operator : RC/JU
 Sample : P4380-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E27H4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.970	8	14	36	rVB	9097173	13082603	100.00%	19.115%
2	3.123	36	40	48	rVV5	17814	36438	0.28%	0.053%
3	3.211	51	55	60	rVV	75009	93027	0.71%	0.136%
4	3.475	94	100	106	rBV5	11653	22837	0.17%	0.033%
5	3.605	118	122	131	rBV	291326	411132	3.14%	0.601%
6	3.928	171	177	184	rVB	41779	68706	0.53%	0.100%
7	4.552	274	283	288	rBV4	20572	39708	0.30%	0.058%
8	4.899	334	342	350	rVV4	8355	24936	0.19%	0.036%
9	4.993	352	358	367	rVV	588858	884335	6.76%	1.292%
10	5.193	388	392	399	rVB7	11010	22576	0.17%	0.033%
11	5.487	436	442	445	rBV2	16652	29473	0.23%	0.043%
12	5.705	474	479	482	rBV2	21274	29594	0.23%	0.043%
13	6.052	533	538	540	rBV2	29647	44620	0.34%	0.065%
14	6.081	540	543	549	rVB	37759	56294	0.43%	0.082%
15	6.222	561	567	570	rBV3	23706	38123	0.29%	0.056%
16	6.452	600	606	611	rBV5	15777	32005	0.24%	0.047%
17	6.552	617	623	627	rVB2	24709	43823	0.33%	0.064%
18	6.658	633	641	648	rBV6	10487	23983	0.18%	0.035%
19	6.834	663	671	685	rVB	257681	460458	3.52%	0.673%
20	7.005	692	700	707	rBV	1154385	1704341	13.03%	2.490%
21	7.199	726	733	744	rBV	1000662	1529409	11.69%	2.235%
22	7.663	805	812	820	rBV	1099930	1655380	12.65%	2.419%
23	7.740	820	825	832	rVB	84149	128135	0.98%	0.187%
24	8.158	890	896	905	rBV4	26087	50879	0.39%	0.074%
25	8.363	924	931	936	rBV3	28555	59643	0.46%	0.087%
26	8.422	936	941	945	rVV5	23809	45098	0.34%	0.066%
27	8.475	945	950	956	rVB	40730	66362	0.51%	0.097%
28	8.546	956	962	967	rBV4	19495	35649	0.27%	0.052%
29	8.758	992	998	1000	rBV2	20492	31629	0.24%	0.046%
30	8.805	1000	1006	1017	rVV	1241353	1991377	15.22%	2.910%
31	8.893	1017	1021	1026	rVV3	60782	112488	0.86%	0.164%
32	8.940	1026	1029	1034	rVV3	23948	37603	0.29%	0.055%
33	8.987	1034	1037	1043	rVV6	13522	26920	0.21%	0.039%
34	9.052	1043	1048	1055	rVV8	15217	36457	0.28%	0.053%
35	9.216	1068	1076	1084	rVV8	23631	58880	0.45%	0.086%
36	9.293	1084	1089	1097	rVB2	15259	27406	0.21%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034644.D
 Acq On : 18 Oct 2024 10:25
 Operator : RC/JU
 Sample : P4380-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E27H4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

37	9.375	1097	1103	1109	rBV9	10849	21168	0.16%	0.031%
38	9.522	1121	1128	1136	rBV	855108	1389974	10.62%	2.031%
39	9.769	1165	1170	1177	rBV9	19087	36482	0.28%	0.053%
40	9.863	1181	1186	1190	rVV3	47469	81428	0.62%	0.119%
41	9.910	1190	1194	1203	rVV4	41646	90556	0.69%	0.132%
42	9.999	1203	1209	1213	rVV3	54903	86513	0.66%	0.126%
43	10.057	1213	1219	1229	rVB	974228	1578726	12.07%	2.307%
44	10.228	1240	1248	1255	rBV3	32056	68029	0.52%	0.099%
45	10.304	1255	1261	1267	rBV	85678	147115	1.12%	0.215%
46	10.440	1277	1284	1291	rBV	1332887	2166268	16.56%	3.165%
47	10.510	1291	1296	1301	rVB	74772	117681	0.90%	0.172%
48	10.575	1301	1307	1310	rBV3	18751	40825	0.31%	0.060%
49	10.963	1367	1373	1383	rBV	44536	89178	0.68%	0.130%
50	11.052	1383	1388	1391	rBV6	11318	23125	0.18%	0.034%
51	11.251	1414	1422	1430	rBV2	708749	1240533	9.48%	1.813%
52	11.540	1467	1471	1481	rVB2	19315	39769	0.30%	0.058%
53	11.699	1492	1498	1504	rVB	66733	112882	0.86%	0.165%
54	11.787	1507	1513	1517	rBV4	13899	28645	0.22%	0.042%
55	11.928	1531	1537	1543	rBV	49737	83250	0.64%	0.122%
56	12.028	1551	1554	1563	rVB4	29372	55434	0.42%	0.081%
57	12.199	1578	1583	1587	rBV2	16042	26330	0.20%	0.038%
58	12.398	1611	1617	1627	rBV5	73721	197453	1.51%	0.289%
59	12.563	1640	1645	1648	rBV6	20209	37035	0.28%	0.054%
60	12.669	1658	1663	1669	rBV7	37266	70653	0.54%	0.103%
61	12.763	1675	1679	1685	rBV7	28017	57178	0.44%	0.084%
62	12.834	1685	1691	1695	rVB3	38450	67205	0.51%	0.098%
63	13.146	1739	1744	1749	rBV7	26195	41890	0.32%	0.061%
64	13.204	1749	1754	1759	rVV	115177	180688	1.38%	0.264%
65	13.251	1759	1762	1766	rVB6	25517	34235	0.26%	0.050%
66	13.410	1783	1789	1792	rBV7	17601	34969	0.27%	0.051%
67	13.451	1792	1796	1801	rVV7	12477	22436	0.17%	0.033%
68	13.510	1802	1806	1810	rBV7	15407	25637	0.20%	0.037%
69	13.651	1826	1830	1835	rVB3	103022	149764	1.14%	0.219%
70	13.716	1835	1841	1851	rVB	2006251	2964346	22.66%	4.331%
71	13.857	1861	1865	1870	rVB6	34612	47843	0.37%	0.070%
72	13.940	1872	1879	1881	rVV7	32004	58745	0.45%	0.086%
73	13.987	1881	1887	1893	rVB	1241219	1815324	13.88%	2.652%
74	14.040	1893	1896	1901	rBV4	14078	20852	0.16%	0.030%
75	14.157	1912	1916	1920	rBV	51612	82321	0.63%	0.120%
76	14.298	1932	1940	1953	rBV	1672470	2468748	18.87%	3.607%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034644.D
 Acq On : 18 Oct 2024 10:25
 Operator : RC/JU
 Sample : P4380-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E27H4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

77	14.481	1966	1971	1978	rVV	358154	534423	4.08%	0.781%
78	14.640	1993	1998	2004	rBV	139123	205834	1.57%	0.301%
79	14.828	2025	2030	2033	rBV	111840	177682	1.36%	0.260%
80	15.016	2058	2062	2067	rBV2	38006	54798	0.42%	0.080%
81	15.292	2103	2109	2122	rVB	3052284	4209605	32.18%	6.151%
82	15.404	2122	2128	2135	rBV	620718	896394	6.85%	1.310%
83	15.792	2191	2194	2199	rBV6	21238	32310	0.25%	0.047%
84	15.851	2201	2204	2208	rVB4	26577	36613	0.28%	0.053%
85	15.928	2214	2217	2219	rBV2	33089	42495	0.32%	0.062%
86	15.957	2220	2222	2225	rVV	48687	72952	0.56%	0.107%
87	15.987	2225	2227	2234	rVB2	78594	106497	0.81%	0.156%
88	16.128	2248	2251	2257	rBV2	31150	50693	0.39%	0.074%
89	16.322	2281	2284	2291	rBV4	30980	52692	0.40%	0.077%
90	16.516	2314	2317	2320	rBV2	34794	46842	0.36%	0.068%
91	17.039	2400	2406	2413	rVB	1803403	2456211	18.77%	3.589%
92	17.139	2417	2423	2431	rVB	2802723	3974751	30.38%	5.808%
93	17.651	2507	2510	2513	rBV3	36657	56020	0.43%	0.082%
94	17.969	2561	2564	2572	rVB5	78879	127300	0.97%	0.186%
95	18.404	2633	2638	2645	rBV2	339368	546259	4.18%	0.798%
96	19.433	2807	2813	2819	rBV	3531288	4722219	36.10%	6.900%
97	20.939	3065	3069	3076	rVB	162722	242201	1.85%	0.354%
98	21.263	3119	3124	3136	rVB	1959661	2647882	20.24%	3.869%
99	23.957	3573	3582	3595	rVB	2179771	5075251	38.79%	7.416%
100	24.151	3606	3615	3630	rVB	1302989	3128819	23.92%	4.572%




Sum of corrected areas: 68440303

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034644.D
Acq On : 18 Oct 2024 10:25
Operator : RC/JU
Sample : P4380-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E27H4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

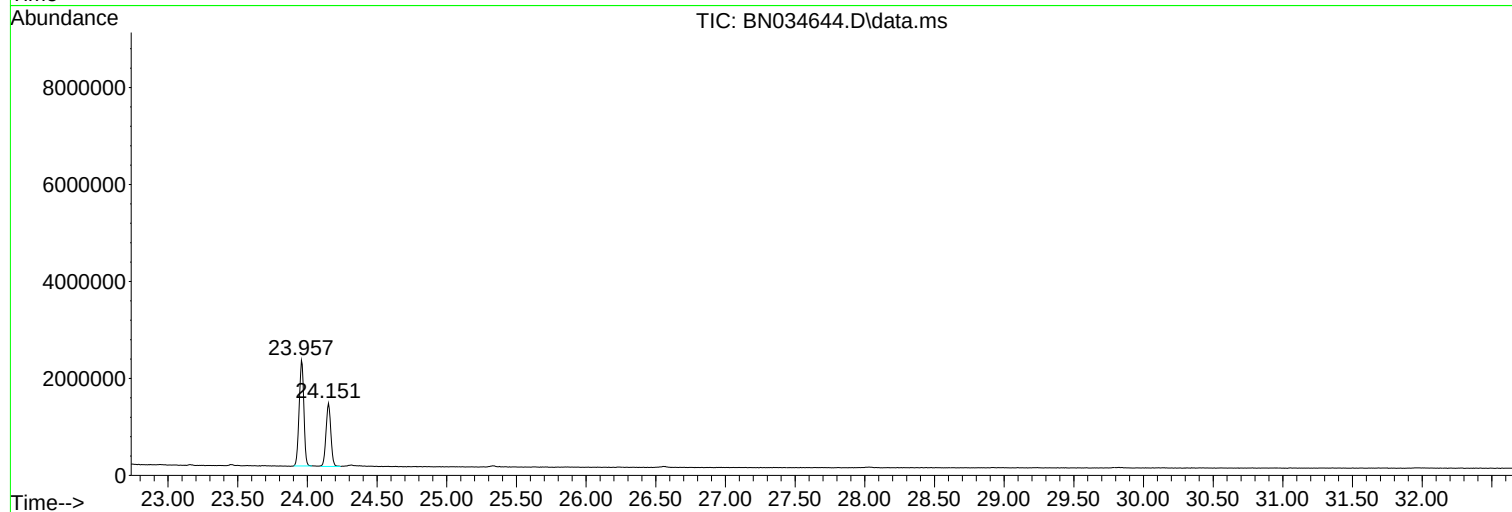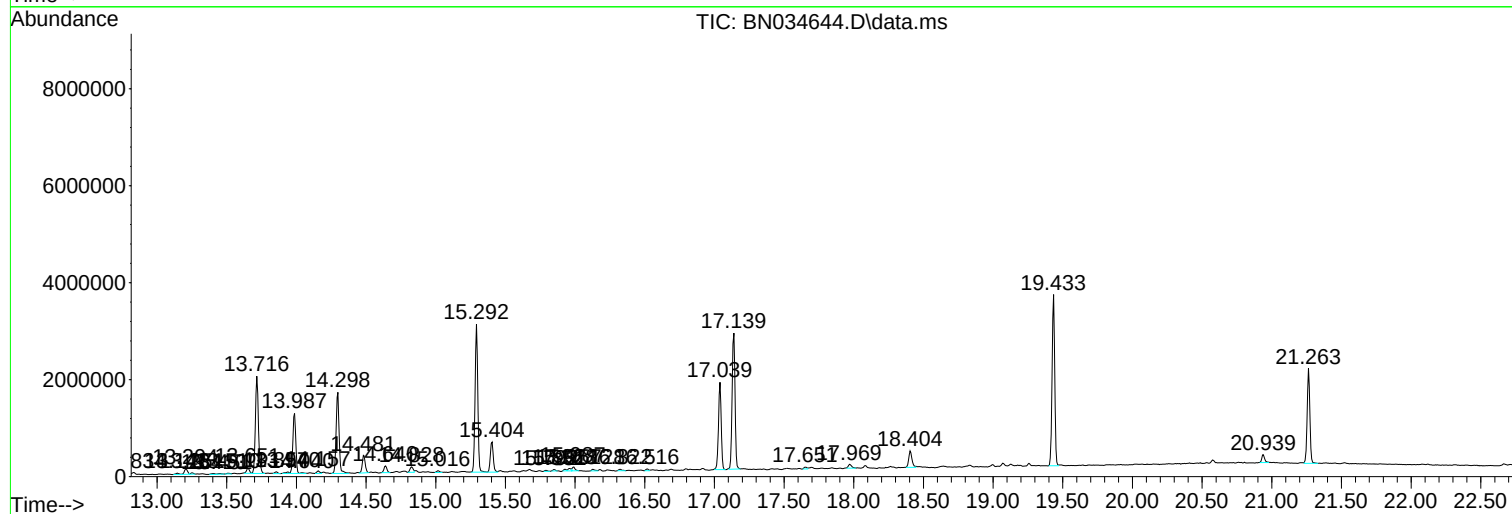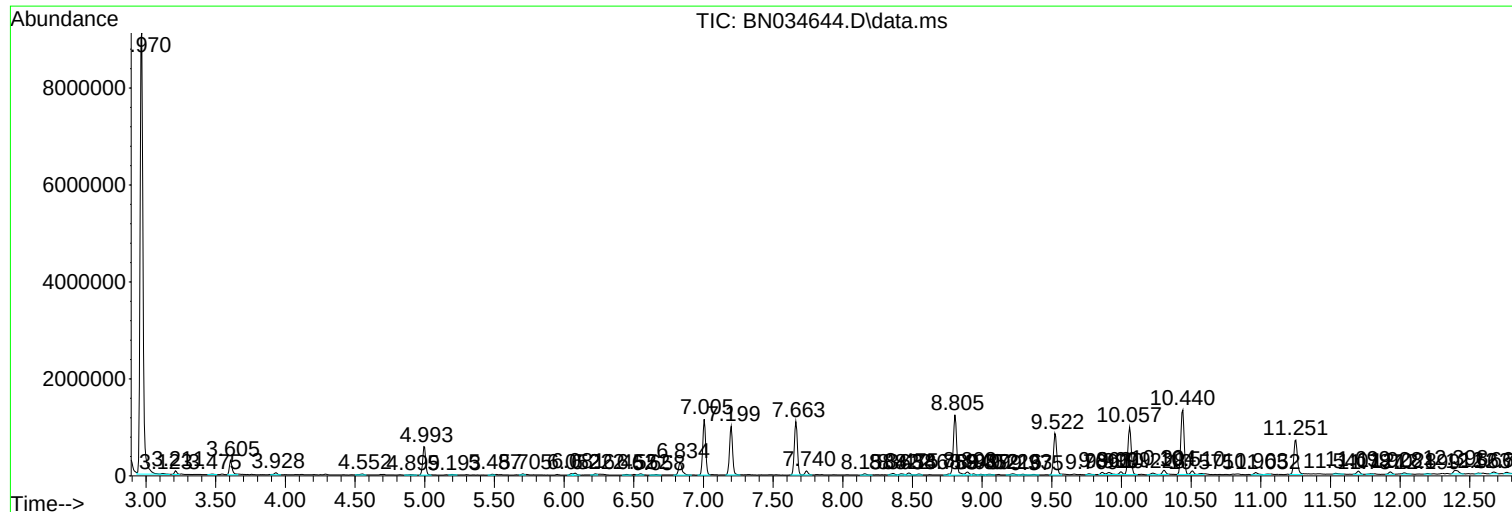

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034644.D
Acq On : 18 Oct 2024 10:25
Operator : RC/JU
Sample : P4380-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E27H4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034644.D
Acq On : 18 Oct 2024 10:25
Operator : RC/JU
Sample : P4380-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E27H4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc