

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034648.D
 Acq On : 18 Oct 2024 13:02
 Operator : RC/JU
 Sample : PB164041BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK041

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	24	rVB	412233	534296	11.47%	0.878%
2	3.211	51	55	62	rVB	104410	126391	2.71%	0.208%
3	3.599	117	121	135	rBV	1320806	1833615	39.35%	3.012%
4	3.928	172	177	184	rVB	33438	48911	1.05%	0.080%
5	4.293	238	239	244	rVB4	4115	4794	0.10%	0.008%
6	4.899	338	342	345	rBV5	3104	4716	0.10%	0.008%
7	6.834	664	671	684	rBV	1367586	2059094	44.19%	3.382%
8	7.005	694	700	711	rVB	1119851	1660157	35.63%	2.727%
9	7.199	726	733	742	rBV	1391166	2088812	44.83%	3.431%
10	7.664	804	812	820	rBV	1292466	1914325	41.09%	3.145%
11	8.364	924	931	944	rBV	1609710	2458744	52.77%	4.039%
12	8.611	969	973	976	rBV5	3311	5028	0.11%	0.008%
13	8.805	995	1006	1014	rBV	1224836	1952442	41.90%	3.207%
14	9.287	1083	1088	1094	rBV2	15003	22486	0.48%	0.037%
15	9.522	1120	1128	1141	rBV	838426	1373479	29.48%	2.256%
16	10.058	1211	1219	1233	rBV	1408072	2264389	48.60%	3.720%
17	10.440	1275	1284	1295	rVB	1612229	2655279	56.99%	4.362%
18	10.569	1295	1306	1315	rBV	1528675	2453256	52.65%	4.030%
19	11.246	1415	1421	1423	rBV6	3177	5845	0.13%	0.010%
20	11.358	1434	1440	1442	rBV4	6782	10754	0.23%	0.018%
21	11.787	1507	1513	1517	rVB2	12249	18225	0.39%	0.030%
22	12.034	1549	1555	1562	rBV	30914	51440	1.10%	0.084%
23	13.263	1761	1764	1769	rBV4	3424	5789	0.12%	0.010%
24	13.716	1834	1841	1851	rBV	2123514	2816338	60.44%	4.626%
25	13.793	1851	1854	1857	rVV4	8934	12966	0.28%	0.021%
26	13.987	1879	1887	1896	rBV	2572749	3704581	79.51%	6.085%
27	14.299	1932	1940	1947	rBV	2011116	2940561	63.11%	4.830%
28	14.487	1965	1972	1987	rBV	876051	1289275	27.67%	2.118%
29	14.722	2008	2012	2015	rVB4	6038	7711	0.17%	0.013%
30	14.957	2048	2052	2054	rBV5	3311	5088	0.11%	0.008%
31	15.293	2102	2109	2116	rBV	2906913	4020181	86.28%	6.604%
32	15.357	2116	2120	2122	rBV3	5041	6568	0.14%	0.011%
33	15.404	2122	2128	2141	rVV	425791	583879	12.53%	0.959%
34	15.534	2147	2150	2156	rVB4	16308	21755	0.47%	0.036%
35	16.081	2240	2243	2246	rVB4	4676	5832	0.13%	0.010%
36	16.616	2330	2334	2335	rBV3	3834	4995	0.11%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034648.D
 Acq On : 18 Oct 2024 13:02
 Operator : RC/JU
 Sample : PB164041BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK041

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

37	16.822	2367	2369	2375	rVB3	4906	5976	0.13%	0.010%
38	17.040	2399	2406	2414	rBV	2029472	2832257	60.79%	4.652%
39	17.134	2416	2422	2433	rVB2	2765869	4038885	86.68%	6.634%
40	17.269	2439	2445	2448	rBV8	8412	11282	0.24%	0.019%
41	17.404	2465	2468	2473	rBV4	4695	8252	0.18%	0.014%
42	17.963	2559	2563	2567	rBV6	4695	8057	0.17%	0.013%
43	18.992	2735	2738	2744	rVB2	32554	42345	0.91%	0.070%
44	19.069	2746	2751	2754	rVB	34917	44880	0.96%	0.074%
45	19.434	2806	2813	2821	rBV	3096161	4162042	89.33%	6.837%
46	21.263	3118	3124	3135	rBV	1999454	2817091	60.46%	4.627%
47	23.951	3572	3581	3595	rVB	2060620	4659343	100.00%	7.654%
48	24.151	3606	3615	3628	rVB	1405178	3275023	70.29%	5.380%




Sum of corrected areas: 60877430

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034648.D
Acq On : 18 Oct 2024 13:02
Operator : RC/JU
Sample : PB164041BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK041

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

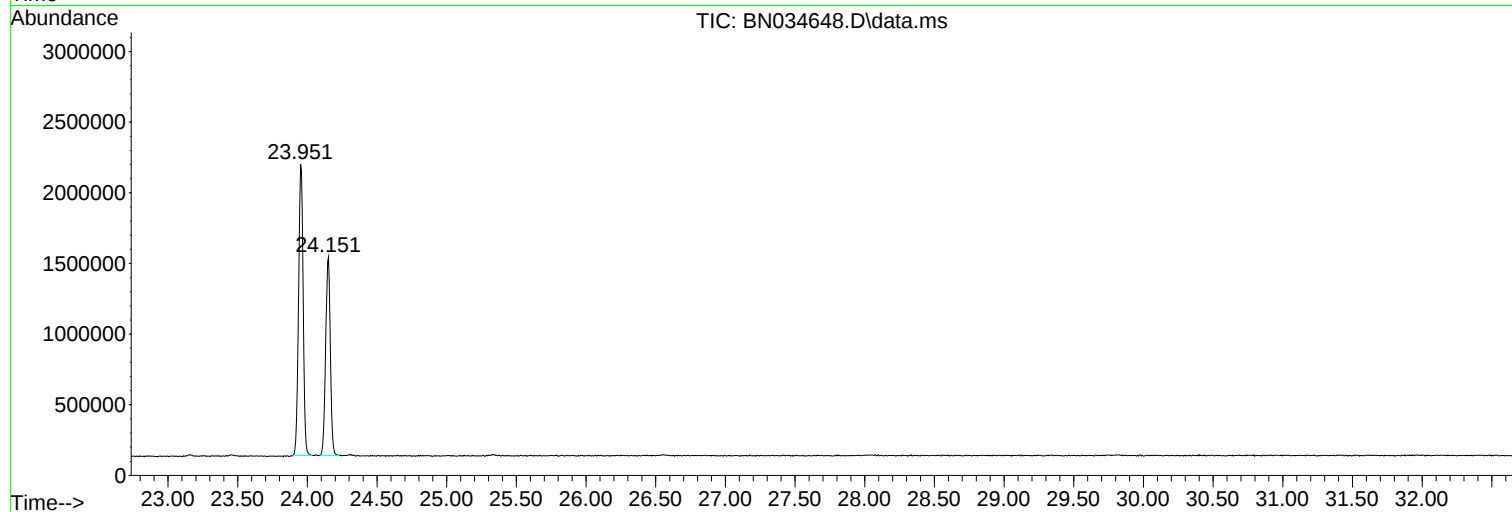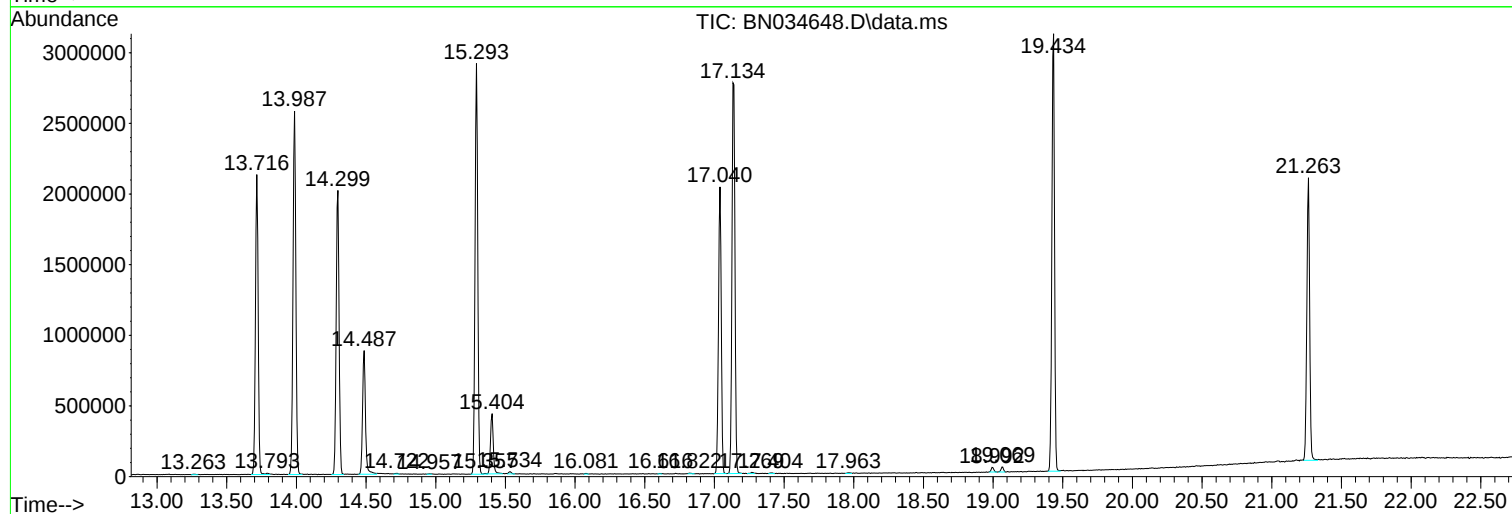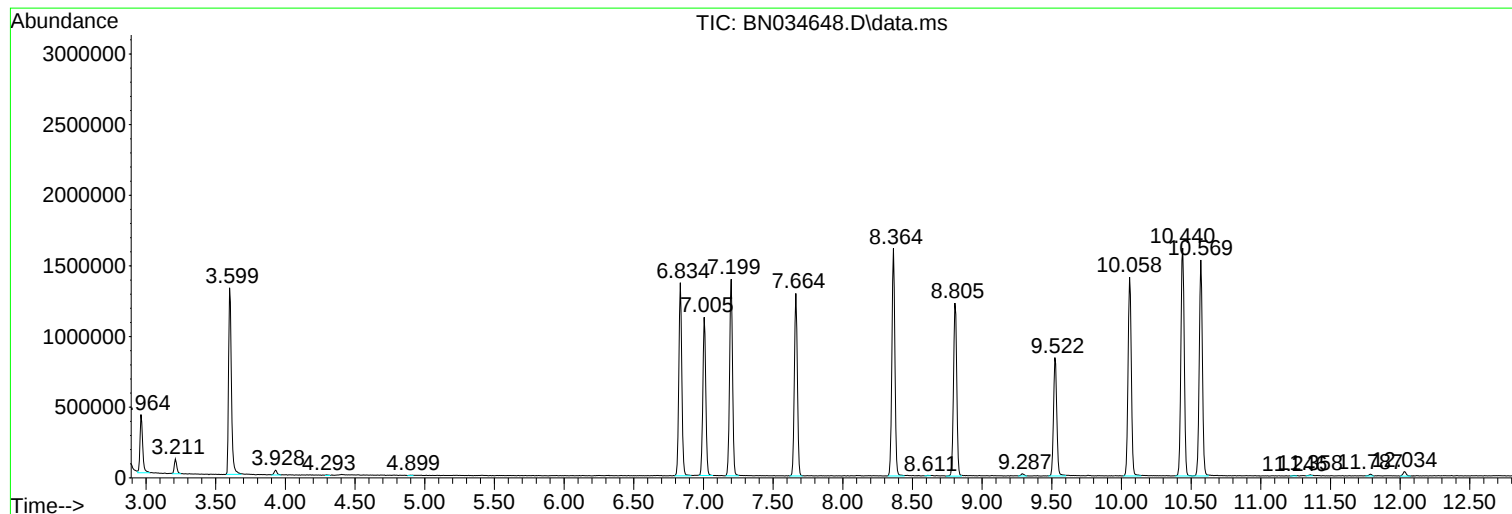

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034648.D
Acq On : 18 Oct 2024 13:02
Operator : RC/JU
Sample : PB164041BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK041

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034648.D
Acq On : 18 Oct 2024 13:02
Operator : RC/JU
Sample : PB164041BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK041

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc