

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034650.D
 Acq On : 18 Oct 2024 15:19
 Operator : RC/JU
 Sample : PB164050BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK050

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034650.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	8	13	26	rVB	276045	396030	7.23%	0.544%
2	3.205	50	54	63	rVB	96239	129769	2.37%	0.178%
3	3.599	116	121	142	rBV	1379874	2008181	36.66%	2.761%
4	3.928	172	177	182	rVB	18986	29150	0.53%	0.040%
5	6.828	660	670	679	rBV	1471542	2262672	41.30%	3.111%
6	6.999	693	699	713	rVB	1190240	1857558	33.91%	2.554%
7	7.193	725	732	745	rBV	1470668	2271957	41.47%	3.123%
8	7.657	803	811	819	rBV	1357194	2129164	38.87%	2.927%
9	8.357	923	930	942	rBV	1764619	2799505	51.10%	3.849%
10	8.804	997	1006	1017	rBV	1378630	2224811	40.61%	3.059%
11	9.287	1083	1088	1094	rVB	13580	19833	0.36%	0.027%
12	9.522	1120	1128	1142	rBV	996020	1579428	28.83%	2.171%
13	10.057	1211	1219	1230	rBV	1658756	2647568	48.33%	3.640%
14	10.434	1276	1283	1294	rVB	1906655	3170822	57.88%	4.359%
15	10.569	1298	1306	1319	rBV	1761215	2953214	53.91%	4.060%
16	11.787	1507	1513	1516	rBV4	10123	16249	0.30%	0.022%
17	12.028	1549	1554	1559	rBV2	35136	55977	1.02%	0.077%
18	13.716	1834	1841	1848	rBV	2836184	3787417	69.14%	5.207%
19	13.792	1851	1854	1861	rVB5	8511	11517	0.21%	0.016%
20	13.987	1880	1887	1894	rBV	3315929	4806682	87.74%	6.608%
21	14.298	1932	1940	1947	rBV	2677904	3960592	72.30%	5.445%
22	14.487	1965	1972	1988	rBV	1129627	1661591	30.33%	2.284%
23	14.716	2008	2011	2016	rVB6	10511	14405	0.26%	0.020%
24	15.292	2102	2109	2117	rBV	3935361	5478019	100.00%	7.531%
25	15.404	2122	2128	2139	rBV	617356	863158	15.76%	1.187%
26	15.528	2146	2149	2156	rVB2	19227	30340	0.55%	0.042%
27	15.857	2202	2205	2207	rBV4	4809	6029	0.11%	0.008%
28	16.081	2240	2243	2246	rVB4	6966	7457	0.14%	0.010%
29	16.610	2329	2333	2336	rVB5	4444	7046	0.13%	0.010%
30	16.822	2366	2369	2374	rVB5	7733	9889	0.18%	0.014%
31	17.039	2399	2406	2415	rVB	2977799	4068761	74.27%	5.594%
32	17.139	2416	2423	2433	rBV	3939310	5477711	99.99%	7.531%
33	17.269	2443	2445	2449	rVB5	5085	7142	0.13%	0.010%
34	17.410	2465	2469	2472	rBV4	6757	10124	0.18%	0.014%
35	17.963	2560	2563	2570	rBV7	9198	14132	0.26%	0.019%
36	18.998	2734	2739	2744	rVB	43966	58924	1.08%	0.081%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034650.D
Acq On : 18 Oct 2024 15:19
Operator : RC/JU
Sample : PB164050BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK050

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Title : SVOA CALIBRATION

37	19.063	2746	2750	2757	rBV	41957	59570	1.09%	0.082%
38	19.251	2779	2782	2786	rBV6	8648	10124	0.18%	0.014%
39	19.433	2806	2813	2821	rBV	3954953	5170503	94.39%	7.108%
40	21.263	3118	3124	3135	rVB	2201519	2976892	54.34%	4.093%
41	23.957	3573	3582	3594	rVB	1944259	4463570	81.48%	6.136%
42	24.151	3606	3615	3626	rVB	1361112	3224891	58.87%	4.434%




Sum of corrected areas: 72738374

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034650.D
Acq On : 18 Oct 2024 15:19
Operator : RC/JU
Sample : PB164050BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK050

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

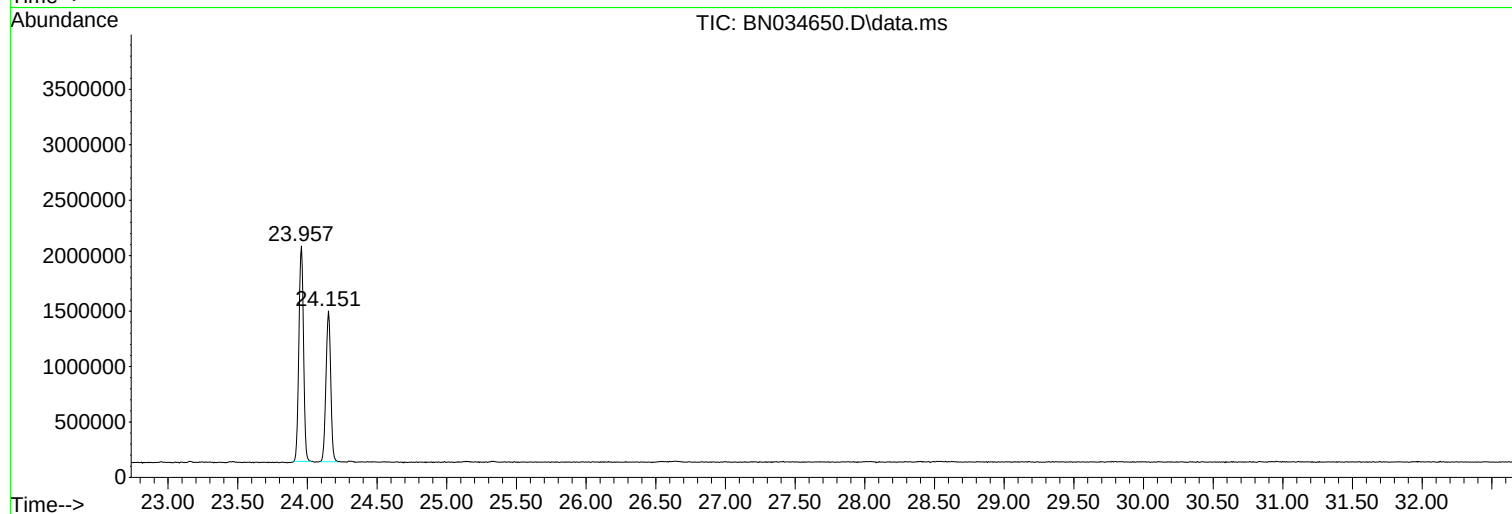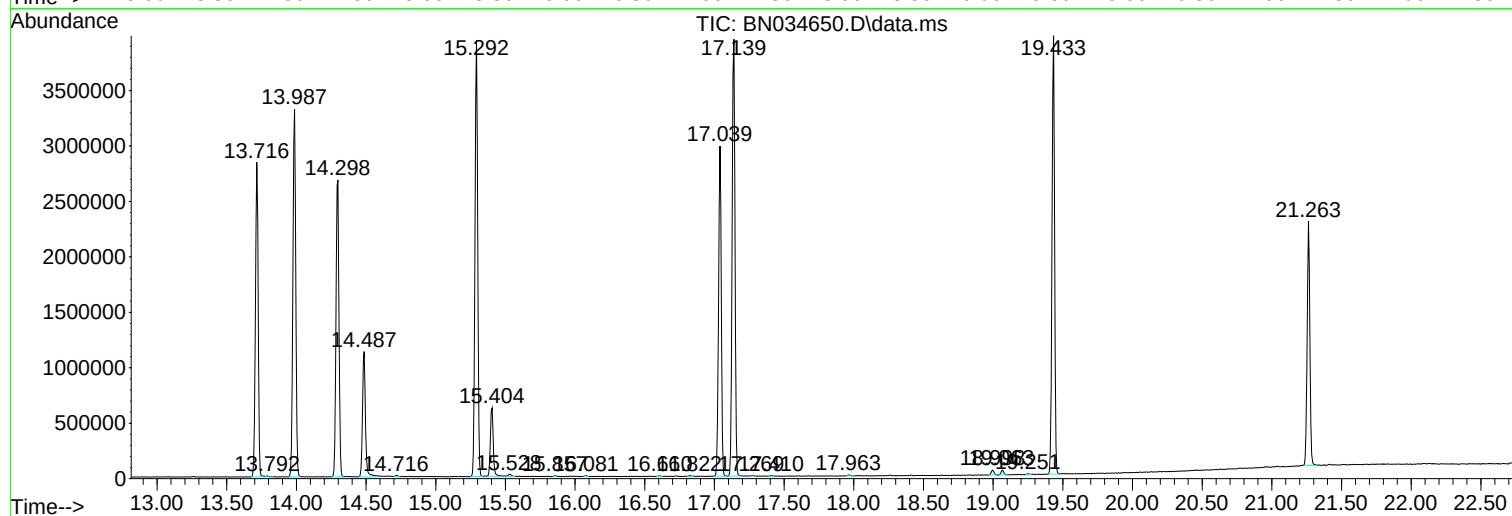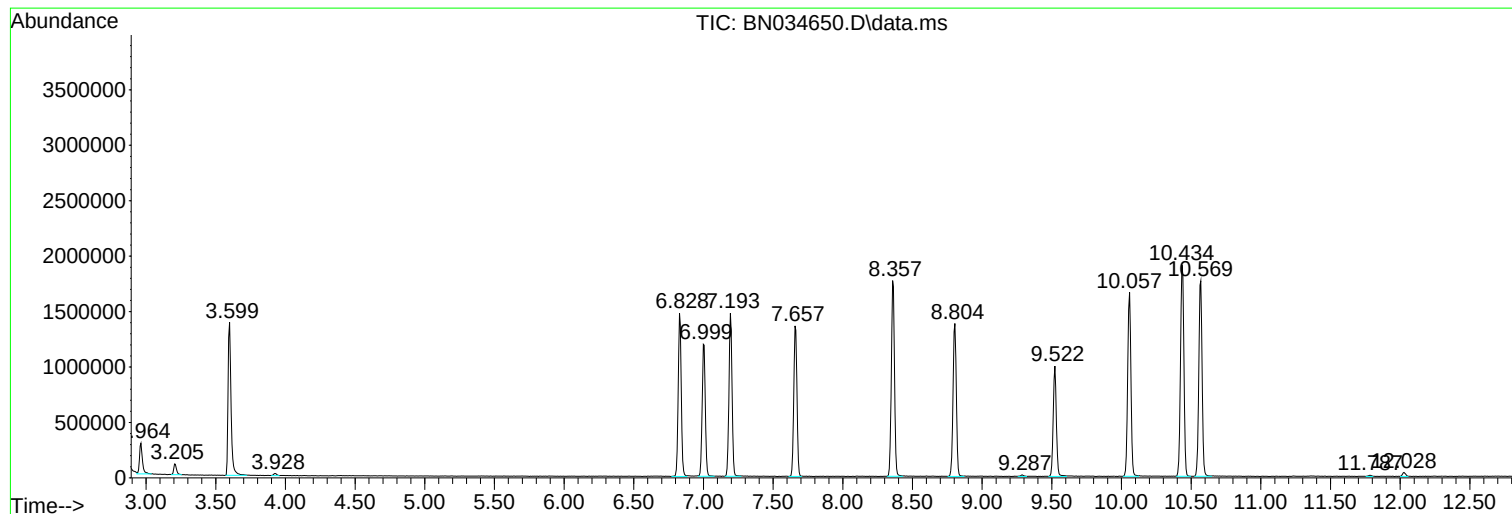

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034650.D
Acq On : 18 Oct 2024 15:19
Operator : RC/JU
Sample : PB164050BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK050

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034650.D
Acq On : 18 Oct 2024 15:19
Operator : RC/JU
Sample : PB164050BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK050

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc