

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034651.D
 Acq On : 18 Oct 2024 15:59
 Operator : RC/JU
 Sample : PB164094BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK094

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	26	rVB	319813	426196	7.36%	0.543%
2	3.211	51	55	64	rVB	119621	148063	2.56%	0.189%
3	3.599	117	121	139	rBV	1557190	2185066	37.71%	2.783%
4	3.928	173	177	182	rVB	23463	29136	0.50%	0.037%
5	6.834	663	671	683	rBV	1640193	2504903	43.23%	3.190%
6	7.005	694	700	709	rVB	1352633	2028389	35.01%	2.583%
7	7.199	725	733	743	rBV	1637014	2489718	42.97%	3.171%
8	7.664	805	812	823	rVB	1507456	2300354	39.70%	2.930%
9	8.363	922	931	944	rBV	1983440	3077843	53.12%	3.920%
10	8.805	996	1006	1017	rBV	1558982	2449530	42.28%	3.120%
11	9.287	1083	1088	1094	rVB3	17330	26302	0.45%	0.033%
12	9.522	1120	1128	1138	rBV	1062032	1693205	29.22%	2.157%
13	10.058	1212	1219	1232	rBV	1819087	2890491	49.89%	3.681%
14	10.440	1276	1284	1293	rVB	2065965	3375581	58.26%	4.299%
15	10.569	1297	1306	1319	rBV	1972832	3235132	55.83%	4.120%
16	11.787	1506	1513	1518	rVB3	14487	26408	0.46%	0.034%
17	12.028	1549	1554	1563	rVB2	38816	61309	1.06%	0.078%
18	12.299	1597	1600	1605	rVB2	6884	9447	0.16%	0.012%
19	13.075	1727	1732	1737	rBV6	4024	7221	0.12%	0.009%
20	13.269	1760	1765	1768	rBV5	6499	11797	0.20%	0.015%
21	13.716	1834	1841	1850	rBV	3057406	4021594	69.41%	5.122%
22	13.787	1851	1853	1857	rVB3	7892	9614	0.17%	0.012%
23	13.987	1880	1887	1896	rVB	3604713	5138198	88.68%	6.544%
24	14.293	1931	1939	1947	rBV	2786339	4149805	71.62%	5.285%
25	14.487	1965	1972	1984	rBV	1224992	1780957	30.74%	2.268%
26	14.716	2006	2011	2015	rBV8	8263	12888	0.22%	0.016%
27	15.293	2102	2109	2116	rBV	4253545	5794249	100.00%	7.380%
28	15.357	2116	2120	2122	rVV3	5708	7827	0.14%	0.010%
29	15.404	2122	2128	2142	rVV	668398	947665	16.36%	1.207%
30	15.534	2146	2150	2156	rVB3	20037	30714	0.53%	0.039%
31	15.863	2199	2206	2208	rBV8	5008	8621	0.15%	0.011%
32	16.081	2239	2243	2249	rVB7	5958	8253	0.14%	0.011%
33	16.728	2349	2353	2356	rBV5	5361	6017	0.10%	0.008%
34	16.822	2366	2369	2375	rVB3	7811	10183	0.18%	0.013%
35	17.039	2398	2406	2416	rBV	3144626	4221755	72.86%	5.377%
36	17.139	2416	2423	2431	rBV	4090997	5743131	99.12%	7.315%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034651.D
Acq On : 18 Oct 2024 15:59
Operator : RC/JU
Sample : PB164094BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK094

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Title : SVOA CALIBRATION

37	17.275	2443	2446	2451	rVB7	5015	6873	0.12%	0.009%
38	18.257	2610	2613	2617	rBV4	5334	8132	0.14%	0.010%
39	18.998	2733	2739	2744	rBV	47647	68089	1.18%	0.087%
40	19.069	2746	2751	2755	rVV	45470	61587	1.06%	0.078%
41	19.433	2806	2813	2819	rBV	3949891	5442662	93.93%	6.932%
42	21.263	3118	3124	3134	rBV	2347695	3298469	56.93%	4.201%
43	23.951	3572	3581	3595	rBV	2167384	5108856	88.17%	6.507%
44	24.151	3606	3615	3629	rVB	1543016	3654007	63.06%	4.654%




Sum of corrected areas: 78516237

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034651.D
Acq On : 18 Oct 2024 15:59
Operator : RC/JU
Sample : PB164094BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK094

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

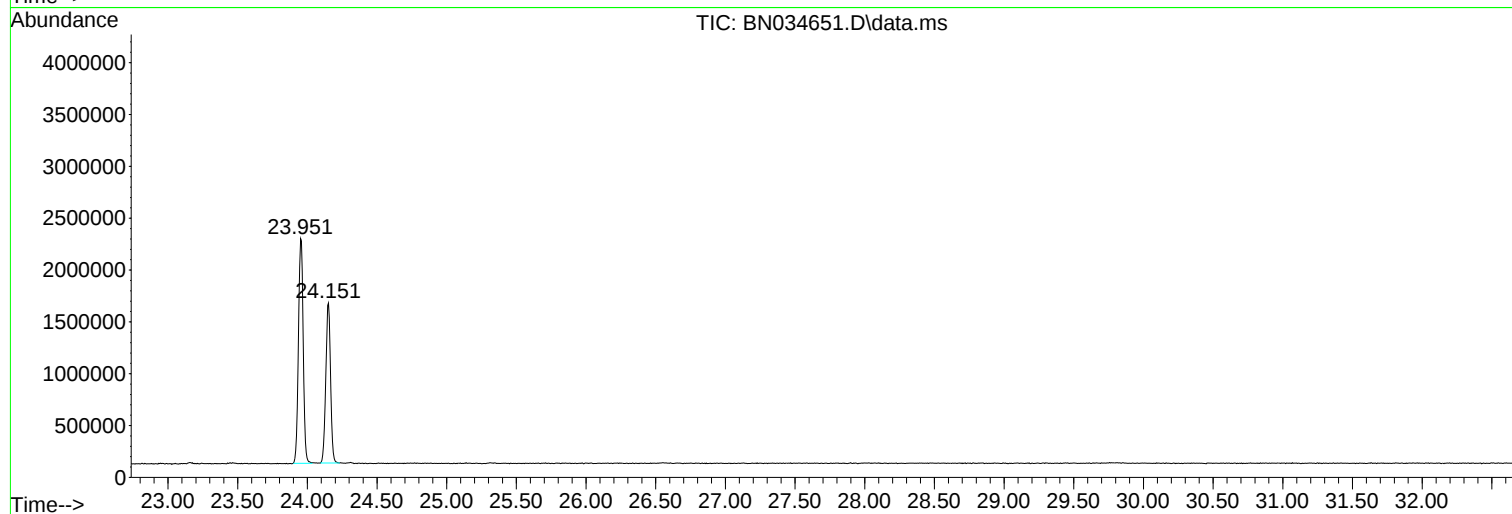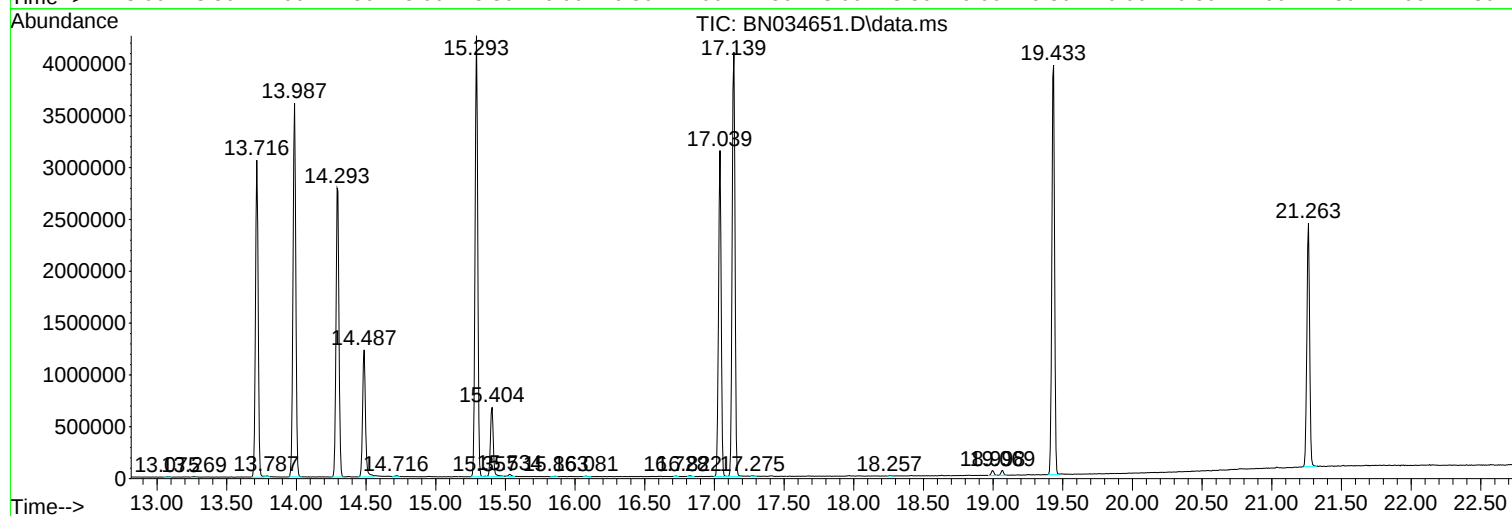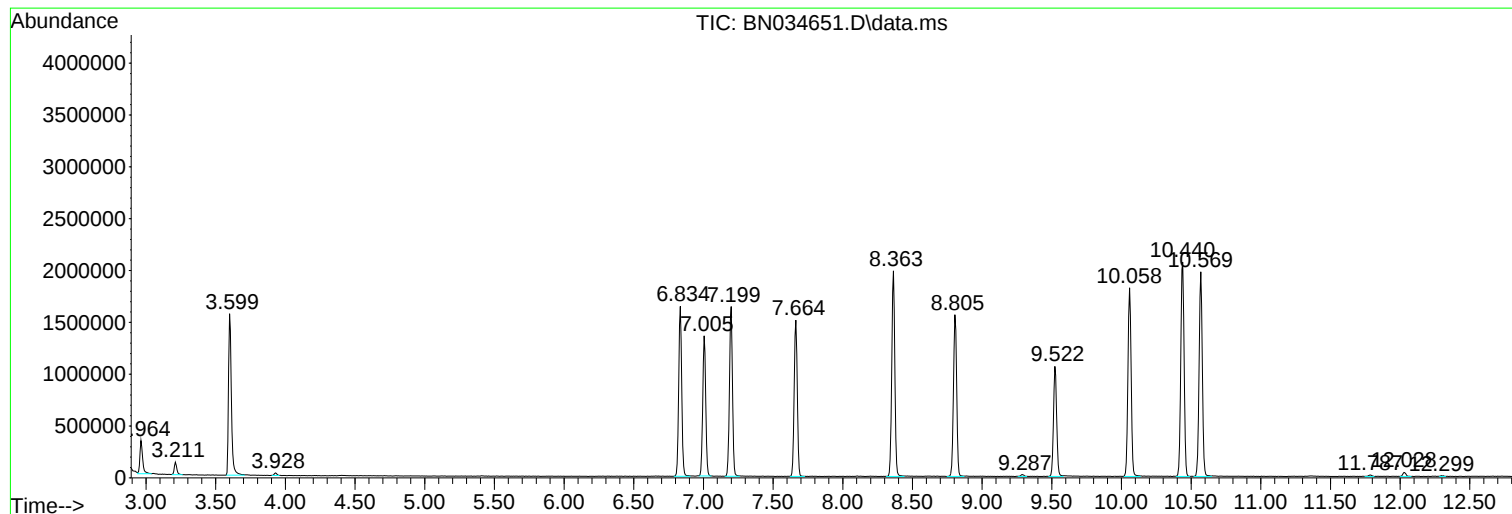

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034651.D
Acq On : 18 Oct 2024 15:59
Operator : RC/JU
Sample : PB164094BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK094

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034651.D
Acq On : 18 Oct 2024 15:59
Operator : RC/JU
Sample : PB164094BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK094

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc