

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034657.D
 Acq On : 18 Oct 2024 19:54
 Operator : RC/JU
 Sample : P4380-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E27G6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	8	13	36	rVB	12105381	18976008	100.00%	20.090%
2	3.117	37	39	46	rVB4	13631	19572	0.10%	0.021%
3	3.211	51	55	61	rBV	89134	110212	0.58%	0.117%
4	3.611	119	123	133	rBV	210396	303541	1.60%	0.321%
5	3.928	174	177	182	rVB	27624	35793	0.19%	0.038%
6	4.505	271	275	281	rBV	12024	21507	0.11%	0.023%
7	4.993	353	358	364	rBV	62637	95619	0.50%	0.101%
8	6.281	571	577	582	rVB6	13651	28986	0.15%	0.031%
9	6.675	635	644	649	rBV8	14035	37194	0.20%	0.039%
10	6.834	664	671	679	rBV	673191	1074649	5.66%	1.138%
11	6.905	681	683	693	rVB5	13253	20404	0.11%	0.022%
12	7.005	693	700	708	rBV	1555984	2359735	12.44%	2.498%
13	7.199	726	733	742	rBV	1849575	2827242	14.90%	2.993%
14	7.664	805	812	822	rBV	1515930	2338142	12.32%	2.475%
15	7.893	847	851	855	rBV6	13170	22602	0.12%	0.024%
16	8.158	890	896	900	rBV5	11835	21134	0.11%	0.022%
17	8.364	925	931	938	rBV	1672342	2569624	13.54%	2.720%
18	8.552	957	963	967	rBV6	18113	33011	0.17%	0.035%
19	8.805	999	1006	1018	rVV	1709052	2814470	14.83%	2.980%
20	8.899	1019	1022	1027	rVB2	22706	35685	0.19%	0.038%
21	9.075	1048	1052	1058	rVB7	13625	23805	0.13%	0.025%
22	9.287	1083	1088	1093	rVB2	24076	42048	0.22%	0.045%
23	9.363	1093	1101	1107	rBV6	13588	38212	0.20%	0.040%
24	9.522	1121	1128	1137	rBV	1314559	2114676	11.14%	2.239%
25	9.658	1147	1151	1158	rVB4	41305	70312	0.37%	0.074%
26	9.863	1179	1186	1192	rBV2	50103	91218	0.48%	0.097%
27	9.928	1192	1197	1204	rVV	116358	177130	0.93%	0.188%
28	9.993	1204	1208	1212	rVV3	24652	37505	0.20%	0.040%
29	10.058	1212	1219	1230	rVV	2094491	3447695	18.17%	3.650%
30	10.134	1230	1232	1242	rVB9	11820	25935	0.14%	0.027%
31	10.222	1242	1247	1253	rBV3	27587	53913	0.28%	0.057%
32	10.305	1256	1261	1267	rVV4	43691	83017	0.44%	0.088%
33	10.363	1267	1271	1276	rVB	24088	37326	0.20%	0.040%
34	10.440	1276	1284	1291	rBV	1991408	3282861	17.30%	3.476%
35	10.487	1291	1292	1300	rVB4	18263	26619	0.14%	0.028%
36	10.569	1300	1306	1315	rBV2	87085	187993	0.99%	0.199%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034657.D
 Acq On : 18 Oct 2024 19:54
 Operator : RC/JU
 Sample : P4380-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E27G6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

37	10.799	1340	1345	1349	rBV	41360	68096	0.36%	0.072%
38	10.987	1370	1377	1381	rBV6	11285	24198	0.13%	0.026%
39	11.075	1387	1392	1397	rVB6	16836	32362	0.17%	0.034%
40	11.246	1415	1421	1423	rBV3	25768	44097	0.23%	0.047%
41	11.540	1464	1471	1480	rVB6	25587	68407	0.36%	0.072%
42	11.787	1509	1513	1526	rVB7	21866	54026	0.28%	0.057%
43	12.028	1545	1554	1559	rBV	43170	91445	0.48%	0.097%
44	12.316	1601	1603	1610	rVB5	17026	32076	0.17%	0.034%
45	12.416	1612	1620	1626	rBV5	21943	70152	0.37%	0.074%
46	12.681	1659	1665	1671	rVB5	26103	51742	0.27%	0.055%
47	12.804	1683	1686	1695	rVB2	36297	75350	0.40%	0.080%
48	13.010	1717	1721	1724	rBV6	11828	21388	0.11%	0.023%
49	13.087	1731	1734	1739	rVB5	27023	35962	0.19%	0.038%
50	13.152	1739	1745	1751	rBV	128023	186216	0.98%	0.197%
51	13.457	1793	1797	1799	rBV4	18223	30572	0.16%	0.032%
52	13.522	1803	1808	1811	rVV	75143	104654	0.55%	0.111%
53	13.557	1811	1814	1818	rVB2	41662	55896	0.29%	0.059%
54	13.716	1835	1841	1848	rVB	2964798	4056856	21.38%	4.295%
55	13.793	1851	1854	1857	rBV2	30843	41175	0.22%	0.044%
56	13.987	1880	1887	1897	rBV	3761298	5512094	29.05%	5.836%
57	14.299	1933	1940	1947	rBV	2474709	3690725	19.45%	3.907%
58	14.487	1967	1972	1978	rBV	444874	646538	3.41%	0.684%
59	15.293	2103	2109	2115	rBV	4080121	5981403	31.52%	6.332%
60	15.404	2122	2128	2137	rBV	968729	1418738	7.48%	1.502%
61	15.987	2224	2227	2237	rVB	197750	306195	1.61%	0.324%
62	16.345	2285	2288	2292	rBV	73176	90058	0.47%	0.095%
63	17.040	2400	2406	2412	rBV	2543580	3443149	18.14%	3.645%
64	17.140	2417	2423	2436	rVB2	4052783	5633250	29.69%	5.964%
65	17.422	2467	2471	2476	rVB	396942	508161	2.68%	0.538%
66	17.975	2561	2565	2571	rVB3	151820	211219	1.11%	0.224%
67	19.257	2781	2783	2789	rVB2	126838	138368	0.73%	0.146%
68	19.434	2807	2813	2820	rBV	4099660	5589080	29.45%	5.917%
69	21.263	3119	3124	3131	rVB	2315072	3084311	16.25%	3.265%
70	23.957	3573	3582	3593	rVB	2583687	6008233	31.66%	6.361%
71	24.151	3607	3615	3626	rVB	1493976	3565585	18.79%	3.775%




Sum of corrected areas: 94457172

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034657.D
Acq On : 18 Oct 2024 19:54
Operator : RC/JU
Sample : P4380-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E27G6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

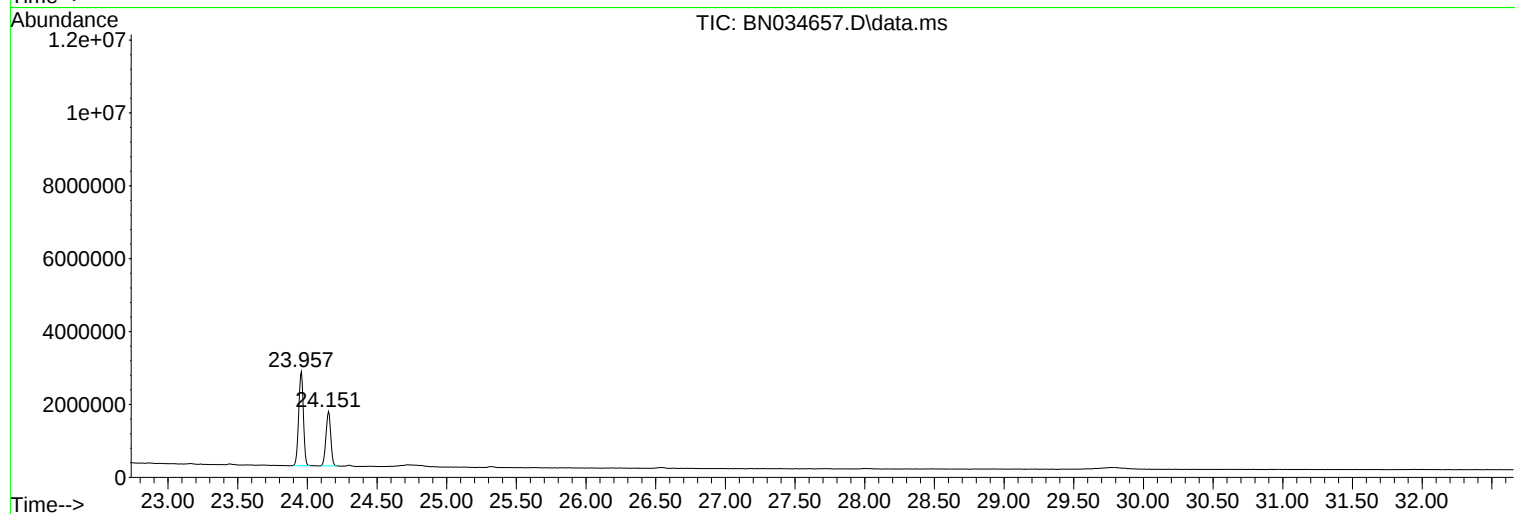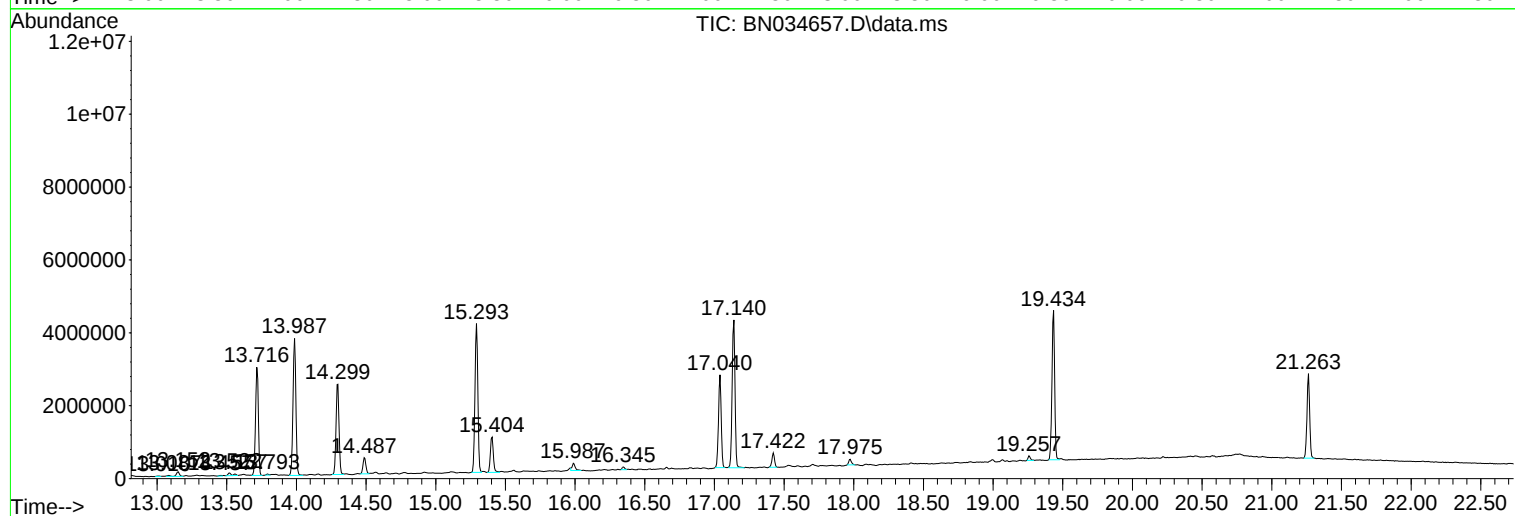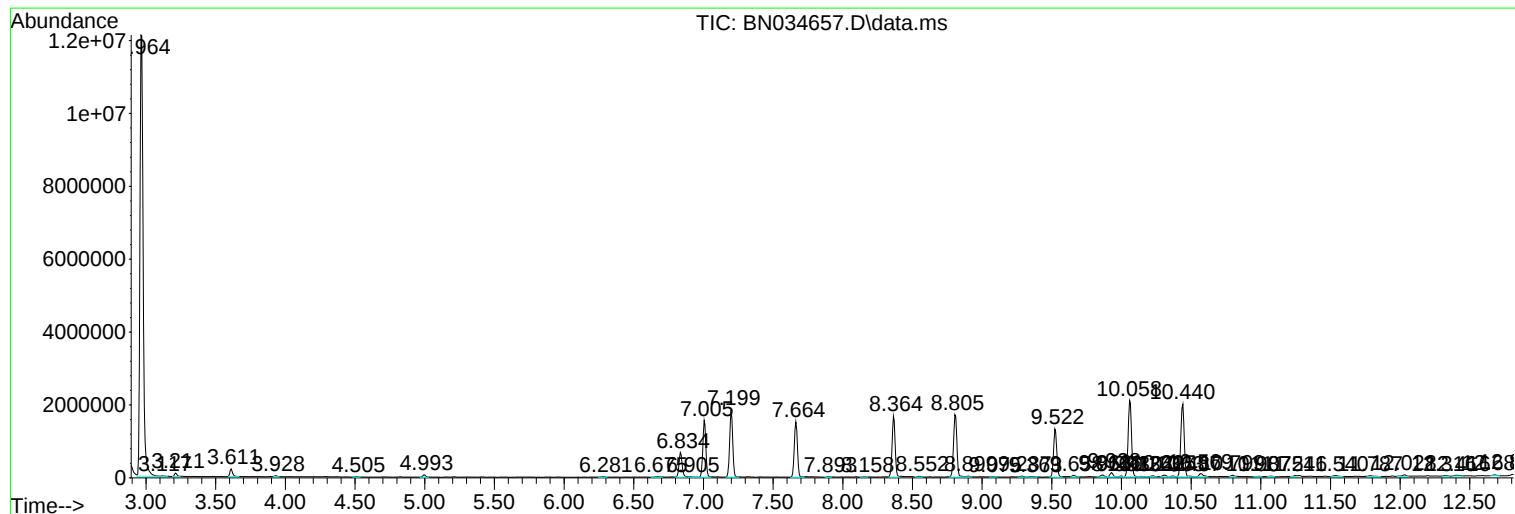

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034657.D
Acq On : 18 Oct 2024 19:54
Operator : RC/JU
Sample : P4380-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E27G6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Phenol, 4-(1-methyl-1-pheny... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.422	2.95 ng/ul	508161	Phenanthrene-d10	17.040

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Phenol, 4-(1-methyl-1-phenylethyl)-	212	C15H16O	000599-64-4	99
2			Phenol, 4-(1-methyl-1-phenylethyl)-	212	C15H16O	000599-64-4	99
3			Phenol, 4-(1-methyl-1-phenylethyl)-	212	C15H16O	000599-64-4	91
4			Dimethyl diphenylsilane	212	C14H16Si	000778-24-5	62
5			Dimethyl diphenylsilane	212	C14H16Si	000778-24-5	62

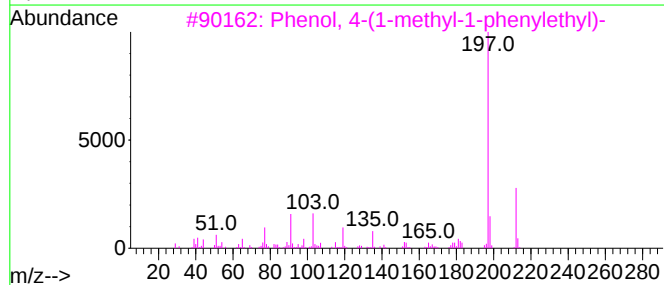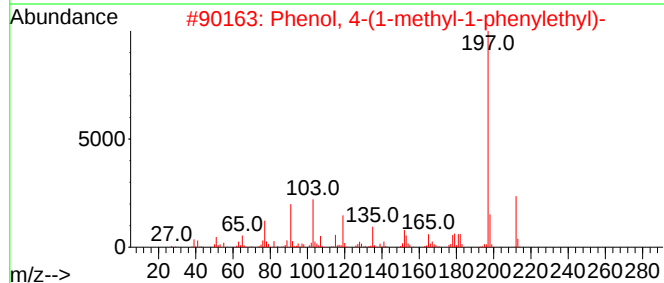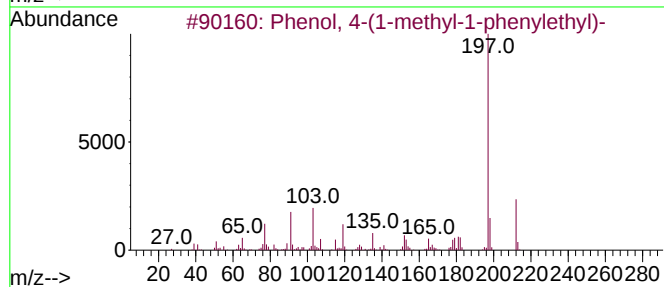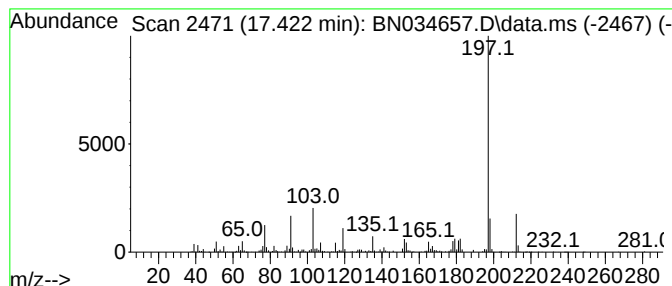

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034657.D
Acq On : 18 Oct 2024 19:54
Operator : RC/JU
Sample : P4380-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E27G6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Phenol, 4-(1-me...	17.422	3.0	ng/ul	508161	4	17.040	3443150	20.0