

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
 Data File : BN034663.D
 Acq On : 19 Oct 2024 00:29
 Operator : RC/JU
 Sample : PB164251BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034663.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.964	9	13	28	rVB	323922	460797	7.94%	0.631%
2	3.211	51	55	66	rVB	112732	155461	2.68%	0.213%
3	3.605	118	122	144	rBV	1525853	2117475	36.49%	2.898%
4	3.928	172	177	181	rBV	21167	30852	0.53%	0.042%
5	6.840	663	672	682	rBV	1544419	2404761	41.44%	3.291%
6	7.005	693	700	708	rVB	1319194	1963514	33.83%	2.687%
7	7.199	725	733	741	rBV	1603278	2423737	41.76%	3.317%
8	7.663	803	812	820	rBV	1447210	2204252	37.98%	3.017%
9	8.363	923	931	944	rBV	1853643	2889683	49.79%	3.955%
10	8.804	999	1006	1016	rBV	1413715	2284112	39.36%	3.126%
11	9.522	1120	1128	1140	rBV	1024262	1664997	28.69%	2.279%
12	10.057	1212	1219	1230	rBV	1600926	2659522	45.83%	3.640%
13	10.440	1275	1284	1295	rVB	1866449	3054856	52.64%	4.181%
14	10.569	1299	1306	1320	rBV	1740117	2900523	49.98%	3.969%
15	11.775	1507	1511	1516	rBV7	3938	6358	0.11%	0.009%
16	12.028	1547	1554	1562	rVB2	33092	54977	0.95%	0.075%
17	12.304	1598	1601	1607	rVB4	4501	7572	0.13%	0.010%
18	13.716	1834	1841	1849	rBV	2395250	3307716	57.00%	4.527%
19	13.986	1880	1887	1896	rBV2	2913140	4351325	74.98%	5.955%
20	14.292	1932	1939	1946	rBV	2357166	3426341	59.04%	4.689%
21	14.492	1966	1973	1991	rBV	1042016	1607842	27.71%	2.200%
22	14.716	2007	2011	2017	rVB9	8738	13216	0.23%	0.018%
23	14.951	2049	2051	2057	rBV7	6710	7966	0.14%	0.011%
24	15.292	2102	2109	2116	rBV	3488905	4859212	83.73%	6.650%
25	15.404	2122	2128	2139	rBV	537441	762679	13.14%	1.044%
26	15.533	2145	2150	2156	rVB2	18666	30304	0.52%	0.041%
27	16.722	2348	2352	2357	rVB8	5465	7694	0.13%	0.011%
28	16.822	2366	2369	2377	rVB4	6099	9782	0.17%	0.013%
29	17.039	2399	2406	2416	rBV	2481702	3481918	60.00%	4.765%
30	17.133	2416	2422	2435	rBV2	3500724	5002315	86.20%	6.846%
31	17.275	2443	2446	2451	rVB7	7180	9041	0.16%	0.012%
32	17.410	2465	2469	2474	rBV3	5429	9922	0.17%	0.014%
33	18.992	2734	2738	2743	rBV2	45718	63390	1.09%	0.087%
34	19.063	2745	2750	2755	rBV	50352	68390	1.18%	0.094%
35	19.427	2806	2812	2823	rBV	3987584	5388541	92.85%	7.374%
36	21.263	3118	3124	3132	rVB	2477417	3564609	61.42%	4.878%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034663.D
Acq On : 19 Oct 2024 00:29
Operator : RC/JU
Sample : PB164251BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK251

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Title : SVOA CALIBRATION

37	23.951	3572	3581	3596	rVB	2522483	5803340	100.00%	7.942%
38	24.145	3605	3614	3624	rBV	1734125	4013899	69.17%	5.493%




Sum of corrected areas: 73072891

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034663.D
Acq On : 19 Oct 2024 00:29
Operator : RC/JU
Sample : PB164251BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

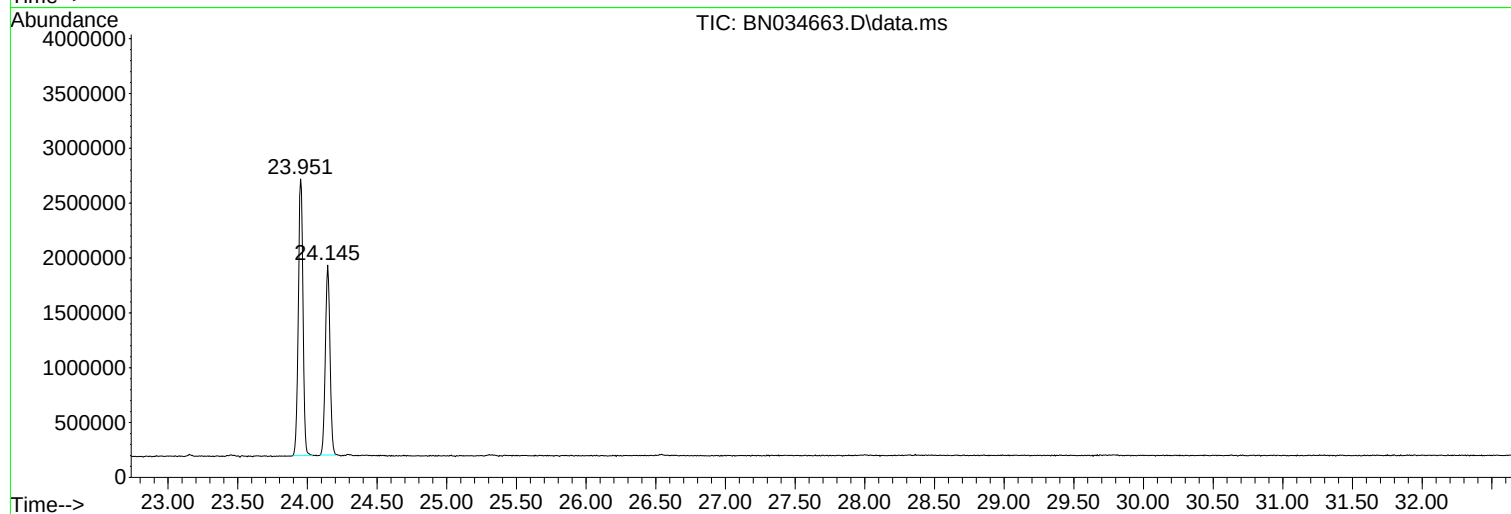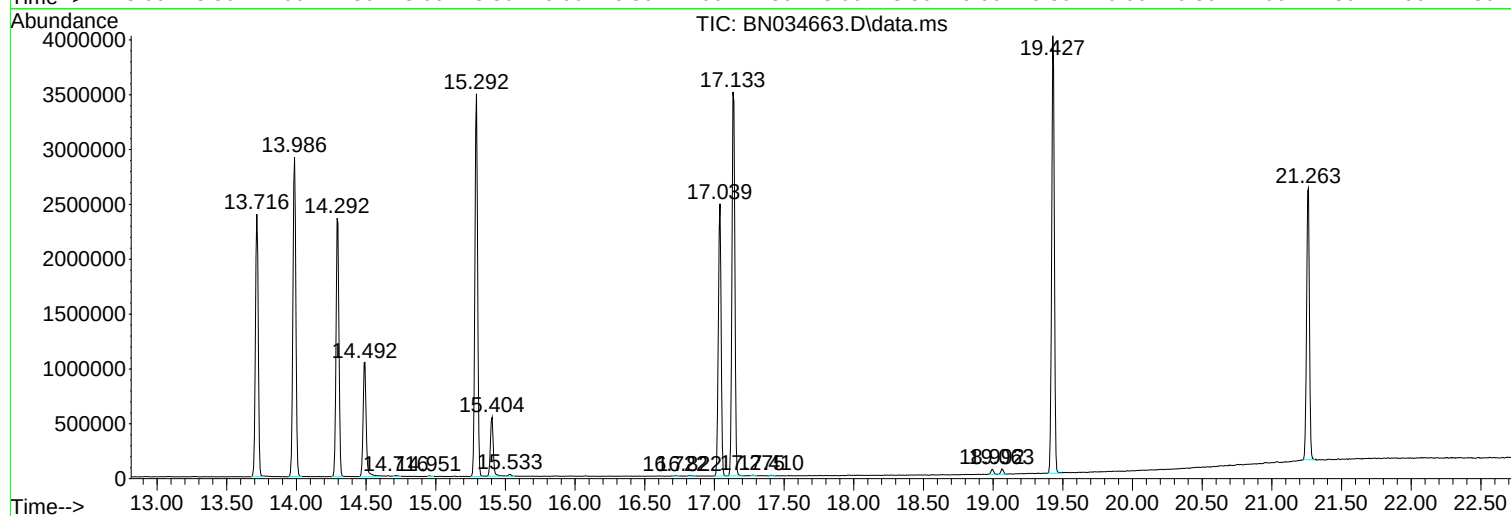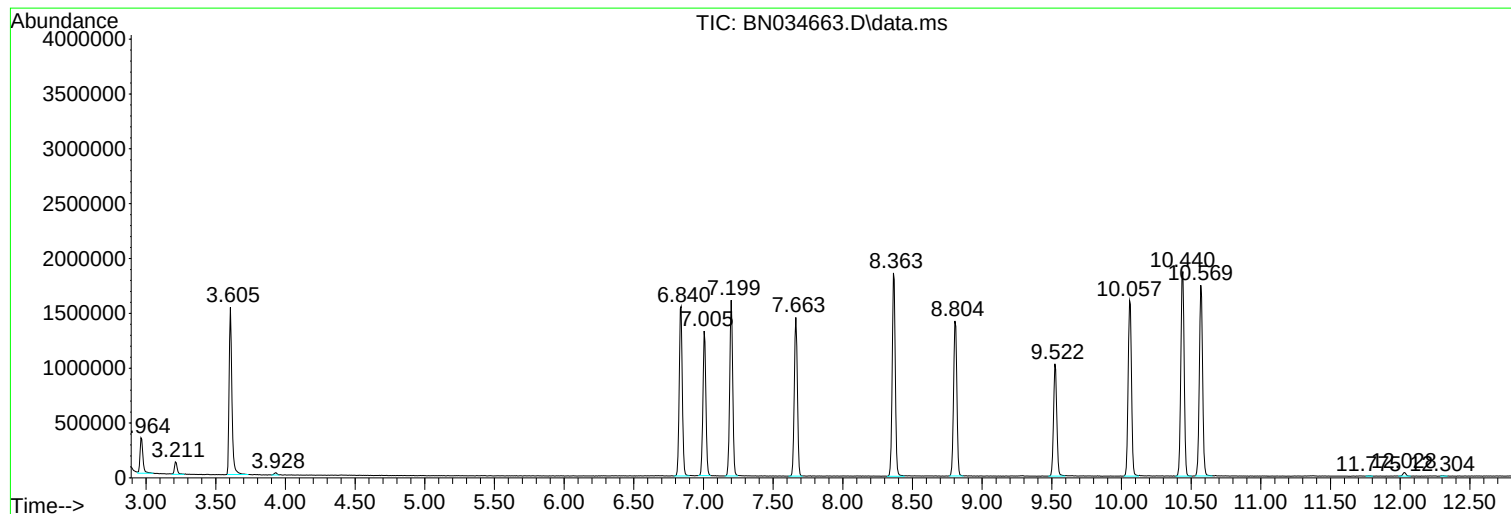

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034663.D
Acq On : 19 Oct 2024 00:29
Operator : RC/JU
Sample : PB164251BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101724\
Data File : BN034663.D
Acq On : 19 Oct 2024 00:29
Operator : RC/JU
Sample : PB164251BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------