
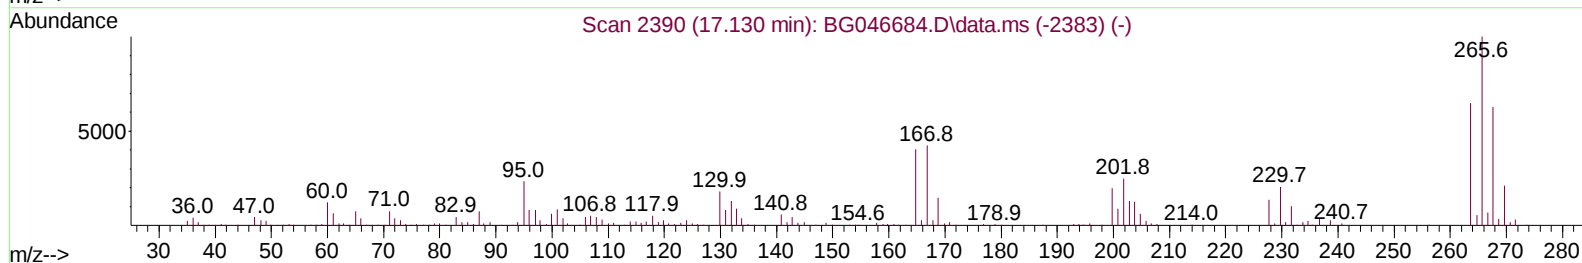
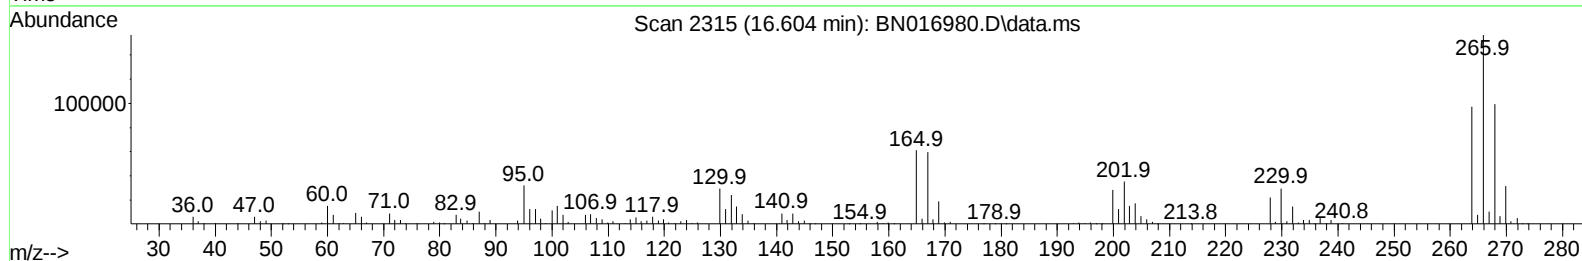


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101821\
Data File : BN016980.D
Acq On : 18 Oct 2021 09:41
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 11:32:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 17:23:48 2021
Response via : Initial Calibration

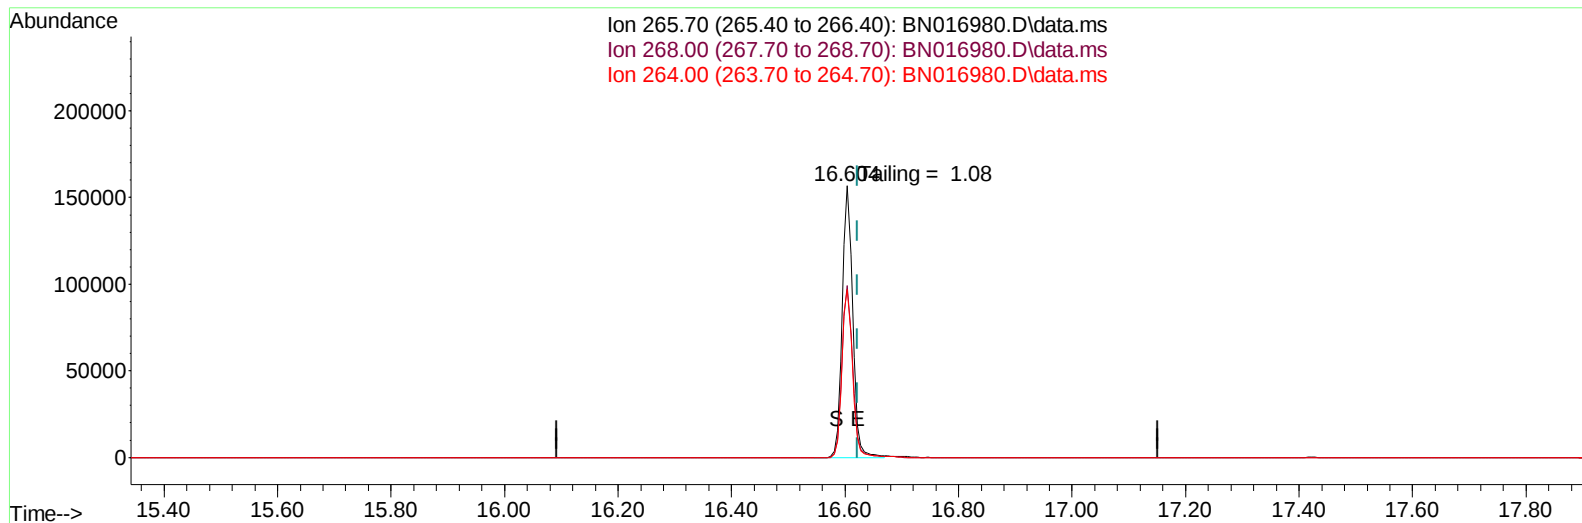

TIC: BN016980.D\data.ms

(70) Pentachlorophenol (C)




16.604min (-0.018) 27072.33 ng

response 201834

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.38
264.00	61.60	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101821\
Data File : BN016980.D
Acq On : 18 Oct 2021 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 11:32:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 17:23:48 2021
Response via : Initial Calibration

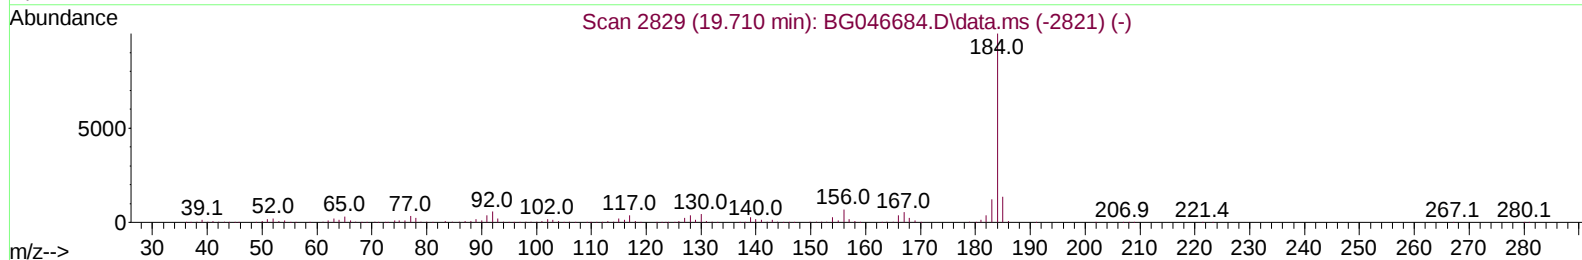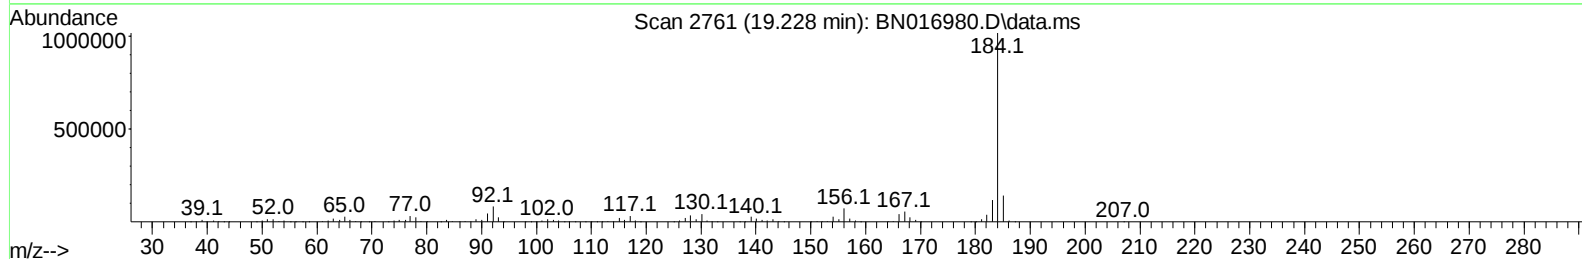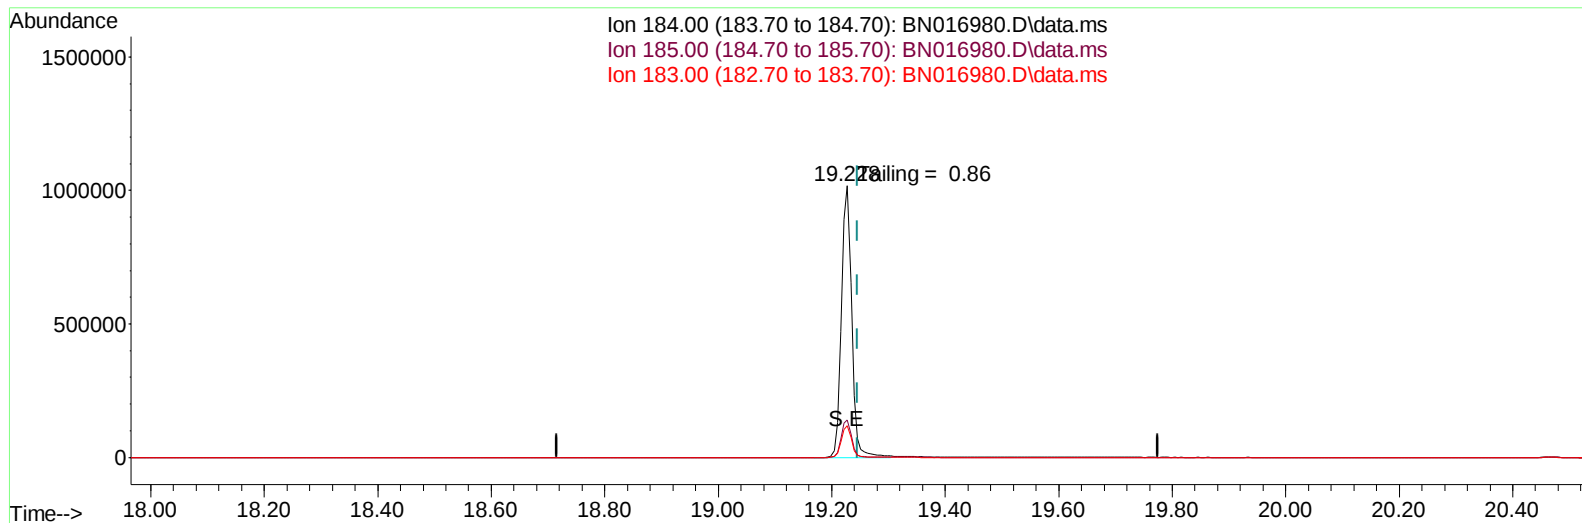

TIC: BN016980.D\data.ms

(77) Benzidine

19.228min (-0.018) 0.00 ng

response 1298919

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	11.63
0.00	0.00	0.00