
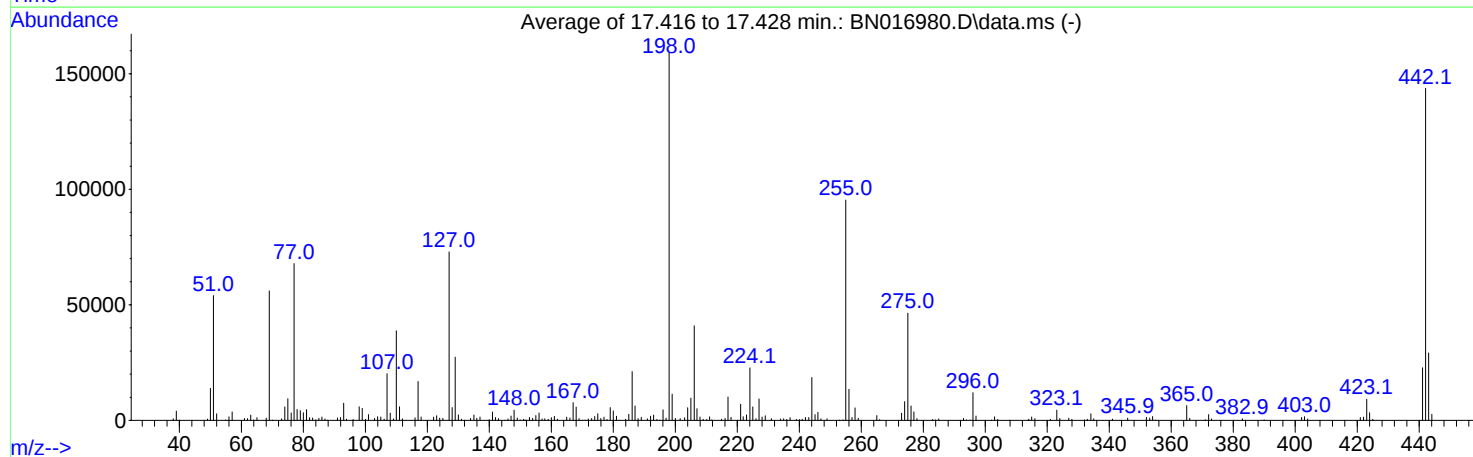


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101821\
 Data File : BN016980.D
 Acq On : 18 Oct 2021 09:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 18 15:14:53 2021

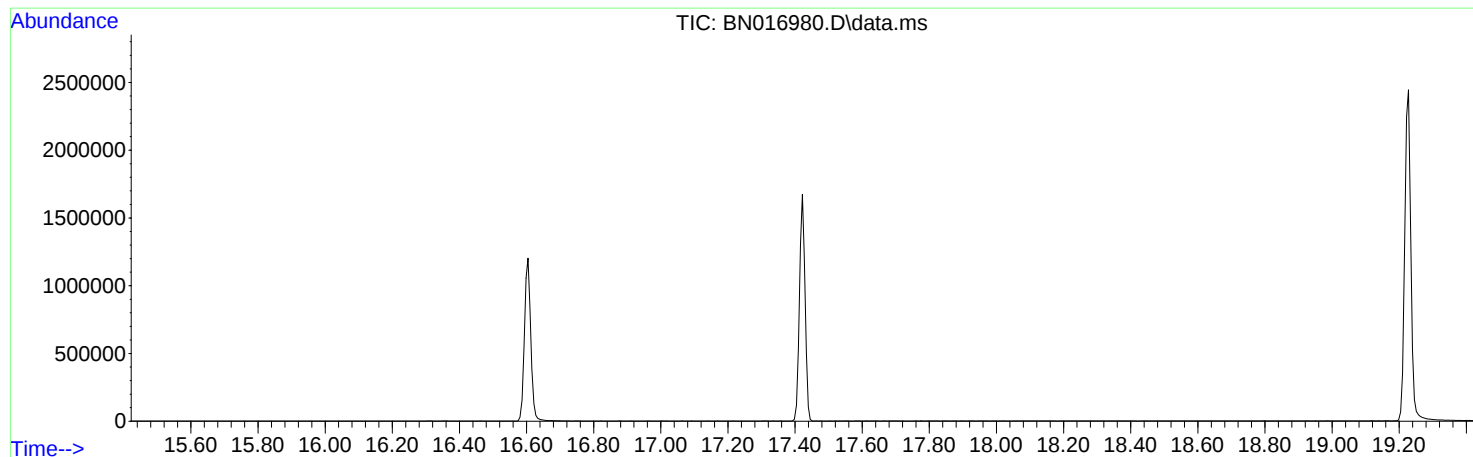




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	54045	PASS
68	69	0.00	2	1.8	993	PASS
69	198	0.00	100	35.2	56024	PASS
70	69	0.00	2	0.2	125	PASS
127	198	10	80	45.8	72947	PASS
197	198	0.00	2	0.6	944	PASS
198	198	100	100	100.0	159211	PASS
199	198	5	9	7.1	11332	PASS
275	198	10	60	29.2	46432	PASS
365	198	1	100	4.0	6403	PASS
441	198	0.01	100	14.3	22800	PASS
442	442	50	100	100.0	143688	PASS
443	442	15	24	20.3	29171	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101821\
Data File : BN016980.D
Acq On : 18 Oct 2021 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 18 11:32:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 17:23:48 2021
Response via : Initial Calibration

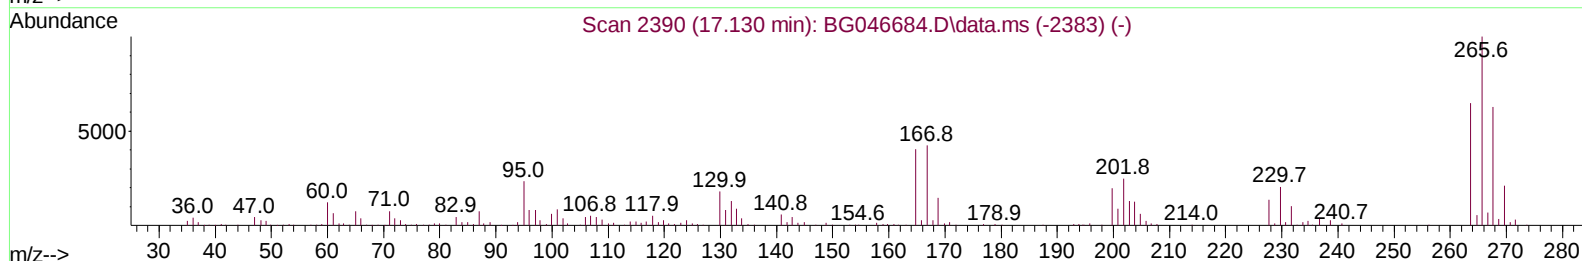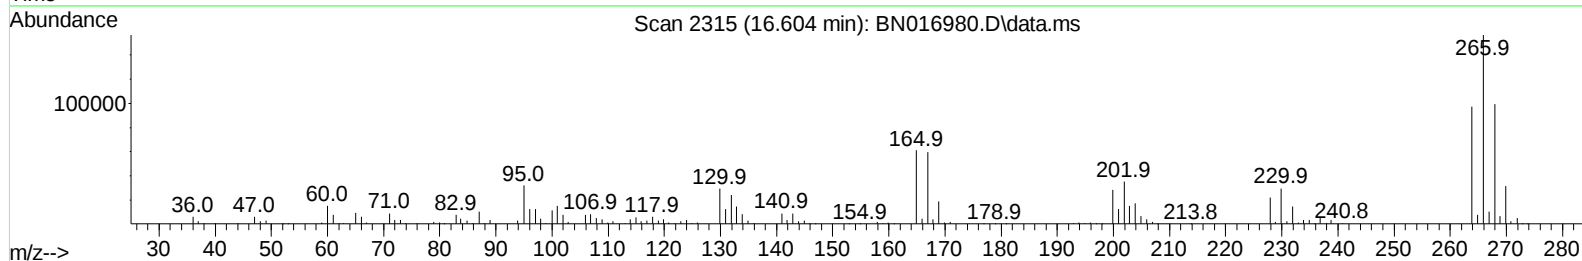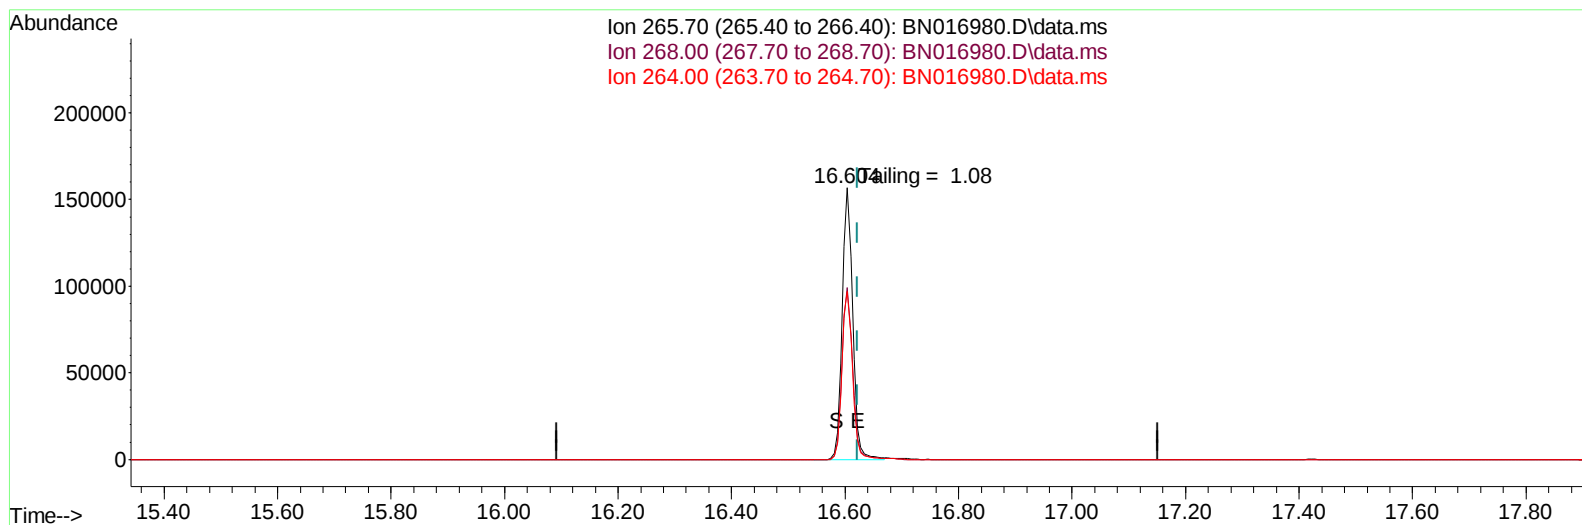

TIC: BN016980.D\data.ms

(70) Pentachlorophenol (C)

16.604min (-0.018) 27072.33 ng




response 201834

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.38
264.00	61.60	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101821\
Data File : BN016980.D
Acq On : 18 Oct 2021 09:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 18 11:32:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 17:23:48 2021
Response via : Initial Calibration

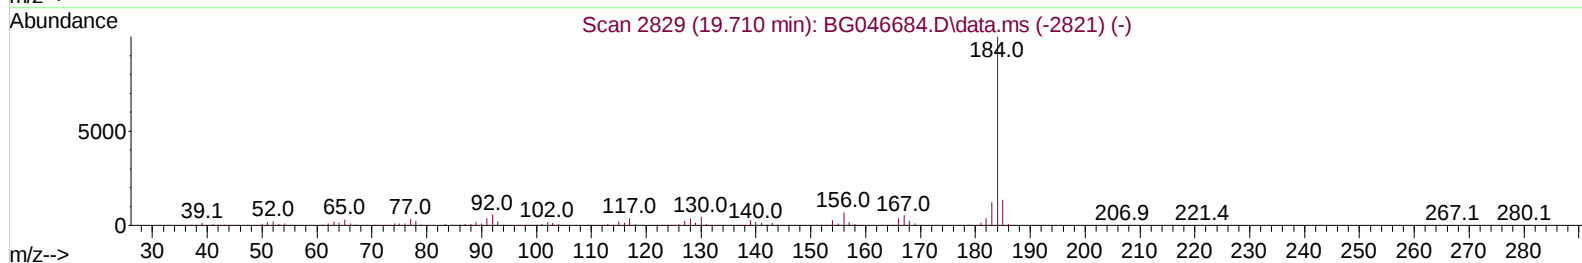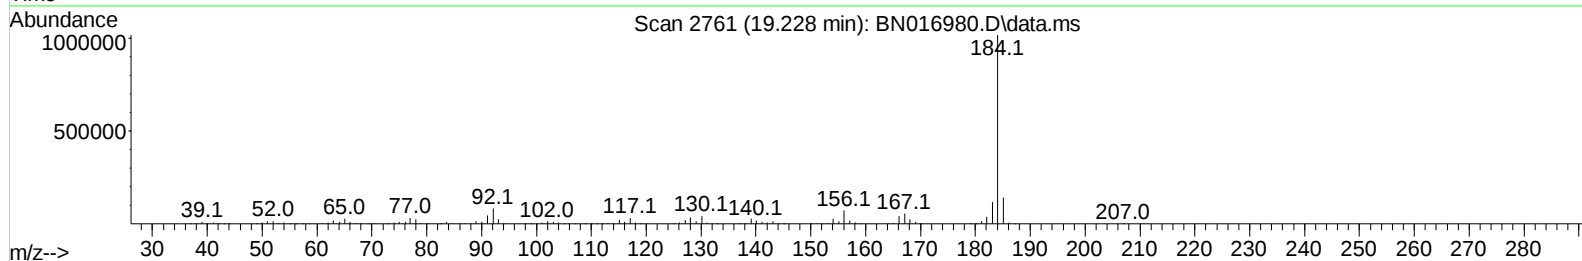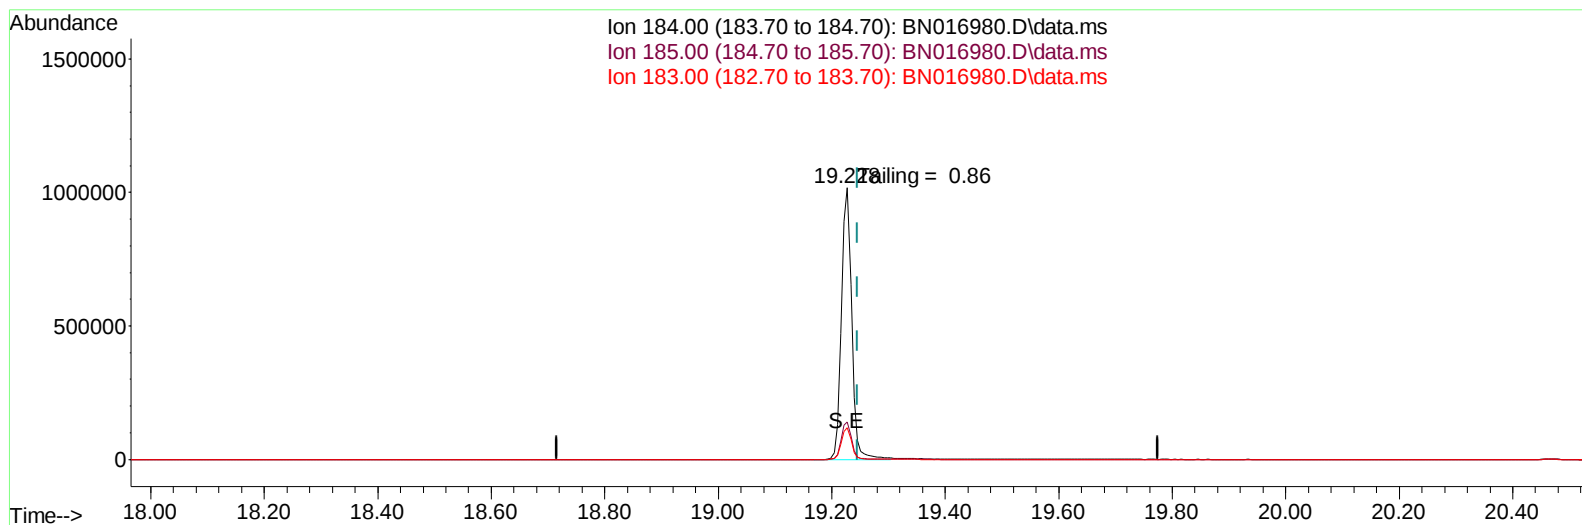

TIC: BN016980.D\data.ms

(77) Benzidine

19.228min (-0.018) 0.00 ng

response 1298919

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/18/2021	BNA_N	<u>BN016980.D</u>
Compound Name	Response	Retention Time
DDT	614057	20.469
DDD	2146	20.028
DDE	0	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2146	616203	0.35

Instrument :
BNA_N
ClientSampleId :
DFTPP